

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030419.D
 Acq On : 05 Aug 2022 10:45
 Operator : JC/MD
 Sample : N4021-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030419.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	56	rVB2	257150	305137	24.33%	3.157%
2	1.666	91	95	103	rVB	128826	156510	12.48%	1.620%
3	2.306	194	200	209	rBV	254668	387523	30.90%	4.010%
4	2.392	211	214	219	rBV3	1361	1830	0.15%	0.019%
5	2.489	227	230	231	rBV	443	505	0.04%	0.005%
6	2.501	231	232	233	rBV	592	396	0.03%	0.004%
7	2.696	262	264	268	rVB2	431	522	0.04%	0.005%
8	2.751	271	273	275	rVB2	524	404	0.03%	0.004%
9	2.892	294	296	297	rBV2	366	316	0.03%	0.003%
10	2.977	308	310	312	rBV2	294	391	0.03%	0.004%
11	3.020	315	317	318	rBV	588	306	0.02%	0.003%
12	3.093	322	329	335	rBV2	10146	18166	1.45%	0.188%
13	3.263	355	357	360	rBV2	587	517	0.04%	0.005%
14	3.654	420	421	424	rBV	494	557	0.04%	0.006%
15	3.885	456	459	462	rBV2	427	615	0.05%	0.006%
16	3.922	462	465	468	rVV2	330	474	0.04%	0.005%
17	4.032	480	483	489	rBV	489	817	0.07%	0.008%
18	4.080	489	491	494	rBV	254	328	0.03%	0.003%
19	4.257	518	520	523	rBV	360	461	0.04%	0.005%
20	4.477	545	556	574	rBV3	145528	539250	43.00%	5.580%
21	5.056	639	651	673	rVV2	166086	510855	40.74%	5.286%
22	5.208	675	676	682	rVB2	693	826	0.07%	0.009%
23	5.287	687	689	691	rBV	553	348	0.03%	0.004%
24	5.379	700	704	705	rBV2	811	672	0.05%	0.007%
25	5.519	724	727	729	rBV3	601	776	0.06%	0.008%
26	5.544	729	731	732	rBV	787	435	0.03%	0.005%
27	5.726	759	761	766	rVB2	320	464	0.04%	0.005%
28	5.775	766	769	770	rBV3	535	439	0.04%	0.005%
29	5.818	775	776	779	rBV	527	425	0.03%	0.004%
30	5.842	779	780	783	rVB2	417	400	0.03%	0.004%
31	5.970	788	801	819	rBV2	420569	1253997	100.00%	12.976%
32	6.293	852	854	855	rBV	690	457	0.04%	0.005%
33	6.330	859	860	863	rBV	429	411	0.03%	0.004%
34	6.354	863	864	866	rVB2	545	335	0.03%	0.003%
35	6.458	878	881	882	rBV2	543	553	0.04%	0.006%
36	6.763	920	931	946	rBV	279983	659026	52.55%	6.819%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030419.D
 Acq On : 05 Aug 2022 10:45
 Operator : JC/MD
 Sample : N4021-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.897	952	953	956	rVB	591	381	0.03%	0.004%
38	7.129	982	991	1006	rVB4	59393	143921	11.48%	1.489%
39	7.238	1006	1009	1012	rBV3	333	557	0.04%	0.006%
40	7.312	1012	1021	1034	rBV	256026	566178	45.15%	5.859%
41	7.580	1063	1065	1067	rVV	399	381	0.03%	0.004%
42	7.598	1067	1068	1073	rVV2	550	637	0.05%	0.007%
43	7.781	1095	1098	1100	rBV2	497	495	0.04%	0.005%
44	7.946	1119	1125	1130	rVV4	983	1985	0.16%	0.021%
45	8.256	1174	1176	1178	rVB	709	555	0.04%	0.006%
46	8.324	1181	1187	1198	rBV	178241	298057	23.77%	3.084%
47	8.458	1207	1209	1211	rVB3	639	413	0.03%	0.004%
48	8.494	1211	1215	1217	rBV3	833	1191	0.09%	0.012%
49	8.561	1222	1226	1227	rBV2	678	651	0.05%	0.007%
50	8.653	1234	1241	1250	rBV	610662	989353	78.90%	10.238%
51	8.842	1270	1272	1273	rBV	418	372	0.03%	0.004%
52	8.951	1284	1290	1297	rBV	135763	198386	15.82%	2.053%
53	9.281	1340	1344	1348	rVB5	4026	5495	0.44%	0.057%
54	9.336	1352	1353	1356	rBV2	471	444	0.04%	0.005%
55	9.384	1356	1361	1377	rBV	478112	689751	55.00%	7.137%
56	9.781	1424	1426	1428	rBV2	478	387	0.03%	0.004%
57	10.055	1465	1471	1480	rBV	584334	770432	61.44%	7.972%
58	10.250	1501	1503	1505	rVB2	812	550	0.04%	0.006%
59	10.274	1505	1507	1509	rBV2	445	403	0.03%	0.004%
60	10.299	1509	1511	1512	rBV	493	325	0.03%	0.003%
61	10.317	1512	1514	1517	rVB3	435	394	0.03%	0.004%
62	10.390	1524	1526	1527	rBV2	441	331	0.03%	0.003%
63	10.537	1549	1550	1555	rBV4	460	638	0.05%	0.007%
64	10.585	1555	1558	1561	rVV2	442	612	0.05%	0.006%
65	10.616	1561	1563	1565	rVB	618	376	0.03%	0.004%
66	10.726	1580	1581	1585	rBV2	374	499	0.04%	0.005%
67	10.805	1593	1594	1596	rBV2	390	351	0.03%	0.004%
68	10.860	1602	1603	1607	rVB	598	429	0.03%	0.004%
69	10.963	1618	1620	1621	rBV	669	353	0.03%	0.004%
70	11.012	1626	1628	1630	rBV	606	464	0.04%	0.005%
71	11.036	1630	1632	1633	rBV	426	314	0.03%	0.003%
72	11.085	1638	1640	1648	rVB2	553	826	0.07%	0.009%
73	11.195	1653	1658	1667	rVB	440632	573042	45.70%	5.930%
74	11.317	1675	1678	1680	rBV	662	661	0.05%	0.007%
75	11.353	1682	1684	1688	rBV3	497	782	0.06%	0.008%
76	11.402	1688	1692	1694	rBV2	219	314	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030419.D
 Acq On : 05 Aug 2022 10:45
 Operator : JC/MD
 Sample : N4021-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.445	1697	1699	1702	rBV	415	318	0.03%	0.003%
78	11.677	1735	1737	1741	rVB2	380	469	0.04%	0.005%
79	11.713	1741	1743	1744	rBV2	557	381	0.03%	0.004%
80	12.024	1788	1794	1802	rBV	597089	717952	57.25%	7.429%
81	12.219	1824	1826	1828	rBV	328	336	0.03%	0.003%
82	12.268	1832	1834	1836	rBV2	290	335	0.03%	0.003%
83	12.323	1837	1843	1850	rBV	663393	839300	66.93%	8.685%
84	12.628	1890	1893	1896	rBV	463	846	0.07%	0.009%
85	12.774	1916	1917	1920	rBV	535	414	0.03%	0.004%
86	13.036	1959	1960	1963	rBV	429	319	0.03%	0.003%
87	13.067	1963	1965	1967	rBV	417	328	0.03%	0.003%
88	13.146	1976	1978	1979	rBV2	530	474	0.04%	0.005%
89	13.262	1995	1997	1998	rBV	577	383	0.03%	0.004%
90	13.280	1998	2000	2002	rVV	424	387	0.03%	0.004%
91	13.493	2033	2035	2041	rBV3	482	860	0.07%	0.009%
92	13.615	2053	2055	2057	rBV2	322	339	0.03%	0.004%
93	13.634	2057	2058	2061	rVB2	389	321	0.03%	0.003%
94	13.969	2110	2113	2114	rBV2	431	473	0.04%	0.005%
95	14.005	2117	2119	2120	rVB2	674	462	0.04%	0.005%
96	14.030	2120	2123	2124	rBV	663	560	0.04%	0.006%
97	14.444	2190	2191	2193	rVV	564	344	0.03%	0.004%
98	14.469	2193	2195	2197	rVV2	544	406	0.03%	0.004%
99	14.493	2197	2199	2201	rVB	516	415	0.03%	0.004%
100	16.292	2493	2494	2496	rBV2	769	388	0.03%	0.004%




Sum of corrected areas: 9663940

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030419.D
Acq On : 05 Aug 2022 10:45
Operator : JC/MD
Sample : N4021-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

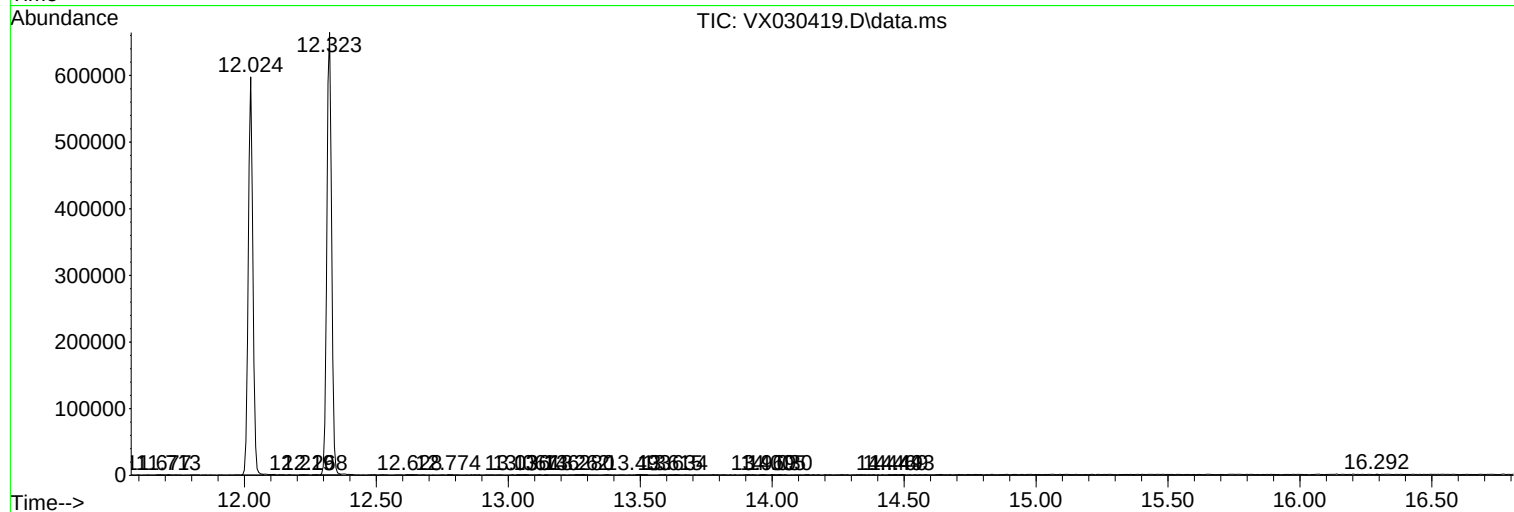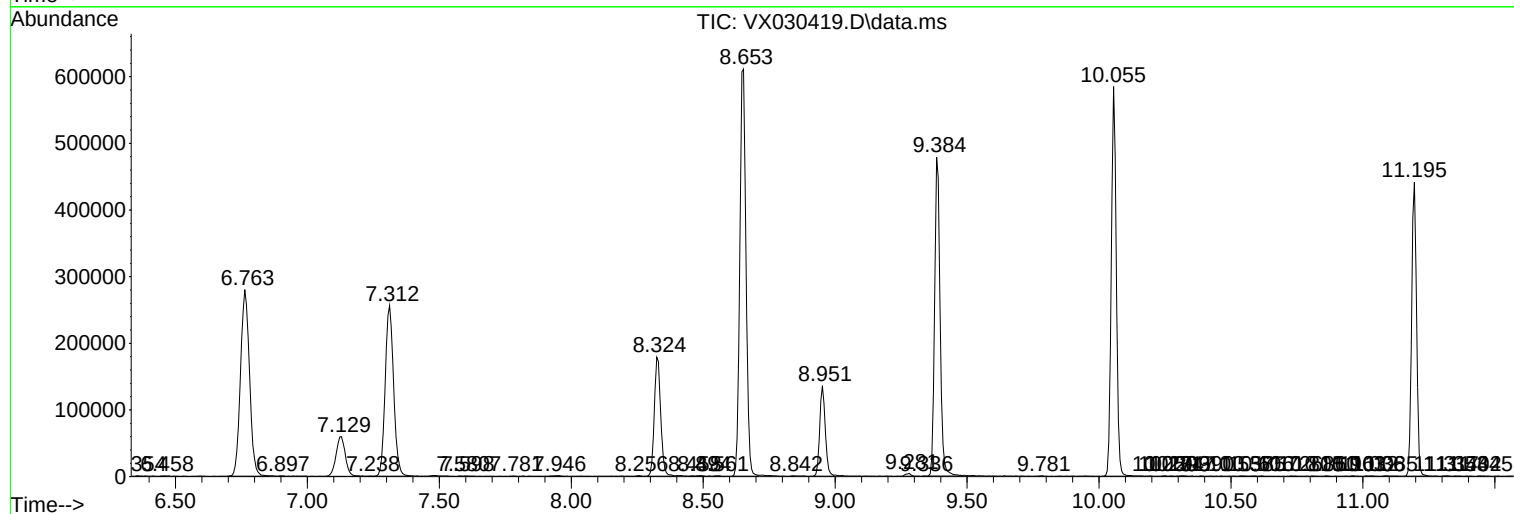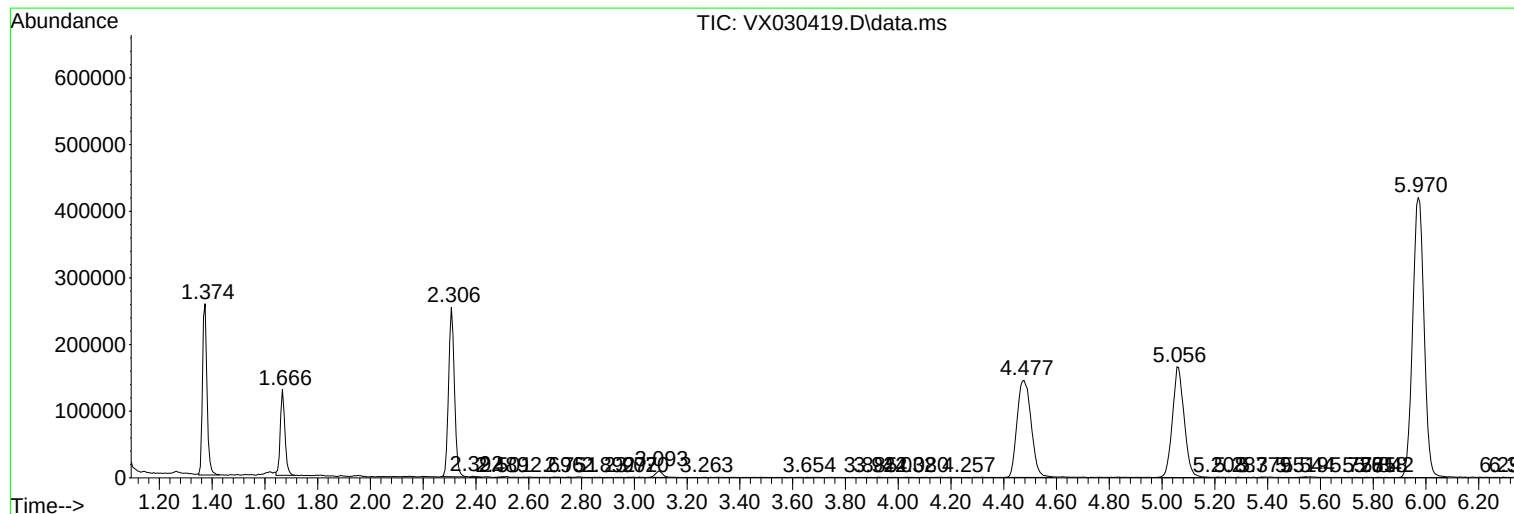

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030419.D
Acq On : 05 Aug 2022 10:45
Operator : JC/MD
Sample : N4021-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030419.D
Acq On : 05 Aug 2022 10:45
Operator : JC/MD
Sample : N4021-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc