

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030420.D
 Acq On : 05 Aug 2022 11:08
 Operator : JC/MD
 Sample : N4021-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030420.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB2	258424	297506	24.15%	3.142%
2	1.666	91	95	104	rVB	117915	149561	12.14%	1.579%
3	2.306	194	200	210	rVB	239315	371028	30.12%	3.918%
4	2.611	248	250	254	rBV2	548	635	0.05%	0.007%
5	2.648	254	256	257	rBV	471	328	0.03%	0.003%
6	2.715	264	267	270	rBV2	454	721	0.06%	0.008%
7	2.782	276	278	280	rBV3	495	470	0.04%	0.005%
8	3.099	321	330	337	rBV	8774	17623	1.43%	0.186%
9	3.251	351	355	356	rBV2	441	589	0.05%	0.006%
10	3.331	365	368	370	rBV2	366	380	0.03%	0.004%
11	3.434	384	385	392	rVB2	306	539	0.04%	0.006%
12	3.648	417	420	423	rVV2	336	358	0.03%	0.004%
13	3.739	432	435	437	rBV2	449	581	0.05%	0.006%
14	3.849	449	453	454	rBV2	344	538	0.04%	0.006%
15	3.873	456	457	459	rVV	438	310	0.03%	0.003%
16	4.099	491	494	496	rVV2	484	411	0.03%	0.004%
17	4.306	525	528	530	rBV	429	416	0.03%	0.004%
18	4.330	530	532	534	rVV2	414	379	0.03%	0.004%
19	4.379	539	540	543	rBV2	385	344	0.03%	0.004%
20	4.477	543	556	573	rBV2	144997	528593	42.90%	5.582%
21	4.739	595	599	601	rVB4	339	309	0.03%	0.003%
22	4.940	630	632	633	rBV2	436	287	0.02%	0.003%
23	4.971	635	637	639	rVV2	549	419	0.03%	0.004%
24	5.056	641	651	670	rVV	156360	494063	40.10%	5.218%
25	5.233	678	680	682	rBV	638	402	0.03%	0.004%
26	5.251	682	683	685	rBV2	365	281	0.02%	0.003%
27	5.385	700	705	707	rBV4	1318	2198	0.18%	0.023%
28	5.556	727	733	742	rVB3	2910	6715	0.55%	0.071%
29	5.623	742	744	747	rBV2	369	437	0.04%	0.005%
30	5.653	747	749	752	rVB2	372	373	0.03%	0.004%
31	5.696	754	756	758	rBV2	321	277	0.02%	0.003%
32	5.977	789	802	822	rBV2	414935	1232025	100.00%	13.011%
33	6.257	842	848	850	rBV2	302	670	0.05%	0.007%
34	6.342	861	862	864	rBV	366	299	0.02%	0.003%
35	6.373	864	867	868	rVV	415	406	0.03%	0.004%
36	6.428	875	876	878	rVB	610	298	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030420.D
 Acq On : 05 Aug 2022 11:08
 Operator : JC/MD
 Sample : N4021-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.458	878	881	884	rBV3	572	836	0.07%	0.009%
38	6.647	910	912	914	rBV2	455	474	0.04%	0.005%
39	6.702	920	921	922	rBV	515	316	0.03%	0.003%
40	6.763	922	931	945	rVV	270853	664283	53.92%	7.015%
41	6.958	961	963	964	rBV2	465	397	0.03%	0.004%
42	7.001	966	970	971	rVB3	495	444	0.04%	0.005%
43	7.129	982	991	1000	rVV6	50616	124193	10.08%	1.312%
44	7.226	1005	1007	1009	rVB	654	370	0.03%	0.004%
45	7.312	1013	1021	1034	rBV	253805	560685	45.51%	5.921%
46	7.488	1045	1050	1053	rBV2	910	1578	0.13%	0.017%
47	7.623	1071	1072	1073	rBV	496	333	0.03%	0.004%
48	7.659	1076	1078	1079	rVV	479	393	0.03%	0.004%
49	7.684	1080	1082	1084	rVB2	528	365	0.03%	0.004%
50	7.812	1099	1103	1105	rBV2	608	792	0.06%	0.008%
51	7.836	1105	1107	1111	rVV2	466	546	0.04%	0.006%
52	7.879	1111	1114	1117	rVV	540	476	0.04%	0.005%
53	8.165	1158	1161	1162	rBV2	356	351	0.03%	0.004%
54	8.330	1180	1188	1197	rBV	180653	295478	23.98%	3.120%
55	8.580	1228	1229	1232	rVB2	660	489	0.04%	0.005%
56	8.653	1234	1241	1249	rBV	623211	966528	78.45%	10.207%
57	8.854	1272	1274	1276	rBV	511	639	0.05%	0.007%
58	8.952	1284	1290	1300	rBV	131445	193254	15.69%	2.041%
59	9.055	1306	1307	1310	rVB2	687	555	0.05%	0.006%
60	9.086	1310	1312	1315	rVV2	650	538	0.04%	0.006%
61	9.128	1317	1319	1320	rVB2	560	287	0.02%	0.003%
62	9.275	1336	1343	1349	rBV3	3515	5453	0.44%	0.058%
63	9.391	1356	1362	1375	rBV	479693	693486	56.29%	7.324%
64	9.720	1413	1416	1421	rBV2	442	505	0.04%	0.005%
65	9.817	1430	1432	1434	rVB	452	379	0.03%	0.004%
66	9.842	1434	1436	1437	rBV2	316	302	0.02%	0.003%
67	9.884	1441	1443	1444	rBV	425	344	0.03%	0.004%
68	9.994	1458	1461	1463	rBV2	396	526	0.04%	0.006%
69	10.055	1465	1471	1482	rBV	563751	753300	61.14%	7.955%
70	10.250	1499	1503	1505	rBV3	404	623	0.05%	0.007%
71	10.354	1518	1520	1524	rBV2	384	342	0.03%	0.004%
72	10.494	1540	1543	1544	rBV2	244	287	0.02%	0.003%
73	10.567	1554	1555	1558	rBV	396	359	0.03%	0.004%
74	10.622	1562	1564	1566	rBV2	286	300	0.02%	0.003%
75	10.781	1589	1590	1594	rVV2	334	364	0.03%	0.004%
76	10.896	1607	1609	1610	rBV2	423	305	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030420.D
 Acq On : 05 Aug 2022 11:08
 Operator : JC/MD
 Sample : N4021-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.195	1652	1658	1665	rBV	446520	562308	45.64%	5.938%
78	11.567	1718	1719	1722	rBV	497	457	0.04%	0.005%
79	11.799	1755	1757	1760	rVB3	462	431	0.03%	0.005%
80	11.902	1772	1774	1778	rVV2	315	292	0.02%	0.003%
81	12.024	1789	1794	1802	rBV	570749	688658	55.90%	7.273%
82	12.323	1837	1843	1855	rBV	644360	826328	67.07%	8.727%
83	12.408	1855	1857	1860	rVB2	843	666	0.05%	0.007%
84	12.439	1860	1862	1865	rVB2	542	458	0.04%	0.005%
85	12.677	1900	1901	1903	rBV	385	283	0.02%	0.003%
86	12.780	1917	1918	1920	rBV2	382	309	0.03%	0.003%
87	12.847	1926	1929	1930	rBV2	352	341	0.03%	0.004%
88	13.109	1969	1972	1973	rBV	509	410	0.03%	0.004%
89	13.280	1999	2000	2003	rBV	421	420	0.03%	0.004%
90	13.500	2034	2036	2041	rBV2	400	547	0.04%	0.006%
91	13.682	2065	2066	2068	rBV	503	311	0.03%	0.003%
92	13.847	2091	2093	2095	rBV2	373	376	0.03%	0.004%
93	14.085	2130	2132	2134	rBV	384	313	0.03%	0.003%
94	14.231	2154	2156	2157	rBV2	626	524	0.04%	0.006%
95	14.329	2169	2172	2175	rVB3	584	574	0.05%	0.006%
96	14.737	2237	2239	2241	rBV2	416	313	0.03%	0.003%
97	14.816	2250	2252	2253	rBV	605	316	0.03%	0.003%
98	15.469	2358	2359	2363	rVB4	807	995	0.08%	0.011%
99	15.511	2363	2366	2368	rBV3	517	678	0.06%	0.007%
100	16.298	2494	2495	2497	rBV2	785	556	0.05%	0.006%




Sum of corrected areas: 9469108

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030420.D
Acq On : 05 Aug 2022 11:08
Operator : JC/MD
Sample : N4021-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

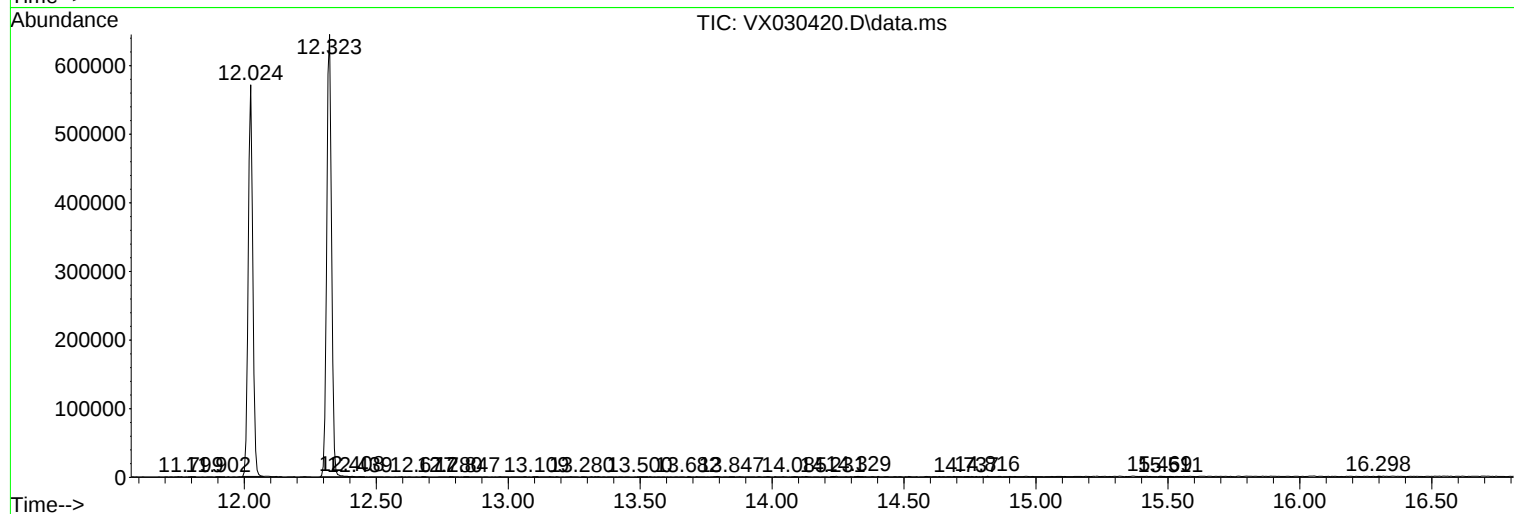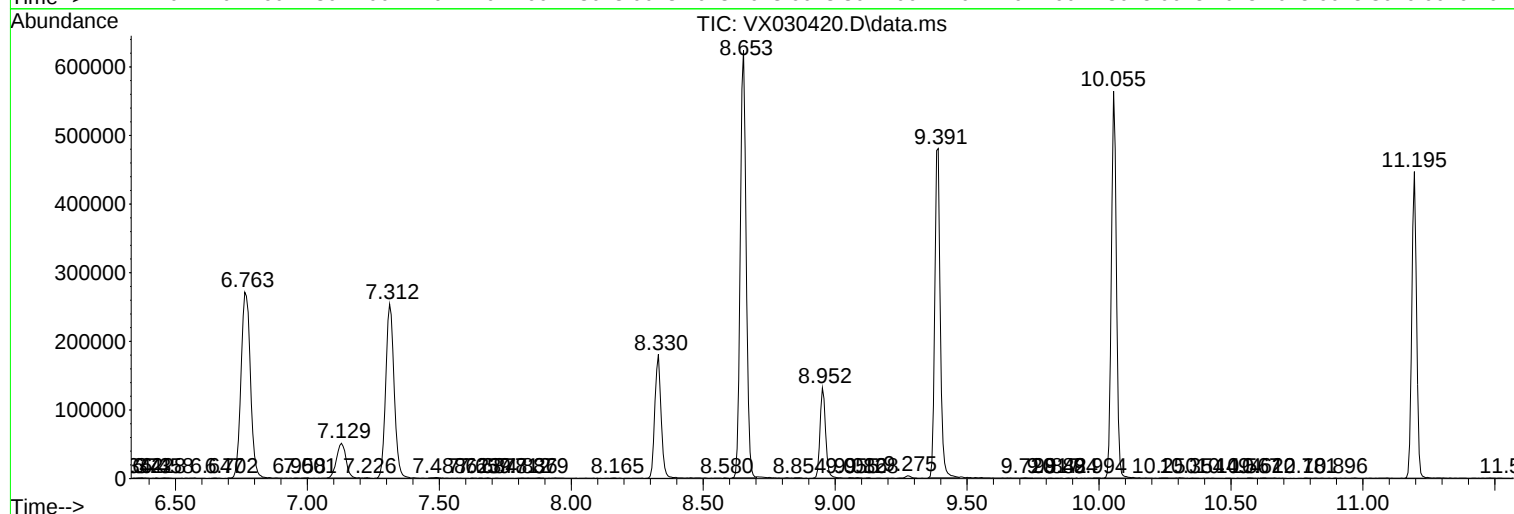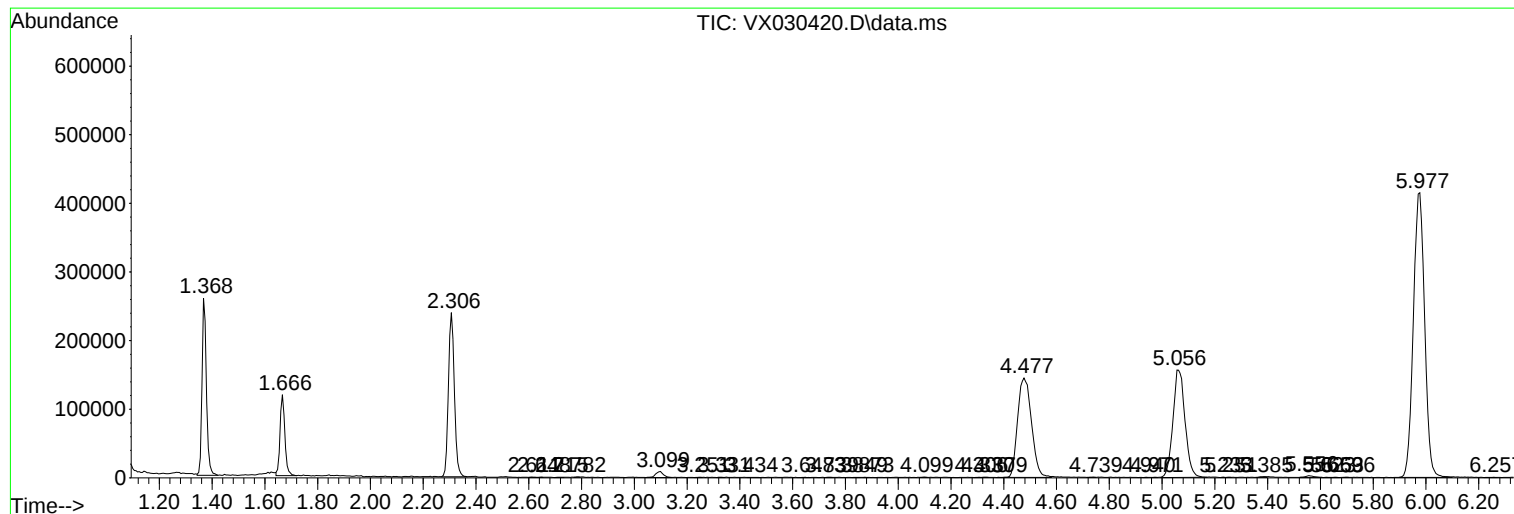

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030420.D
Acq On : 05 Aug 2022 11:08
Operator : JC/MD
Sample : N4021-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030420.D
Acq On : 05 Aug 2022 11:08
Operator : JC/MD
Sample : N4021-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc