

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030424.D
 Acq On : 05 Aug 2022 13:02
 Operator : JC/MD
 Sample : N4003-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030424.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB	159095	161303	13.71%	1.732%
2	1.666	91	95	107	rVB	112551	140005	11.90%	1.503%
3	2.050	156	158	159	rBV2	1057	852	0.07%	0.009%
4	2.221	184	186	187	rBV	847	434	0.04%	0.005%
5	2.306	194	200	210	rVB	243789	364124	30.94%	3.909%
6	2.508	229	233	235	rBV2	821	1082	0.09%	0.012%
7	2.550	238	240	242	rVB2	485	371	0.03%	0.004%
8	2.636	252	254	257	rVB	425	389	0.03%	0.004%
9	2.721	267	268	271	rVB	786	497	0.04%	0.005%
10	2.782	276	278	284	rVV3	1258	1875	0.16%	0.020%
11	3.093	323	329	338	rVB3	4595	8591	0.73%	0.092%
12	3.172	338	342	345	rBV3	322	404	0.03%	0.004%
13	3.251	350	355	356	rBV2	277	345	0.03%	0.004%
14	3.453	385	388	390	rVB4	476	505	0.04%	0.005%
15	3.611	411	414	416	rBV	463	454	0.04%	0.005%
16	3.733	431	434	436	rVB3	410	523	0.04%	0.006%
17	4.343	531	534	536	rBV	542	456	0.04%	0.005%
18	4.489	545	558	574	rBV2	261095	883576	75.09%	9.486%
19	4.672	585	588	589	rBV2	554	475	0.04%	0.005%
20	4.776	604	605	608	rBV	473	435	0.04%	0.005%
21	5.062	639	652	667	rBV	162241	487476	41.43%	5.233%
22	5.349	695	699	701	rBV2	477	573	0.05%	0.006%
23	5.397	701	707	712	rVV4	1171	3321	0.28%	0.036%
24	5.562	726	734	739	rBV4	1724	4321	0.37%	0.046%
25	5.977	790	802	821	rBV2	397313	1176692	100.00%	12.633%
26	6.251	842	847	848	rBV	245	373	0.03%	0.004%
27	6.348	861	863	865	rBV2	492	504	0.04%	0.005%
28	6.452	878	880	883	rVB	572	639	0.05%	0.007%
29	6.483	883	885	887	rVB2	802	494	0.04%	0.005%
30	6.531	891	893	894	rBV	593	517	0.04%	0.006%
31	6.769	922	932	945	rBV	275508	657969	55.92%	7.064%
32	7.117	982	989	999	rVV5	13745	35520	3.02%	0.381%
33	7.312	1013	1021	1033	rBV	237778	535290	45.49%	5.747%
34	7.470	1045	1047	1049	rBV2	615	586	0.05%	0.006%
35	7.818	1101	1104	1106	rVB2	437	394	0.03%	0.004%
36	7.933	1121	1123	1125	rBV	789	702	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030424.D
 Acq On : 05 Aug 2022 13:02
 Operator : JC/MD
 Sample : N4003-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	8.226	1168	1171	1174	rBV2	245	382	0.03%	0.004%
38	8.330	1181	1188	1200	rBV	166240	276358	23.49%	2.967%
39	8.586	1225	1230	1233	rBV3	672	1166	0.10%	0.013%
40	8.653	1234	1241	1253	rVV	610654	923559	78.49%	9.915%
41	8.781	1260	1262	1264	rBV2	764	433	0.04%	0.005%
42	8.866	1274	1276	1278	rVB	520	369	0.03%	0.004%
43	8.903	1281	1282	1285	rBV	504	420	0.04%	0.005%
44	8.952	1285	1290	1299	rBV	121710	180977	15.38%	1.943%
45	9.061	1307	1308	1312	rVB2	687	639	0.05%	0.007%
46	9.208	1328	1332	1336	rVB2	599	917	0.08%	0.010%
47	9.281	1339	1344	1349	rVB3	1626	2046	0.17%	0.022%
48	9.384	1356	1361	1375	rBV	460712	680991	57.87%	7.311%
49	9.543	1385	1387	1389	rVB	808	483	0.04%	0.005%
50	9.586	1392	1394	1395	rBV	508	521	0.04%	0.006%
51	9.842	1435	1436	1439	rVB	511	479	0.04%	0.005%
52	9.878	1439	1442	1443	rBV2	558	514	0.04%	0.006%
53	9.915	1446	1448	1449	rBV	488	373	0.03%	0.004%
54	10.055	1466	1471	1480	rVV	549948	746111	63.41%	8.010%
55	10.159	1487	1488	1490	rBV	441	344	0.03%	0.004%
56	10.409	1526	1529	1531	rVB2	420	481	0.04%	0.005%
57	10.439	1531	1534	1536	rBV2	505	510	0.04%	0.005%
58	10.512	1543	1546	1548	rBV2	472	523	0.04%	0.006%
59	10.610	1560	1562	1565	rBB2	417	374	0.03%	0.004%
60	10.640	1565	1567	1571	rBV	348	438	0.04%	0.005%
61	10.695	1574	1576	1578	rVB	704	387	0.03%	0.004%
62	10.841	1598	1600	1603	rVB2	412	437	0.04%	0.005%
63	10.945	1615	1617	1619	rBV	408	429	0.04%	0.005%
64	11.098	1639	1642	1645	rBV2	762	701	0.06%	0.008%
65	11.195	1653	1658	1666	rVV	451674	548418	46.61%	5.888%
66	11.433	1694	1697	1698	rBV2	496	591	0.05%	0.006%
67	11.616	1725	1727	1729	rBV2	437	470	0.04%	0.005%
68	11.719	1741	1744	1745	rVB2	518	505	0.04%	0.005%
69	11.799	1755	1757	1760	rVV2	460	542	0.05%	0.006%
70	11.829	1760	1762	1764	rVB	626	457	0.04%	0.005%
71	11.860	1764	1767	1770	rBV	480	814	0.07%	0.009%
72	11.884	1770	1771	1774	rVB2	537	439	0.04%	0.005%
73	12.024	1789	1794	1801	rBV	567362	684288	58.15%	7.346%
74	12.183	1816	1820	1823	rBV5	630	843	0.07%	0.009%
75	12.225	1823	1827	1829	rBV4	649	824	0.07%	0.009%
76	12.323	1837	1843	1851	rBV	612007	770165	65.45%	8.268%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030424.D
 Acq On : 05 Aug 2022 13:02
 Operator : JC/MD
 Sample : N4003-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.591	1884	1887	1888	rBV2	706	527	0.04%	0.006%
78	12.707	1902	1906	1908	rBV2	612	866	0.07%	0.009%
79	12.737	1910	1911	1913	rBV2	353	348	0.03%	0.004%
80	12.811	1920	1923	1924	rBV	419	541	0.05%	0.006%
81	12.866	1931	1932	1936	rBV	621	594	0.05%	0.006%
82	13.158	1978	1980	1984	rVB2	487	664	0.06%	0.007%
83	13.201	1984	1987	1990	rBV2	455	650	0.06%	0.007%
84	13.304	2002	2004	2008	rVB3	360	387	0.03%	0.004%
85	13.670	2062	2064	2066	rVB	575	482	0.04%	0.005%
86	13.859	2092	2095	2098	rBV	422	579	0.05%	0.006%
87	13.932	2105	2107	2109	rBV2	527	488	0.04%	0.005%
88	14.006	2118	2119	2121	rBV	642	411	0.03%	0.004%
89	14.152	2142	2143	2145	rBV2	714	395	0.03%	0.004%
90	14.207	2149	2152	2153	rBV2	389	418	0.04%	0.004%
91	14.365	2176	2178	2183	rVB2	575	795	0.07%	0.009%
92	14.457	2191	2193	2195	rVB2	567	430	0.04%	0.005%
93	14.963	2274	2276	2278	rBV2	476	350	0.03%	0.004%
94	15.109	2298	2300	2305	rVB4	692	873	0.07%	0.009%
95	15.658	2388	2390	2391	rBV2	741	597	0.05%	0.006%
96	15.731	2400	2402	2403	rBV2	471	360	0.03%	0.004%
97	15.767	2406	2408	2411	rBV3	512	614	0.05%	0.007%
98	16.011	2446	2448	2450	rBV3	616	632	0.05%	0.007%
99	16.395	2509	2511	2513	rBV2	528	416	0.04%	0.004%
100	16.712	2561	2563	2564	rBV2	615	352	0.03%	0.004%




Sum of corrected areas: 9314554

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030424.D
Acq On : 05 Aug 2022 13:02
Operator : JC/MD
Sample : N4003-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

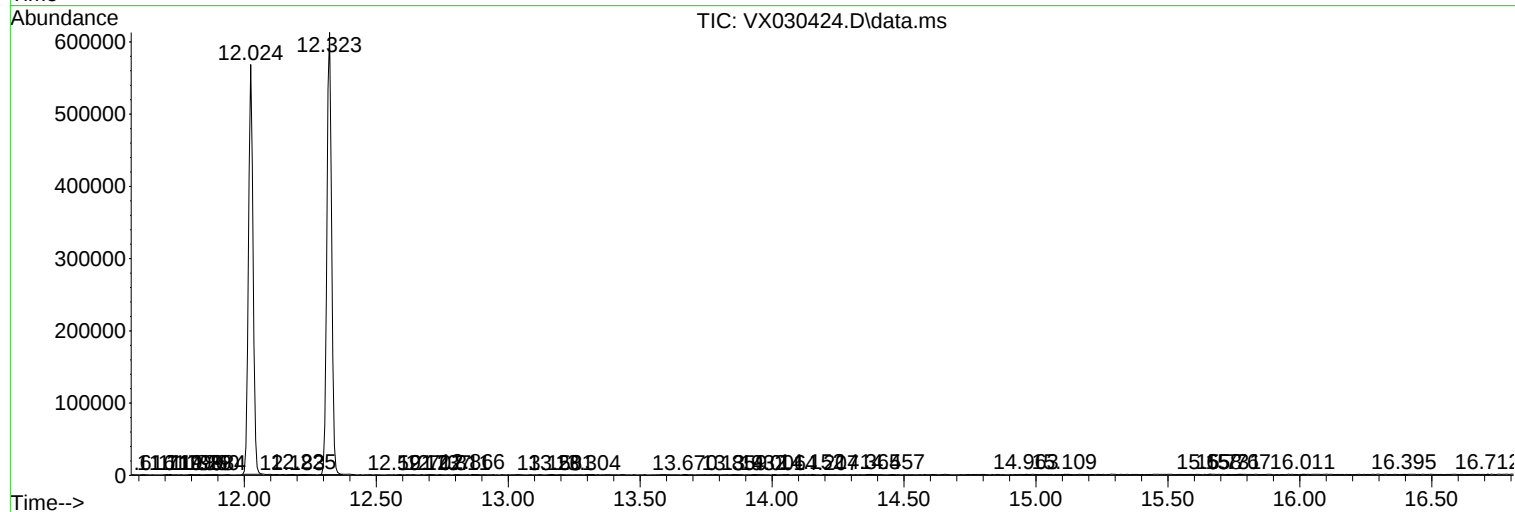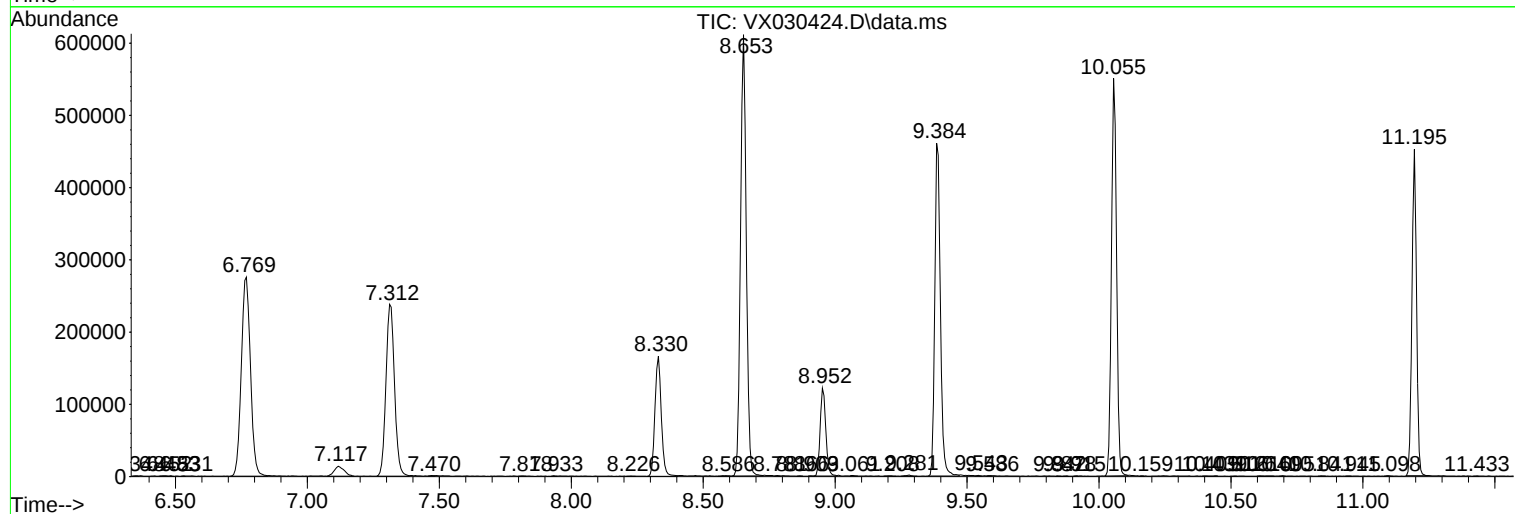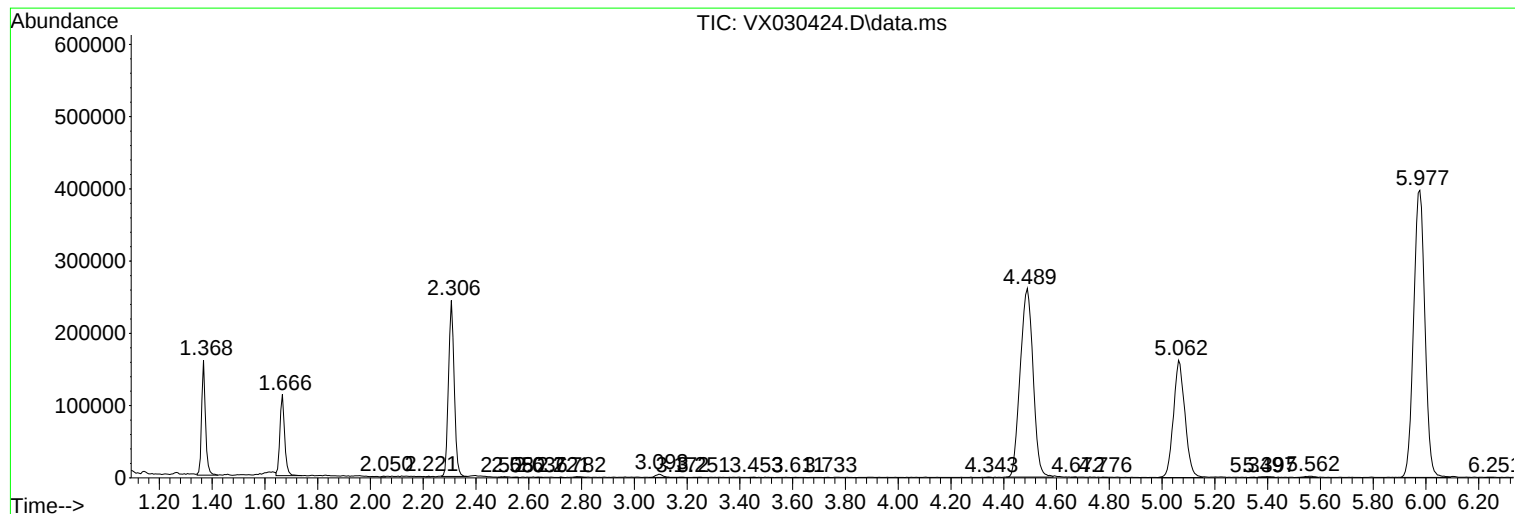

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030424.D
Acq On : 05 Aug 2022 13:02
Operator : JC/MD
Sample : N4003-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030424.D
Acq On : 05 Aug 2022 13:02
Operator : JC/MD
Sample : N4003-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc