

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030425.D
 Acq On : 05 Aug 2022 13:25
 Operator : JC/MD
 Sample : N4003-15DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D64DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030425.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	56	rVB	156796	168081	14.16%	1.810%
2	1.666	91	95	104	rVB	117108	143902	12.13%	1.550%
3	2.306	194	200	210	rVB	243432	370837	31.25%	3.994%
4	2.788	274	279	287	rVB2	5119	9471	0.80%	0.102%
5	2.952	298	306	315	rVV2	10126	23977	2.02%	0.258%
6	3.093	323	329	336	rVB2	5599	10865	0.92%	0.117%
7	3.263	354	357	361	rVB	468	673	0.06%	0.007%
8	3.300	361	363	366	rBV2	498	697	0.06%	0.008%
9	3.446	383	387	390	rBV2	590	582	0.05%	0.006%
10	3.507	396	397	400	rBV	449	407	0.03%	0.004%
11	3.611	411	414	416	rBV2	309	336	0.03%	0.004%
12	3.714	426	431	432	rBV	369	488	0.04%	0.005%
13	3.739	433	435	439	rVB3	518	536	0.05%	0.006%
14	3.769	439	440	443	rBV2	430	383	0.03%	0.004%
15	3.879	454	458	460	rVV3	354	510	0.04%	0.005%
16	3.964	468	472	475	rBV2	547	764	0.06%	0.008%
17	3.995	475	477	480	rBV	467	389	0.03%	0.004%
18	4.080	488	491	492	rBV	479	436	0.04%	0.005%
19	4.300	526	527	530	rBV	545	359	0.03%	0.004%
20	4.483	545	557	569	rBV2	209918	735902	62.01%	7.926%
21	4.964	634	636	639	rVV2	308	340	0.03%	0.004%
22	5.062	640	652	667	rVV2	157882	481441	40.57%	5.186%
23	5.306	690	692	694	rBV2	671	626	0.05%	0.007%
24	5.391	699	706	709	rBV2	1132	2290	0.19%	0.025%
25	5.543	726	731	734	rBV3	1275	2271	0.19%	0.024%
26	5.623	743	744	747	rBV2	488	375	0.03%	0.004%
27	5.665	749	751	753	rVB	565	322	0.03%	0.003%
28	5.775	767	769	774	rVB2	404	606	0.05%	0.007%
29	5.818	774	776	778	rBV	477	410	0.03%	0.004%
30	5.976	789	802	819	rVV2	398884	1186660	100.00%	12.782%
31	6.220	839	842	844	rVB2	326	323	0.03%	0.003%
32	6.245	844	846	849	rBV	386	363	0.03%	0.004%
33	6.458	879	881	882	rBV	502	488	0.04%	0.005%
34	6.525	889	892	893	rBV2	511	555	0.05%	0.006%
35	6.549	893	896	899	rVV2	650	821	0.07%	0.009%
36	6.769	921	932	947	rBV	278360	664969	56.04%	7.162%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030425.D
 Acq On : 05 Aug 2022 13:25
 Operator : JC/MD
 Sample : N4003-15DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D64DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
 Title : VOC Analysis

37	7.116	981	989	1001	rBV5	12261	31259	2.63%	0.337%
38	7.311	1012	1021	1035	rVV	242287	544186	45.86%	5.861%
39	7.452	1042	1044	1045	rBV	419	428	0.04%	0.005%
40	7.580	1062	1065	1066	rBV2	554	390	0.03%	0.004%
41	7.726	1086	1089	1091	rBV2	485	531	0.04%	0.006%
42	7.830	1105	1106	1108	rBV	487	324	0.03%	0.003%
43	7.933	1121	1123	1124	rBV	645	464	0.04%	0.005%
44	8.037	1139	1140	1141	rBV	483	336	0.03%	0.004%
45	8.104	1149	1151	1154	rBV2	301	415	0.03%	0.004%
46	8.159	1156	1160	1162	rBV2	372	408	0.03%	0.004%
47	8.232	1167	1172	1175	rBV2	483	722	0.06%	0.008%
48	8.329	1181	1188	1200	rBV	164884	278581	23.48%	3.001%
49	8.500	1213	1216	1219	rBV3	493	640	0.05%	0.007%
50	8.579	1226	1229	1233	rVB3	587	775	0.07%	0.008%
51	8.653	1234	1241	1254	rBV	612240	935901	78.87%	10.081%
52	8.817	1265	1268	1269	rBV	468	525	0.04%	0.006%
53	8.872	1273	1277	1279	rBV3	621	657	0.06%	0.007%
54	8.951	1284	1290	1301	rBV	117509	181037	15.26%	1.950%
55	9.281	1338	1344	1347	rVB4	731	1044	0.09%	0.011%
56	9.390	1356	1362	1377	rBV	454341	682552	57.52%	7.352%
57	9.707	1409	1414	1417	rBV5	1547	2982	0.25%	0.032%
58	9.805	1427	1430	1432	rBV3	562	543	0.05%	0.006%
59	9.829	1432	1434	1437	rBV2	544	621	0.05%	0.007%
60	9.860	1437	1439	1441	rVV2	461	345	0.03%	0.004%
61	9.933	1448	1451	1453	rVB2	499	479	0.04%	0.005%
62	9.976	1457	1458	1461	rBV	405	352	0.03%	0.004%
63	10.055	1466	1471	1483	rVV	573657	771197	64.99%	8.307%
64	10.549	1549	1552	1553	rBV	339	329	0.03%	0.004%
65	10.640	1565	1567	1573	rBV3	379	785	0.07%	0.008%
66	10.853	1601	1602	1604	rBV2	477	356	0.03%	0.004%
67	10.975	1619	1622	1623	rBV2	527	457	0.04%	0.005%
68	11.091	1640	1641	1643	rBV2	460	443	0.04%	0.005%
69	11.140	1647	1649	1651	rVV	438	407	0.03%	0.004%
70	11.195	1653	1658	1669	rVV	440921	545973	46.01%	5.881%
71	11.280	1669	1672	1675	rVB3	479	520	0.04%	0.006%
72	11.311	1675	1677	1679	rBV	657	587	0.05%	0.006%
73	11.335	1679	1681	1684	rBV2	363	324	0.03%	0.003%
74	11.652	1726	1733	1735	rVB2	710	1189	0.10%	0.013%
75	11.670	1735	1736	1738	rBV	517	364	0.03%	0.004%
76	11.744	1747	1748	1750	rVV2	409	344	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030425.D
 Acq On : 05 Aug 2022 13:25
 Operator : JC/MD
 Sample : N4003-15DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D64DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.841	1763	1764	1768	rBV	390	491	0.04%	0.005%
78	11.890	1771	1772	1775	rBV	406	330	0.03%	0.004%
79	11.957	1782	1783	1786	rVB2	507	428	0.04%	0.005%
80	12.024	1789	1794	1803	rVV	573882	696321	58.68%	7.500%
81	12.164	1814	1817	1822	rBV2	409	872	0.07%	0.009%
82	12.225	1825	1827	1829	rBV	663	466	0.04%	0.005%
83	12.323	1837	1843	1859	rVB	602152	772961	65.14%	8.326%
84	12.756	1912	1914	1916	rVV2	571	458	0.04%	0.005%
85	12.816	1922	1924	1927	rBV3	395	472	0.04%	0.005%
86	13.292	2001	2002	2005	rVV	637	454	0.04%	0.005%
87	13.475	2029	2032	2035	rBV3	502	630	0.05%	0.007%
88	13.591	2050	2051	2053	rBV	422	368	0.03%	0.004%
89	13.780	2078	2082	2085	rBV3	547	1012	0.09%	0.011%
90	14.200	2150	2151	2154	rBV2	414	382	0.03%	0.004%
91	14.255	2158	2160	2165	rBV3	471	787	0.07%	0.008%
92	14.365	2176	2178	2179	rVB2	561	343	0.03%	0.004%
93	14.627	2220	2221	2226	rBV	654	652	0.05%	0.007%
94	15.097	2296	2298	2299	rBV	848	584	0.05%	0.006%
95	15.145	2304	2306	2309	rVB2	665	682	0.06%	0.007%
96	15.895	2428	2429	2431	rBV	771	426	0.04%	0.005%
97	16.042	2450	2453	2454	rBV2	665	845	0.07%	0.009%
98	16.426	2513	2516	2517	rBV2	734	758	0.06%	0.008%
99	16.584	2540	2542	2543	rVB	869	366	0.03%	0.004%
100	16.676	2555	2557	2560	rBV2	656	786	0.07%	0.008%




Sum of corrected areas: 9284101

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030425.D
Acq On : 05 Aug 2022 13:25
Operator : JC/MD
Sample : N4003-15DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D64DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

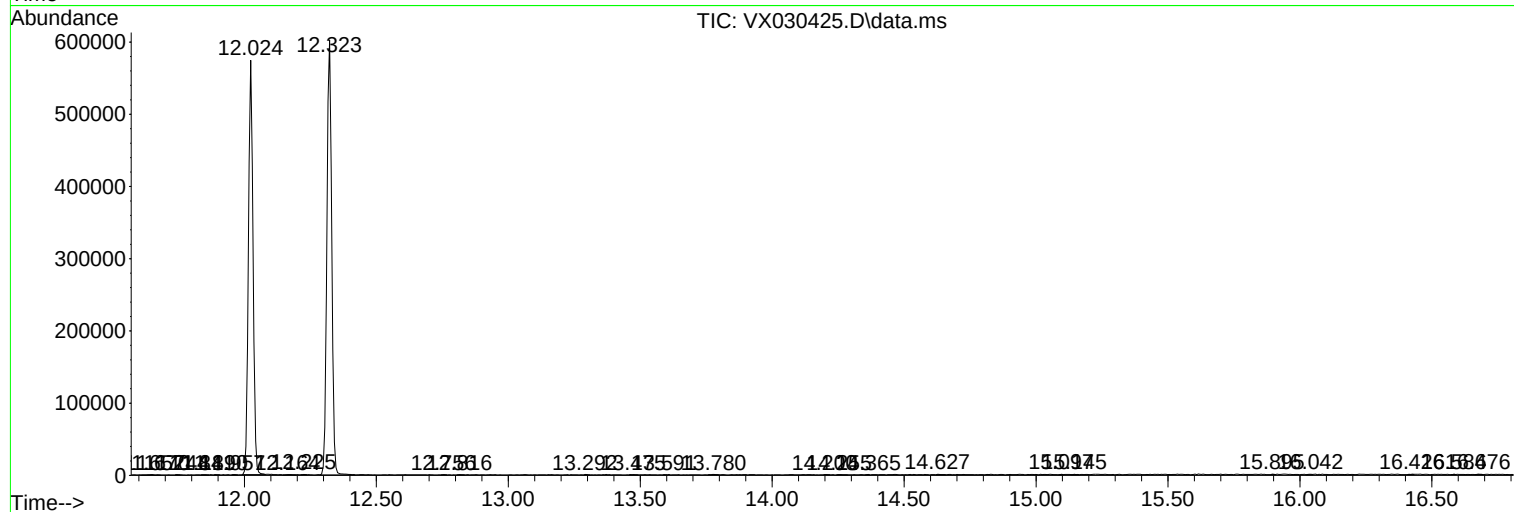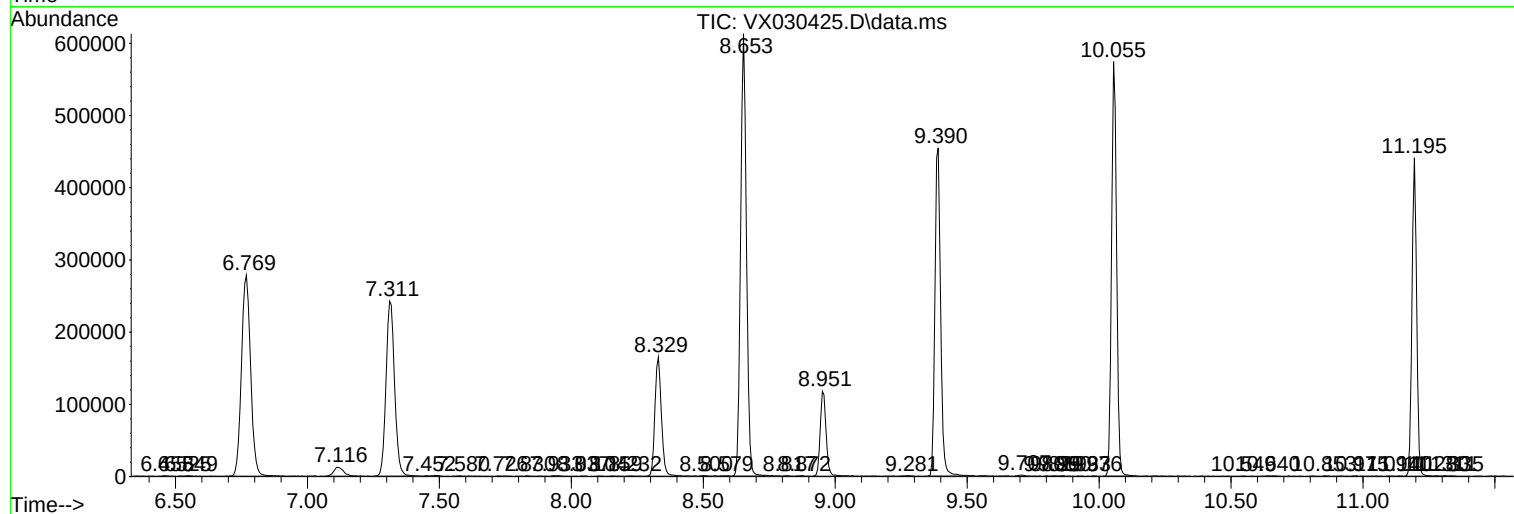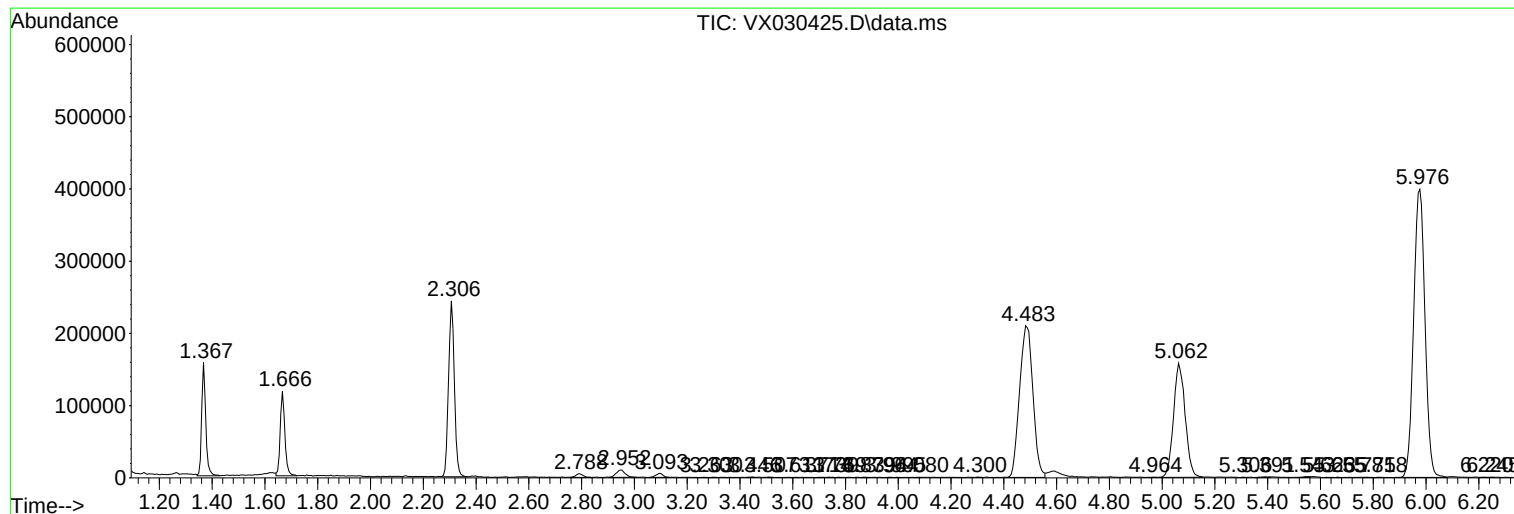

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030425.D
Acq On : 05 Aug 2022 13:25
Operator : JC/MD
Sample : N4003-15DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D64DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030425.D
Acq On : 05 Aug 2022 13:25
Operator : JC/MD
Sample : N4003-15DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D64DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------