

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030426.D
 Acq On : 05 Aug 2022 13:48
 Operator : JC/MD
 Sample : N4003-16DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D65DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030426.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB	163558	164001	13.74%	1.767%
2	1.666	91	95	105	rVB	121617	147811	12.38%	1.593%
3	2.307	193	200	211	rVB	232758	362617	30.37%	3.907%
4	2.569	242	243	247	rBV2	536	497	0.04%	0.005%
5	2.788	275	279	287	rVB4	3436	6634	0.56%	0.071%
6	2.947	299	305	313	rVB3	4928	10869	0.91%	0.117%
7	3.099	323	330	337	rVB3	5475	11364	0.95%	0.122%
8	3.294	360	362	365	rBV	470	575	0.05%	0.006%
9	3.440	384	386	388	rBV2	497	307	0.03%	0.003%
10	3.593	409	411	415	rVB	557	574	0.05%	0.006%
11	3.642	418	419	420	rBV	577	348	0.03%	0.004%
12	3.703	427	429	431	rVB2	566	414	0.03%	0.004%
13	3.764	437	439	443	rVB2	321	451	0.04%	0.005%
14	3.800	443	445	448	rBV	307	333	0.03%	0.004%
15	3.965	470	472	473	rBV	397	314	0.03%	0.003%
16	4.099	492	494	496	rVB2	580	369	0.03%	0.004%
17	4.331	528	532	535	rBV2	336	560	0.05%	0.006%
18	4.489	545	558	571	rBV2	214542	732353	61.34%	7.891%
19	4.861	616	619	621	rBV2	393	508	0.04%	0.005%
20	4.940	630	632	634	rBV	414	306	0.03%	0.003%
21	5.062	640	652	668	rBV	160269	487902	40.87%	5.257%
22	5.282	685	688	691	rVB2	414	478	0.04%	0.005%
23	5.483	719	721	723	rBV	566	357	0.03%	0.004%
24	5.556	727	733	735	rBV3	1888	3261	0.27%	0.035%
25	5.635	744	746	752	rVB3	648	888	0.07%	0.010%
26	5.684	752	754	756	rBV2	403	379	0.03%	0.004%
27	5.739	761	763	764	rVB	592	323	0.03%	0.003%
28	5.977	790	802	816	rBV2	408531	1193877	100.00%	12.864%
29	6.111	822	824	828	rVB3	853	849	0.07%	0.009%
30	6.141	828	829	831	rVB2	695	452	0.04%	0.005%
31	6.178	831	835	836	rBV2	326	397	0.03%	0.004%
32	6.251	844	847	849	rBV2	590	621	0.05%	0.007%
33	6.348	861	863	866	rBV2	427	470	0.04%	0.005%
34	6.495	885	887	891	rBV2	333	395	0.03%	0.004%
35	6.544	891	895	899	rBV3	657	754	0.06%	0.008%
36	6.629	906	909	910	rBV	435	498	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030426.D
 Acq On : 05 Aug 2022 13:48
 Operator : JC/MD
 Sample : N4003-16DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D65DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.696	917	920	921	rBV2	479	409	0.03%	0.004%
38	6.769	922	932	953	rVV	268600	640921	53.68%	6.906%
39	7.050	975	978	979	rBV	347	355	0.03%	0.004%
40	7.123	982	990	999	rVV6	12382	32353	2.71%	0.349%
41	7.196	1001	1002	1005	rBV	506	350	0.03%	0.004%
42	7.226	1005	1007	1010	rBV2	424	375	0.03%	0.004%
43	7.312	1013	1021	1036	rBV	247523	550645	46.12%	5.933%
44	7.604	1067	1069	1073	rVB3	575	608	0.05%	0.007%
45	7.671	1077	1080	1082	rBV	353	468	0.04%	0.005%
46	7.763	1091	1095	1096	rVB2	381	313	0.03%	0.003%
47	7.885	1112	1115	1116	rBV2	411	454	0.04%	0.005%
48	8.123	1149	1154	1155	rVB2	338	498	0.04%	0.005%
49	8.257	1174	1176	1177	rBV	390	303	0.03%	0.003%
50	8.330	1181	1188	1201	rVV	166973	279919	23.45%	3.016%
51	8.464	1208	1210	1213	rBV3	659	951	0.08%	0.010%
52	8.653	1234	1241	1253	rVV	602303	935210	78.33%	10.077%
53	8.757	1257	1258	1260	rVB2	814	434	0.04%	0.005%
54	8.952	1285	1290	1299	rVV	121650	180998	15.16%	1.950%
55	9.116	1314	1317	1318	rBV2	623	519	0.04%	0.006%
56	9.177	1325	1327	1329	rBV	522	444	0.04%	0.005%
57	9.275	1341	1343	1347	rVB	498	397	0.03%	0.004%
58	9.391	1356	1362	1374	rBV	489878	701838	58.79%	7.562%
59	9.610	1396	1398	1403	rBV3	717	728	0.06%	0.008%
60	9.653	1403	1405	1406	rVB	736	441	0.04%	0.005%
61	9.677	1406	1409	1410	rBV	395	541	0.05%	0.006%
62	9.756	1420	1422	1423	rVB	620	314	0.03%	0.003%
63	9.787	1426	1427	1433	rBV2	417	597	0.05%	0.006%
64	9.854	1437	1438	1440	rBV	683	470	0.04%	0.005%
65	10.055	1465	1471	1481	rVV	563322	742670	62.21%	8.002%
66	10.177	1490	1491	1492	rBV	669	313	0.03%	0.003%
67	10.317	1511	1514	1516	rBV2	364	371	0.03%	0.004%
68	10.403	1526	1528	1529	rBV2	384	410	0.03%	0.004%
69	10.586	1556	1558	1561	rBV2	462	519	0.04%	0.006%
70	10.701	1572	1577	1579	rBV2	575	779	0.07%	0.008%
71	10.805	1593	1594	1595	rBV	610	331	0.03%	0.004%
72	10.866	1601	1604	1606	rBV2	483	491	0.04%	0.005%
73	11.079	1637	1639	1640	rBV2	436	307	0.03%	0.003%
74	11.122	1644	1646	1648	rBV	303	317	0.03%	0.003%
75	11.195	1652	1658	1666	rBV	441113	560307	46.93%	6.037%
76	11.512	1707	1710	1713	rVB3	415	561	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030426.D
 Acq On : 05 Aug 2022 13:48
 Operator : JC/MD
 Sample : N4003-16DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D65DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.543	1713	1715	1718	rBV	432	538	0.05%	0.006%
78	11.604	1723	1725	1726	rBV	430	372	0.03%	0.004%
79	11.823	1758	1761	1762	rBV	322	353	0.03%	0.004%
80	12.024	1789	1794	1805	rVB	545205	679687	56.93%	7.324%
81	12.323	1837	1843	1850	rBV	674773	818044	68.52%	8.814%
82	12.445	1861	1863	1864	rVB	636	400	0.03%	0.004%
83	12.591	1885	1887	1888	rBV	338	315	0.03%	0.003%
84	13.152	1976	1979	1980	rBV	384	429	0.04%	0.005%
85	13.353	2010	2012	2013	rBV	377	334	0.03%	0.004%
86	13.439	2024	2026	2029	rBV2	387	493	0.04%	0.005%
87	13.512	2035	2038	2039	rBV2	348	440	0.04%	0.005%
88	13.872	2094	2097	2098	rBV2	469	425	0.04%	0.005%
89	13.890	2098	2100	2105	rVV	581	858	0.07%	0.009%
90	13.975	2113	2114	2117	rBV	464	376	0.03%	0.004%
91	14.000	2117	2118	2119	rVV	552	308	0.03%	0.003%
92	14.042	2123	2125	2129	rVB2	653	534	0.04%	0.006%
93	14.359	2174	2177	2178	rBV2	566	576	0.05%	0.006%
94	14.439	2188	2190	2194	rVB4	574	702	0.06%	0.008%
95	14.475	2194	2196	2199	rBV3	543	797	0.07%	0.009%
96	14.615	2216	2219	2220	rBV	581	695	0.06%	0.007%
97	15.188	2311	2313	2315	rBV2	461	425	0.04%	0.005%
98	15.572	2374	2376	2377	rBV	688	371	0.03%	0.004%
99	15.609	2380	2382	2386	rBV4	474	447	0.04%	0.005%
100	15.725	2399	2401	2402	rVB	1016	575	0.05%	0.006%




Sum of corrected areas: 9280829

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030426.D
Acq On : 05 Aug 2022 13:48
Operator : JC/MD
Sample : N4003-16DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D65DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

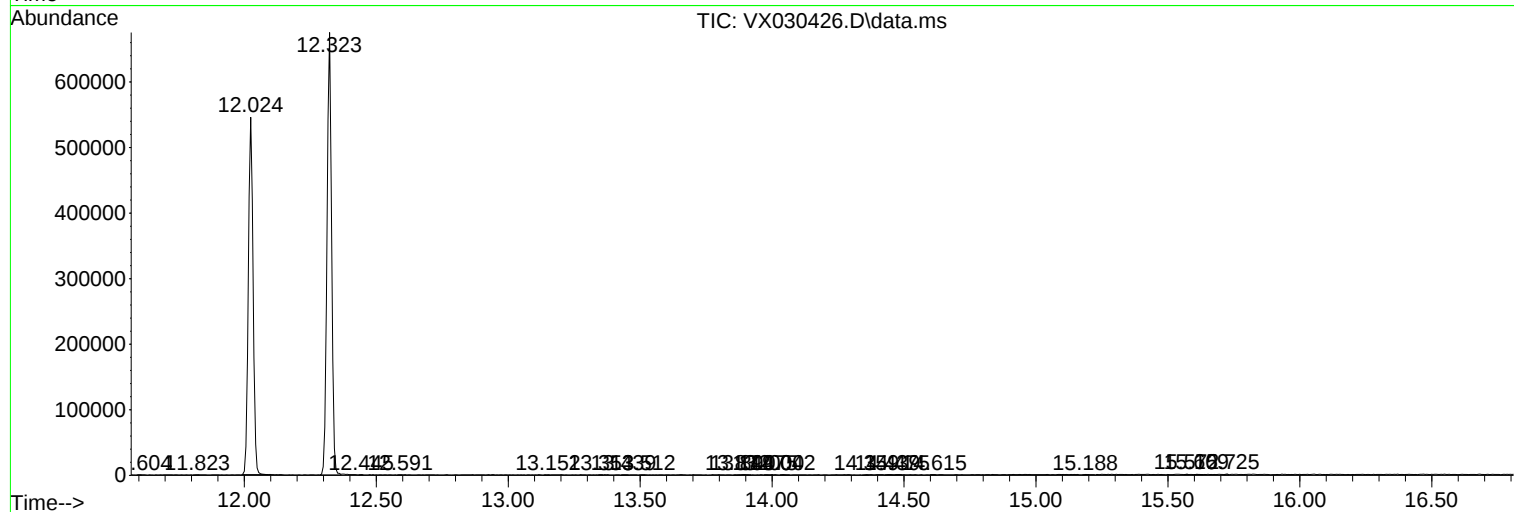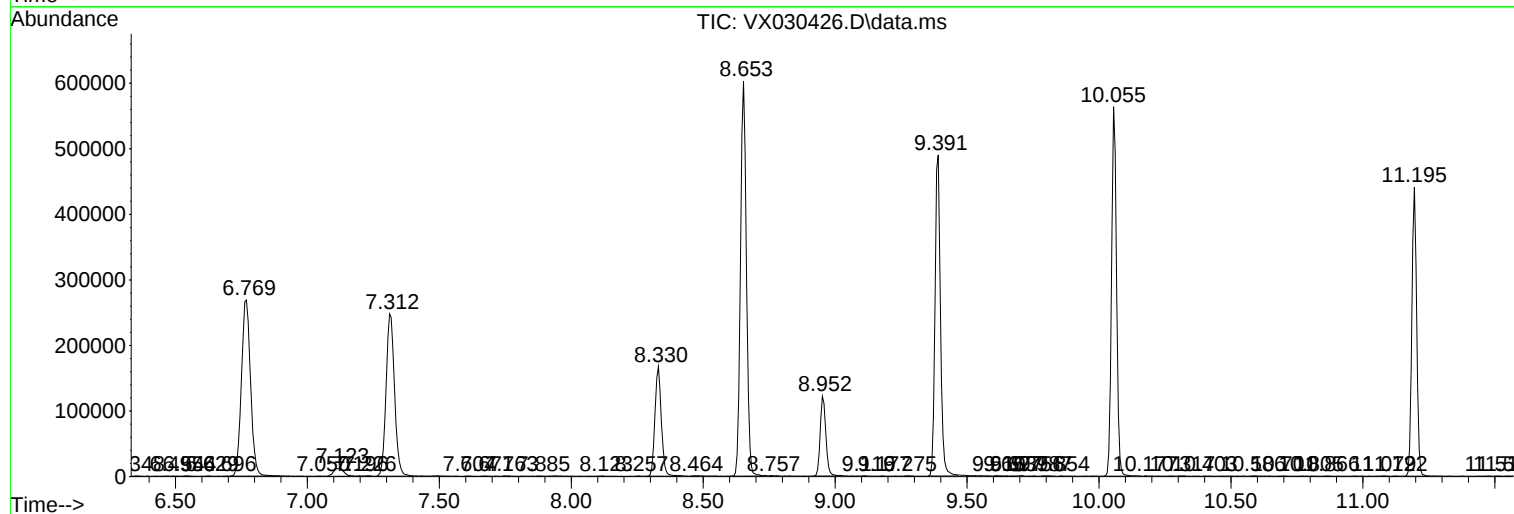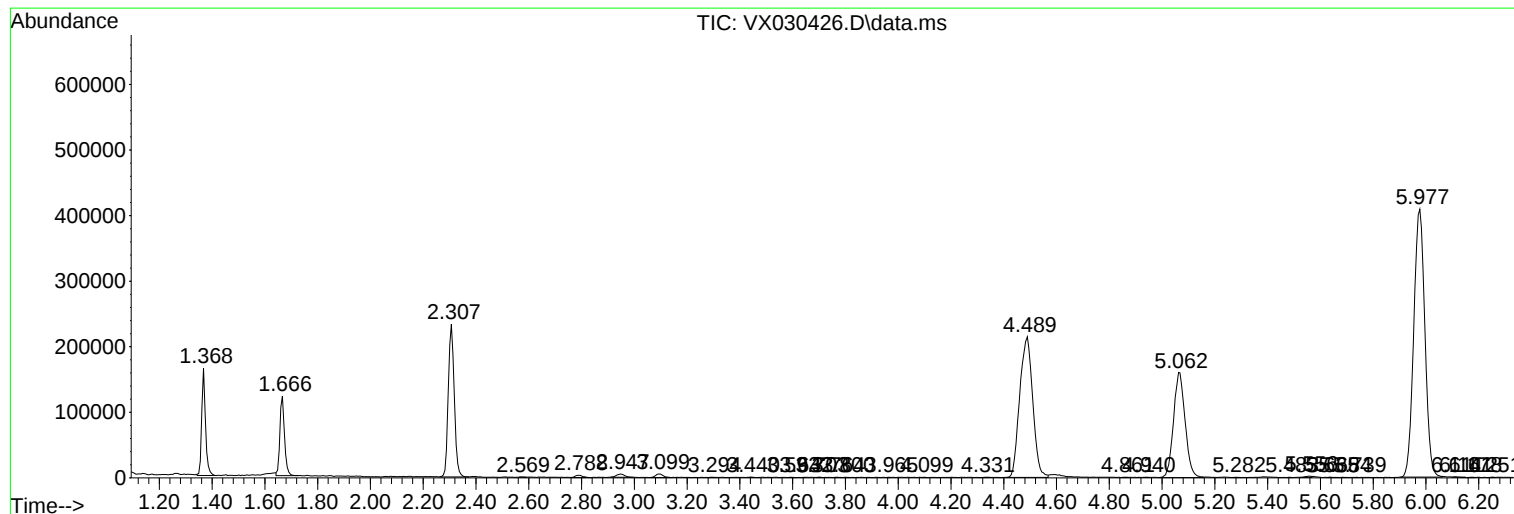

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030426.D
Acq On : 05 Aug 2022 13:48
Operator : JC/MD
Sample : N4003-16DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D65DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030426.D
Acq On : 05 Aug 2022 13:48
Operator : JC/MD
Sample : N4003-16DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D65DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------