

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030427.D
 Acq On : 05 Aug 2022 14:12
 Operator : JC/MD
 Sample : N4003-07DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D32DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030427.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB2	190660	208891	17.22%	2.213%
2	1.666	91	95	101	rVB	122014	145613	12.00%	1.542%
3	2.307	193	200	210	rVB	264412	390602	32.20%	4.137%
4	2.380	210	212	216	rBV3	1083	1458	0.12%	0.015%
5	2.794	272	280	285	rVV5	3241	6941	0.57%	0.074%
6	2.867	289	292	293	rVV2	493	474	0.04%	0.005%
7	2.947	298	305	315	rVV2	6497	15637	1.29%	0.166%
8	3.044	320	321	323	rBV	499	454	0.04%	0.005%
9	3.093	323	329	337	rVV2	7224	14790	1.22%	0.157%
10	3.197	344	346	351	rVB2	309	417	0.03%	0.004%
11	3.514	393	398	401	rBV4	334	658	0.05%	0.007%
12	3.556	403	405	407	rVV	359	346	0.03%	0.004%
13	3.849	452	453	457	rVV2	544	399	0.03%	0.004%
14	4.245	516	518	521	rBV	515	566	0.05%	0.006%
15	4.489	543	558	570	rBV2	239101	807499	66.57%	8.553%
16	4.769	602	604	606	rBV2	403	353	0.03%	0.004%
17	4.946	631	633	636	rVB2	383	453	0.04%	0.005%
18	5.062	639	652	668	rVV	163772	494099	40.73%	5.233%
19	5.239	680	681	685	rBV2	415	615	0.05%	0.007%
20	5.385	699	705	707	rBV2	781	1380	0.11%	0.015%
21	5.483	719	721	725	rVB2	501	624	0.05%	0.007%
22	5.532	727	729	730	rBV	604	428	0.04%	0.005%
23	5.544	730	731	733	rBV2	1000	918	0.08%	0.010%
24	5.635	744	746	749	rVB2	465	466	0.04%	0.005%
25	5.812	771	775	778	rVB2	389	510	0.04%	0.005%
26	5.873	781	785	788	rBV2	224	410	0.03%	0.004%
27	5.977	788	802	821	rBV2	409160	1212978	100.00%	12.847%
28	6.153	829	831	835	rVB2	554	667	0.05%	0.007%
29	6.190	835	837	838	rBV	650	450	0.04%	0.005%
30	6.476	880	884	885	rBV3	382	413	0.03%	0.004%
31	6.769	922	932	945	rBV	259706	622182	51.29%	6.590%
32	7.117	982	989	1001	rBV4	17475	44731	3.69%	0.474%
33	7.220	1005	1006	1009	rVB	486	376	0.03%	0.004%
34	7.312	1012	1021	1034	rBV	248970	560239	46.19%	5.934%
35	7.482	1045	1049	1051	rBV3	862	1101	0.09%	0.012%
36	7.562	1059	1062	1064	rBV2	450	449	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030427.D
 Acq On : 05 Aug 2022 14:12
 Operator : JC/MD
 Sample : N4003-07DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D32DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.921	1118	1121	1123	rBV	514	737	0.06%	0.008%
38	7.946	1123	1125	1126	rVV2	738	476	0.04%	0.005%
39	7.964	1126	1128	1133	rVB3	579	910	0.08%	0.010%
40	8.013	1133	1136	1137	rBV2	497	552	0.05%	0.006%
41	8.049	1140	1142	1146	rVB3	447	417	0.03%	0.004%
42	8.123	1150	1154	1156	rBV2	637	714	0.06%	0.008%
43	8.238	1171	1173	1177	rVB2	433	414	0.03%	0.004%
44	8.330	1181	1188	1199	rBV	172036	281678	23.22%	2.983%
45	8.476	1209	1212	1213	rBV3	462	466	0.04%	0.005%
46	8.537	1221	1222	1224	rVB2	792	437	0.04%	0.005%
47	8.653	1234	1241	1253	rBV	627788	953956	78.65%	10.104%
48	8.805	1264	1266	1267	rVB2	695	365	0.03%	0.004%
49	8.952	1284	1290	1304	rBV	124581	187704	15.47%	1.988%
50	9.135	1317	1320	1322	rVV2	762	879	0.07%	0.009%
51	9.159	1322	1324	1327	rVB2	586	616	0.05%	0.007%
52	9.275	1337	1343	1349	rVB4	3229	5703	0.47%	0.060%
53	9.324	1349	1351	1353	rBV2	445	413	0.03%	0.004%
54	9.391	1356	1362	1377	rBV	485237	711641	58.67%	7.537%
55	9.702	1410	1413	1417	rVV3	577	1091	0.09%	0.012%
56	9.738	1417	1419	1421	rVB2	641	433	0.04%	0.005%
57	9.878	1439	1442	1443	rBV	781	516	0.04%	0.005%
58	9.915	1446	1448	1450	rBV2	301	371	0.03%	0.004%
59	9.982	1455	1459	1461	rBV3	545	604	0.05%	0.006%
60	10.055	1466	1471	1486	rVB	533716	720460	59.40%	7.631%
61	10.153	1486	1487	1489	rBV	598	578	0.05%	0.006%
62	10.214	1494	1497	1500	rVB2	396	504	0.04%	0.005%
63	10.336	1515	1517	1520	rVB2	854	720	0.06%	0.008%
64	10.372	1520	1523	1524	rBV2	522	418	0.03%	0.004%
65	10.409	1527	1529	1533	rVB2	754	657	0.05%	0.007%
66	10.439	1533	1534	1537	rBV2	377	345	0.03%	0.004%
67	10.567	1550	1555	1557	rVB3	443	656	0.05%	0.007%
68	10.592	1557	1559	1561	rBV2	441	432	0.04%	0.005%
69	10.744	1582	1584	1586	rBV	371	426	0.04%	0.005%
70	10.884	1603	1607	1610	rVV	533	517	0.04%	0.005%
71	10.945	1615	1617	1620	rVV2	552	499	0.04%	0.005%
72	11.195	1652	1658	1665	rBV	451682	562225	46.35%	5.955%
73	11.628	1727	1729	1735	rVB2	526	804	0.07%	0.009%
74	11.701	1738	1741	1743	rBV	432	651	0.05%	0.007%
75	11.744	1746	1748	1751	rVB	341	358	0.03%	0.004%
76	11.823	1758	1761	1762	rBV2	294	368	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030427.D
 Acq On : 05 Aug 2022 14:12
 Operator : JC/MD
 Sample : N4003-07DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D32DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.921	1775	1777	1780	rVB2	471	425	0.04%	0.005%
78	12.024	1788	1794	1804	rVV	546032	653021	53.84%	6.917%
79	12.323	1837	1843	1851	rBV	641917	795528	65.58%	8.426%
80	12.671	1897	1900	1903	rVB2	471	426	0.04%	0.005%
81	12.994	1951	1953	1957	rVB2	475	519	0.04%	0.005%
82	13.048	1961	1962	1965	rBV2	294	353	0.03%	0.004%
83	13.347	2008	2011	2012	rBV2	287	349	0.03%	0.004%
84	13.494	2033	2035	2038	rVB	515	519	0.04%	0.005%
85	13.548	2041	2044	2046	rVV2	481	457	0.04%	0.005%
86	13.573	2046	2048	2050	rVB	520	345	0.03%	0.004%
87	13.737	2071	2075	2077	rBV	280	414	0.03%	0.004%
88	13.780	2080	2082	2085	rBV2	628	651	0.05%	0.007%
89	13.957	2109	2111	2113	rBV	415	418	0.03%	0.004%
90	14.378	2178	2180	2181	rVB2	651	400	0.03%	0.004%
91	14.408	2181	2185	2188	rBV2	469	822	0.07%	0.009%
92	14.499	2196	2200	2204	rVB3	613	1045	0.09%	0.011%
93	14.536	2204	2206	2207	rBV	565	392	0.03%	0.004%
94	14.713	2233	2235	2238	rVB2	436	427	0.04%	0.005%
95	14.743	2238	2240	2243	rBV2	420	408	0.03%	0.004%
96	14.780	2243	2246	2249	rBV2	790	886	0.07%	0.009%
97	14.810	2249	2251	2254	rBV2	421	357	0.03%	0.004%
98	14.963	2273	2276	2277	rBV2	515	486	0.04%	0.005%
99	15.816	2412	2416	2420	rBV4	986	1877	0.15%	0.020%
100	16.743	2566	2568	2570	rBV2	820	571	0.05%	0.006%




Sum of corrected areas: 9441394

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030427.D
Acq On : 05 Aug 2022 14:12
Operator : JC/MD
Sample : N4003-07DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D32DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

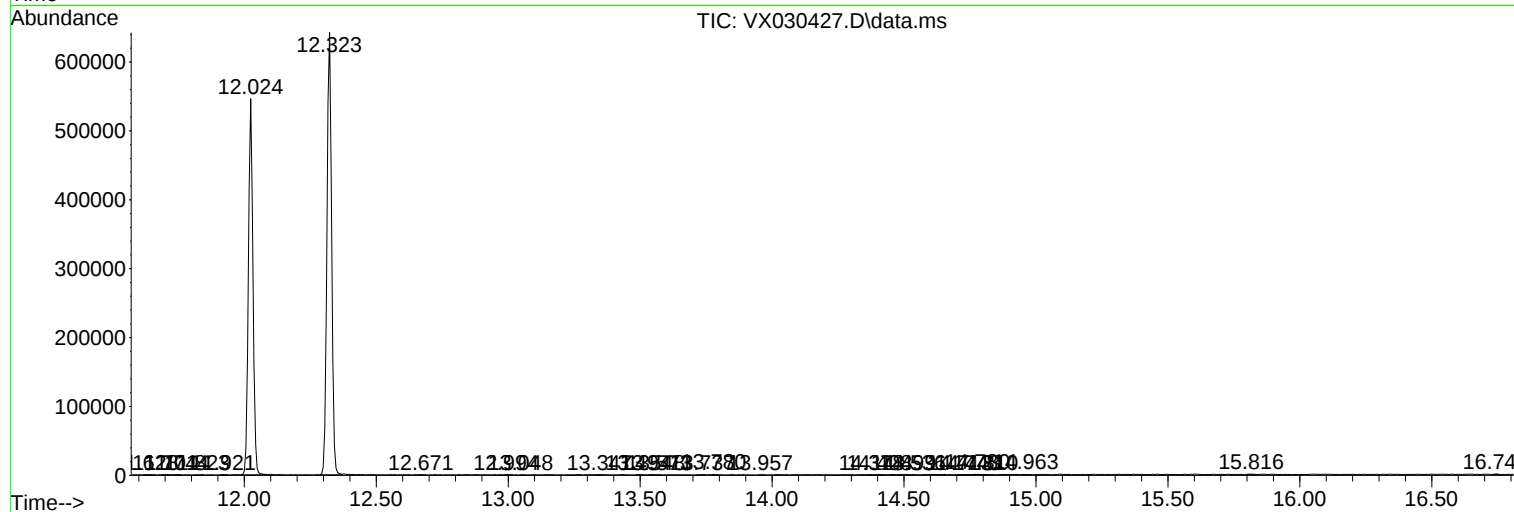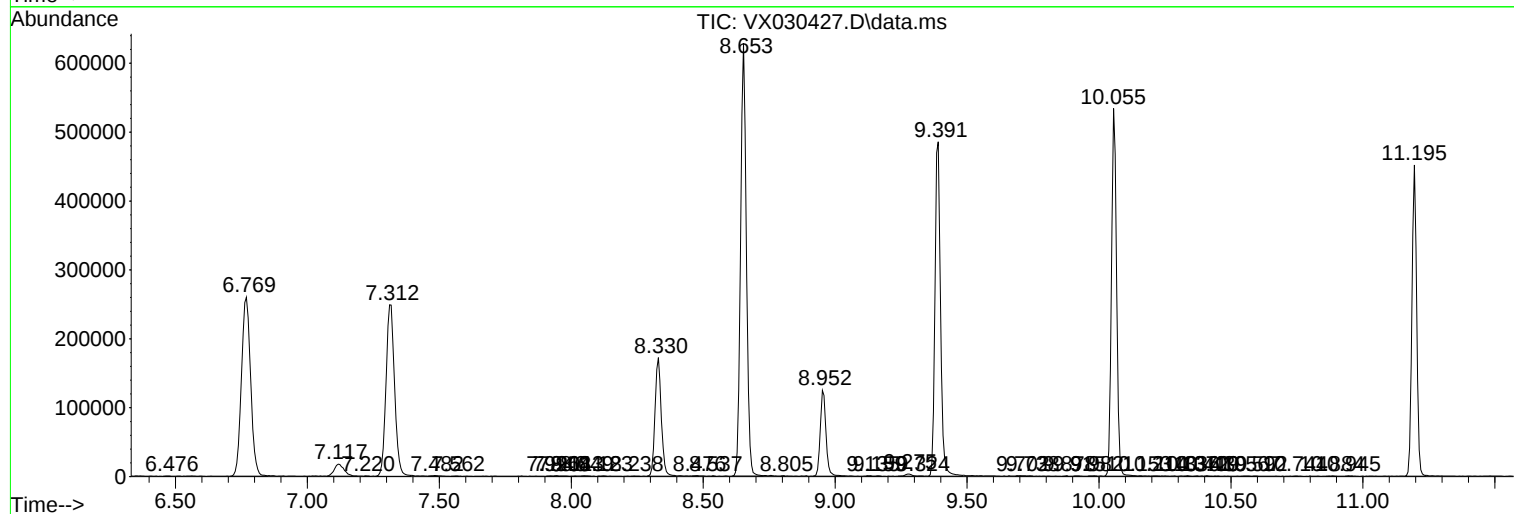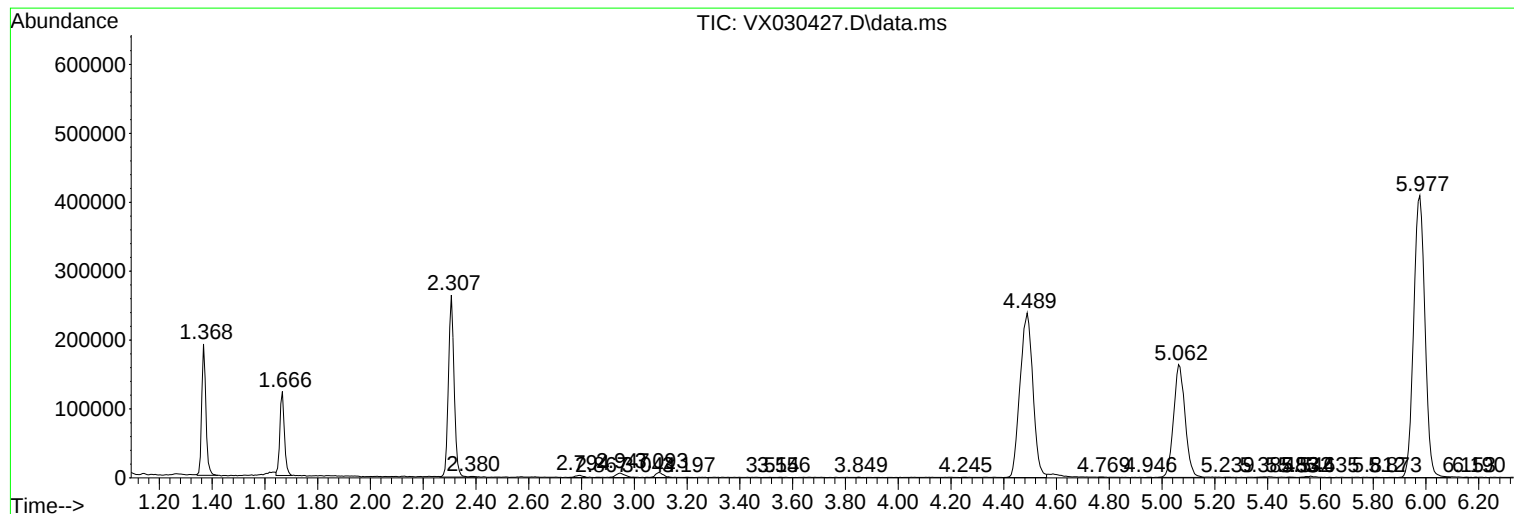

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030427.D
Acq On : 05 Aug 2022 14:12
Operator : JC/MD
Sample : N4003-07DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D32DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030427.D
Acq On : 05 Aug 2022 14:12
Operator : JC/MD
Sample : N4003-07DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D32DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc