

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030428.D
 Acq On : 05 Aug 2022 14:35
 Operator : JC/MD
 Sample : N4003-11DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D58DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030428.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	57	rVB2	181194	189403	16.36%	2.078%
2	1.666	91	95	103	rVB	112530	138653	11.98%	1.521%
3	2.307	194	200	210	rVB	244610	367119	31.71%	4.027%
4	2.788	275	279	285	rVB4	2856	5524	0.48%	0.061%
5	2.873	291	293	294	rBV	514	307	0.03%	0.003%
6	2.953	297	306	315	rVV2	7674	19377	1.67%	0.213%
7	3.044	318	321	323	rBV2	304	420	0.04%	0.005%
8	3.093	323	329	338	rVB4	5476	11761	1.02%	0.129%
9	3.282	356	360	362	rVB2	406	499	0.04%	0.005%
10	3.312	362	365	367	rBV2	295	277	0.02%	0.003%
11	3.416	379	382	383	rVB	517	415	0.04%	0.005%
12	3.447	383	387	392	rBV5	674	1408	0.12%	0.015%
13	3.587	406	410	411	rVB2	393	428	0.04%	0.005%
14	3.654	417	421	422	rVB	481	388	0.03%	0.004%
15	3.672	422	424	428	rBV2	269	346	0.03%	0.004%
16	3.843	450	452	455	rVV2	378	416	0.04%	0.005%
17	3.916	462	464	466	rBV2	486	478	0.04%	0.005%
18	4.154	500	503	504	rBV	349	291	0.03%	0.003%
19	4.495	545	559	571	rBV2	261323	889695	76.85%	9.759%
20	5.068	639	653	670	rBV	155924	476124	41.13%	5.222%
21	5.257	682	684	688	rBV2	445	381	0.03%	0.004%
22	5.379	702	704	705	rBV	583	446	0.04%	0.005%
23	5.550	726	732	734	rBV3	1679	2804	0.24%	0.031%
24	5.727	758	761	763	rVB	356	357	0.03%	0.004%
25	5.977	790	802	815	rBV2	395128	1157669	100.00%	12.698%
26	6.160	830	832	836	rVV3	572	856	0.07%	0.009%
27	6.214	839	841	846	rBV2	363	614	0.05%	0.007%
28	6.373	864	867	868	rBV3	535	470	0.04%	0.005%
29	6.422	873	875	878	rBV	471	511	0.04%	0.006%
30	6.678	916	917	919	rVV2	440	330	0.03%	0.004%
31	6.769	922	932	947	rVV	251373	601535	51.96%	6.598%
32	7.043	974	977	981	rBV2	480	782	0.07%	0.009%
33	7.111	981	988	996	rBV4	13283	30497	2.63%	0.335%
34	7.208	1002	1004	1006	rBV2	657	452	0.04%	0.005%
35	7.232	1006	1008	1010	rVB2	519	363	0.03%	0.004%
36	7.312	1012	1021	1033	rBV	244849	532273	45.98%	5.838%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030428.D
 Acq On : 05 Aug 2022 14:35
 Operator : JC/MD
 Sample : N4003-11DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D58DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.501	1046	1052	1055	rVB4	1004	2037	0.18%	0.022%
38	7.623	1070	1072	1079	rBV2	407	655	0.06%	0.007%
39	7.678	1079	1081	1084	rBV2	379	446	0.04%	0.005%
40	7.738	1088	1091	1093	rVB2	492	415	0.04%	0.005%
41	7.781	1093	1098	1100	rBV2	420	645	0.06%	0.007%
42	7.824	1102	1105	1107	rVB2	489	511	0.04%	0.006%
43	7.860	1109	1111	1113	rVB2	464	355	0.03%	0.004%
44	7.946	1121	1125	1126	rBV3	645	600	0.05%	0.007%
45	8.275	1175	1179	1181	rBV2	546	708	0.06%	0.008%
46	8.330	1181	1188	1200	rVV	168761	270231	23.34%	2.964%
47	8.653	1234	1241	1255	rBV	604148	915401	79.07%	10.041%
48	8.751	1255	1257	1258	rVV	615	311	0.03%	0.003%
49	8.866	1274	1276	1279	rVB3	362	355	0.03%	0.004%
50	8.952	1284	1290	1298	rBV	119936	174210	15.05%	1.911%
51	9.189	1324	1329	1331	rBV3	497	802	0.07%	0.009%
52	9.214	1331	1333	1334	rBV	442	299	0.03%	0.003%
53	9.391	1356	1362	1375	rBV	471302	676151	58.41%	7.417%
54	9.622	1399	1400	1403	rBV3	505	450	0.04%	0.005%
55	9.702	1411	1413	1416	rBV3	700	919	0.08%	0.010%
56	9.854	1435	1438	1440	rVB2	435	503	0.04%	0.006%
57	9.878	1440	1442	1445	rBV3	334	379	0.03%	0.004%
58	9.939	1450	1452	1459	rBV2	665	1218	0.11%	0.013%
59	9.994	1459	1461	1464	rBV2	428	326	0.03%	0.004%
60	10.055	1465	1471	1482	rVV	502118	689691	59.58%	7.565%
61	10.470	1537	1539	1541	rBV2	508	467	0.04%	0.005%
62	10.653	1566	1569	1571	rVB3	683	639	0.06%	0.007%
63	10.671	1571	1572	1575	rBV2	382	443	0.04%	0.005%
64	10.781	1588	1590	1591	rBV	429	365	0.03%	0.004%
65	10.903	1608	1610	1612	rVB2	502	381	0.03%	0.004%
66	11.024	1628	1630	1634	rVB	423	413	0.04%	0.005%
67	11.195	1652	1658	1665	rBV	424908	538173	46.49%	5.903%
68	11.396	1690	1691	1694	rBV2	334	309	0.03%	0.003%
69	11.555	1715	1717	1719	rVB	346	304	0.03%	0.003%
70	11.817	1758	1760	1762	rVB	485	282	0.02%	0.003%
71	11.848	1763	1765	1767	rVB	614	391	0.03%	0.004%
72	11.890	1770	1772	1774	rVB2	456	277	0.02%	0.003%
73	11.988	1786	1788	1789	rVV	415	279	0.02%	0.003%
74	12.024	1789	1794	1804	rVV	516028	624608	53.95%	6.851%
75	12.213	1823	1825	1828	rBV	335	349	0.03%	0.004%
76	12.323	1837	1843	1850	rBV	614795	766308	66.19%	8.405%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030428.D
 Acq On : 05 Aug 2022 14:35
 Operator : JC/MD
 Sample : N4003-11DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D58DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.530	1874	1877	1879	rVB2	445	495	0.04%	0.005%
78	12.573	1881	1884	1885	rVV2	574	515	0.04%	0.006%
79	12.603	1888	1889	1890	rVV	641	326	0.03%	0.004%
80	12.652	1896	1897	1900	rVB	673	443	0.04%	0.005%
81	12.731	1909	1910	1912	rVB2	485	318	0.03%	0.003%
82	12.799	1920	1921	1925	rBV3	296	313	0.03%	0.003%
83	12.847	1927	1929	1930	rVB	651	378	0.03%	0.004%
84	12.890	1934	1936	1938	rBV2	329	344	0.03%	0.004%
85	12.988	1950	1952	1954	rBV2	375	375	0.03%	0.004%
86	13.030	1957	1959	1962	rVB2	400	406	0.04%	0.004%
87	13.298	2002	2003	2008	rVB	619	346	0.03%	0.004%
88	13.542	2041	2043	2047	rVB	450	379	0.03%	0.004%
89	13.780	2080	2082	2087	rVB3	619	623	0.05%	0.007%
90	13.902	2101	2102	2104	rBV	532	366	0.03%	0.004%
91	13.975	2112	2114	2116	rBV2	641	533	0.05%	0.006%
92	14.256	2158	2160	2164	rVB3	482	460	0.04%	0.005%
93	14.548	2206	2208	2211	rVB	512	448	0.04%	0.005%
94	14.634	2220	2222	2225	rBV2	481	735	0.06%	0.008%
95	14.756	2240	2242	2244	rBV2	730	744	0.06%	0.008%
96	15.652	2388	2389	2391	rBV2	536	390	0.03%	0.004%
97	16.072	2457	2458	2461	rBV2	918	796	0.07%	0.009%
98	16.103	2461	2463	2465	rVV	793	588	0.05%	0.006%
99	16.267	2488	2490	2491	rBV2	910	567	0.05%	0.006%
100	16.383	2507	2509	2510	rBV	1069	671	0.06%	0.007%

Sum of corrected areas: 9116834




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030428.D
Acq On : 05 Aug 2022 14:35
Operator : JC/MD
Sample : N4003-11DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D58DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

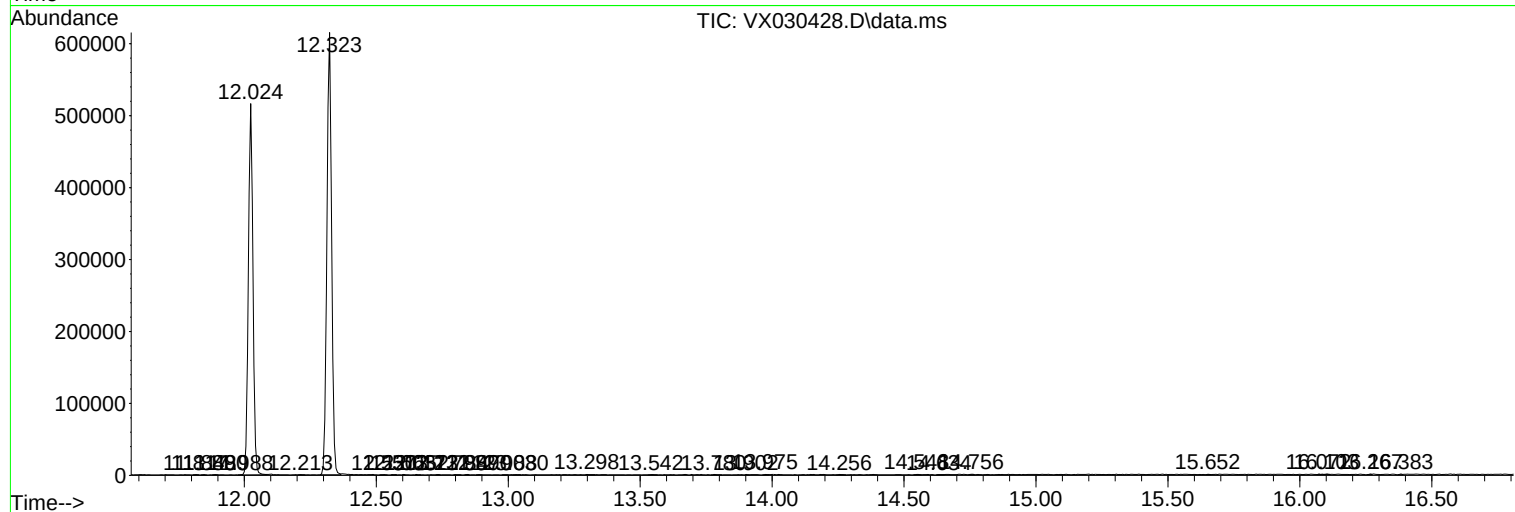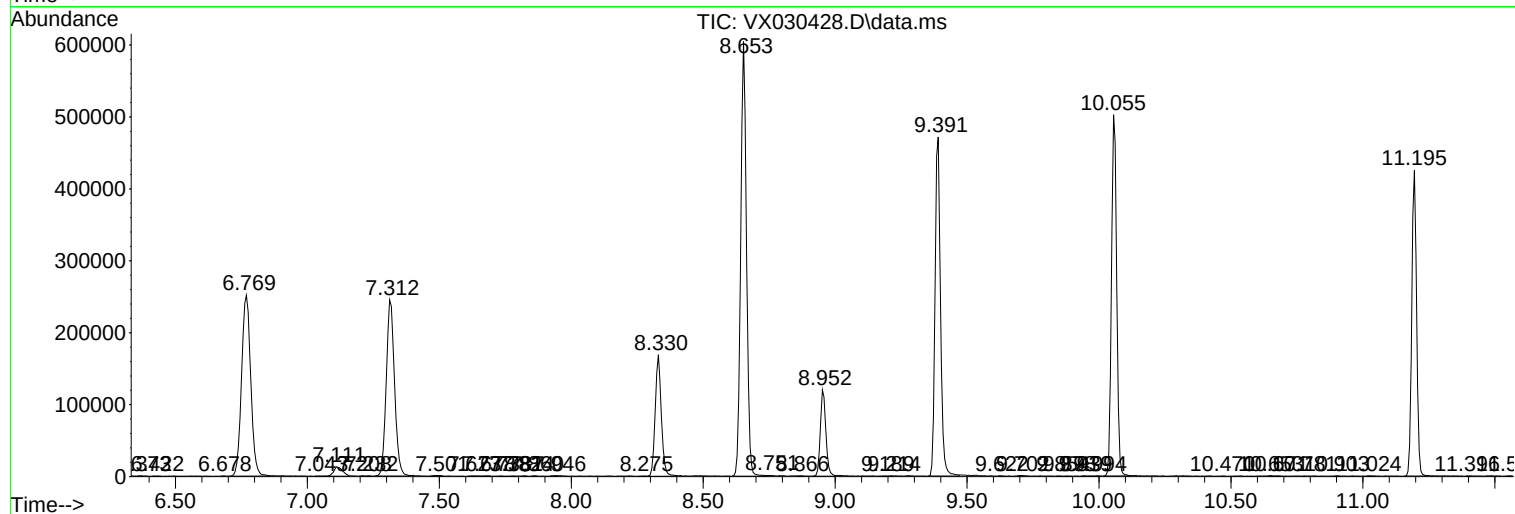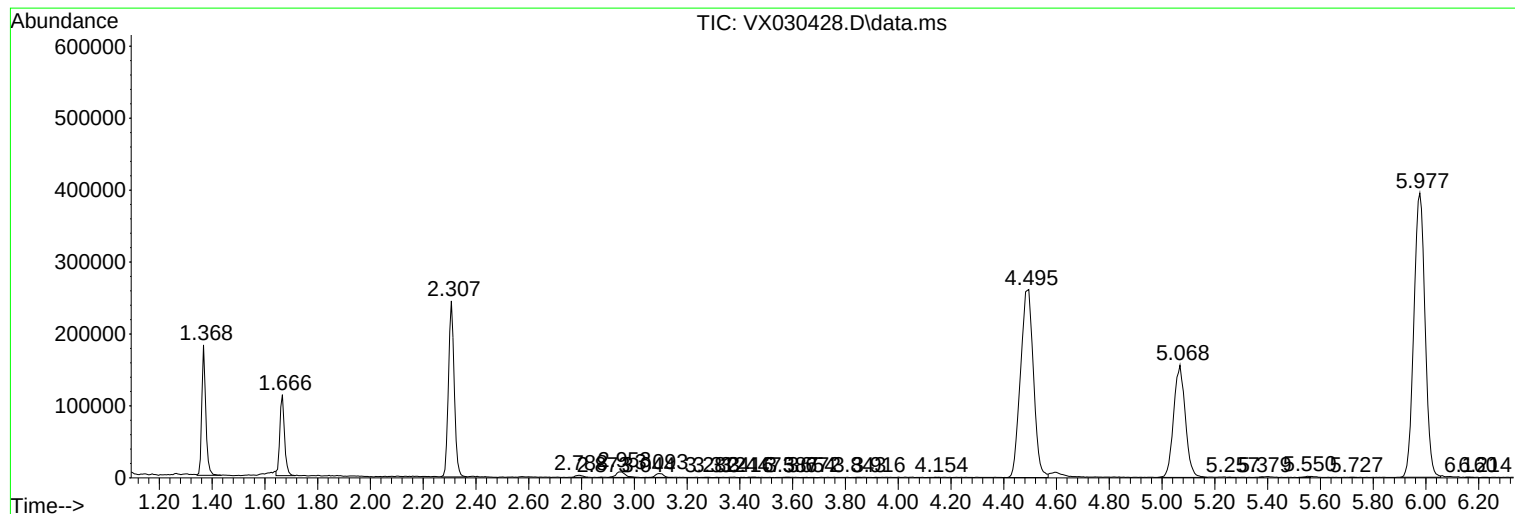

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030428.D
Acq On : 05 Aug 2022 14:35
Operator : JC/MD
Sample : N4003-11DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D58DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030428.D
Acq On : 05 Aug 2022 14:35
Operator : JC/MD
Sample : N4003-11DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D58DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc