

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030429.D
 Acq On : 05 Aug 2022 14:59
 Operator : JC/MD
 Sample : N4003-12DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D59DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030429.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	55	rVB2	176099	184724	15.63%	1.968%
2	1.666	91	95	104	rVB	115407	142935	12.10%	1.523%
3	2.178	177	179	182	rBV4	866	1049	0.09%	0.011%
4	2.306	193	200	211	rVB	232767	362750	30.70%	3.865%
5	2.550	238	240	241	rBV2	419	320	0.03%	0.003%
6	2.568	241	243	246	rBV2	734	959	0.08%	0.010%
7	2.703	261	265	266	rBV3	558	777	0.07%	0.008%
8	2.794	275	280	286	rVB4	2537	4918	0.42%	0.052%
9	2.952	300	306	312	rVV	4922	10546	0.89%	0.112%
10	3.099	324	330	338	rBV4	5614	10726	0.91%	0.114%
11	3.239	351	353	357	rBV	303	381	0.03%	0.004%
12	3.343	366	370	372	rVB2	482	569	0.05%	0.006%
13	3.373	372	375	378	rBV2	384	453	0.04%	0.005%
14	3.672	423	424	427	rVV	592	355	0.03%	0.004%
15	3.782	439	442	443	rBV2	347	392	0.03%	0.004%
16	3.879	456	458	461	rBV	426	521	0.04%	0.006%
17	4.227	513	515	518	rBV2	527	566	0.05%	0.006%
18	4.294	522	526	527	rBV	420	450	0.04%	0.005%
19	4.489	545	558	570	rBV2	266650	897402	75.95%	9.561%
20	4.727	595	597	599	rBV	640	644	0.05%	0.007%
21	4.897	622	625	626	rBV2	438	399	0.03%	0.004%
22	5.068	638	653	669	rBV	153521	477175	40.39%	5.084%
23	5.263	683	685	687	rVB2	475	417	0.04%	0.004%
24	5.287	687	689	690	rBV	686	486	0.04%	0.005%
25	5.550	726	732	734	rBV3	2377	3724	0.32%	0.040%
26	5.690	751	755	758	rVB	446	520	0.04%	0.006%
27	5.720	758	760	763	rBV2	413	465	0.04%	0.005%
28	5.879	783	786	787	rBV	290	377	0.03%	0.004%
29	5.976	790	802	819	rBV2	404804	1181535	100.00%	12.589%
30	6.135	826	828	829	rBV2	415	361	0.03%	0.004%
31	6.257	846	848	849	rVB2	515	310	0.03%	0.003%
32	6.293	851	854	857	rBV2	508	545	0.05%	0.006%
33	6.330	857	860	861	rBV2	419	335	0.03%	0.004%
34	6.391	868	870	871	rBV2	510	336	0.03%	0.004%
35	6.525	891	892	896	rBV3	385	490	0.04%	0.005%
36	6.574	898	900	901	rVV2	546	344	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030429.D
 Acq On : 05 Aug 2022 14:59
 Operator : JC/MD
 Sample : N4003-12DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D59DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.769	921	932	946	rBV	274942	655567	55.48%	6.985%
38	6.970	963	965	966	rBV2	414	312	0.03%	0.003%
39	7.031	972	975	977	rBV2	705	589	0.05%	0.006%
40	7.068	979	981	982	rBV	381	354	0.03%	0.004%
41	7.116	982	989	1000	rVB4	12703	31102	2.63%	0.331%
42	7.311	1012	1021	1037	rVV	255315	549621	46.52%	5.856%
43	7.433	1040	1041	1043	rBV2	594	440	0.04%	0.005%
44	7.726	1085	1089	1091	rVB2	539	674	0.06%	0.007%
45	7.756	1091	1094	1095	rBV	343	312	0.03%	0.003%
46	7.952	1120	1126	1129	rBV3	781	1570	0.13%	0.017%
47	8.019	1133	1137	1138	rBV2	361	499	0.04%	0.005%
48	8.043	1140	1141	1144	rBV	438	521	0.04%	0.006%
49	8.189	1163	1165	1167	rVB2	756	545	0.05%	0.006%
50	8.330	1181	1188	1198	rBV	166152	275940	23.35%	2.940%
51	8.488	1212	1214	1216	rVV3	749	593	0.05%	0.006%
52	8.543	1221	1223	1225	rVB2	509	336	0.03%	0.004%
53	8.653	1234	1241	1254	rBV	617875	932948	78.96%	9.940%
54	8.842	1270	1272	1275	rBV	566	430	0.04%	0.005%
55	8.872	1275	1277	1280	rVB2	592	462	0.04%	0.005%
56	8.951	1283	1290	1303	rBV	119140	179459	15.19%	1.912%
57	9.079	1309	1311	1315	rVB3	756	820	0.07%	0.009%
58	9.232	1332	1336	1338	rBV2	449	611	0.05%	0.007%
59	9.281	1342	1344	1348	rVB3	474	504	0.04%	0.005%
60	9.390	1356	1362	1376	rBV	485847	695811	58.89%	7.414%
61	9.695	1408	1412	1414	rBV3	518	690	0.06%	0.007%
62	9.823	1430	1433	1436	rBV2	492	573	0.05%	0.006%
63	9.988	1459	1460	1463	rVB2	461	315	0.03%	0.003%
64	10.055	1466	1471	1485	rVV	550491	749539	63.44%	7.986%
65	10.415	1529	1530	1533	rBV2	385	355	0.03%	0.004%
66	10.543	1548	1551	1552	rBV2	367	395	0.03%	0.004%
67	10.744	1581	1584	1586	rBV2	267	372	0.03%	0.004%
68	10.805	1592	1594	1596	rBV2	544	396	0.03%	0.004%
69	10.835	1598	1599	1602	rBV	488	385	0.03%	0.004%
70	11.067	1635	1637	1638	rBV	499	333	0.03%	0.004%
71	11.091	1638	1641	1643	rBV2	749	493	0.04%	0.005%
72	11.195	1653	1658	1666	rVB	426820	545471	46.17%	5.812%
73	11.847	1764	1765	1768	rBV2	382	334	0.03%	0.004%
74	11.933	1778	1779	1781	rBV	529	335	0.03%	0.004%
75	12.024	1789	1794	1804	rVV	543865	675596	57.18%	7.198%
76	12.207	1822	1824	1826	rBV3	608	580	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030429.D
 Acq On : 05 Aug 2022 14:59
 Operator : JC/MD
 Sample : N4003-12DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D59DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.323	1838	1843	1849	rBV	632338	778787	65.91%	8.298%
78	12.475	1865	1868	1869	rBV	526	386	0.03%	0.004%
79	12.597	1886	1888	1890	rBV	597	662	0.06%	0.007%
80	12.682	1899	1902	1905	rBV	371	569	0.05%	0.006%
81	12.878	1931	1934	1936	rBV3	314	418	0.04%	0.004%
82	13.006	1954	1955	1957	rBV	367	337	0.03%	0.004%
83	13.073	1965	1966	1968	rBV	548	394	0.03%	0.004%
84	13.365	2012	2014	2016	rBV	465	453	0.04%	0.005%
85	13.518	2037	2039	2040	rVB	577	321	0.03%	0.003%
86	14.115	2135	2137	2138	rBV	484	356	0.03%	0.004%
87	14.310	2168	2169	2172	rBV	342	329	0.03%	0.004%
88	14.383	2179	2181	2184	rVB3	593	475	0.04%	0.005%
89	14.444	2188	2191	2192	rBV	541	402	0.03%	0.004%
90	14.481	2195	2197	2199	rBV	401	361	0.03%	0.004%
91	14.670	2226	2228	2230	rBV	418	381	0.03%	0.004%
92	14.810	2249	2251	2253	rBV2	605	437	0.04%	0.005%
93	14.920	2267	2269	2271	rBV2	690	685	0.06%	0.007%
94	15.182	2310	2312	2316	rBV	708	787	0.07%	0.008%
95	15.310	2331	2333	2334	rBV2	527	414	0.04%	0.004%
96	15.584	2376	2378	2381	rBV3	691	765	0.06%	0.008%
97	15.999	2444	2446	2450	rBV2	760	887	0.08%	0.009%
98	16.224	2482	2483	2484	rBV	530	311	0.03%	0.003%
99	16.389	2508	2510	2513	rVB	727	562	0.05%	0.006%
100	16.432	2513	2517	2519	rBV3	600	763	0.06%	0.008%




Sum of corrected areas: 9385680

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030429.D
Acq On : 05 Aug 2022 14:59
Operator : JC/MD
Sample : N4003-12DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D59DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

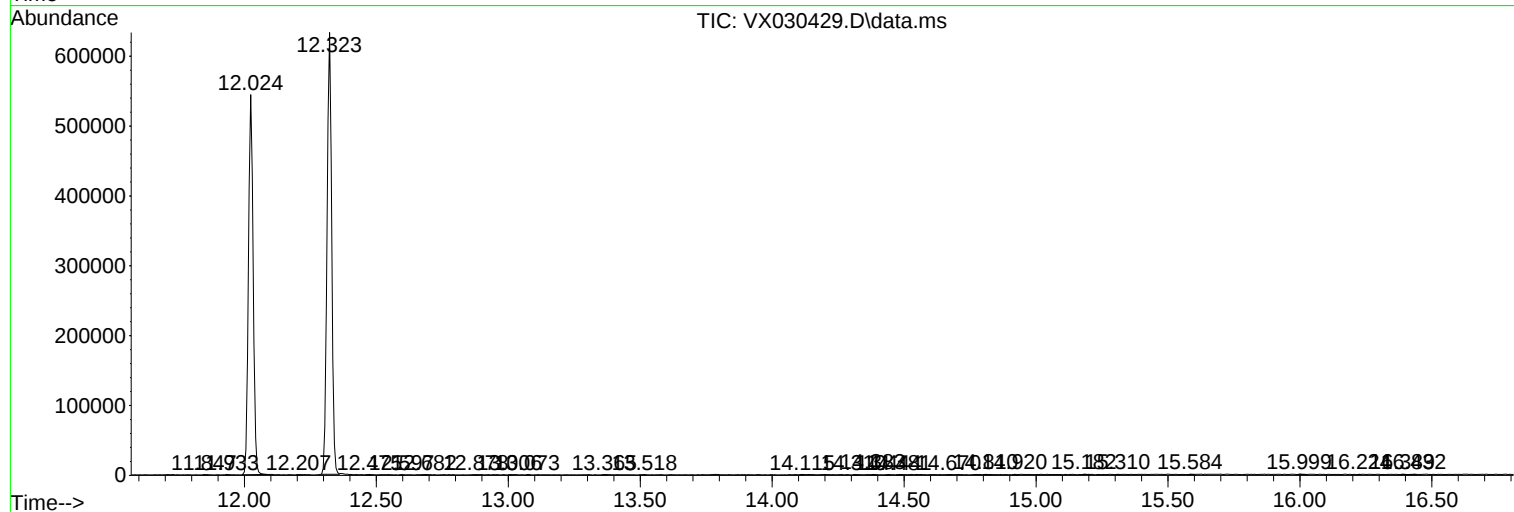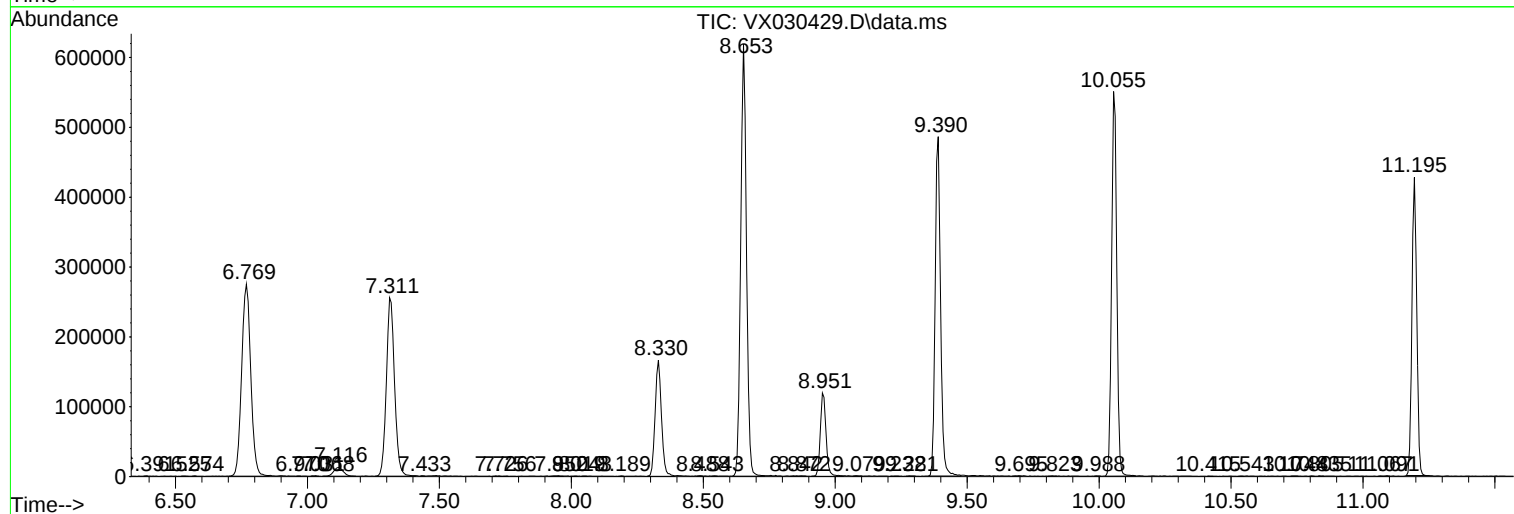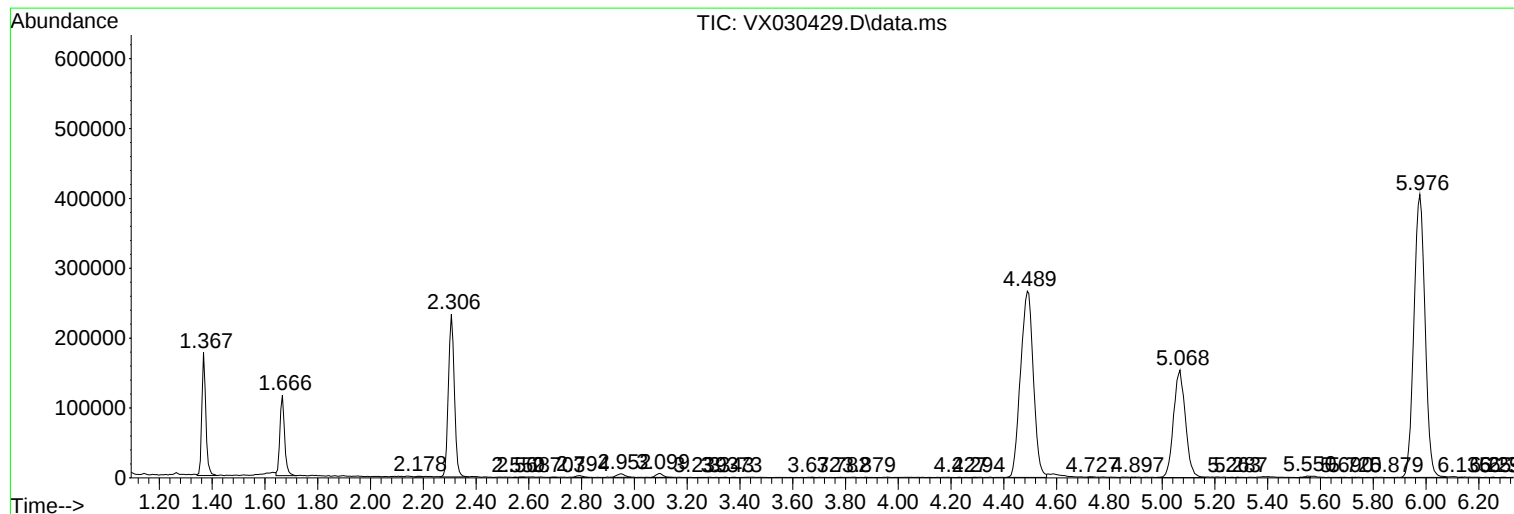

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030429.D
Acq On : 05 Aug 2022 14:59
Operator : JC/MD
Sample : N4003-12DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D59DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030429.D
Acq On : 05 Aug 2022 14:59
Operator : JC/MD
Sample : N4003-12DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D59DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc