

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030430.D
 Acq On : 05 Aug 2022 15:22
 Operator : JC/MD
 Sample : N4003-17DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D86DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030430.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	52	rBV	137655	135746	12.59%	1.467%
2	1.666	91	95	103	rVB	101657	125408	11.63%	1.356%
3	2.307	194	200	210	rVB	222270	349519	32.41%	3.778%
4	2.392	210	214	218	rVB4	1103	1702	0.16%	0.018%
5	2.575	239	244	246	rBV3	980	1617	0.15%	0.017%
6	2.788	274	279	287	rBV5	3948	7455	0.69%	0.081%
7	2.947	297	305	318	rVB3	10848	27615	2.56%	0.298%
8	3.093	322	329	342	rVB	71370	135641	12.58%	1.466%
9	3.215	347	349	353	rBV	321	301	0.03%	0.003%
10	3.373	371	375	376	rBV2	299	382	0.04%	0.004%
11	3.837	449	451	454	rVV	510	489	0.05%	0.005%
12	3.861	454	455	461	rVB2	407	442	0.04%	0.005%
13	3.971	470	473	475	rBV2	510	452	0.04%	0.005%
14	4.020	479	481	482	rVV	429	295	0.03%	0.003%
15	4.038	482	484	486	rVV	501	322	0.03%	0.003%
16	4.087	490	492	494	rVB	607	566	0.05%	0.006%
17	4.111	494	496	499	rBV2	432	551	0.05%	0.006%
18	4.148	499	502	507	rVB2	432	714	0.07%	0.008%
19	4.282	523	524	527	rBV	435	505	0.05%	0.005%
20	4.489	546	558	570	rBV2	340787	1078272	100.00%	11.655%
21	4.855	616	618	620	rBV3	622	578	0.05%	0.006%
22	5.068	639	653	670	rVB	140402	426627	39.57%	4.612%
23	5.391	703	706	715	rVB4	1133	3085	0.29%	0.033%
24	5.471	715	719	720	rBV2	378	372	0.03%	0.004%
25	5.556	727	733	744	rVB6	1824	5772	0.54%	0.062%
26	5.641	744	747	749	rBV3	474	536	0.05%	0.006%
27	5.666	749	751	757	rVB2	455	685	0.06%	0.007%
28	5.721	757	760	762	rBV2	422	388	0.04%	0.004%
29	5.800	771	773	776	rBV2	399	414	0.04%	0.004%
30	5.977	789	802	819	rBV2	363485	1064013	98.68%	11.501%
31	6.196	836	838	839	rBV2	478	326	0.03%	0.004%
32	6.227	842	843	845	rVB	441	283	0.03%	0.003%
33	6.257	845	848	851	rBV2	546	616	0.06%	0.007%
34	6.361	863	865	869	rBV2	668	955	0.09%	0.010%
35	6.446	875	879	880	rVB2	336	289	0.03%	0.003%
36	6.580	899	901	904	rVB2	594	357	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030430.D
 Acq On : 05 Aug 2022 15:22
 Operator : JC/MD
 Sample : N4003-17DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D86DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.617	904	907	911	rBV2	399	468	0.04%	0.005%
38	6.769	922	932	948	rBV	266795	634373	58.83%	6.857%
39	6.970	963	965	968	rVB	467	530	0.05%	0.006%
40	7.001	968	970	973	rVB	636	531	0.05%	0.006%
41	7.037	973	976	978	rBV	410	466	0.04%	0.005%
42	7.129	982	991	1004	rVB2	139988	315693	29.28%	3.412%
43	7.318	1012	1022	1036	rBV	218960	486808	45.15%	5.262%
44	7.476	1046	1048	1049	rBV	698	683	0.06%	0.007%
45	7.568	1061	1063	1064	rBV	642	368	0.03%	0.004%
46	7.678	1078	1081	1083	rBV2	483	564	0.05%	0.006%
47	7.787	1097	1099	1102	rBV2	341	348	0.03%	0.004%
48	7.946	1121	1125	1128	rVV2	570	775	0.07%	0.008%
49	7.988	1130	1132	1134	rBV	294	288	0.03%	0.003%
50	8.269	1176	1178	1181	rBV	266	369	0.03%	0.004%
51	8.330	1181	1188	1200	rVV	148286	243965	22.63%	2.637%
52	8.653	1234	1241	1255	rBV	529101	828718	76.86%	8.958%
53	8.811	1265	1267	1271	rVB2	992	764	0.07%	0.008%
54	8.952	1284	1290	1300	rBV	102549	160243	14.86%	1.732%
55	9.171	1324	1326	1330	rVB3	440	528	0.05%	0.006%
56	9.275	1339	1343	1348	rVB3	10458	16416	1.52%	0.177%
57	9.391	1356	1362	1375	rBV	419228	615861	57.12%	6.657%
58	9.634	1400	1402	1408	rVB3	445	672	0.06%	0.007%
59	9.708	1410	1414	1420	rVV4	1733	2633	0.24%	0.028%
60	9.842	1434	1436	1439	rVB3	529	581	0.05%	0.006%
61	10.055	1466	1471	1485	rVB	522024	707074	65.57%	7.643%
62	10.220	1497	1498	1499	rBV	451	316	0.03%	0.003%
63	10.256	1502	1504	1507	rVB2	493	424	0.04%	0.005%
64	10.348	1517	1519	1520	rBV2	418	395	0.04%	0.004%
65	10.476	1538	1540	1543	rBV2	315	337	0.03%	0.004%
66	10.573	1554	1556	1558	rBV	366	307	0.03%	0.003%
67	10.726	1579	1581	1582	rBV	337	350	0.03%	0.004%
68	10.909	1608	1611	1612	rBV2	586	442	0.04%	0.005%
69	10.976	1620	1622	1625	rBV	520	454	0.04%	0.005%
70	11.006	1625	1627	1629	rVB2	575	505	0.05%	0.005%
71	11.195	1652	1658	1670	rVB	388167	485234	45.00%	5.245%
72	11.695	1738	1740	1741	rBV2	384	292	0.03%	0.003%
73	11.835	1761	1763	1766	rVB	498	361	0.03%	0.004%
74	11.872	1766	1769	1772	rVB2	400	532	0.05%	0.006%
75	11.902	1772	1774	1777	rVB2	351	319	0.03%	0.003%
76	12.024	1789	1794	1805	rVB	527617	640817	59.43%	6.927%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030430.D
 Acq On : 05 Aug 2022 15:22
 Operator : JC/MD
 Sample : N4003-17DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D86DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.195	1820	1822	1825	rVB2	700	501	0.05%	0.005%
78	12.268	1831	1834	1835	rBV3	539	399	0.04%	0.004%
79	12.323	1837	1843	1854	rVV	564172	714655	66.28%	7.725%
80	12.500	1871	1872	1875	rVB2	587	422	0.04%	0.005%
81	12.567	1882	1883	1886	rBV	704	499	0.05%	0.005%
82	12.658	1896	1898	1902	rBV3	404	506	0.05%	0.005%
83	12.768	1911	1916	1917	rBV2	386	681	0.06%	0.007%
84	12.841	1926	1928	1930	rBV	693	454	0.04%	0.005%
85	12.872	1930	1933	1936	rVV	520	686	0.06%	0.007%
86	13.274	1997	1999	2001	rBV	466	465	0.04%	0.005%
87	13.292	2001	2002	2004	rVB2	543	346	0.03%	0.004%
88	13.372	2014	2015	2018	rBV2	654	558	0.05%	0.006%
89	13.469	2028	2031	2032	rBV2	421	409	0.04%	0.004%
90	13.518	2036	2039	2040	rVB2	541	398	0.04%	0.004%
91	13.701	2067	2069	2071	rVB2	414	323	0.03%	0.003%
92	13.731	2071	2074	2079	rVB3	607	710	0.07%	0.008%
93	13.792	2079	2084	2085	rBV2	818	957	0.09%	0.010%
94	13.945	2107	2109	2113	rBV2	583	581	0.05%	0.006%
95	14.189	2148	2149	2151	rVB	594	314	0.03%	0.003%
96	14.304	2166	2168	2171	rBV	626	443	0.04%	0.005%
97	14.652	2223	2225	2228	rVB2	524	350	0.03%	0.004%
98	14.884	2260	2263	2265	rBV2	610	539	0.05%	0.006%
99	15.280	2325	2328	2330	rBV3	672	925	0.09%	0.010%
100	15.774	2404	2409	2410	rBV4	832	1131	0.10%	0.012%




Sum of corrected areas: 9251346

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030430.D
Acq On : 05 Aug 2022 15:22
Operator : JC/MD
Sample : N4003-17DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D86DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

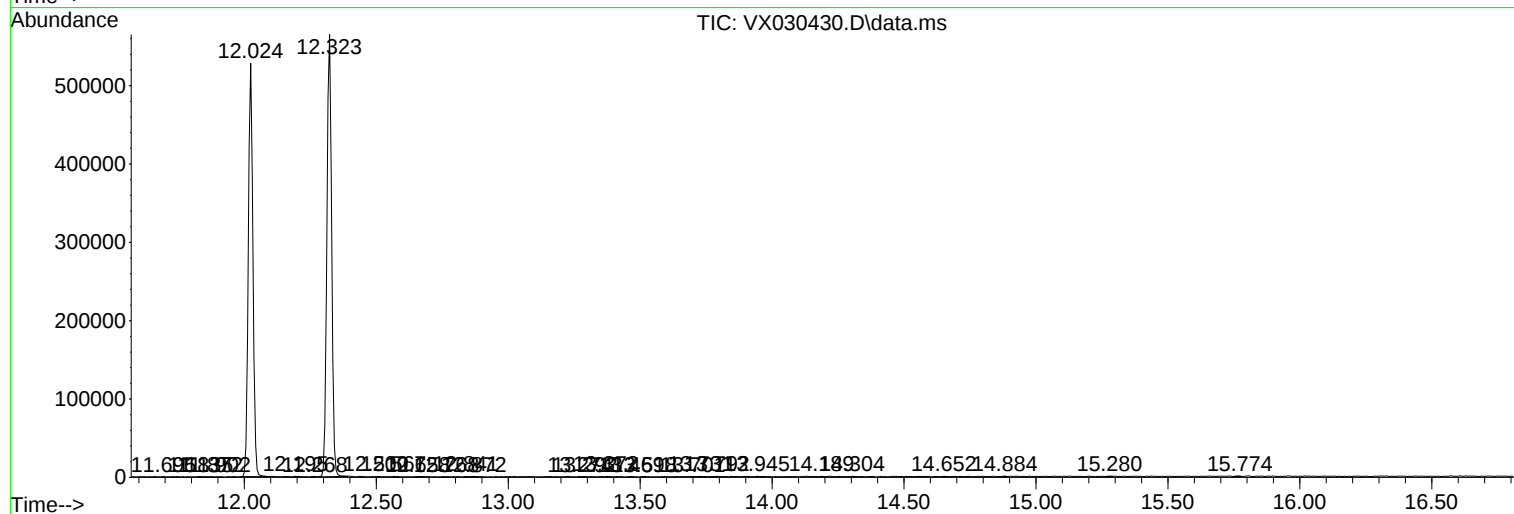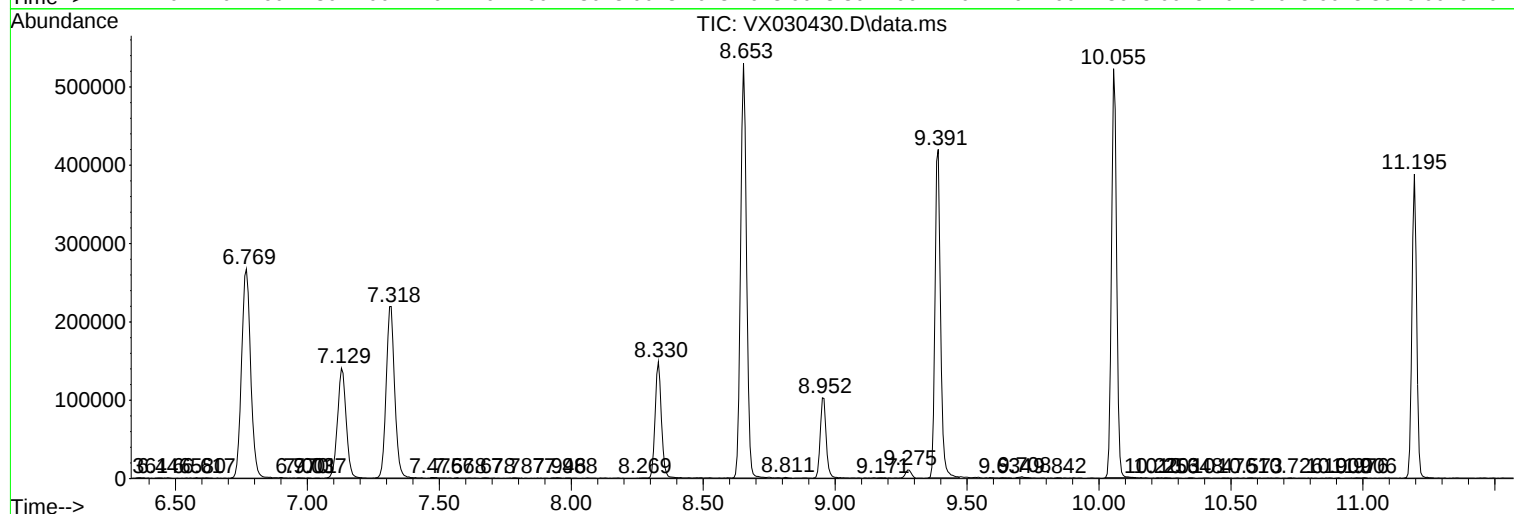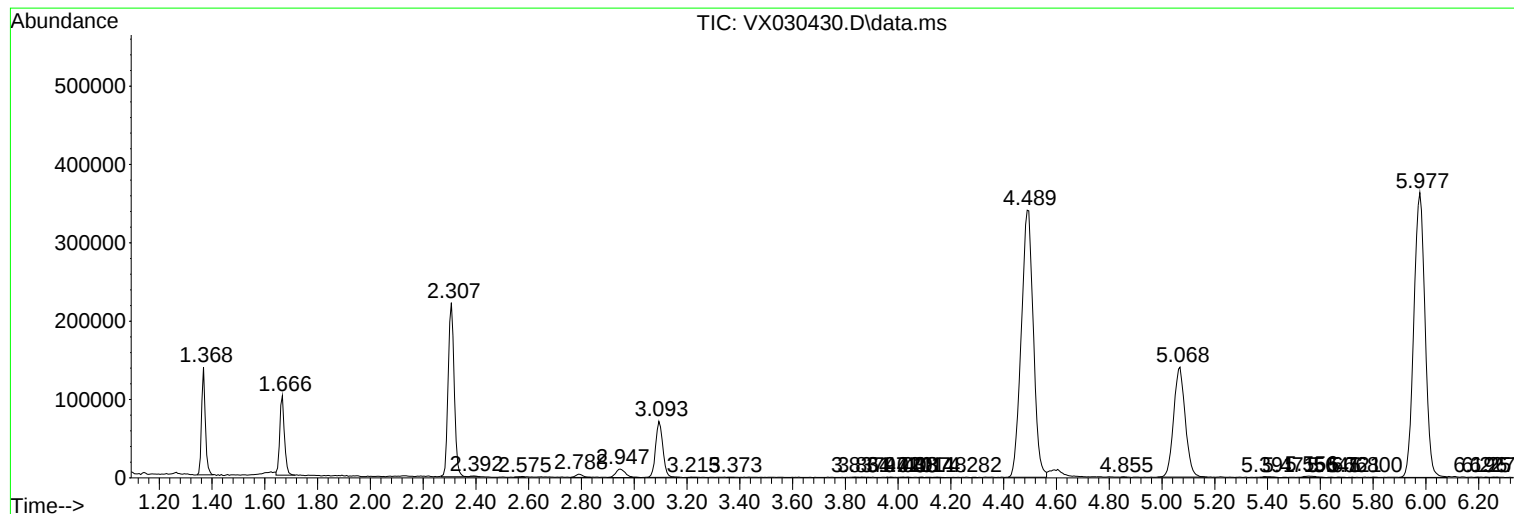

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030430.D
Acq On : 05 Aug 2022 15:22
Operator : JC/MD
Sample : N4003-17DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D86DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030430.D
Acq On : 05 Aug 2022 15:22
Operator : JC/MD
Sample : N4003-17DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D86DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc