

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030431.D
 Acq On : 05 Aug 2022 15:45
 Operator : JC/MD
 Sample : N4003-18DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D88DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030431.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB2	290503	332975	28.49%	3.741%
2	1.666	91	95	105	rVB	108801	137959	11.80%	1.550%
3	2.307	194	200	210	rVB	257523	380674	32.57%	4.277%
4	2.392	212	214	221	rVB5	2049	3375	0.29%	0.038%
5	2.532	235	237	239	rBV2	378	306	0.03%	0.003%
6	2.624	250	252	253	rBV	451	416	0.04%	0.005%
7	2.794	275	280	286	rVB2	3647	6287	0.54%	0.071%
8	2.886	290	295	297	rBV2	431	738	0.06%	0.008%
9	2.947	298	305	315	rVV	9145	20163	1.72%	0.227%
10	3.099	325	330	336	rVB5	3449	7195	0.62%	0.081%
11	3.215	346	349	350	rBV	354	332	0.03%	0.004%
12	3.453	386	388	391	rBV	278	304	0.03%	0.003%
13	3.575	407	408	414	rVB2	375	609	0.05%	0.007%
14	3.910	461	463	466	rVB2	378	352	0.03%	0.004%
15	4.050	483	486	489	rBV2	315	464	0.04%	0.005%
16	4.239	512	517	518	rVV2	380	402	0.03%	0.005%
17	4.251	518	519	522	rVV2	647	501	0.04%	0.006%
18	4.471	545	555	568	rBV2	114162	360641	30.85%	4.052%
19	4.806	609	610	612	rBV	572	334	0.03%	0.004%
20	4.873	618	621	623	rBV3	277	321	0.03%	0.004%
21	5.062	640	652	668	rVV	155082	476062	40.73%	5.348%
22	5.208	674	676	677	rVB2	706	391	0.03%	0.004%
23	5.221	677	678	681	rBV2	639	670	0.06%	0.008%
24	5.269	685	686	688	rBV	507	369	0.03%	0.004%
25	5.294	688	690	694	rVB2	394	439	0.04%	0.005%
26	5.361	698	701	702	rBV3	608	669	0.06%	0.008%
27	5.391	702	706	707	rBV3	1016	1402	0.12%	0.016%
28	5.556	729	733	734	rBV	1822	2295	0.20%	0.026%
29	5.739	761	763	765	rVB2	573	483	0.04%	0.005%
30	5.873	782	785	789	rBV3	456	728	0.06%	0.008%
31	5.977	789	802	815	rBV2	397361	1168871	100.00%	13.131%
32	6.178	833	835	838	rVB2	599	599	0.05%	0.007%
33	6.208	838	840	845	rBV3	462	613	0.05%	0.007%
34	6.379	866	868	872	rVB2	288	399	0.03%	0.004%
35	6.409	872	873	876	rBV2	286	344	0.03%	0.004%
36	6.452	878	880	882	rVB	387	287	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030431.D
 Acq On : 05 Aug 2022 15:45
 Operator : JC/MD
 Sample : N4003-18DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D88DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.476	882	884	886	rBV	370	415	0.04%	0.005%
38	6.623	906	908	910	rVB	494	380	0.03%	0.004%
39	6.684	915	918	922	rBV2	436	432	0.04%	0.005%
40	6.769	922	932	948	rBV	259511	636780	54.48%	7.154%
41	6.909	953	955	957	rBV2	453	321	0.03%	0.004%
42	7.123	982	990	997	rBV5	12585	30237	2.59%	0.340%
43	7.214	1003	1005	1009	rBV	461	539	0.05%	0.006%
44	7.251	1009	1011	1013	rBV2	375	303	0.03%	0.003%
45	7.312	1013	1021	1033	rBV	245290	537817	46.01%	6.042%
46	7.476	1046	1048	1049	rBV2	887	768	0.07%	0.009%
47	7.580	1063	1065	1069	rBV2	360	538	0.05%	0.006%
48	7.641	1072	1075	1077	rBV2	433	415	0.04%	0.005%
49	7.793	1098	1100	1103	rBV2	408	441	0.04%	0.005%
50	7.909	1116	1119	1120	rBV	370	301	0.03%	0.003%
51	7.952	1120	1126	1130	rVV4	698	1372	0.12%	0.015%
52	7.988	1130	1132	1134	rVV	352	404	0.03%	0.005%
53	8.226	1168	1171	1174	rBV	625	685	0.06%	0.008%
54	8.330	1181	1188	1200	rBV	160881	268519	22.97%	3.017%
55	8.580	1226	1229	1234	rBV2	310	503	0.04%	0.006%
56	8.653	1234	1241	1250	rBV	589128	900685	77.06%	10.118%
57	8.958	1285	1291	1298	rBV	114275	174754	14.95%	1.963%
58	9.391	1356	1362	1375	rBV	493599	700809	59.96%	7.873%
59	9.628	1400	1401	1402	rVB	824	302	0.03%	0.003%
60	9.708	1410	1414	1421	rVV4	1419	2707	0.23%	0.030%
61	9.915	1447	1448	1451	rBV2	404	378	0.03%	0.004%
62	10.055	1465	1471	1486	rBV	512846	720755	61.66%	8.097%
63	10.299	1509	1511	1515	rVV3	592	574	0.05%	0.006%
64	10.640	1564	1567	1568	rBV2	443	456	0.04%	0.005%
65	10.781	1589	1590	1592	rVB2	647	354	0.03%	0.004%
66	10.811	1592	1595	1596	rBV	523	422	0.04%	0.005%
67	10.872	1602	1605	1606	rBV2	370	425	0.04%	0.005%
68	10.957	1618	1619	1622	rBV	337	358	0.03%	0.004%
69	11.043	1631	1633	1635	rBV	449	435	0.04%	0.005%
70	11.195	1652	1658	1670	rBV	439657	556340	47.60%	6.250%
71	11.317	1675	1678	1680	rVB2	435	424	0.04%	0.005%
72	11.348	1680	1683	1684	rBV2	537	339	0.03%	0.004%
73	11.549	1714	1716	1718	rBV2	400	420	0.04%	0.005%
74	11.598	1721	1724	1725	rBV	503	423	0.04%	0.005%
75	11.665	1732	1735	1737	rVB2	479	435	0.04%	0.005%
76	11.713	1742	1743	1745	rBV2	446	291	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030431.D
 Acq On : 05 Aug 2022 15:45
 Operator : JC/MD
 Sample : N4003-18DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D88DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.799	1755	1757	1759	rBV2	317	331	0.03%	0.004%
78	12.024	1789	1794	1801	rBV	536664	655146	56.05%	7.360%
79	12.323	1837	1843	1855	rBV	643247	784401	67.11%	8.812%
80	12.585	1885	1886	1888	rVB	710	439	0.04%	0.005%
81	12.616	1890	1891	1894	rVB	553	466	0.04%	0.005%
82	12.646	1894	1896	1898	rBV	437	335	0.03%	0.004%
83	12.786	1917	1919	1921	rVB2	437	316	0.03%	0.004%
84	12.939	1942	1944	1946	rBV2	450	364	0.03%	0.004%
85	13.042	1958	1961	1964	rBV2	409	484	0.04%	0.005%
86	13.091	1967	1969	1971	rBV	474	392	0.03%	0.004%
87	13.378	2014	2016	2018	rVB	525	354	0.03%	0.004%
88	13.396	2018	2019	2022	rBV2	368	335	0.03%	0.004%
89	13.457	2027	2029	2033	rBV2	409	580	0.05%	0.007%
90	13.573	2047	2048	2051	rVB	448	377	0.03%	0.004%
91	13.658	2061	2062	2064	rBV	436	344	0.03%	0.004%
92	13.829	2088	2090	2091	rVB	578	287	0.02%	0.003%
93	13.859	2093	2095	2098	rVB	579	474	0.04%	0.005%
94	14.128	2134	2139	2141	rBV2	488	790	0.07%	0.009%
95	14.426	2187	2188	2192	rVB2	669	477	0.04%	0.005%
96	14.853	2256	2258	2259	rBV	451	332	0.03%	0.004%
97	14.920	2267	2269	2271	rBV2	555	387	0.03%	0.004%
98	14.975	2276	2278	2280	rBV2	671	624	0.05%	0.007%
99	15.268	2324	2326	2327	rVB	643	293	0.03%	0.003%
100	15.597	2379	2380	2384	rBV2	687	856	0.07%	0.010%




Sum of corrected areas: 8901409

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030431.D
Acq On : 05 Aug 2022 15:45
Operator : JC/MD
Sample : N4003-18DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D88DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

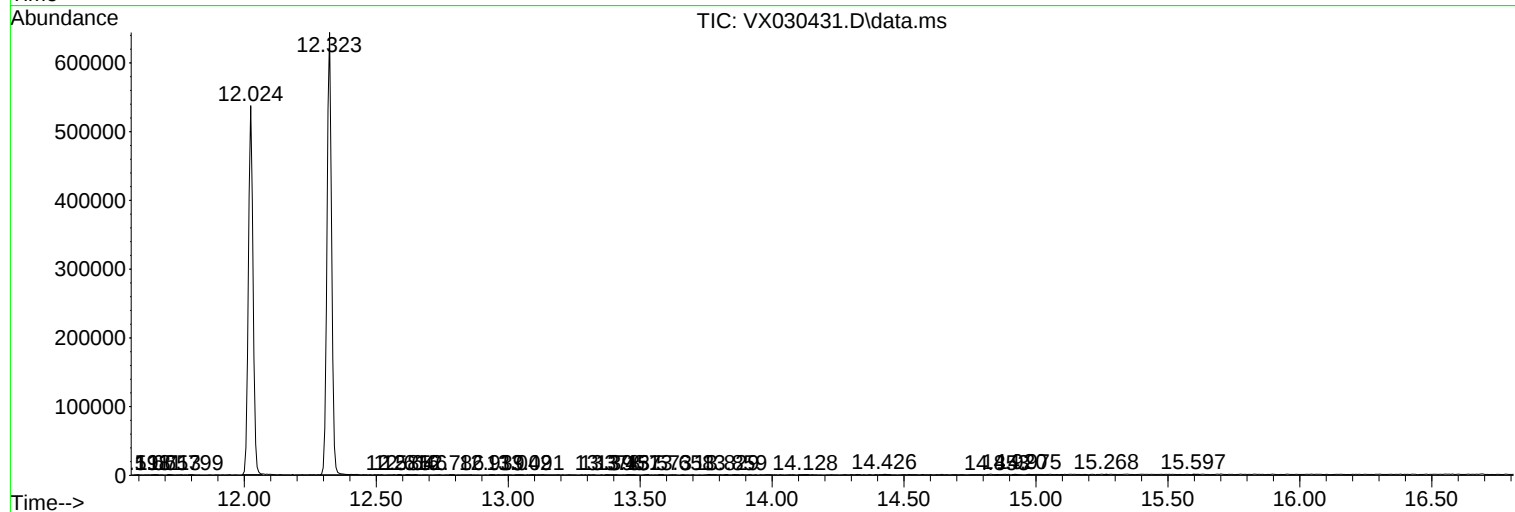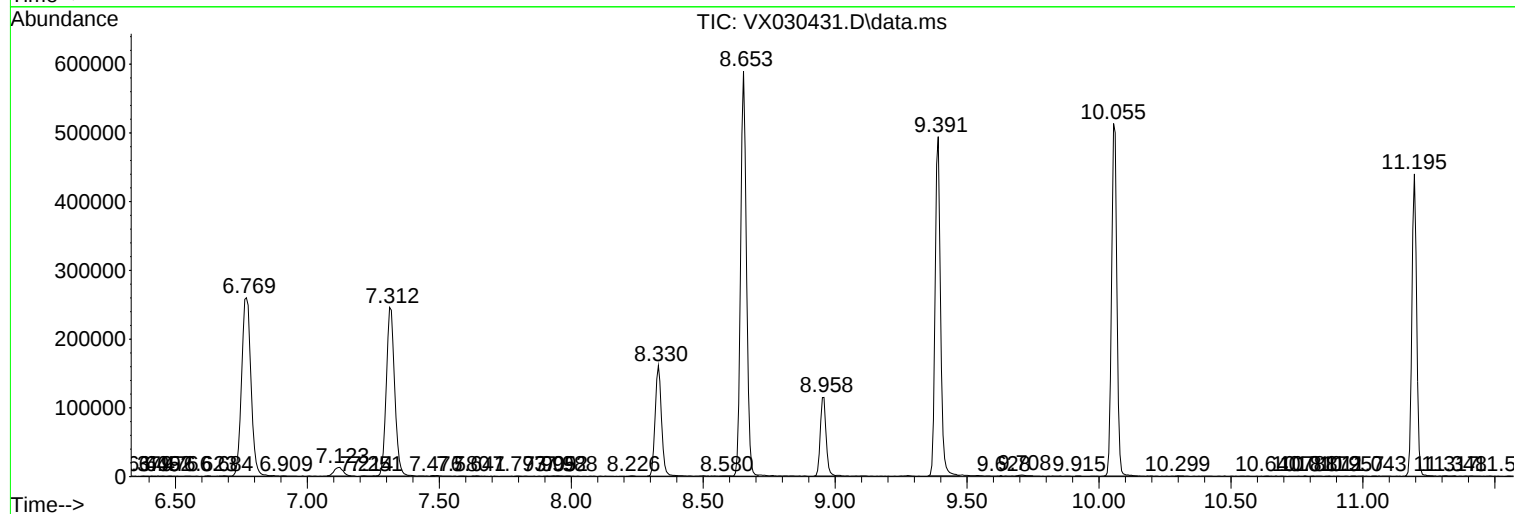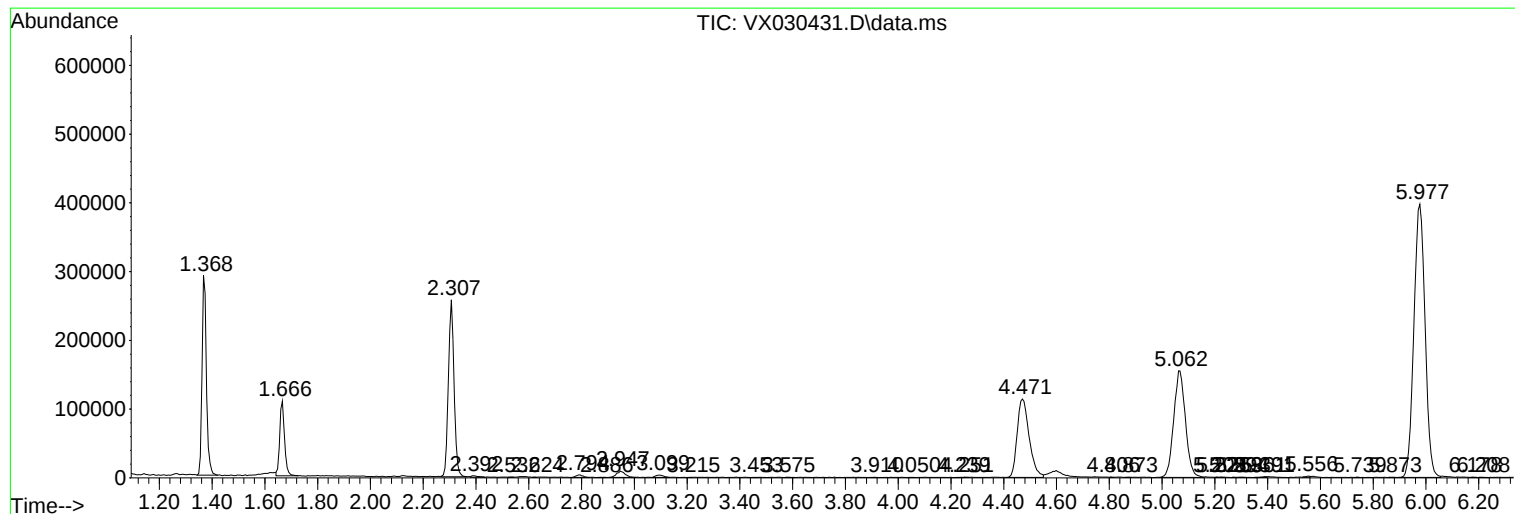

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030431.D
Acq On : 05 Aug 2022 15:45
Operator : JC/MD
Sample : N4003-18DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D88DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030431.D
Acq On : 05 Aug 2022 15:45
Operator : JC/MD
Sample : N4003-18DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D88DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc