

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030432.D
 Acq On : 05 Aug 2022 16:09
 Operator : JC/MD
 Sample : N4003-19DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D89DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030432.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB2	229466	251946	21.40%	2.793%
2	1.666	91	95	104	rVB	110806	138783	11.79%	1.539%
3	2.020	151	153	154	rBV2	822	419	0.04%	0.005%
4	2.306	194	200	211	rVB	247230	381980	32.44%	4.235%
5	2.794	274	280	289	rBV6	3616	10171	0.86%	0.113%
6	2.947	298	305	317	rBV	7503	17187	1.46%	0.191%
7	3.093	324	329	340	rBV4	8298	18726	1.59%	0.208%
8	3.172	340	342	343	rVB	547	333	0.03%	0.004%
9	3.221	347	350	353	rBV2	326	407	0.03%	0.005%
10	3.379	373	376	378	rVB2	347	417	0.04%	0.005%
11	3.428	380	384	385	rBV2	776	935	0.08%	0.010%
12	3.446	385	387	388	rVV2	570	345	0.03%	0.004%
13	3.568	402	407	408	rBV	489	540	0.05%	0.006%
14	3.617	413	415	417	rVV2	420	384	0.03%	0.004%
15	3.782	439	442	444	rBV	374	365	0.03%	0.004%
16	4.001	476	478	479	rBV2	425	373	0.03%	0.004%
17	4.160	500	504	507	rBV3	441	644	0.05%	0.007%
18	4.263	517	521	523	rBV	664	874	0.07%	0.010%
19	4.300	523	527	529	rBV3	1061	1638	0.14%	0.018%
20	4.477	546	556	568	rBV2	142348	509313	43.25%	5.647%
21	4.946	631	633	635	rVB2	541	409	0.03%	0.005%
22	5.062	639	652	672	rBV2	156756	477240	40.53%	5.291%
23	5.324	693	695	698	rVB	640	708	0.06%	0.008%
24	5.373	700	703	704	rBV3	640	609	0.05%	0.007%
25	5.464	715	718	719	rBV2	1065	947	0.08%	0.010%
26	5.556	727	733	734	rBV3	1989	2783	0.24%	0.031%
27	5.800	771	773	775	rBV	312	352	0.03%	0.004%
28	5.885	784	787	788	rBV2	366	355	0.03%	0.004%
29	5.977	788	802	821	rVV2	400464	1177572	100.00%	13.056%
30	6.141	827	829	830	rBV2	458	377	0.03%	0.004%
31	6.251	844	847	849	rBV2	736	767	0.07%	0.009%
32	6.294	851	854	855	rBV	336	398	0.03%	0.004%
33	6.318	855	858	859	rVV	649	373	0.03%	0.004%
34	6.367	863	866	869	rVB2	758	964	0.08%	0.011%
35	6.464	880	882	884	rBV	471	456	0.04%	0.005%
36	6.483	884	885	888	rVB	508	436	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030432.D
 Acq On : 05 Aug 2022 16:09
 Operator : JC/MD
 Sample : N4003-19DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D89DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.568	897	899	902	rVB2	584	510	0.04%	0.006%
38	6.690	916	919	920	rBV	386	352	0.03%	0.004%
39	6.769	922	932	947	rVV2	268609	642793	54.59%	7.127%
40	6.873	947	949	953	rVB2	805	758	0.06%	0.008%
41	6.964	962	964	966	rBV3	438	411	0.03%	0.005%
42	7.110	981	988	1001	rBV4	12206	28915	2.46%	0.321%
43	7.232	1006	1008	1012	rVB2	594	735	0.06%	0.008%
44	7.318	1012	1022	1033	rBV	246105	553043	46.96%	6.132%
45	7.464	1044	1046	1047	rBV	709	498	0.04%	0.006%
46	7.488	1047	1050	1054	rVV4	1064	1742	0.15%	0.019%
47	7.519	1054	1055	1059	rVB	974	616	0.05%	0.007%
48	7.592	1064	1067	1070	rBV	560	517	0.04%	0.006%
49	7.623	1070	1072	1076	rVB2	602	525	0.04%	0.006%
50	7.671	1078	1080	1082	rVB2	668	465	0.04%	0.005%
51	7.744	1089	1092	1093	rVB	423	345	0.03%	0.004%
52	7.873	1110	1113	1114	rBV	594	375	0.03%	0.004%
53	7.952	1122	1126	1129	rVV3	800	1372	0.12%	0.015%
54	8.122	1152	1154	1157	rBV3	448	428	0.04%	0.005%
55	8.330	1181	1188	1199	rBV	167725	268185	22.77%	2.973%
56	8.452	1205	1208	1211	rVB4	749	913	0.08%	0.010%
57	8.488	1212	1214	1216	rBV2	550	492	0.04%	0.005%
58	8.653	1234	1241	1256	rBV	602745	920882	78.20%	10.210%
59	8.952	1285	1290	1299	rBV	111768	170718	14.50%	1.893%
60	9.080	1308	1311	1313	rBV3	586	833	0.07%	0.009%
61	9.159	1321	1324	1325	rBV2	532	437	0.04%	0.005%
62	9.177	1325	1327	1329	rVB2	454	362	0.03%	0.004%
63	9.244	1336	1338	1340	rBV2	419	407	0.03%	0.005%
64	9.323	1348	1351	1353	rBV2	473	523	0.04%	0.006%
65	9.391	1356	1362	1379	rBV	468776	687400	58.37%	7.621%
66	9.860	1437	1439	1442	rBV2	423	387	0.03%	0.004%
67	10.006	1462	1463	1465	rBV	427	408	0.03%	0.005%
68	10.055	1466	1471	1484	rVV	524784	726405	61.69%	8.054%
69	10.354	1519	1520	1522	rBV2	410	390	0.03%	0.004%
70	10.640	1565	1567	1572	rVV2	410	535	0.05%	0.006%
71	10.799	1592	1593	1598	rBV2	506	719	0.06%	0.008%
72	10.835	1598	1599	1603	rVV2	376	438	0.04%	0.005%
73	10.963	1617	1620	1621	rBV2	399	339	0.03%	0.004%
74	11.091	1639	1641	1642	rVB2	591	357	0.03%	0.004%
75	11.116	1642	1645	1647	rBV2	354	502	0.04%	0.006%
76	11.195	1653	1658	1667	rVB	430464	537772	45.67%	5.962%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030432.D
 Acq On : 05 Aug 2022 16:09
 Operator : JC/MD
 Sample : N4003-19DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D89DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.469	1699	1703	1704	rBV2	362	496	0.04%	0.005%
78	11.482	1704	1705	1711	rVB2	485	466	0.04%	0.005%
79	11.610	1723	1726	1729	rVB3	435	482	0.04%	0.005%
80	11.823	1757	1761	1763	rBV	506	762	0.06%	0.008%
81	11.866	1767	1768	1771	rBV	477	447	0.04%	0.005%
82	11.927	1776	1778	1781	rBV	323	334	0.03%	0.004%
83	12.024	1789	1794	1804	rBV	541689	655748	55.69%	7.270%
84	12.219	1823	1826	1828	rBV2	739	826	0.07%	0.009%
85	12.323	1837	1843	1850	rBV	650236	797290	67.71%	8.840%
86	12.658	1894	1898	1900	rBV2	480	558	0.05%	0.006%
87	12.744	1910	1912	1917	rVV2	554	806	0.07%	0.009%
88	12.811	1920	1923	1924	rBV2	402	427	0.04%	0.005%
89	13.292	2001	2002	2004	rVB2	515	348	0.03%	0.004%
90	13.634	2056	2058	2060	rVB2	641	473	0.04%	0.005%
91	13.780	2080	2082	2085	rVB2	627	725	0.06%	0.008%
92	13.810	2085	2087	2089	rBV2	479	455	0.04%	0.005%
93	13.999	2115	2118	2119	rBV2	474	436	0.04%	0.005%
94	14.140	2138	2141	2143	rBV2	606	548	0.05%	0.006%
95	14.292	2164	2166	2167	rVB	680	339	0.03%	0.004%
96	14.603	2215	2217	2220	rVB3	727	575	0.05%	0.006%
97	14.780	2243	2246	2247	rBV2	628	557	0.05%	0.006%
98	14.999	2280	2282	2284	rBV3	607	564	0.05%	0.006%
99	15.133	2301	2304	2307	rBV2	758	840	0.07%	0.009%
100	16.493	2526	2527	2529	rBV2	870	566	0.05%	0.006%




Sum of corrected areas: 9019398

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030432.D
Acq On : 05 Aug 2022 16:09
Operator : JC/MD
Sample : N4003-19DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D89DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

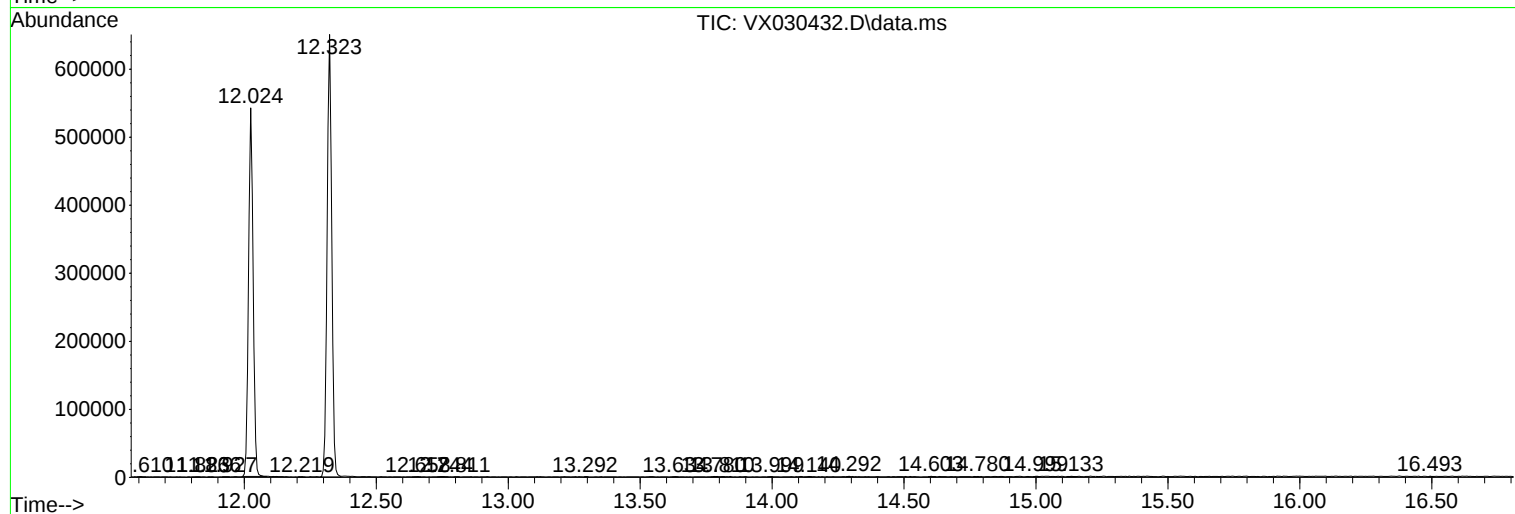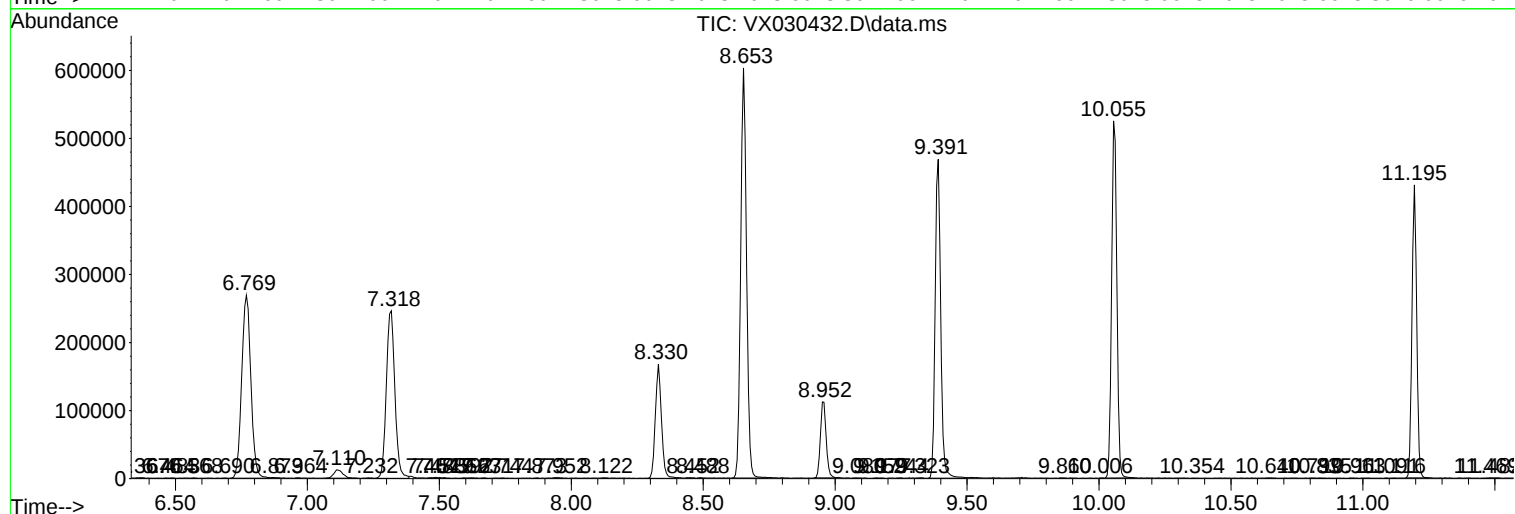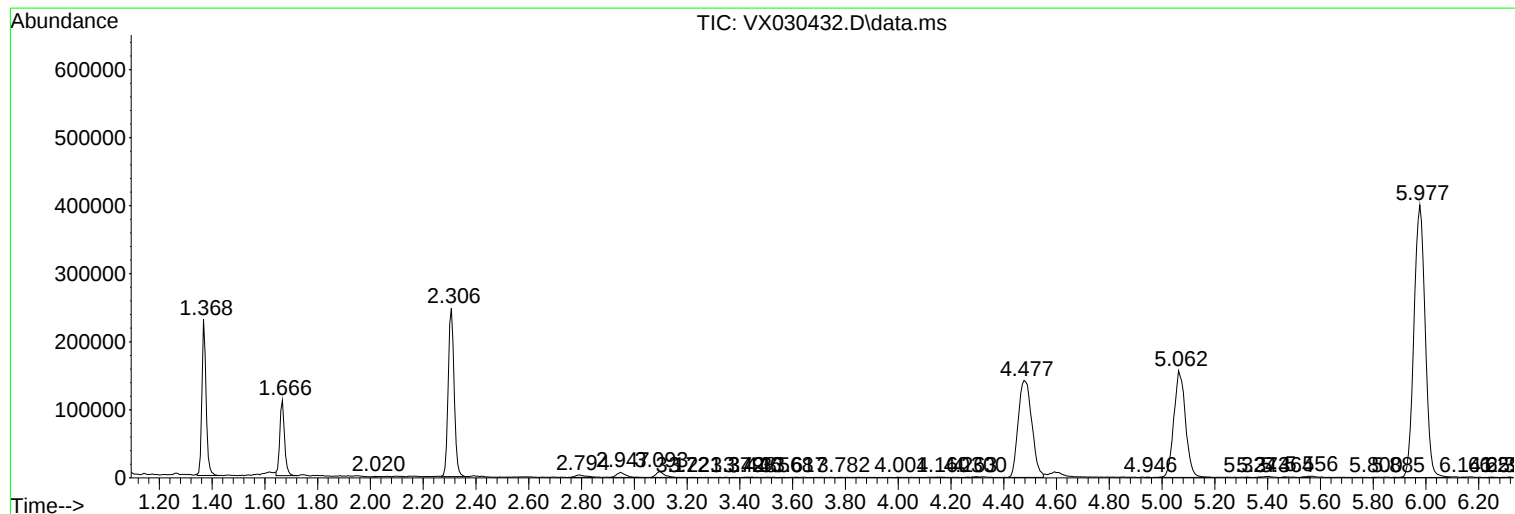

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030432.D
Acq On : 05 Aug 2022 16:09
Operator : JC/MD
Sample : N4003-19DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D89DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030432.D
Acq On : 05 Aug 2022 16:09
Operator : JC/MD
Sample : N4003-19DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D89DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc