

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030433.D
 Acq On : 05 Aug 2022 16:33
 Operator : JC/MD
 Sample : N4003-20DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D91DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030433.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	58	rVB2	372348	431698	25.68%	4.149%
2	1.666	91	95	102	rVB	103090	133906	7.96%	1.287%
3	2.307	194	200	211	rVB	256486	403170	23.98%	3.875%
4	2.794	274	280	286	rBV2	3433	6658	0.40%	0.064%
5	2.880	290	294	295	rBV2	365	415	0.02%	0.004%
6	2.953	300	306	317	rVV	7290	16199	0.96%	0.156%
7	3.093	323	329	340	rVV	32694	65540	3.90%	0.630%
8	3.215	348	349	351	rBV	382	299	0.02%	0.003%
9	3.239	351	353	354	rBV2	466	283	0.02%	0.003%
10	3.410	378	381	383	rBV2	442	532	0.03%	0.005%
11	3.434	383	385	388	rVV2	472	510	0.03%	0.005%
12	3.465	388	390	392	rVV	358	337	0.02%	0.003%
13	3.514	396	398	401	rBV	398	517	0.03%	0.005%
14	3.636	413	418	419	rVB2	456	395	0.02%	0.004%
15	3.721	430	432	434	rVV2	436	360	0.02%	0.003%
16	3.776	438	441	444	rVB	382	444	0.03%	0.004%
17	3.806	444	446	447	rVB	430	310	0.02%	0.003%
18	3.855	449	454	455	rBV2	621	535	0.03%	0.005%
19	3.873	455	457	460	rVV2	324	382	0.02%	0.004%
20	4.001	477	478	480	rBV	354	325	0.02%	0.003%
21	4.056	484	487	489	rBV2	344	390	0.02%	0.004%
22	4.111	495	496	499	rVB	558	278	0.02%	0.003%
23	4.343	533	534	536	rBV	402	349	0.02%	0.003%
24	4.495	545	559	571	rBV2	564952	1681273	100.00%	16.160%
25	5.068	637	653	670	rBV	157965	477299	28.39%	4.588%
26	5.221	676	678	680	rBV3	473	332	0.02%	0.003%
27	5.318	691	694	696	rBV2	422	497	0.03%	0.005%
28	5.391	700	706	708	rBV4	1020	1727	0.10%	0.017%
29	5.489	720	722	724	rBV2	286	312	0.02%	0.003%
30	5.666	749	751	753	rVV3	410	298	0.02%	0.003%
31	5.721	758	760	762	rBV2	589	537	0.03%	0.005%
32	5.977	789	802	815	rBV2	407325	1177544	70.04%	11.318%
33	6.202	836	839	842	rVB2	513	679	0.04%	0.007%
34	6.257	845	848	849	rVB2	357	371	0.02%	0.004%
35	6.379	866	868	871	rBV	577	385	0.02%	0.004%
36	6.416	873	874	876	rBV2	454	349	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030433.D
 Acq On : 05 Aug 2022 16:33
 Operator : JC/MD
 Sample : N4003-20DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D91DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.440	876	878	881	rVB2	560	633	0.04%	0.006%
38	6.470	881	883	886	rBV	802	938	0.06%	0.009%
39	6.507	886	889	891	rBV2	482	724	0.04%	0.007%
40	6.769	922	932	946	rBV	283266	670707	39.89%	6.447%
41	6.934	957	959	963	rVB3	695	821	0.05%	0.008%
42	7.044	975	977	978	rVV2	533	461	0.03%	0.004%
43	7.117	981	989	999	rVV4	12098	29274	1.74%	0.281%
44	7.190	999	1001	1004	rVB	535	596	0.04%	0.006%
45	7.312	1010	1021	1036	rBV	245875	542388	32.26%	5.213%
46	7.489	1046	1050	1054	rBV4	1138	1498	0.09%	0.014%
47	7.586	1064	1066	1069	rVB	713	432	0.03%	0.004%
48	7.684	1079	1082	1084	rBV2	366	346	0.02%	0.003%
49	7.818	1100	1104	1105	rBV2	437	594	0.04%	0.006%
50	7.885	1112	1115	1118	rBV2	754	1126	0.07%	0.011%
51	8.330	1181	1188	1200	rBV	164971	268462	15.97%	2.580%
52	8.476	1210	1212	1213	rBV	581	377	0.02%	0.004%
53	8.580	1227	1229	1231	rBV2	349	390	0.02%	0.004%
54	8.653	1235	1241	1250	rVV	601692	918406	54.63%	8.828%
55	8.885	1277	1279	1283	rVB2	486	460	0.03%	0.004%
56	8.952	1285	1290	1302	rVV	115001	175910	10.46%	1.691%
57	9.098	1311	1314	1315	rBV2	369	359	0.02%	0.003%
58	9.116	1315	1317	1320	rVB2	914	935	0.06%	0.009%
59	9.391	1356	1362	1376	rBV	486955	682580	40.60%	6.561%
60	9.708	1411	1414	1417	rBV4	1119	1161	0.07%	0.011%
61	9.836	1434	1435	1438	rVB	536	332	0.02%	0.003%
62	9.891	1438	1444	1446	rBV2	315	535	0.03%	0.005%
63	10.055	1466	1471	1480	rBV	532484	719372	42.79%	6.914%
64	10.171	1488	1490	1492	rBV2	967	687	0.04%	0.007%
65	10.250	1501	1503	1507	rVB3	553	688	0.04%	0.007%
66	10.494	1541	1543	1546	rBV2	551	524	0.03%	0.005%
67	10.677	1571	1573	1574	rVB	565	286	0.02%	0.003%
68	10.695	1574	1576	1579	rBV3	490	640	0.04%	0.006%
69	10.762	1585	1587	1589	rVB2	711	633	0.04%	0.006%
70	10.793	1589	1592	1593	rBV2	497	542	0.03%	0.005%
71	10.866	1601	1604	1606	rVB2	362	406	0.02%	0.004%
72	10.964	1618	1620	1622	rBV2	612	553	0.03%	0.005%
73	11.043	1631	1633	1636	rBV2	247	364	0.02%	0.003%
74	11.195	1652	1658	1667	rBV	426510	540924	32.17%	5.199%
75	11.433	1694	1697	1698	rBV2	324	322	0.02%	0.003%
76	11.488	1703	1706	1707	rBV	321	329	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030433.D
 Acq On : 05 Aug 2022 16:33
 Operator : JC/MD
 Sample : N4003-20DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D91DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.579	1720	1721	1722	rBV	542	287	0.02%	0.003%
78	11.659	1732	1734	1736	rBV2	308	317	0.02%	0.003%
79	11.793	1755	1756	1757	rBV	703	319	0.02%	0.003%
80	11.866	1765	1768	1769	rVB2	583	378	0.02%	0.004%
81	11.969	1784	1785	1786	rBV	524	275	0.02%	0.003%
82	12.024	1789	1794	1805	rVV	538472	651696	38.76%	6.264%
83	12.323	1837	1843	1853	rBV	613202	770820	45.85%	7.409%
84	12.512	1871	1874	1876	rBV2	445	560	0.03%	0.005%
85	12.762	1913	1915	1917	rVB	472	277	0.02%	0.003%
86	12.847	1928	1929	1930	rBV	613	321	0.02%	0.003%
87	13.433	2022	2025	2027	rBV	435	452	0.03%	0.004%
88	13.561	2043	2046	2047	rBV2	531	435	0.03%	0.004%
89	13.780	2079	2082	2084	rBV2	440	560	0.03%	0.005%
90	13.902	2099	2102	2105	rVB2	355	468	0.03%	0.004%
91	13.987	2114	2116	2119	rBV2	279	356	0.02%	0.003%
92	14.030	2121	2123	2126	rVB	670	676	0.04%	0.006%
93	14.061	2126	2128	2129	rBV	609	463	0.03%	0.004%
94	14.085	2130	2132	2134	rVB2	570	411	0.02%	0.004%
95	14.225	2153	2155	2157	rBV	566	499	0.03%	0.005%
96	14.250	2157	2159	2162	rVB3	601	551	0.03%	0.005%
97	14.384	2178	2181	2182	rBV	394	398	0.02%	0.004%
98	15.036	2286	2288	2291	rVB2	725	481	0.03%	0.005%
99	15.207	2314	2316	2318	rBV2	515	299	0.02%	0.003%
100	15.566	2373	2375	2377	rBV3	559	423	0.03%	0.004%

Sum of corrected areas: 10403872



Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030433.D
Acq On : 05 Aug 2022 16:33
Operator : JC/MD
Sample : N4003-20DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D91DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

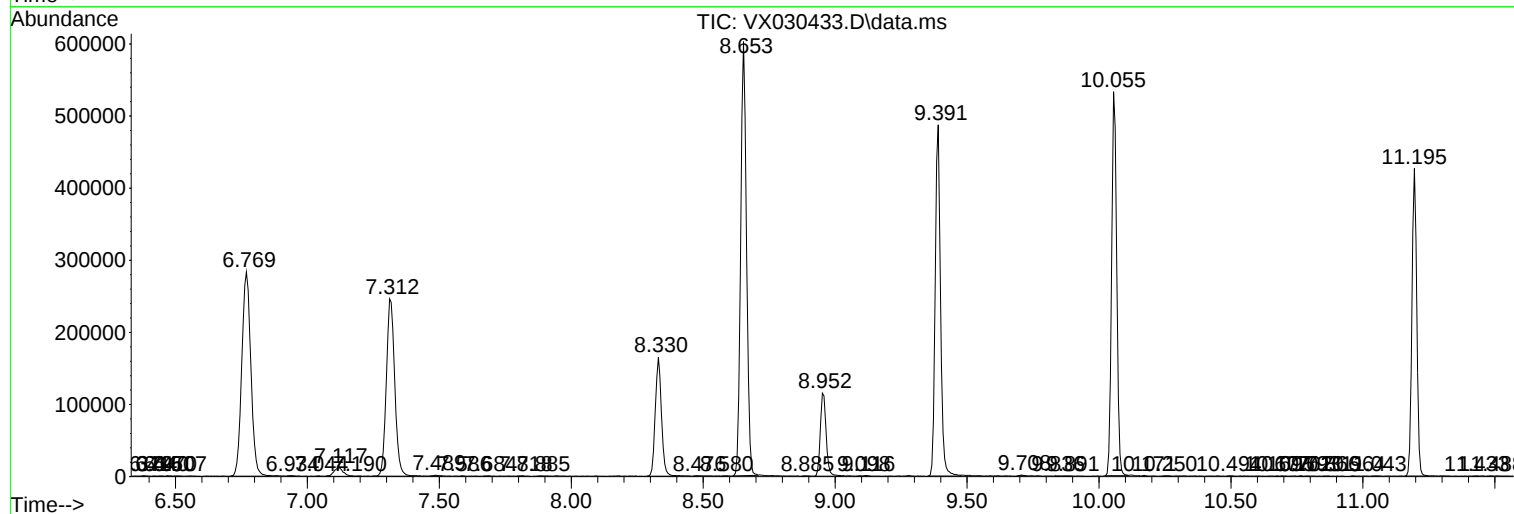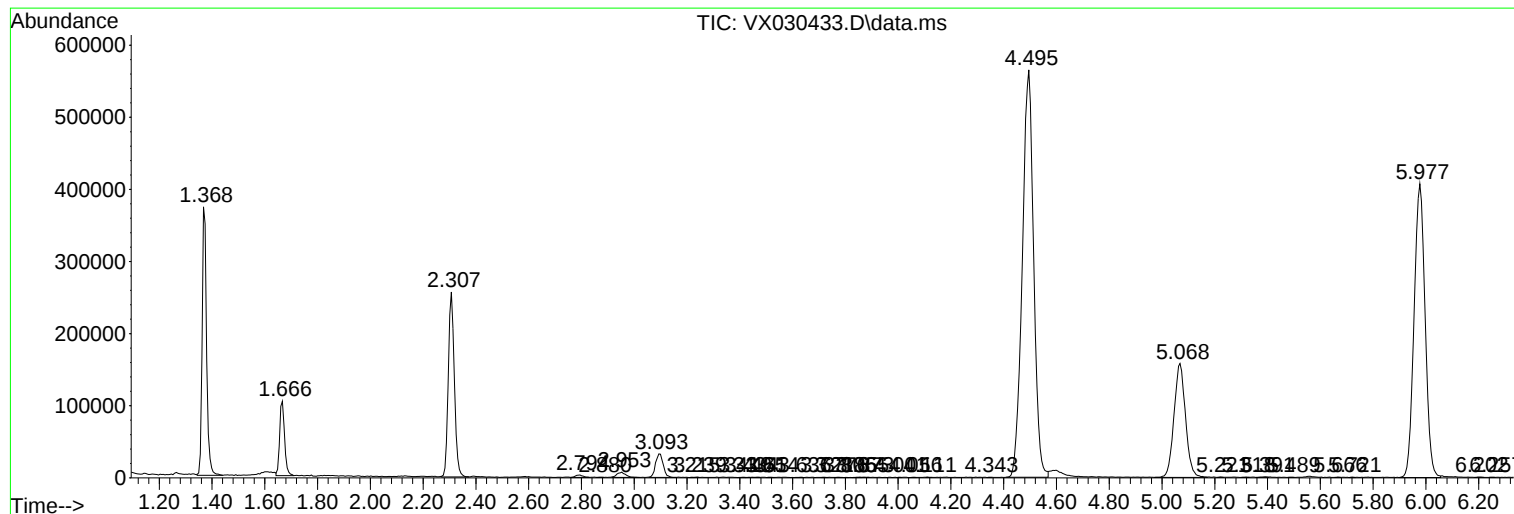

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030433.D
Acq On : 05 Aug 2022 16:33
Operator : JC/MD
Sample : N4003-20DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D91DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030433.D
Acq On : 05 Aug 2022 16:33
Operator : JC/MD
Sample : N4003-20DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D91DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc