

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030434.D
 Acq On : 05 Aug 2022 16:56
 Operator : JC/MD
 Sample : N4003-21DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D92DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030434.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	58	rVB2	233610	266561	22.87%	2.736%
2	1.666	91	95	104	rVB	110979	134781	11.56%	1.383%
3	2.306	194	200	210	rVB	252382	369856	31.73%	3.796%
4	2.386	211	213	216	rBV2	1476	1291	0.11%	0.013%
5	2.477	225	228	229	rBV2	417	436	0.04%	0.004%
6	2.532	235	237	239	rBV2	804	639	0.05%	0.007%
7	2.562	239	242	243	rBV2	673	741	0.06%	0.008%
8	2.721	266	268	271	rVB2	534	469	0.04%	0.005%
9	2.788	271	279	283	rBV6	4498	9974	0.86%	0.102%
10	2.947	296	305	312	rBV	11343	25759	2.21%	0.264%
11	3.050	318	322	323	rVB2	406	391	0.03%	0.004%
12	3.093	323	329	341	rBV2	15224	30885	2.65%	0.317%
13	3.215	347	349	353	rVB3	463	403	0.03%	0.004%
14	3.257	353	356	359	rVB2	588	634	0.05%	0.007%
15	3.306	362	364	368	rBV2	340	376	0.03%	0.004%
16	3.410	379	381	383	rBV2	419	353	0.03%	0.004%
17	3.538	400	402	404	rVB	644	386	0.03%	0.004%
18	3.611	404	414	420	rBV	678	1578	0.14%	0.016%
19	4.056	486	487	490	rBV2	572	575	0.05%	0.006%
20	4.221	512	514	516	rVB	478	378	0.03%	0.004%
21	4.239	516	517	520	rVB	377	344	0.03%	0.004%
22	4.306	520	528	535	rBV6	2100	5738	0.49%	0.059%
23	4.361	535	537	540	rVB2	578	567	0.05%	0.006%
24	4.404	540	544	545	rBV2	365	481	0.04%	0.005%
25	4.495	545	559	570	rBV2	334702	1090853	93.57%	11.197%
26	4.812	607	611	612	rVB2	787	943	0.08%	0.010%
27	4.836	612	615	616	rBV2	598	462	0.04%	0.005%
28	5.062	639	652	667	rBV	151863	468999	40.23%	4.814%
29	5.361	699	701	702	rBV2	631	513	0.04%	0.005%
30	5.385	702	705	706	rVV2	1247	1454	0.12%	0.015%
31	5.416	709	710	714	rVV	1202	770	0.07%	0.008%
32	5.470	714	719	726	rVV4	1689	3721	0.32%	0.038%
33	5.550	729	732	740	rVV5	2048	4622	0.40%	0.047%
34	5.635	744	746	747	rVV	670	392	0.03%	0.004%
35	5.678	750	753	756	rBV2	488	647	0.06%	0.007%
36	5.714	756	759	761	rBV	387	365	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030434.D
 Acq On : 05 Aug 2022 16:56
 Operator : JC/MD
 Sample : N4003-21DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D92DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	5.806	769	774	777	rBV2	473	944	0.08%	0.010%
38	5.976	790	802	821	rBV2	401246	1165782	100.00%	11.966%
39	6.135	826	828	830	rBV3	480	555	0.05%	0.006%
40	6.251	845	847	848	rBV	599	550	0.05%	0.006%
41	6.361	861	865	871	rBV4	647	1439	0.12%	0.015%
42	6.562	895	898	899	rBV2	420	388	0.03%	0.004%
43	6.769	922	932	946	rBV	269680	641481	55.03%	6.584%
44	6.988	966	968	969	rBV2	539	372	0.03%	0.004%
45	7.129	982	991	1005	rBV4	66475	158815	13.62%	1.630%
46	7.318	1013	1022	1044	rVB	238577	543032	46.58%	5.574%
47	7.482	1044	1049	1050	rBV2	789	1074	0.09%	0.011%
48	7.568	1060	1063	1065	rVB2	646	672	0.06%	0.007%
49	7.592	1065	1067	1070	rBV3	714	775	0.07%	0.008%
50	7.940	1122	1124	1125	rBV2	710	582	0.05%	0.006%
51	8.330	1182	1188	1198	rBV	165877	264066	22.65%	2.710%
52	8.543	1221	1223	1226	rVB3	406	391	0.03%	0.004%
53	8.586	1228	1230	1234	rVB2	751	764	0.07%	0.008%
54	8.653	1234	1241	1252	rBV	582748	907342	77.83%	9.313%
55	8.769	1259	1260	1265	rVB3	848	926	0.08%	0.010%
56	8.958	1284	1291	1301	rBV	112365	174042	14.93%	1.786%
57	9.226	1333	1335	1338	rBV2	347	398	0.03%	0.004%
58	9.275	1338	1343	1349	rVV2	25821	39641	3.40%	0.407%
59	9.390	1356	1362	1381	rBV	483477	695604	59.67%	7.140%
60	9.708	1408	1414	1419	rVB6	2406	4395	0.38%	0.045%
61	9.817	1429	1432	1433	rBV2	552	469	0.04%	0.005%
62	9.921	1446	1449	1451	rBV2	382	456	0.04%	0.005%
63	10.055	1465	1471	1481	rBV	540156	737080	63.23%	7.566%
64	10.317	1510	1514	1515	rVB3	607	725	0.06%	0.007%
65	10.396	1525	1527	1530	rVV2	498	593	0.05%	0.006%
66	10.457	1536	1537	1541	rVV2	397	396	0.03%	0.004%
67	10.634	1563	1566	1567	rBV	479	358	0.03%	0.004%
68	10.701	1576	1577	1581	rBV2	394	341	0.03%	0.004%
69	10.884	1605	1607	1609	rBV2	350	375	0.03%	0.004%
70	10.988	1622	1624	1626	rBV2	341	366	0.03%	0.004%
71	11.195	1652	1658	1668	rVB	438392	539824	46.31%	5.541%
72	11.341	1679	1682	1686	rVB2	589	846	0.07%	0.009%
73	11.372	1686	1687	1689	rBV2	479	410	0.04%	0.004%
74	11.482	1702	1705	1707	rBV3	308	388	0.03%	0.004%
75	11.524	1711	1712	1714	rBV2	324	339	0.03%	0.003%
76	11.799	1751	1757	1758	rVB3	433	561	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030434.D
 Acq On : 05 Aug 2022 16:56
 Operator : JC/MD
 Sample : N4003-21DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D92DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.024	1788	1794	1801	rBV	545659	667696	57.27%	6.853%
78	12.323	1837	1843	1852	rBV	597397	747542	64.12%	7.673%
79	12.524	1874	1876	1880	rVB3	615	625	0.05%	0.006%
80	12.811	1921	1923	1925	rBV	445	384	0.03%	0.004%
81	13.012	1954	1956	1959	rVV2	443	492	0.04%	0.005%
82	13.042	1959	1961	1962	rVV2	425	372	0.03%	0.004%
83	13.237	1992	1993	1997	rVB2	562	570	0.05%	0.006%
84	13.414	2020	2022	2024	rVB2	421	374	0.03%	0.004%
85	13.439	2024	2026	2030	rVB2	442	512	0.04%	0.005%
86	13.603	2050	2053	2055	rBV2	411	475	0.04%	0.005%
87	13.731	2072	2074	2077	rBV	311	408	0.03%	0.004%
88	13.926	2103	2106	2107	rBV2	519	573	0.05%	0.006%
89	13.981	2113	2115	2118	rBV2	488	397	0.03%	0.004%
90	14.054	2125	2127	2129	rBV	550	529	0.05%	0.005%
91	14.353	2175	2176	2179	rBV2	504	575	0.05%	0.006%
92	14.554	2205	2209	2212	rBV2	367	592	0.05%	0.006%
93	14.737	2237	2239	2242	rBV3	514	517	0.04%	0.005%
94	14.969	2275	2277	2281	rBV3	766	789	0.07%	0.008%
95	15.005	2281	2283	2288	rBV2	677	1034	0.09%	0.011%
96	15.139	2304	2305	2308	rVB3	430	367	0.03%	0.004%
97	15.877	2425	2426	2428	rBV	682	419	0.04%	0.004%
98	16.255	2485	2488	2489	rBV2	670	734	0.06%	0.008%
99	16.511	2529	2530	2533	rBV3	756	786	0.07%	0.008%
100	16.627	2546	2549	2551	rBV2	801	928	0.08%	0.010%




Sum of corrected areas: 9742584

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030434.D
Acq On : 05 Aug 2022 16:56
Operator : JC/MD
Sample : N4003-21DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D92DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

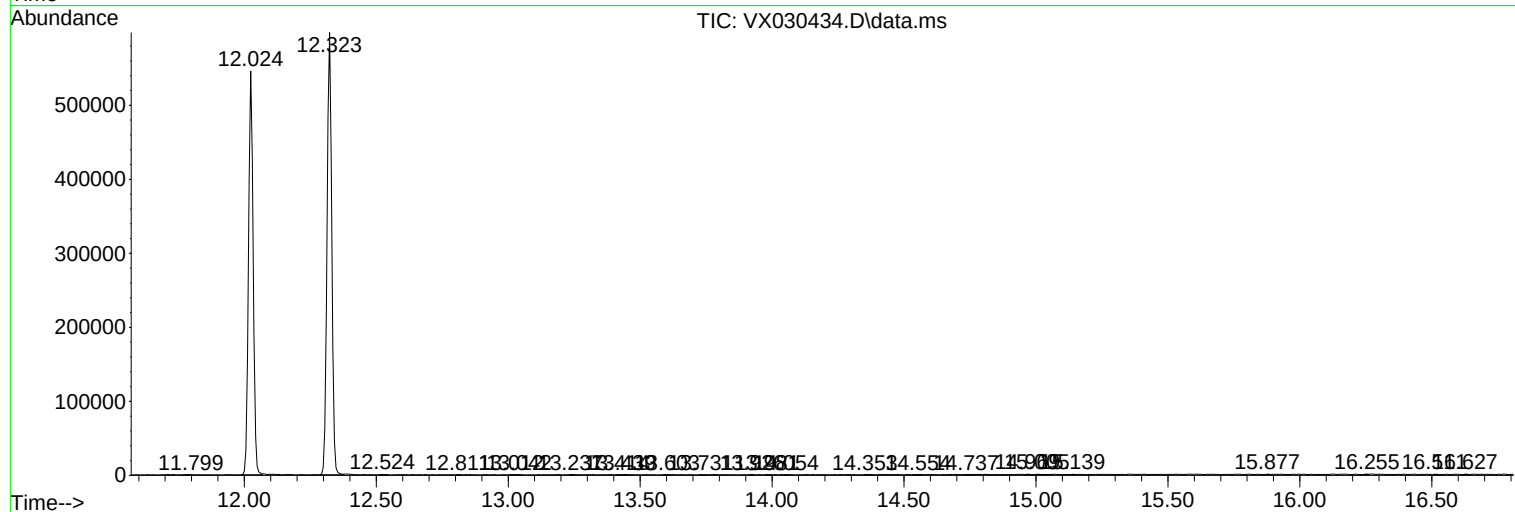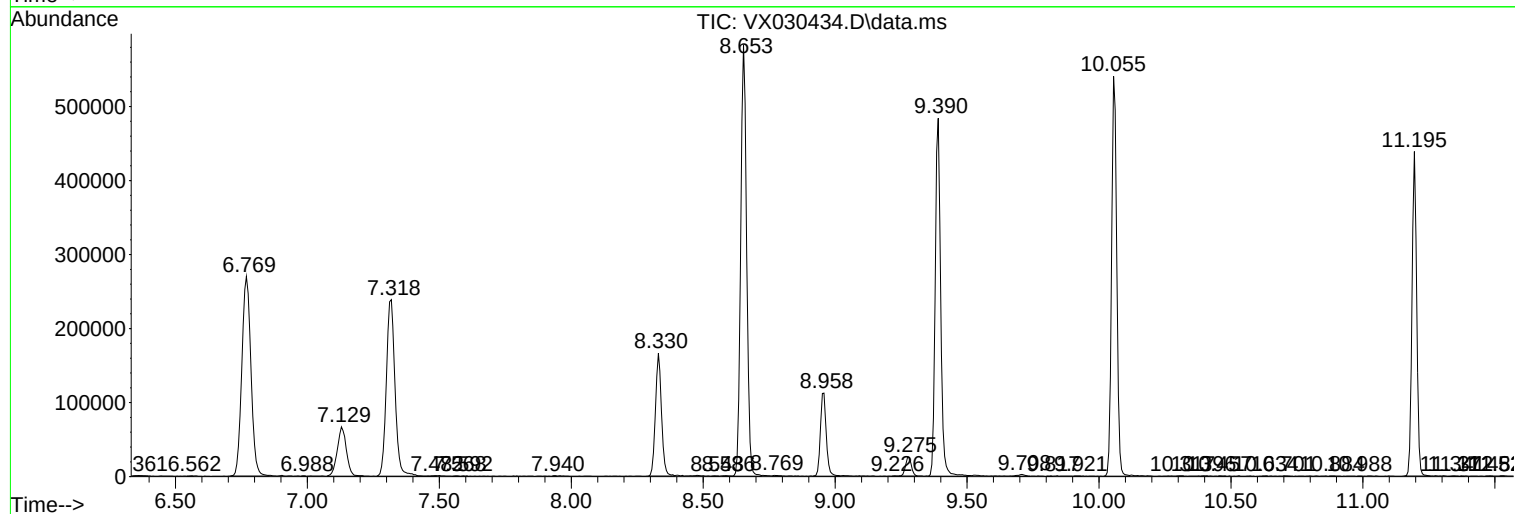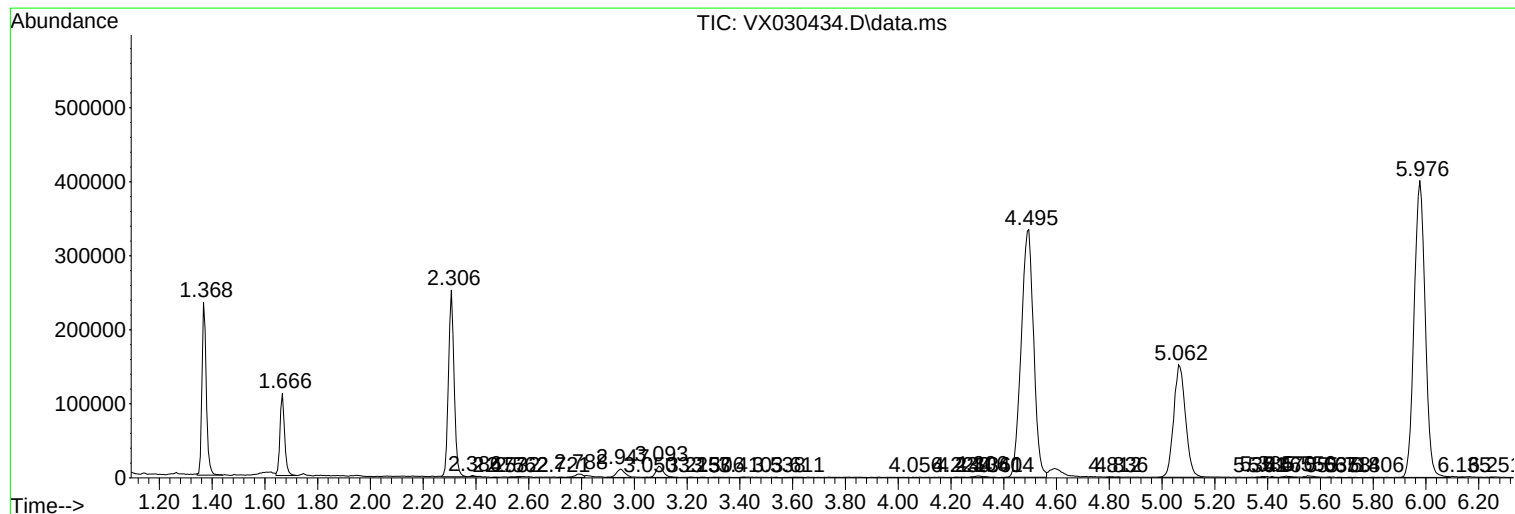

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030434.D
Acq On : 05 Aug 2022 16:56
Operator : JC/MD
Sample : N4003-21DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D92DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030434.D
Acq On : 05 Aug 2022 16:56
Operator : JC/MD
Sample : N4003-21DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D92DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc