

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030435.D
 Acq On : 05 Aug 2022 17:20
 Operator : JC/MD
 Sample : N4003-10DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D36DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030435.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	58	rVB2	215432	237876	17.43%	2.424%
2	1.666	91	95	105	rVB	109277	133204	9.76%	1.358%
3	2.306	194	200	212	rVB	248006	389370	28.53%	3.968%
4	2.501	230	232	234	rVB2	582	429	0.03%	0.004%
5	2.568	239	243	245	rBV4	1167	1692	0.12%	0.017%
6	2.684	260	262	263	rVB	590	361	0.03%	0.004%
7	2.751	270	273	274	rVB2	432	420	0.03%	0.004%
8	2.794	274	280	288	rBV5	3456	6948	0.51%	0.071%
9	2.946	298	305	318	rVB2	5998	14544	1.07%	0.148%
10	3.038	318	320	323	rVB2	570	741	0.05%	0.008%
11	3.093	323	329	336	rBV3	6391	13520	0.99%	0.138%
12	3.154	336	339	344	rVB2	436	702	0.05%	0.007%
13	3.452	383	388	390	rBV3	604	752	0.06%	0.008%
14	3.654	420	421	424	rVB	497	355	0.03%	0.004%
15	3.684	424	426	427	rBV2	574	418	0.03%	0.004%
16	3.751	435	437	440	rBV2	430	532	0.04%	0.005%
17	3.830	448	450	452	rVV	460	373	0.03%	0.004%
18	3.928	463	466	467	rBV2	422	359	0.03%	0.004%
19	4.154	501	503	505	rBV2	486	458	0.03%	0.005%
20	4.410	542	545	546	rBV	409	413	0.03%	0.004%
21	4.489	546	558	572	rBV2	430304	1364559	100.00%	13.908%
22	4.934	629	631	633	rVB	451	395	0.03%	0.004%
23	5.062	641	652	671	rBV	153139	484486	35.50%	4.938%
24	5.312	692	693	696	rVB2	644	463	0.03%	0.005%
25	5.403	701	708	711	rBV4	1555	3216	0.24%	0.033%
26	5.544	727	731	732	rBV3	1182	1610	0.12%	0.016%
27	5.562	732	734	742	rVB5	2765	4265	0.31%	0.043%
28	5.879	785	786	789	rBV	321	372	0.03%	0.004%
29	5.976	790	802	817	rVV2	408838	1176153	86.19%	11.987%
30	6.263	847	849	856	rVB2	387	549	0.04%	0.006%
31	6.342	859	862	864	rBV2	446	506	0.04%	0.005%
32	6.434	875	877	880	rBV	384	534	0.04%	0.005%
33	6.568	897	899	902	rVB3	559	557	0.04%	0.006%
34	6.769	921	932	948	rBV	273065	637413	46.71%	6.496%
35	6.976	963	966	970	rVB2	637	891	0.07%	0.009%
36	7.019	970	973	977	rBV3	361	600	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030435.D
 Acq On : 05 Aug 2022 17:20
 Operator : JC/MD
 Sample : N4003-10DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D36DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.123	981	990	1001	rVB5	18470	47129	3.45%	0.480%
38	7.318	1012	1022	1036	rBV	243525	535578	39.25%	5.459%
39	7.488	1046	1050	1052	rBV2	829	1088	0.08%	0.011%
40	7.586	1064	1066	1069	rVB2	535	512	0.04%	0.005%
41	7.629	1069	1073	1074	rBV2	406	554	0.04%	0.006%
42	7.915	1116	1120	1122	rBV3	549	603	0.04%	0.006%
43	8.330	1180	1188	1197	rBV	165502	264063	19.35%	2.691%
44	8.482	1211	1213	1215	rVB2	600	389	0.03%	0.004%
45	8.653	1234	1241	1252	rBV	582577	915341	67.08%	9.329%
46	8.823	1268	1269	1272	rVB3	590	511	0.04%	0.005%
47	8.860	1272	1275	1277	rVB	664	662	0.05%	0.007%
48	8.951	1285	1290	1304	rVB	116558	172061	12.61%	1.754%
49	9.159	1323	1324	1327	rBV	570	392	0.03%	0.004%
50	9.281	1340	1344	1347	rBV4	2076	2839	0.21%	0.029%
51	9.390	1356	1362	1378	rBV	475636	696444	51.04%	7.098%
52	9.628	1399	1401	1403	rBV2	418	535	0.04%	0.005%
53	9.701	1411	1413	1417	rVB2	936	1183	0.09%	0.012%
54	9.817	1430	1432	1434	rBV2	410	368	0.03%	0.004%
55	9.970	1453	1457	1459	rBV3	388	616	0.05%	0.006%
56	10.055	1466	1471	1479	rBV	518186	712680	52.23%	7.264%
57	10.207	1495	1496	1499	rBV2	456	389	0.03%	0.004%
58	10.244	1500	1502	1503	rVV	674	370	0.03%	0.004%
59	10.280	1506	1508	1510	rVB	576	347	0.03%	0.004%
60	10.372	1521	1523	1525	rBV	737	444	0.03%	0.005%
61	10.537	1548	1550	1553	rBV2	319	424	0.03%	0.004%
62	10.805	1591	1594	1597	rBV2	492	649	0.05%	0.007%
63	10.963	1618	1620	1624	rVB2	434	453	0.03%	0.005%
64	11.049	1632	1634	1637	rVB	519	462	0.03%	0.005%
65	11.195	1653	1658	1668	rVV	415027	535264	39.23%	5.455%
66	11.372	1686	1687	1690	rBV	477	453	0.03%	0.005%
67	11.427	1694	1696	1698	rVB2	617	422	0.03%	0.004%
68	11.469	1699	1703	1704	rVV2	331	386	0.03%	0.004%
69	11.482	1704	1705	1708	rVB2	557	435	0.03%	0.004%
70	11.652	1731	1733	1734	rBV2	682	511	0.04%	0.005%
71	11.817	1756	1760	1761	rBV	436	493	0.04%	0.005%
72	11.890	1770	1772	1777	rBV3	505	609	0.04%	0.006%
73	11.963	1779	1784	1785	rBV2	364	474	0.03%	0.005%
74	12.024	1789	1794	1804	rVB	530552	636199	46.62%	6.484%
75	12.225	1824	1827	1828	rBV2	541	508	0.04%	0.005%
76	12.323	1837	1843	1849	rBV	642384	785078	57.53%	8.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030435.D
 Acq On : 05 Aug 2022 17:20
 Operator : JC/MD
 Sample : N4003-10DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D36DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.573	1882	1884	1885	rBV2	493	465	0.03%	0.005%
78	12.628	1891	1893	1897	rBV2	469	668	0.05%	0.007%
79	12.780	1915	1918	1921	rBV	527	639	0.05%	0.007%
80	12.884	1933	1935	1937	rVV2	416	349	0.03%	0.004%
81	12.920	1939	1941	1943	rBV2	381	435	0.03%	0.004%
82	13.054	1961	1963	1967	rBV2	419	535	0.04%	0.005%
83	13.463	2029	2030	2032	rVB	508	358	0.03%	0.004%
84	13.506	2034	2037	2039	rBV2	417	475	0.03%	0.005%
85	13.573	2045	2048	2049	rVB	452	406	0.03%	0.004%
86	13.597	2049	2052	2055	rBV2	342	479	0.04%	0.005%
87	13.725	2071	2073	2079	rBV2	472	712	0.05%	0.007%
88	13.786	2079	2083	2085	rBV2	515	778	0.06%	0.008%
89	13.999	2115	2118	2119	rBV	626	625	0.05%	0.006%
90	14.079	2129	2131	2134	rBV2	426	415	0.03%	0.004%
91	14.121	2136	2138	2141	rVV2	520	521	0.04%	0.005%
92	14.152	2141	2143	2146	rVB2	643	459	0.03%	0.005%
93	14.213	2151	2153	2155	rVV2	528	569	0.04%	0.006%
94	14.231	2155	2156	2159	rVB2	783	711	0.05%	0.007%
95	14.609	2216	2218	2221	rVB2	598	603	0.04%	0.006%
96	14.859	2257	2259	2260	rBV2	498	359	0.03%	0.004%
97	15.304	2328	2332	2333	rBV2	782	1107	0.08%	0.011%
98	15.432	2350	2353	2354	rBV	440	471	0.03%	0.005%
99	16.426	2515	2516	2519	rBV2	727	568	0.04%	0.006%
100	16.731	2564	2566	2570	rBV3	799	989	0.07%	0.010%




Sum of corrected areas: 9811650

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030435.D
Acq On : 05 Aug 2022 17:20
Operator : JC/MD
Sample : N4003-10DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D36DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

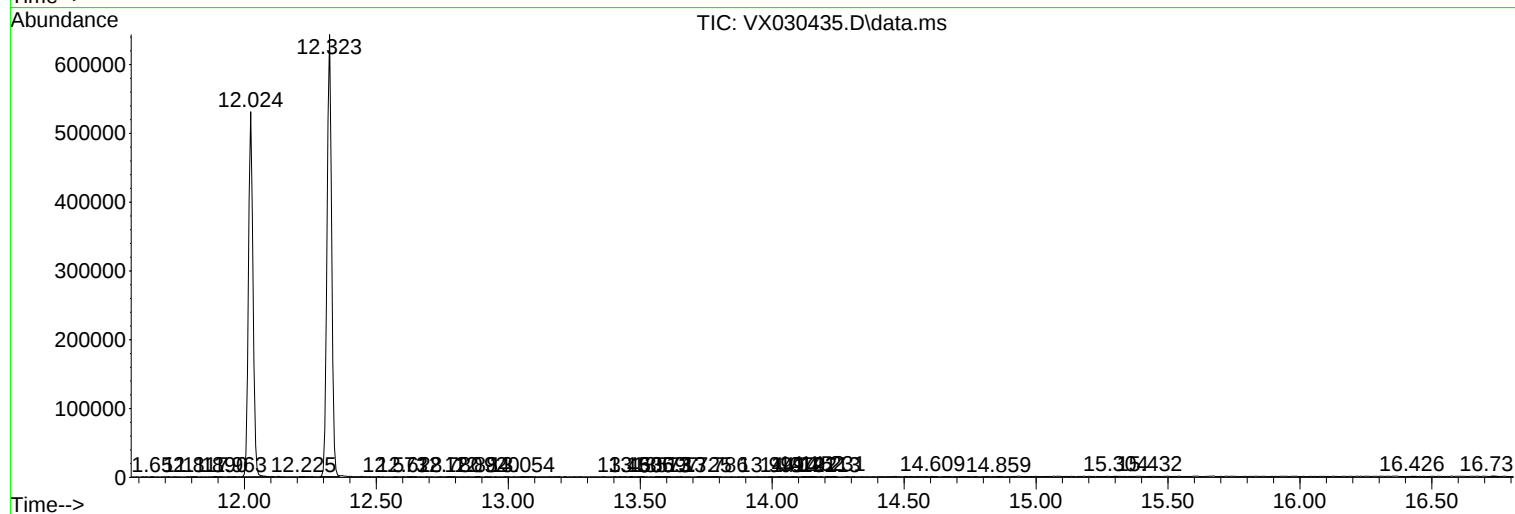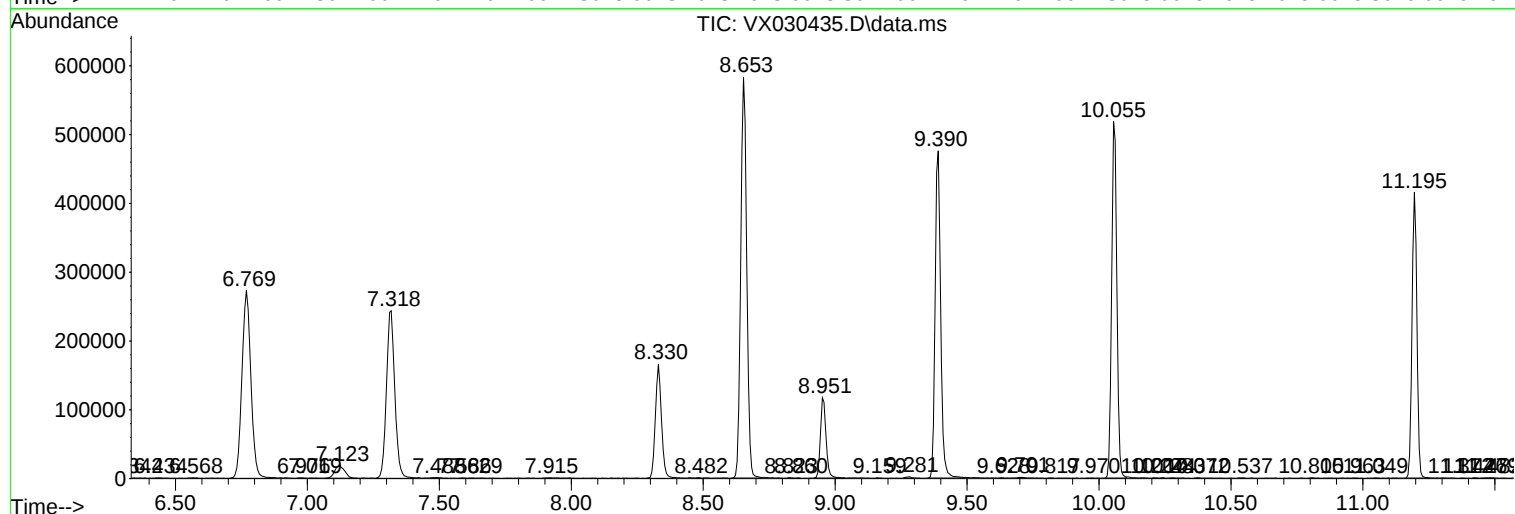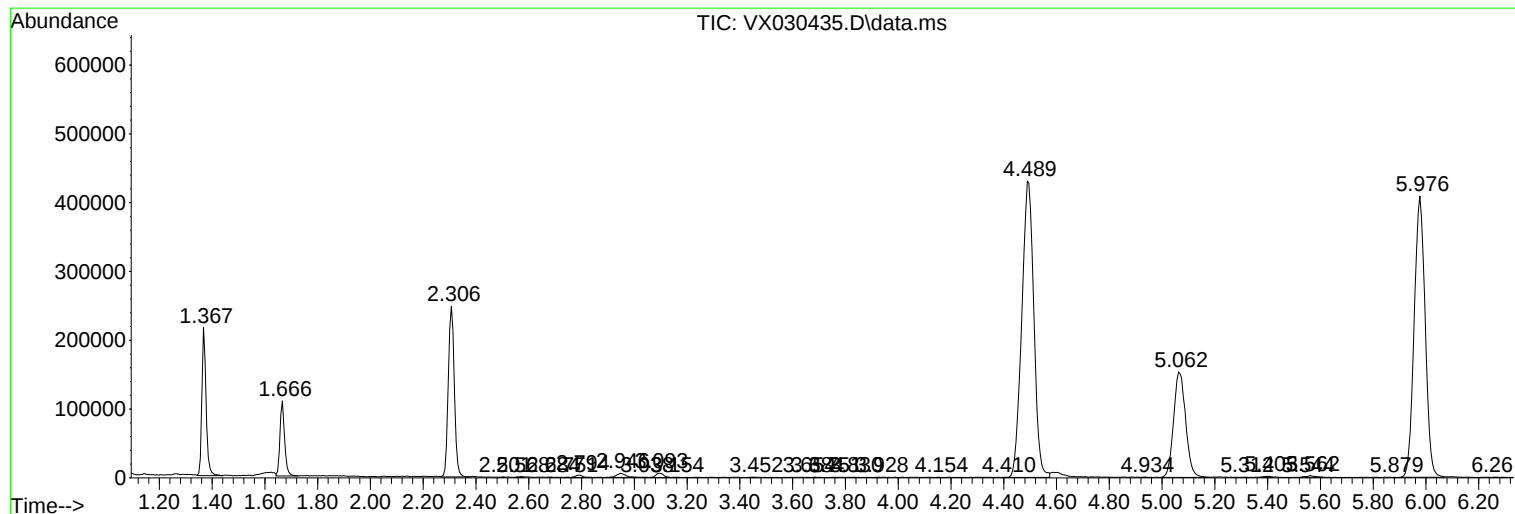

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030435.D
Acq On : 05 Aug 2022 17:20
Operator : JC/MD
Sample : N4003-10DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D36DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030435.D
Acq On : 05 Aug 2022 17:20
Operator : JC/MD
Sample : N4003-10DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D36DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc