

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030436.D
 Acq On : 05 Aug 2022 17:43
 Operator : JC/MD
 Sample : N4003-09DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D34DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB2	157834	168227	14.32%	1.741%
2	1.666	91	95	103	rVB	105470	136120	11.59%	1.409%
3	2.105	165	167	169	rBV2	1124	735	0.06%	0.008%
4	2.307	194	200	210	rVB	227760	359082	30.57%	3.716%
5	2.489	228	230	231	rBV2	578	448	0.04%	0.005%
6	2.794	273	280	288	rVB4	4017	7576	0.64%	0.078%
7	2.947	297	305	317	rVB	9407	23575	2.01%	0.244%
8	3.093	323	329	338	rBV2	10235	20141	1.71%	0.208%
9	3.441	384	386	388	rVV2	470	355	0.03%	0.004%
10	3.501	394	396	399	rVB2	543	449	0.04%	0.005%
11	3.550	399	404	405	rBV	304	342	0.03%	0.004%
12	3.569	405	407	410	rVB	375	343	0.03%	0.004%
13	3.593	410	411	413	rBV2	465	387	0.03%	0.004%
14	3.648	418	420	421	rVB2	613	395	0.03%	0.004%
15	3.684	421	426	428	rBV	606	820	0.07%	0.008%
16	3.721	428	432	435	rVV2	328	371	0.03%	0.004%
17	3.806	441	446	447	rBV2	414	651	0.06%	0.007%
18	3.922	461	465	467	rBV2	288	385	0.03%	0.004%
19	3.965	470	472	474	rBV2	385	391	0.03%	0.004%
20	4.032	481	483	485	rBV	522	450	0.04%	0.005%
21	4.136	497	500	504	rVB2	443	560	0.05%	0.006%
22	4.257	518	520	523	rBV3	434	500	0.04%	0.005%
23	4.495	546	559	570	rBV3	322971	1042916	88.77%	10.794%
24	4.879	620	622	625	rVB2	594	601	0.05%	0.006%
25	4.934	628	631	634	rBV2	456	464	0.04%	0.005%
26	5.068	639	653	676	rBV	156481	485968	41.37%	5.030%
27	5.367	700	702	704	rBV2	491	602	0.05%	0.006%
28	5.397	704	707	711	rVV3	1128	1888	0.16%	0.020%
29	5.452	715	716	721	rVB2	559	648	0.06%	0.007%
30	5.495	721	723	726	rVB2	460	544	0.05%	0.006%
31	5.562	729	734	738	rBV4	1576	3593	0.31%	0.037%
32	5.812	772	775	777	rBV2	395	414	0.04%	0.004%
33	5.977	790	802	818	rBV2	404274	1174793	100.00%	12.159%
34	6.361	862	865	867	rVB3	346	390	0.03%	0.004%
35	6.434	875	877	880	rBV	358	347	0.03%	0.004%
36	6.562	895	898	899	rBV	532	369	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030436.D
 Acq On : 05 Aug 2022 17:43
 Operator : JC/MD
 Sample : N4003-09DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D34DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.769	920	932	945	rBV	251880	603927	51.41%	6.250%
38	6.958	962	963	965	rBV2	534	462	0.04%	0.005%
39	7.129	979	991	1002	rBV2	160741	358984	30.56%	3.715%
40	7.312	1013	1021	1034	rVV	239703	537813	45.78%	5.566%
41	7.476	1043	1048	1049	rBV2	958	1231	0.10%	0.013%
42	7.708	1084	1086	1089	rVB	628	418	0.04%	0.004%
43	7.745	1089	1092	1095	rVB2	529	442	0.04%	0.005%
44	7.775	1095	1097	1100	rBV2	377	511	0.04%	0.005%
45	7.940	1121	1124	1128	rBV2	537	950	0.08%	0.010%
46	8.147	1155	1158	1161	rBV2	329	563	0.05%	0.006%
47	8.232	1170	1172	1173	rBV	478	350	0.03%	0.004%
48	8.251	1173	1175	1178	rBV	413	374	0.03%	0.004%
49	8.330	1182	1188	1196	rBV	161452	260924	22.21%	2.700%
50	8.574	1227	1228	1232	rBV3	631	755	0.06%	0.008%
51	8.653	1234	1241	1255	rVV	603098	914738	77.86%	9.467%
52	8.860	1273	1275	1277	rBV2	549	495	0.04%	0.005%
53	8.952	1285	1290	1298	rBV	115931	174754	14.88%	1.809%
54	9.214	1329	1333	1334	rBV2	600	632	0.05%	0.007%
55	9.275	1338	1343	1349	rBV	23571	35367	3.01%	0.366%
56	9.391	1356	1362	1374	rBV	484521	689123	58.66%	7.132%
57	9.708	1410	1414	1419	rBV4	3553	5513	0.47%	0.057%
58	9.842	1434	1436	1438	rBV	473	578	0.05%	0.006%
59	9.878	1440	1442	1444	rVV	495	400	0.03%	0.004%
60	9.903	1444	1446	1449	rVB2	638	756	0.06%	0.008%
61	9.945	1451	1453	1456	rBV2	378	427	0.04%	0.004%
62	10.055	1466	1471	1481	rBV	512489	697892	59.41%	7.223%
63	10.256	1501	1504	1506	rBV2	310	421	0.04%	0.004%
64	10.317	1510	1514	1516	rVB2	722	931	0.08%	0.010%
65	10.360	1516	1521	1523	rBV2	461	700	0.06%	0.007%
66	10.409	1528	1529	1532	rBV	588	343	0.03%	0.004%
67	10.567	1551	1555	1556	rVV2	793	670	0.06%	0.007%
68	10.610	1560	1562	1564	rBV	304	358	0.03%	0.004%
69	10.756	1584	1586	1590	rBV2	266	375	0.03%	0.004%
70	10.829	1595	1598	1600	rBV	578	599	0.05%	0.006%
71	10.921	1611	1613	1615	rBV2	605	670	0.06%	0.007%
72	11.043	1630	1633	1635	rVV	540	421	0.04%	0.004%
73	11.195	1652	1658	1669	rVV	422284	542112	46.15%	5.611%
74	11.287	1672	1673	1676	rVV2	642	518	0.04%	0.005%
75	11.348	1681	1683	1685	rVB2	679	499	0.04%	0.005%
76	11.366	1685	1686	1688	rVB	533	343	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030436.D
 Acq On : 05 Aug 2022 17:43
 Operator : JC/MD
 Sample : N4003-09DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D34DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.433	1695	1697	1698	rBV	598	385	0.03%	0.004%
78	11.652	1732	1733	1736	rBV2	310	369	0.03%	0.004%
79	11.878	1765	1770	1772	rBV2	520	745	0.06%	0.008%
80	12.024	1788	1794	1806	rBV	519258	625408	53.24%	6.473%
81	12.250	1829	1831	1832	rBV	566	389	0.03%	0.004%
82	12.323	1837	1843	1856	rVV	603833	751240	63.95%	7.775%
83	12.841	1926	1928	1930	rBV2	385	422	0.04%	0.004%
84	12.988	1950	1952	1956	rVB2	474	457	0.04%	0.005%
85	13.292	2001	2002	2006	rBV2	427	524	0.04%	0.005%
86	13.378	2014	2016	2020	rVB2	391	447	0.04%	0.005%
87	13.506	2031	2037	2040	rVB2	773	1233	0.10%	0.013%
88	13.603	2049	2053	2054	rBV3	504	609	0.05%	0.006%
89	14.195	2149	2150	2156	rVB3	683	1071	0.09%	0.011%
90	14.286	2163	2165	2168	rVB3	357	409	0.03%	0.004%
91	14.384	2179	2181	2184	rBV2	642	514	0.04%	0.005%
92	14.414	2184	2186	2189	rBV2	353	519	0.04%	0.005%
93	14.542	2206	2207	2209	rBV2	581	352	0.03%	0.004%
94	14.603	2215	2217	2219	rBV2	520	433	0.04%	0.004%
95	14.725	2234	2237	2239	rBV2	712	816	0.07%	0.008%
96	14.743	2239	2240	2243	rVV2	468	437	0.04%	0.005%
97	15.127	2301	2303	2305	rBV	619	485	0.04%	0.005%
98	15.426	2350	2352	2353	rBV	717	378	0.03%	0.004%
99	15.457	2353	2357	2358	rBV2	657	617	0.05%	0.006%
100	15.859	2421	2423	2426	rBV2	564	638	0.05%	0.007%




Sum of corrected areas: 9662076

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030436.D
Acq On : 05 Aug 2022 17:43
Operator : JC/MD
Sample : N4003-09DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D34DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

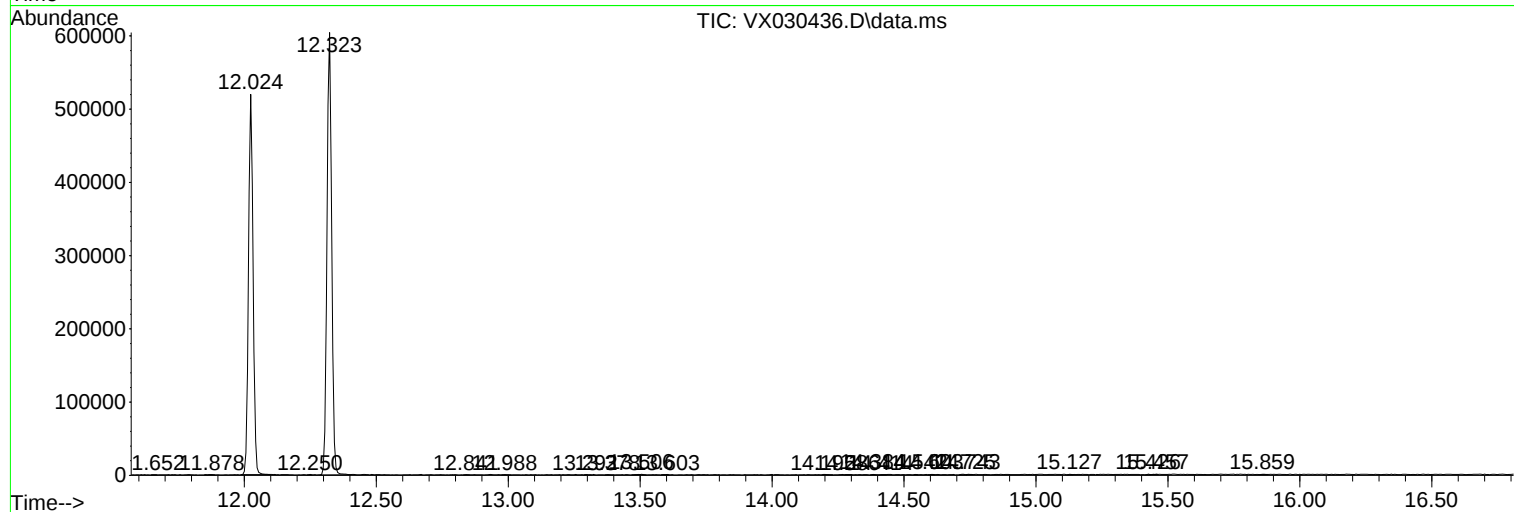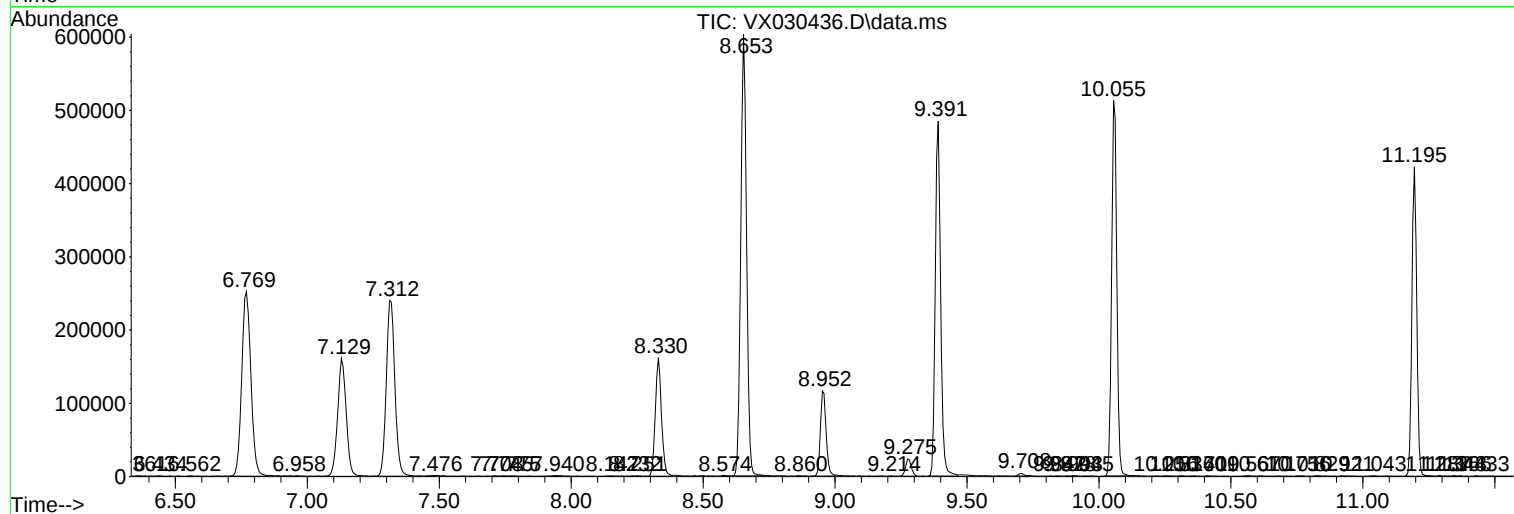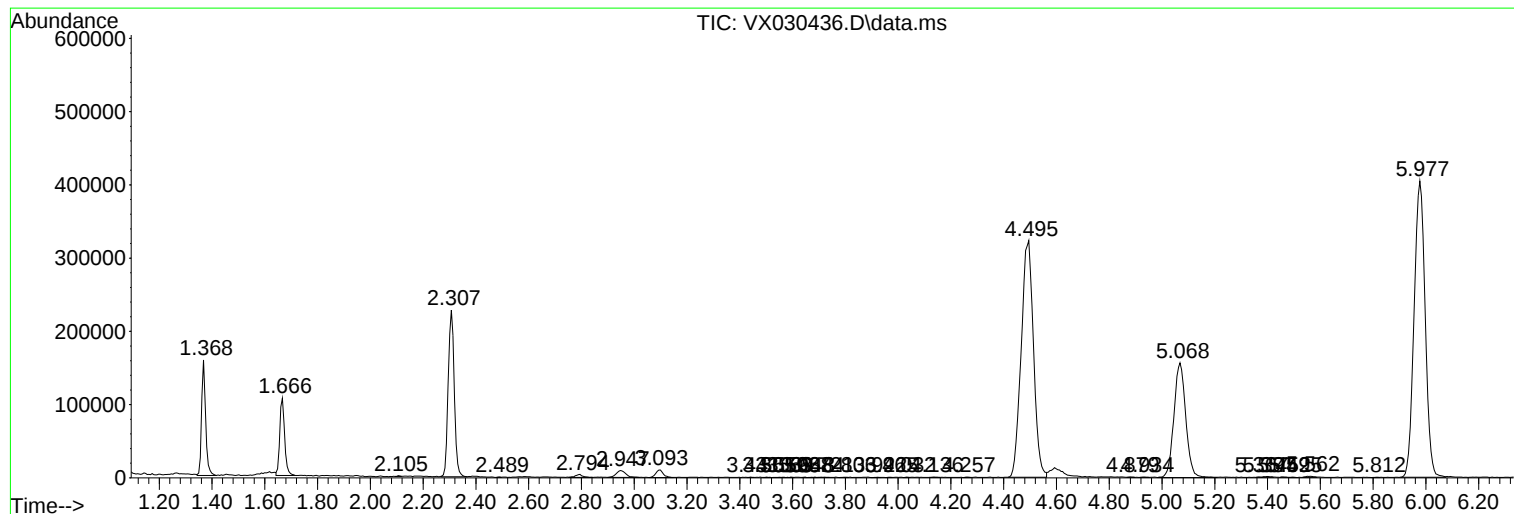

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030436.D
Acq On : 05 Aug 2022 17:43
Operator : JC/MD
Sample : N4003-09DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D34DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030436.D
Acq On : 05 Aug 2022 17:43
Operator : JC/MD
Sample : N4003-09DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D34DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc