

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030437.D
 Acq On : 05 Aug 2022 18:07
 Operator : JC/MD
 Sample : N4003-08DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D33DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030437.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB2	162890	173106	14.54%	1.791%
2	1.666	91	95	103	rVB	110655	138863	11.66%	1.437%
3	2.307	194	200	210	rVB	237393	370641	31.13%	3.835%
4	2.715	264	267	269	rBV	402	431	0.04%	0.004%
5	2.788	275	279	286	rVB4	3528	6161	0.52%	0.064%
6	2.947	300	305	313	rVV	7273	16603	1.39%	0.172%
7	3.093	323	329	339	rVB2	10167	19935	1.67%	0.206%
8	3.331	365	368	372	rVB2	464	712	0.06%	0.007%
9	3.410	379	381	383	rVB2	520	434	0.04%	0.004%
10	3.428	383	384	386	rBV	547	478	0.04%	0.005%
11	3.544	400	403	404	rBV	344	440	0.04%	0.005%
12	3.770	439	440	444	rVB2	472	577	0.05%	0.006%
13	3.818	444	448	449	rBV2	397	440	0.04%	0.005%
14	4.129	497	499	504	rBV3	344	422	0.04%	0.004%
15	4.294	521	526	528	rBV3	378	618	0.05%	0.006%
16	4.495	546	559	570	rBV2	307879	1014814	85.24%	10.500%
17	5.062	641	652	672	rVB	149535	482239	40.51%	4.990%
18	5.196	672	674	676	rBV	379	393	0.03%	0.004%
19	5.257	682	684	685	rBV2	561	408	0.03%	0.004%
20	5.391	700	706	707	rBV	1440	1672	0.14%	0.017%
21	5.562	728	734	740	rBV5	1856	4471	0.38%	0.046%
22	5.873	779	785	786	rVB2	499	618	0.05%	0.006%
23	5.885	786	787	789	rBV2	414	392	0.03%	0.004%
24	5.977	790	802	818	rVV2	413157	1190483	100.00%	12.318%
25	6.257	845	848	850	rBV2	430	470	0.04%	0.005%
26	6.373	862	867	869	rBV3	728	897	0.08%	0.009%
27	6.629	906	909	911	rBV	489	472	0.04%	0.005%
28	6.769	922	932	943	rBV	259498	620405	52.11%	6.419%
29	6.946	959	961	963	rVB3	641	545	0.05%	0.006%
30	6.970	963	965	967	rBV	477	515	0.04%	0.005%
31	7.050	976	978	980	rBV2	374	462	0.04%	0.005%
32	7.129	982	991	1004	rVV3	129509	293609	24.66%	3.038%
33	7.245	1009	1010	1013	rVV2	410	425	0.04%	0.004%
34	7.318	1013	1022	1041	rVB	242219	542767	45.59%	5.616%
35	7.458	1043	1045	1046	rBV	530	426	0.04%	0.004%
36	7.482	1046	1049	1052	rBV4	853	1316	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030437.D
 Acq On : 05 Aug 2022 18:07
 Operator : JC/MD
 Sample : N4003-08DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D33DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.562	1060	1062	1064	rVB	668	363	0.03%	0.004%
38	7.617	1069	1071	1075	rVB2	546	737	0.06%	0.008%
39	7.665	1075	1079	1080	rBV	324	368	0.03%	0.004%
40	7.714	1085	1087	1089	rVB2	576	427	0.04%	0.004%
41	7.763	1091	1095	1097	rBV2	385	452	0.04%	0.005%
42	7.867	1110	1112	1117	rVB2	401	448	0.04%	0.005%
43	7.934	1121	1123	1125	rBV2	731	559	0.05%	0.006%
44	7.976	1128	1130	1131	rBV	460	385	0.03%	0.004%
45	8.062	1140	1144	1145	rBV2	358	403	0.03%	0.004%
46	8.330	1179	1188	1199	rBV	164821	267934	22.51%	2.772%
47	8.482	1211	1213	1215	rBV3	573	669	0.06%	0.007%
48	8.592	1226	1231	1232	rBV4	825	1462	0.12%	0.015%
49	8.653	1234	1241	1252	rBV	586033	914308	76.80%	9.460%
50	8.952	1285	1290	1299	rBV	116425	174986	14.70%	1.811%
51	9.183	1325	1328	1330	rBV2	329	380	0.03%	0.004%
52	9.275	1337	1343	1349	rBV	17492	26834	2.25%	0.278%
53	9.342	1351	1354	1356	rBV2	646	708	0.06%	0.007%
54	9.391	1356	1362	1375	rBV	493510	706831	59.37%	7.313%
55	9.708	1410	1414	1419	rVB2	2315	3102	0.26%	0.032%
56	9.860	1437	1439	1441	rBV2	570	381	0.03%	0.004%
57	9.982	1454	1459	1461	rVB	451	514	0.04%	0.005%
58	10.055	1466	1471	1484	rVB	523429	705845	59.29%	7.303%
59	10.256	1502	1504	1506	rVB	798	443	0.04%	0.005%
60	10.305	1510	1512	1516	rBV2	493	585	0.05%	0.006%
61	10.683	1573	1574	1577	rVV	465	423	0.04%	0.004%
62	10.793	1590	1592	1596	rVB2	582	660	0.06%	0.007%
63	10.890	1605	1608	1611	rBV2	397	451	0.04%	0.005%
64	10.976	1621	1622	1626	rBV2	427	524	0.04%	0.005%
65	11.043	1632	1633	1636	rBV	332	384	0.03%	0.004%
66	11.079	1636	1639	1641	rVV2	495	478	0.04%	0.005%
67	11.195	1652	1658	1670	rVB	450010	548069	46.04%	5.671%
68	11.598	1721	1724	1725	rBV2	367	411	0.03%	0.004%
69	11.707	1740	1742	1745	rBV3	527	513	0.04%	0.005%
70	11.762	1748	1751	1752	rBV2	462	450	0.04%	0.005%
71	11.866	1766	1768	1770	rBV	586	390	0.03%	0.004%
72	12.024	1788	1794	1804	rBV	522412	636284	53.45%	6.583%
73	12.232	1826	1828	1829	rBV2	496	374	0.03%	0.004%
74	12.323	1837	1843	1851	rBV	611836	764489	64.22%	7.910%
75	12.512	1873	1874	1876	rVB	690	356	0.03%	0.004%
76	12.530	1876	1877	1879	rBV	563	429	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030437.D
 Acq On : 05 Aug 2022 18:07
 Operator : JC/MD
 Sample : N4003-08DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D33DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.591	1883	1887	1889	rBV3	669	804	0.07%	0.008%
78	12.738	1910	1911	1913	rVB	822	479	0.04%	0.005%
79	12.768	1913	1916	1918	rBV2	402	579	0.05%	0.006%
80	12.792	1918	1920	1925	rBV2	470	791	0.07%	0.008%
81	12.933	1941	1943	1944	rBV2	390	381	0.03%	0.004%
82	13.042	1959	1961	1962	rBV	522	425	0.04%	0.004%
83	13.219	1988	1990	1992	rBV	406	367	0.03%	0.004%
84	13.292	2001	2002	2005	rBV2	377	417	0.04%	0.004%
85	13.433	2020	2025	2026	rBV3	420	679	0.06%	0.007%
86	13.786	2077	2083	2087	rBV2	640	1309	0.11%	0.014%
87	13.841	2090	2092	2094	rVB2	585	537	0.05%	0.006%
88	13.890	2097	2100	2102	rBV2	409	492	0.04%	0.005%
89	14.122	2136	2138	2142	rBV3	375	487	0.04%	0.005%
90	14.182	2146	2148	2150	rBV	576	519	0.04%	0.005%
91	14.237	2155	2157	2159	rBV2	444	512	0.04%	0.005%
92	14.402	2182	2184	2185	rBV2	629	536	0.05%	0.006%
93	14.670	2226	2228	2231	rBV4	409	527	0.04%	0.005%
94	14.890	2263	2264	2266	rVB	855	585	0.05%	0.006%
95	15.146	2304	2306	2310	rVB2	576	424	0.04%	0.004%
96	15.621	2381	2384	2386	rBV2	602	863	0.07%	0.009%
97	15.835	2418	2419	2422	rBV2	623	477	0.04%	0.005%
98	16.237	2483	2485	2486	rBV	698	462	0.04%	0.005%
99	16.420	2514	2515	2518	rVB	695	444	0.04%	0.005%
100	16.493	2526	2527	2528	rBV	804	358	0.03%	0.004%




Sum of corrected areas: 9664923

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030437.D
Acq On : 05 Aug 2022 18:07
Operator : JC/MD
Sample : N4003-08DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D33DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

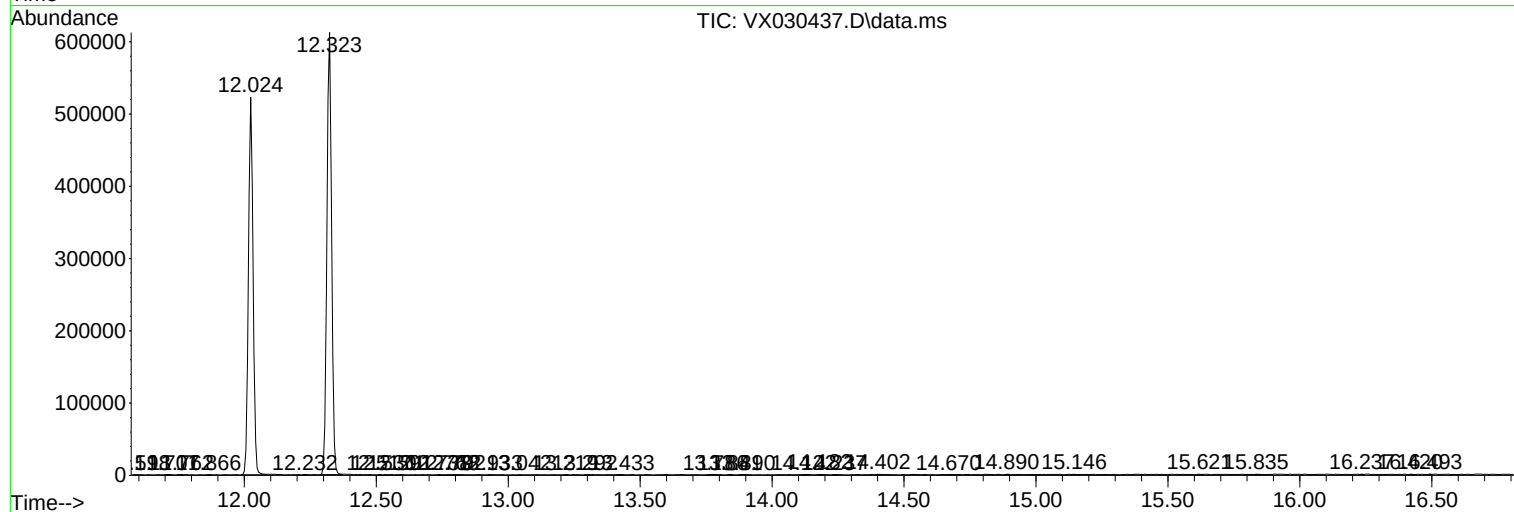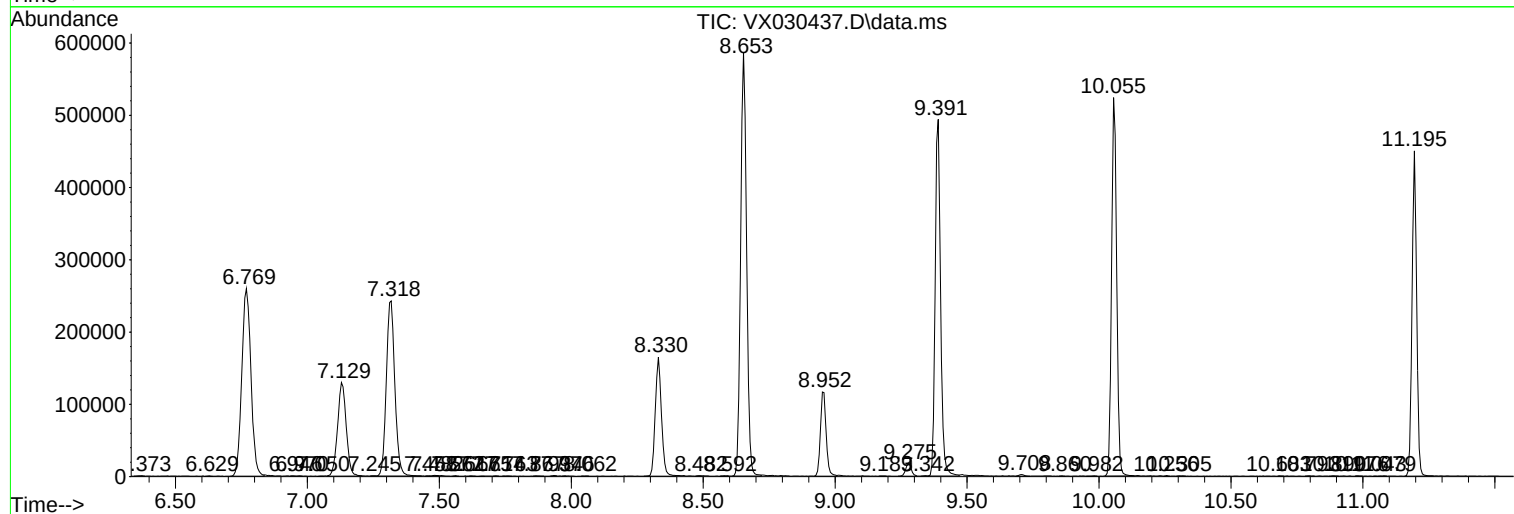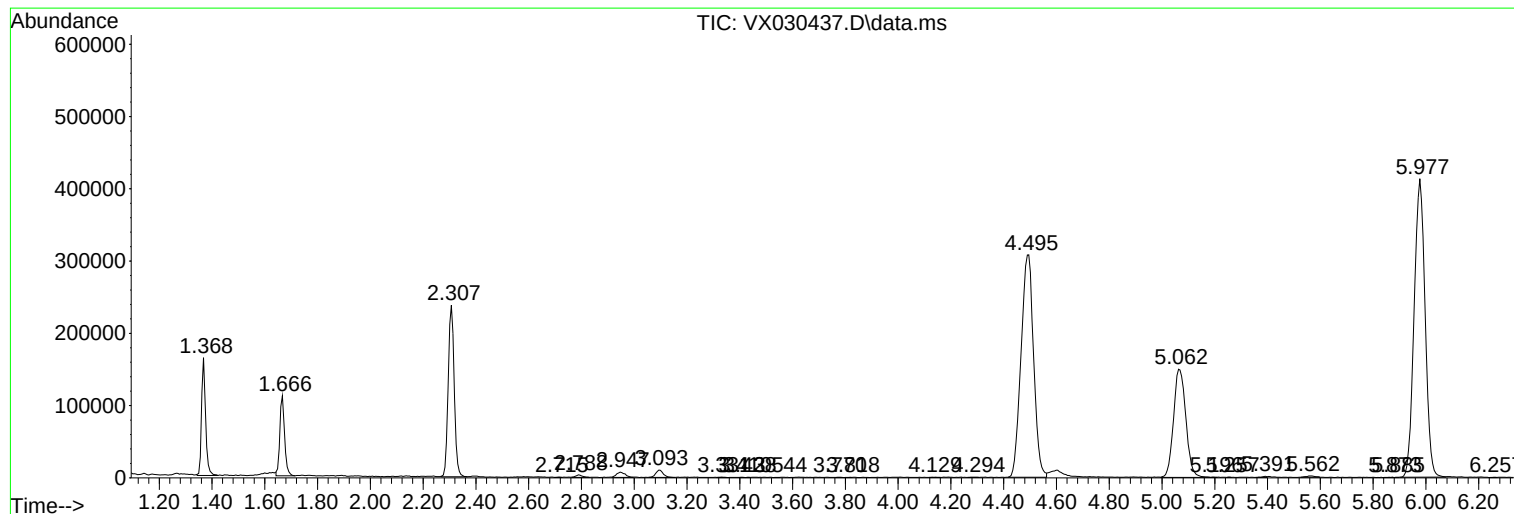

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030437.D
Acq On : 05 Aug 2022 18:07
Operator : JC/MD
Sample : N4003-08DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D33DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030437.D
Acq On : 05 Aug 2022 18:07
Operator : JC/MD
Sample : N4003-08DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D33DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------