

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030443.D
 Acq On : 05 Aug 2022 21:15
 Operator : JC/MD
 Sample : N4066-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030443.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB2	147401	159986	14.71%	1.867%
2	1.666	91	95	102	rVB	96589	120752	11.10%	1.409%
3	2.306	194	200	209	rVB	211523	324185	29.80%	3.784%
4	2.508	229	233	238	rBV5	1012	1944	0.18%	0.023%
5	2.605	248	249	250	rBV	617	322	0.03%	0.004%
6	2.654	254	257	258	rVB	628	601	0.06%	0.007%
7	2.672	258	260	261	rBV	510	427	0.04%	0.005%
8	2.691	261	263	264	rBV	344	307	0.03%	0.004%
9	2.788	278	279	283	rBV2	907	908	0.08%	0.011%
10	2.892	295	296	300	rBV2	491	425	0.04%	0.005%
11	3.099	320	330	337	rBV2	6204	15232	1.40%	0.178%
12	3.203	343	347	349	rVB2	330	387	0.04%	0.005%
13	3.233	349	352	354	rBV2	504	435	0.04%	0.005%
14	3.294	359	362	363	rBV2	338	304	0.03%	0.004%
15	3.453	385	388	389	rVV2	358	391	0.04%	0.005%
16	3.617	413	415	418	rBV2	317	303	0.03%	0.004%
17	3.690	425	427	430	rBV3	310	303	0.03%	0.004%
18	3.800	443	445	449	rBV2	303	426	0.04%	0.005%
19	3.855	452	454	455	rVB2	552	363	0.03%	0.004%
20	3.892	457	460	462	rVB2	389	400	0.04%	0.005%
21	3.922	462	465	466	rBV2	397	428	0.04%	0.005%
22	3.977	472	474	478	rBV2	331	522	0.05%	0.006%
23	4.257	518	520	523	rVB2	359	419	0.04%	0.005%
24	4.343	531	534	536	rBV2	397	366	0.03%	0.004%
25	4.489	545	558	577	rBV2	236410	802399	73.76%	9.365%
26	4.733	595	598	601	rBV3	477	681	0.06%	0.008%
27	4.934	630	631	634	rBV2	332	319	0.03%	0.004%
28	4.977	636	638	640	rVB	560	421	0.04%	0.005%
29	5.062	640	652	672	rBV	146110	457940	42.10%	5.345%
30	5.202	672	675	676	rBV	577	535	0.05%	0.006%
31	5.269	684	686	690	rVV	531	405	0.04%	0.005%
32	5.550	728	732	734	rBV2	520	850	0.08%	0.010%
33	5.696	755	756	759	rBV	443	434	0.04%	0.005%
34	5.977	790	802	817	rBV2	373755	1087826	100.00%	12.696%
35	6.117	824	825	828	rVB2	913	494	0.05%	0.006%
36	6.342	861	862	864	rBV2	648	350	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030443.D
 Acq On : 05 Aug 2022 21:15
 Operator : JC/MD
 Sample : N4066-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.367	864	866	868	rVV2	676	665	0.06%	0.008%
38	6.391	868	870	873	rVB	481	305	0.03%	0.004%
39	6.769	922	932	943	rBV	244760	586032	53.87%	6.840%
40	6.922	956	957	959	rVB	633	334	0.03%	0.004%
41	7.037	974	976	978	rVB2	452	315	0.03%	0.004%
42	7.117	978	989	1000	rVB5	10594	27463	2.52%	0.321%
43	7.220	1004	1006	1008	rBV2	436	347	0.03%	0.004%
44	7.245	1008	1010	1012	rBV2	347	338	0.03%	0.004%
45	7.318	1013	1022	1034	rVV	227805	503325	46.27%	5.874%
46	7.421	1038	1039	1043	rVB4	613	742	0.07%	0.009%
47	7.458	1043	1045	1046	rBV2	481	292	0.03%	0.003%
48	7.488	1048	1050	1052	rVB2	803	663	0.06%	0.008%
49	7.909	1116	1119	1121	rBV2	569	572	0.05%	0.007%
50	8.251	1174	1175	1180	rBV2	474	513	0.05%	0.006%
51	8.330	1181	1188	1198	rBV	151135	245750	22.59%	2.868%
52	8.653	1234	1241	1251	rBV	548776	830309	76.33%	9.691%
53	8.952	1285	1290	1299	rVV	103501	158687	14.59%	1.852%
54	9.275	1341	1343	1347	rVB2	1280	1271	0.12%	0.015%
55	9.311	1347	1349	1350	rBV2	493	353	0.03%	0.004%
56	9.391	1356	1362	1374	rBV	470067	671280	61.71%	7.835%
57	9.647	1402	1404	1406	rBV2	758	430	0.04%	0.005%
58	9.708	1412	1414	1416	rBV	623	658	0.06%	0.008%
59	9.738	1417	1419	1423	rVB3	597	661	0.06%	0.008%
60	9.817	1429	1432	1435	rVB2	430	477	0.04%	0.006%
61	10.055	1466	1471	1485	rVB	498748	681393	62.64%	7.953%
62	10.378	1522	1524	1525	rBV	390	297	0.03%	0.003%
63	10.433	1530	1533	1536	rBV3	578	829	0.08%	0.010%
64	10.592	1557	1559	1561	rBV2	311	369	0.03%	0.004%
65	10.659	1568	1570	1572	rVV2	838	568	0.05%	0.007%
66	10.683	1572	1574	1576	rVB2	414	316	0.03%	0.004%
67	10.781	1589	1590	1593	rBV2	485	422	0.04%	0.005%
68	10.909	1608	1611	1614	rBV2	349	485	0.04%	0.006%
69	11.061	1633	1636	1637	rBV	404	426	0.04%	0.005%
70	11.195	1652	1658	1666	rBV	424213	528234	48.56%	6.165%
71	11.280	1671	1672	1676	rVB	708	576	0.05%	0.007%
72	11.439	1694	1698	1699	rBV2	546	511	0.05%	0.006%
73	11.488	1705	1706	1708	rVB2	669	369	0.03%	0.004%
74	11.506	1708	1709	1711	rBV	550	457	0.04%	0.005%
75	11.713	1739	1743	1745	rVB2	654	719	0.07%	0.008%
76	11.835	1761	1763	1766	rBV2	449	476	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030443.D
 Acq On : 05 Aug 2022 21:15
 Operator : JC/MD
 Sample : N4066-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.024	1789	1794	1804	rVB	515064	620004	56.99%	7.236%
78	12.280	1834	1836	1837	rBV	580	376	0.03%	0.004%
79	12.323	1837	1843	1852	rVV	563534	705390	64.84%	8.233%
80	12.756	1911	1914	1916	rBV2	410	408	0.04%	0.005%
81	12.835	1925	1927	1928	rBV	407	375	0.03%	0.004%
82	12.896	1935	1937	1940	rBV	720	673	0.06%	0.008%
83	12.939	1942	1944	1947	rVB	490	436	0.04%	0.005%
84	13.396	2018	2019	2022	rBV	380	395	0.04%	0.005%
85	13.469	2028	2031	2034	rVB2	461	567	0.05%	0.007%
86	13.871	2095	2097	2098	rVB	553	345	0.03%	0.004%
87	14.402	2182	2184	2185	rBV	608	416	0.04%	0.005%
88	14.463	2192	2194	2197	rBV2	479	457	0.04%	0.005%
89	14.579	2211	2213	2215	rBV2	447	291	0.03%	0.003%
90	14.652	2223	2225	2227	rVV2	573	450	0.04%	0.005%
91	14.676	2227	2229	2231	rVV2	577	500	0.05%	0.006%
92	14.725	2234	2237	2239	rBV2	555	518	0.05%	0.006%
93	14.786	2246	2247	2248	rVB	917	336	0.03%	0.004%
94	14.816	2248	2252	2257	rBV3	709	1474	0.14%	0.017%
95	15.518	2365	2367	2371	rBV4	584	1038	0.10%	0.012%
96	15.579	2375	2377	2378	rBV	726	414	0.04%	0.005%
97	15.975	2441	2442	2446	rVB4	770	857	0.08%	0.010%
98	16.152	2469	2471	2472	rVB2	841	417	0.04%	0.005%
99	16.310	2496	2497	2499	rBV	718	436	0.04%	0.005%
100	16.511	2528	2530	2532	rBV3	780	467	0.04%	0.005%


Sum of corrected areas: 8568059

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030443.D
Acq On : 05 Aug 2022 21:15
Operator : JC/MD
Sample : N4066-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

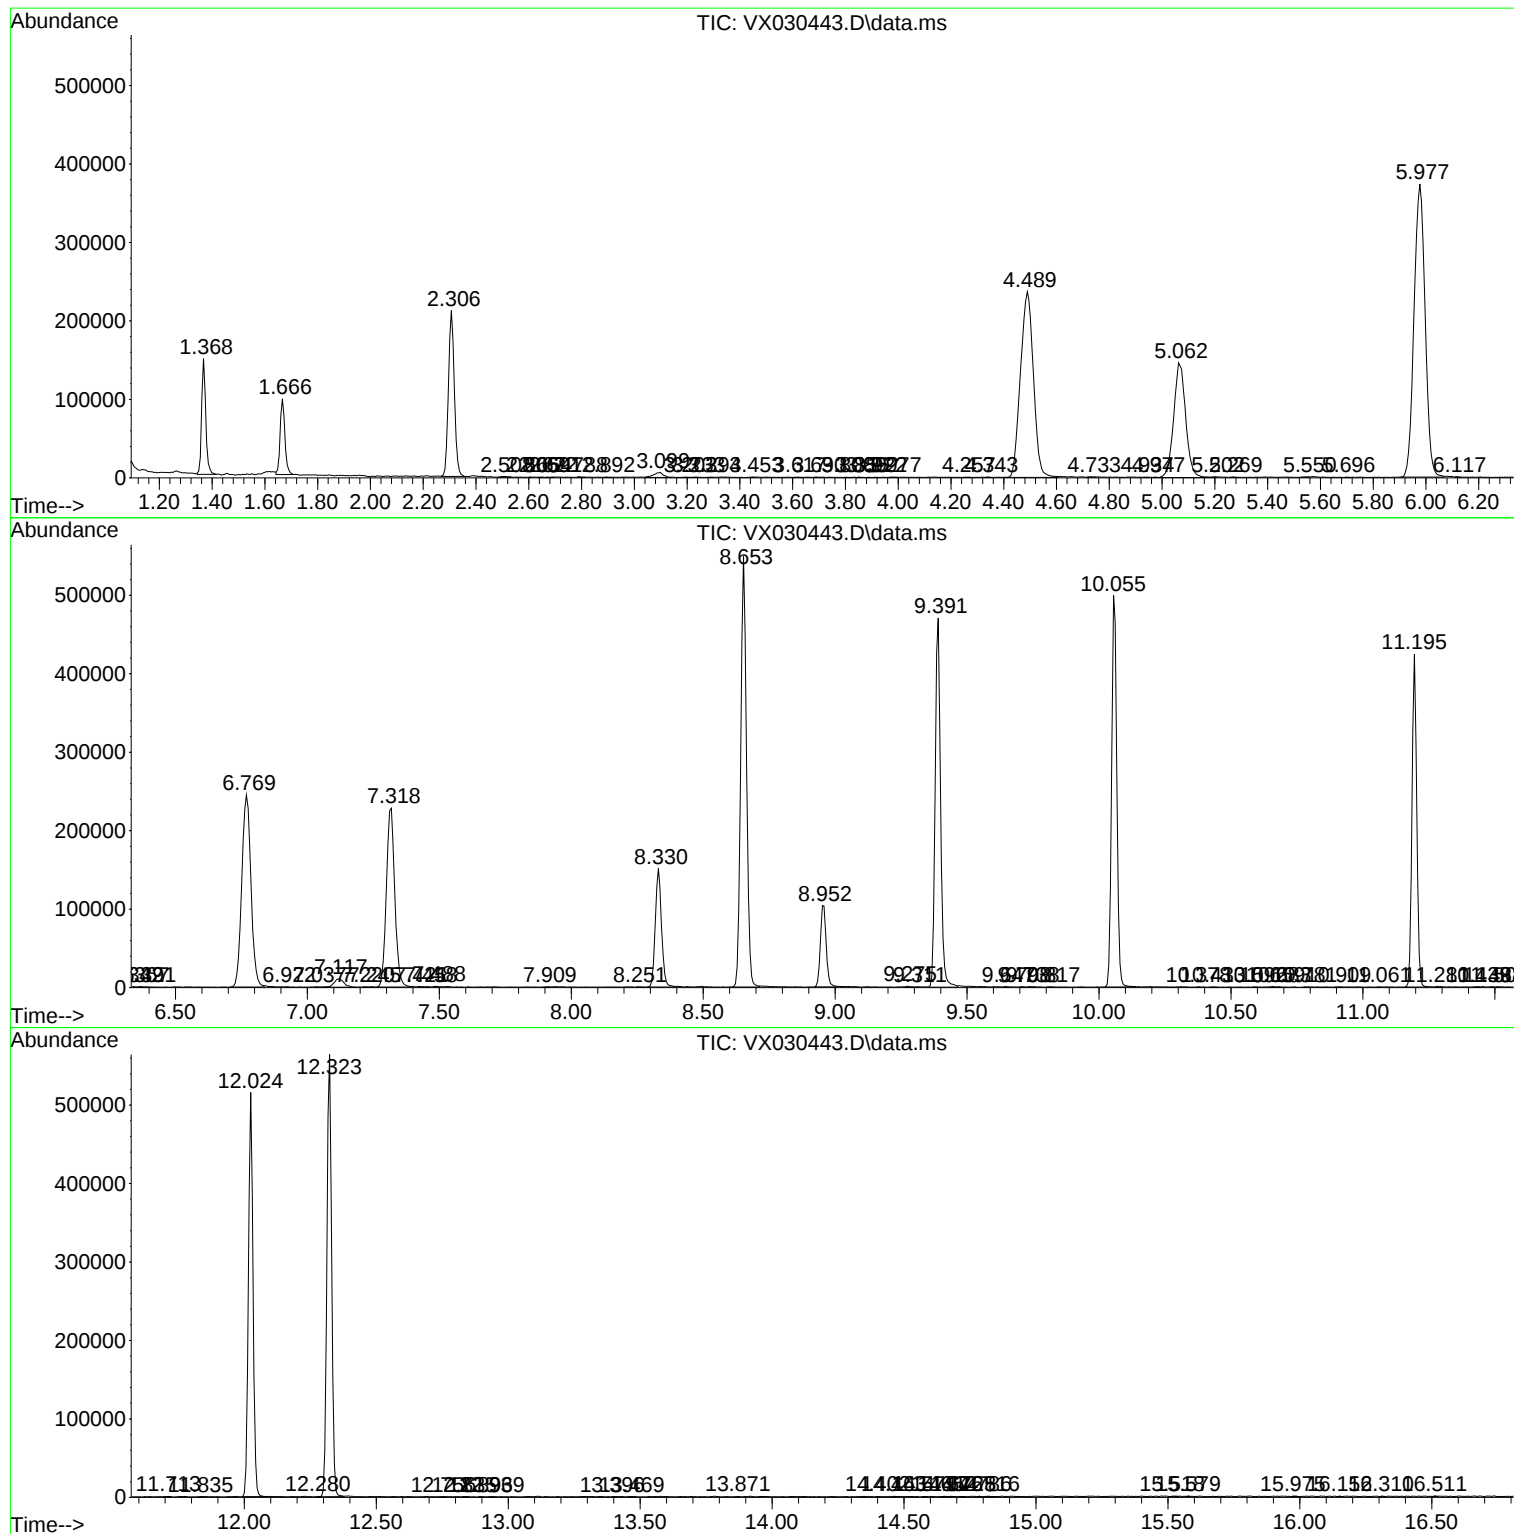

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030443.D
Acq On : 05 Aug 2022 21:15
Operator : JC/MD
Sample : N4066-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030443.D
Acq On : 05 Aug 2022 21:15
Operator : JC/MD
Sample : N4066-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc