

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030446.D
 Acq On : 05 Aug 2022 22:25
 Operator : JC/MD
 Sample : N4066-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030446.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	56	rVB2	406867	480335	11.15%	3.782%
2	1.666	91	95	104	rVB2	110498	152159	3.53%	1.198%
3	2.307	194	200	211	rVB	216048	331153	7.69%	2.608%
4	2.386	211	213	215	rBV3	820	729	0.02%	0.006%
5	2.477	226	228	230	rBV2	434	408	0.01%	0.003%
6	2.514	230	234	235	rVV2	1019	823	0.02%	0.006%
7	2.782	276	278	281	rVV3	667	611	0.01%	0.005%
8	2.806	281	282	286	rVB3	905	616	0.01%	0.005%
9	2.849	287	289	291	rBV2	525	480	0.01%	0.004%
10	2.971	307	309	311	rVV2	396	414	0.01%	0.003%
11	3.099	322	330	343	rVB2	29245	66088	1.53%	0.520%
12	3.239	350	353	356	rVB3	506	589	0.01%	0.005%
13	3.294	360	362	365	rBV2	487	584	0.01%	0.005%
14	3.422	379	383	386	rBV	279	468	0.01%	0.004%
15	3.508	395	397	402	rVB2	409	512	0.01%	0.004%
16	3.581	406	409	411	rBV	321	399	0.01%	0.003%
17	3.733	431	434	437	rVV2	409	563	0.01%	0.004%
18	3.953	468	470	472	rBV2	435	463	0.01%	0.004%
19	4.014	476	480	481	rBV2	425	400	0.01%	0.003%
20	4.160	500	504	506	rVB3	421	483	0.01%	0.004%
21	4.184	506	508	512	rBV2	346	533	0.01%	0.004%
22	4.495	546	559	574	rBV2	1546022	4307704	100.00%	33.921%
23	4.843	614	616	618	rBV2	481	500	0.01%	0.004%
24	4.891	620	624	626	rBV4	576	780	0.02%	0.006%
25	5.068	640	653	669	rBV	153342	470816	10.93%	3.707%
26	5.361	696	701	702	rBV	477	694	0.02%	0.005%
27	5.379	702	704	705	rBV2	390	403	0.01%	0.003%
28	5.483	717	721	723	rBV3	590	832	0.02%	0.007%
29	5.562	729	734	735	rBV2	786	1251	0.03%	0.010%
30	5.812	773	775	779	rVB3	469	642	0.01%	0.005%
31	5.977	790	802	820	rBV2	384273	1121130	26.03%	8.828%
32	6.300	851	855	857	rBV	556	664	0.02%	0.005%
33	6.367	864	866	867	rBV	513	381	0.01%	0.003%
34	6.477	883	884	888	rVB	742	651	0.02%	0.005%
35	6.769	923	932	943	rVV	249112	592377	13.75%	4.665%
36	7.037	975	976	980	rVB2	360	379	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030446.D
 Acq On : 05 Aug 2022 22:25
 Operator : JC/MD
 Sample : N4066-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.129	982	991	1001	rVV3	27421	72798	1.69%	0.573%
38	7.312	1013	1021	1035	rVV	232236	516741	12.00%	4.069%
39	7.434	1040	1041	1046	rBV	564	646	0.01%	0.005%
40	7.482	1046	1049	1052	rBV3	1117	1486	0.03%	0.012%
41	7.836	1104	1107	1110	rBV	450	521	0.01%	0.004%
42	7.940	1121	1124	1126	rBV4	754	963	0.02%	0.008%
43	8.074	1144	1146	1149	rBV3	531	568	0.01%	0.004%
44	8.147	1156	1158	1162	rBV	591	581	0.01%	0.005%
45	8.184	1162	1164	1168	rBV	508	574	0.01%	0.005%
46	8.330	1179	1188	1197	rBV	151621	248449	5.77%	1.956%
47	8.494	1211	1215	1216	rBV2	659	796	0.02%	0.006%
48	8.653	1234	1241	1252	rBV	554801	848389	19.69%	6.681%
49	8.879	1277	1278	1282	rVB2	694	415	0.01%	0.003%
50	8.909	1282	1283	1285	rBV	571	537	0.01%	0.004%
51	8.952	1285	1290	1304	rVV	107755	162980	3.78%	1.283%
52	9.275	1340	1343	1349	rVB5	3737	6187	0.14%	0.049%
53	9.391	1356	1362	1379	rBV	478134	698079	16.21%	5.497%
54	9.592	1393	1395	1397	rBV2	506	423	0.01%	0.003%
55	9.927	1448	1450	1453	rBV2	280	404	0.01%	0.003%
56	10.055	1465	1471	1482	rBV	498899	688105	15.97%	5.418%
57	10.317	1510	1514	1515	rBV2	420	480	0.01%	0.004%
58	10.427	1528	1532	1533	rBV	462	515	0.01%	0.004%
59	10.500	1543	1544	1547	rVB2	634	503	0.01%	0.004%
60	10.531	1547	1549	1553	rBV3	499	735	0.02%	0.006%
61	10.793	1590	1592	1594	rVV2	511	436	0.01%	0.003%
62	11.195	1652	1658	1668	rVB	443362	542844	12.60%	4.275%
63	11.274	1668	1671	1673	rBV2	544	673	0.02%	0.005%
64	11.543	1714	1715	1718	rBV2	425	434	0.01%	0.003%
65	11.866	1765	1768	1770	rBV2	456	509	0.01%	0.004%
66	12.024	1789	1794	1804	rVV	510153	612228	14.21%	4.821%
67	12.134	1809	1812	1816	rVB4	886	1129	0.03%	0.009%
68	12.323	1837	1843	1853	rBV	579003	732132	17.00%	5.765%
69	12.500	1870	1872	1875	rBV	636	660	0.02%	0.005%
70	12.579	1881	1885	1886	rBV3	376	545	0.01%	0.004%
71	12.756	1912	1914	1916	rBV2	487	489	0.01%	0.004%
72	12.805	1919	1922	1926	rVB2	349	564	0.01%	0.004%
73	12.860	1929	1931	1933	rVB	839	595	0.01%	0.005%
74	12.988	1950	1952	1955	rBV2	493	651	0.02%	0.005%
75	13.085	1966	1968	1970	rBV2	361	440	0.01%	0.003%
76	13.213	1987	1989	1993	rVB2	489	602	0.01%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030446.D
 Acq On : 05 Aug 2022 22:25
 Operator : JC/MD
 Sample : N4066-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	13.366	2010	2014	2016	rVB2	348	400	0.01%	0.003%
78	13.481	2030	2033	2034	rBV2	462	512	0.01%	0.004%
79	13.609	2053	2054	2057	rVB	513	431	0.01%	0.003%
80	13.689	2065	2067	2070	rBV2	491	599	0.01%	0.005%
81	13.756	2076	2078	2080	rBV	637	569	0.01%	0.004%
82	13.865	2090	2096	2098	rVB3	652	972	0.02%	0.008%
83	13.963	2109	2112	2114	rBV2	525	598	0.01%	0.005%
84	14.079	2128	2131	2132	rBV2	391	389	0.01%	0.003%
85	14.134	2138	2140	2144	rVB2	716	765	0.02%	0.006%
86	14.286	2162	2165	2168	rBV2	620	1133	0.03%	0.009%
87	14.310	2168	2169	2171	rVV	887	396	0.01%	0.003%
88	14.341	2172	2174	2178	rVB	543	525	0.01%	0.004%
89	14.384	2178	2181	2183	rBV2	443	433	0.01%	0.003%
90	14.493	2196	2199	2201	rBV3	619	809	0.02%	0.006%
91	14.749	2240	2241	2243	rBV	628	444	0.01%	0.003%
92	14.890	2261	2264	2265	rBV3	595	675	0.02%	0.005%
93	14.938	2270	2272	2273	rBV2	501	407	0.01%	0.003%
94	15.414	2348	2350	2352	rBV2	573	496	0.01%	0.004%
95	15.999	2444	2446	2448	rBV2	504	407	0.01%	0.003%
96	16.097	2460	2462	2465	rBV3	768	758	0.02%	0.006%
97	16.194	2475	2478	2482	rBV4	769	993	0.02%	0.008%
98	16.225	2482	2483	2485	rBV	756	447	0.01%	0.004%
99	16.286	2491	2493	2499	rBV3	616	827	0.02%	0.007%
100	16.560	2536	2538	2540	rBV2	523	458	0.01%	0.004%




Sum of corrected areas: 12699263

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030446.D
Acq On : 05 Aug 2022 22:25
Operator : JC/MD
Sample : N4066-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

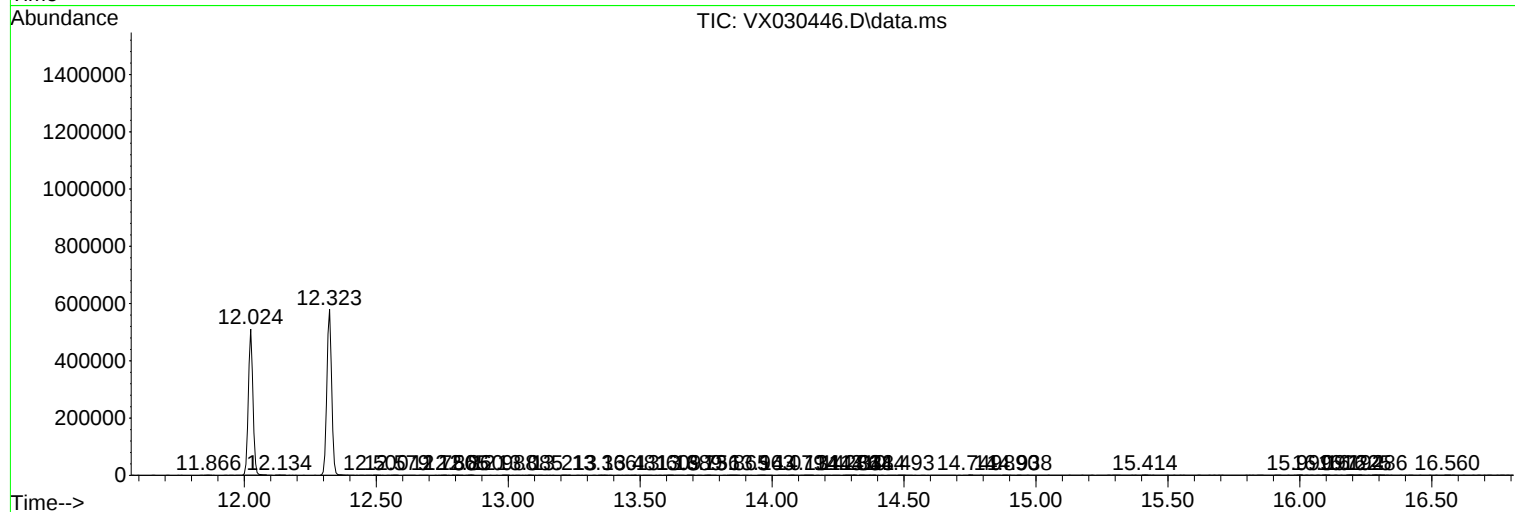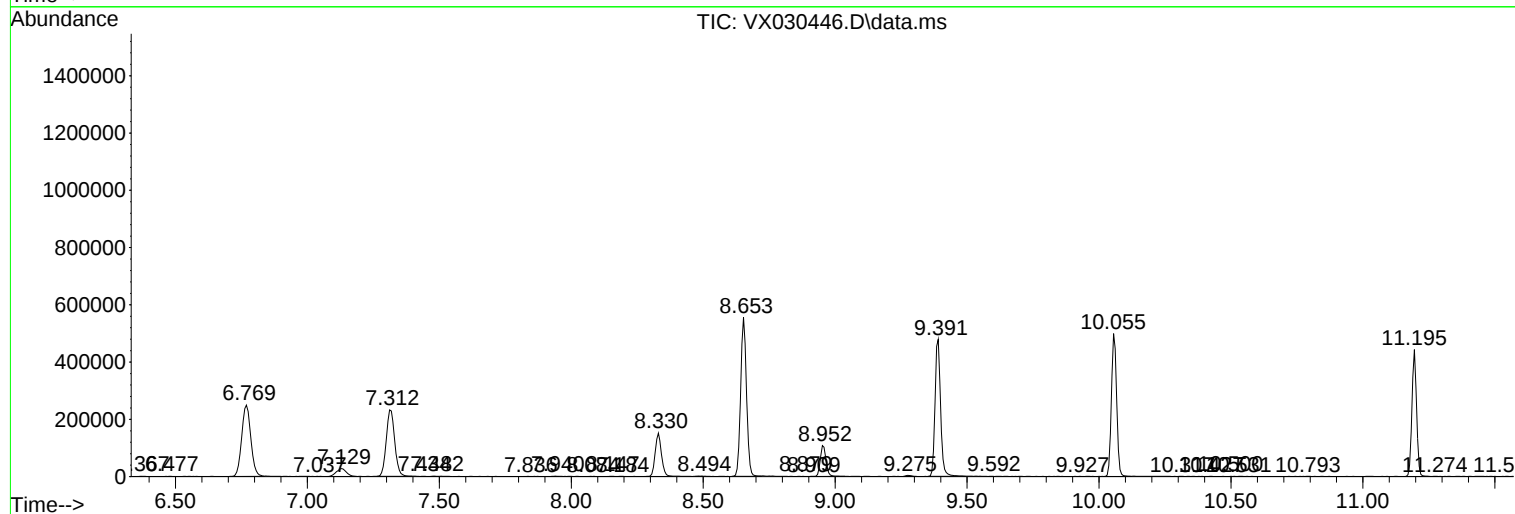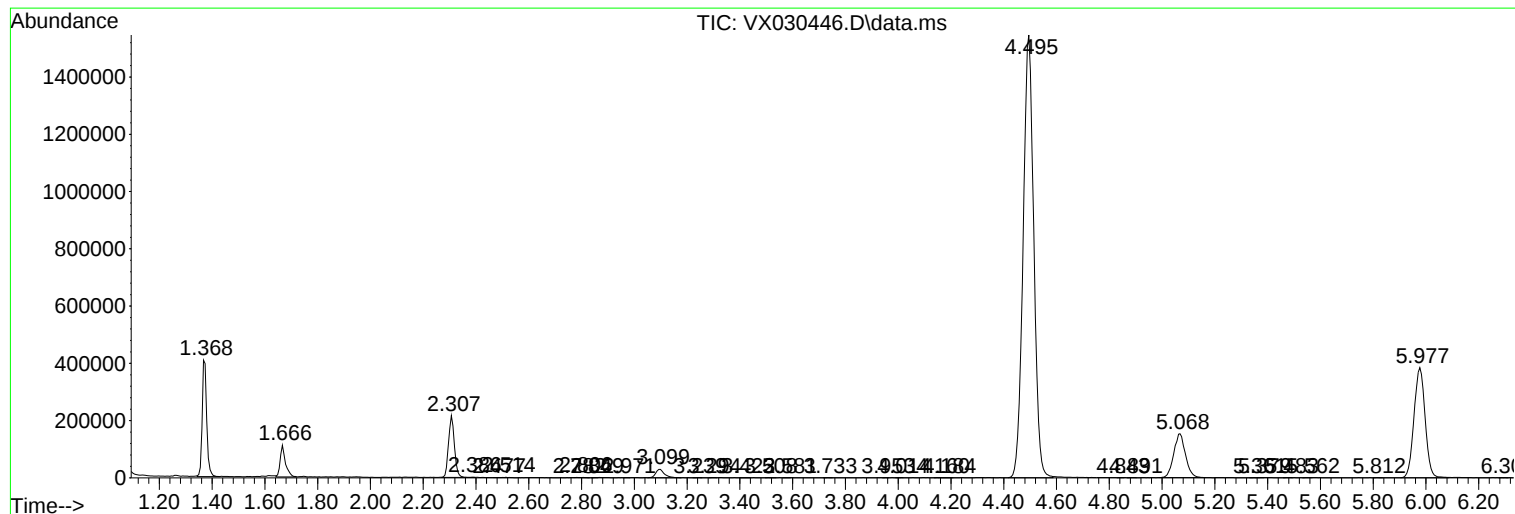

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030446.D
Acq On : 05 Aug 2022 22:25
Operator : JC/MD
Sample : N4066-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030446.D
Acq On : 05 Aug 2022 22:25
Operator : JC/MD
Sample : N4066-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc