

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030447.D
 Acq On : 05 Aug 2022 22:49
 Operator : JC/MD
 Sample : N4066-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E25

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030447.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	41	46	56	rVB2	218605	258410	12.02%	2.053%
2	1.666	91	95	102	rVB	97090	123600	5.75%	0.982%
3	2.197	180	182	186	rBV4	1025	1252	0.06%	0.010%
4	2.306	194	200	211	rVV	204528	318837	14.83%	2.533%
5	2.392	212	214	217	rVB3	1574	1379	0.06%	0.011%
6	2.465	224	226	229	rBV3	614	665	0.03%	0.005%
7	2.636	253	254	257	rVB2	431	249	0.01%	0.002%
8	2.684	260	262	263	rVB	538	250	0.01%	0.002%
9	2.788	275	279	284	rVB4	1123	1565	0.07%	0.012%
10	2.825	284	285	288	rBV3	589	474	0.02%	0.004%
11	2.861	288	291	294	rVB2	521	657	0.03%	0.005%
12	2.953	304	306	308	rBV2	317	259	0.01%	0.002%
13	3.093	323	329	340	rVB2	41996	77399	3.60%	0.615%
14	3.172	340	342	344	rBV2	381	393	0.02%	0.003%
15	3.300	362	363	365	rBV	382	289	0.01%	0.002%
16	3.337	367	369	371	rBV	450	374	0.02%	0.003%
17	3.635	415	418	419	rBV	336	281	0.01%	0.002%
18	3.684	425	426	430	rVB	370	360	0.02%	0.003%
19	3.837	449	451	454	rVB2	294	344	0.02%	0.003%
20	4.013	477	480	483	rVB2	436	595	0.03%	0.005%
21	4.050	483	486	488	rBV2	549	659	0.03%	0.005%
22	4.099	492	494	495	rBV2	602	362	0.02%	0.003%
23	4.160	502	504	507	rBV	625	465	0.02%	0.004%
24	4.495	544	559	580	rBV2	718368	2150113	100.00%	17.082%
25	4.824	612	613	614	rBV	608	320	0.01%	0.003%
26	5.062	640	652	668	rVV	147520	462515	21.51%	3.675%
27	5.318	691	694	695	rBV2	432	449	0.02%	0.004%
28	5.507	723	725	727	rVB	502	269	0.01%	0.002%
29	5.623	742	744	746	rBV2	323	364	0.02%	0.003%
30	5.672	751	752	757	rVV	383	447	0.02%	0.004%
31	5.781	768	770	773	rVB2	342	363	0.02%	0.003%
32	5.848	780	781	783	rVB2	565	341	0.02%	0.003%
33	5.897	785	789	790	rVV	338	320	0.01%	0.003%
34	5.976	790	802	821	rVV2	370582	1092360	50.80%	8.679%
35	6.172	832	834	837	rBV2	461	417	0.02%	0.003%
36	6.226	842	843	847	rBV	369	553	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030447.D
 Acq On : 05 Aug 2022 22:49
 Operator : JC/MD
 Sample : N4066-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E25

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.324	857	859	862	rBV	412	415	0.02%	0.003%
38	6.367	864	866	871	rVB4	840	1139	0.05%	0.009%
39	6.531	892	893	895	rBV2	437	410	0.02%	0.003%
40	6.635	908	910	913	rBV3	350	401	0.02%	0.003%
41	6.702	919	921	922	rBV	323	249	0.01%	0.002%
42	6.769	922	932	943	rBV	260241	609210	28.33%	4.840%
43	6.934	957	959	962	rVB2	602	457	0.02%	0.004%
44	7.001	967	970	972	rBV2	382	427	0.02%	0.003%
45	7.129	979	991	1004	rBV	471714	1049820	48.83%	8.341%
46	7.312	1012	1021	1039	rBV	233396	512379	23.83%	4.071%
47	7.470	1044	1047	1049	rBV2	933	1183	0.06%	0.009%
48	7.592	1062	1067	1069	rBV2	479	788	0.04%	0.006%
49	7.696	1082	1084	1085	rVB	458	276	0.01%	0.002%
50	7.714	1085	1087	1088	rBV	472	275	0.01%	0.002%
51	7.757	1093	1094	1095	rBV	450	267	0.01%	0.002%
52	7.818	1103	1104	1106	rBV2	337	262	0.01%	0.002%
53	8.202	1165	1167	1170	rBV2	281	300	0.01%	0.002%
54	8.330	1181	1188	1195	rBV2	142573	236707	11.01%	1.881%
55	8.574	1225	1228	1229	rVB3	404	327	0.02%	0.003%
56	8.653	1232	1241	1251	rBV	543366	831974	38.69%	6.610%
57	8.952	1285	1290	1303	rBV	103526	158156	7.36%	1.257%
58	9.122	1317	1318	1322	rBV2	349	335	0.02%	0.003%
59	9.214	1331	1333	1334	rVB2	494	308	0.01%	0.002%
60	9.275	1337	1343	1356	rVV	959343	1435345	66.76%	11.404%
61	9.391	1356	1362	1374	rBV	471956	672561	31.28%	5.343%
62	9.634	1400	1402	1405	rBV2	429	646	0.03%	0.005%
63	9.805	1428	1430	1433	rVB3	466	425	0.02%	0.003%
64	9.854	1435	1438	1440	rBV2	445	413	0.02%	0.003%
65	9.927	1449	1450	1452	rBV2	495	336	0.02%	0.003%
66	10.055	1466	1471	1479	rBV	508813	702074	32.65%	5.578%
67	10.244	1500	1502	1505	rBV	346	382	0.02%	0.003%
68	10.311	1512	1513	1517	rVB2	693	558	0.03%	0.004%
69	10.726	1578	1581	1582	rBV3	413	418	0.02%	0.003%
70	10.805	1592	1594	1596	rBV2	277	263	0.01%	0.002%
71	10.854	1599	1602	1604	rBV2	740	626	0.03%	0.005%
72	10.884	1604	1607	1610	rVV3	638	796	0.04%	0.006%
73	10.909	1610	1611	1614	rVB	537	365	0.02%	0.003%
74	10.939	1614	1616	1618	rBV	340	281	0.01%	0.002%
75	11.000	1624	1626	1627	rBV2	507	274	0.01%	0.002%
76	11.195	1652	1658	1665	rBV	420634	528591	24.58%	4.200%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030447.D
 Acq On : 05 Aug 2022 22:49
 Operator : JC/MD
 Sample : N4066-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E25

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.469	1699	1703	1704	rBV2	723	633	0.03%	0.005%
78	11.597	1722	1724	1725	rBV	344	276	0.01%	0.002%
79	11.701	1737	1741	1742	rBV	401	571	0.03%	0.005%
80	11.853	1765	1766	1768	rVB	404	269	0.01%	0.002%
81	12.024	1789	1794	1801	rVV	524216	624348	29.04%	4.960%
82	12.323	1837	1843	1850	rBV	554292	703969	32.74%	5.593%
83	12.646	1895	1896	1898	rBV	506	283	0.01%	0.002%
84	12.744	1911	1912	1913	rBV	451	272	0.01%	0.002%
85	12.817	1922	1924	1925	rBV	493	287	0.01%	0.002%
86	13.243	1992	1994	1997	rBV2	388	312	0.01%	0.002%
87	13.268	1997	1998	1999	rBV	732	275	0.01%	0.002%
88	13.512	2036	2038	2041	rBV2	383	309	0.01%	0.002%
89	13.591	2049	2051	2052	rBV	419	431	0.02%	0.003%
90	13.817	2085	2088	2089	rBV2	272	345	0.02%	0.003%
91	13.841	2090	2092	2095	rVV	626	443	0.02%	0.004%
92	14.457	2191	2193	2195	rBV2	363	256	0.01%	0.002%
93	14.755	2241	2242	2245	rVB	643	499	0.02%	0.004%
94	14.981	2276	2279	2281	rBV3	762	941	0.04%	0.007%
95	15.152	2305	2307	2308	rBV	752	459	0.02%	0.004%
96	15.200	2313	2315	2317	rBV	413	369	0.02%	0.003%
97	15.383	2344	2345	2348	rBV2	966	989	0.05%	0.008%
98	15.969	2439	2441	2444	rBV2	745	1063	0.05%	0.008%
99	16.225	2481	2483	2486	rBV3	567	465	0.02%	0.004%
100	16.731	2564	2566	2567	rBV2	514	352	0.02%	0.003%




Sum of corrected areas: 12586784

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030447.D
Acq On : 05 Aug 2022 22:49
Operator : JC/MD
Sample : N4066-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

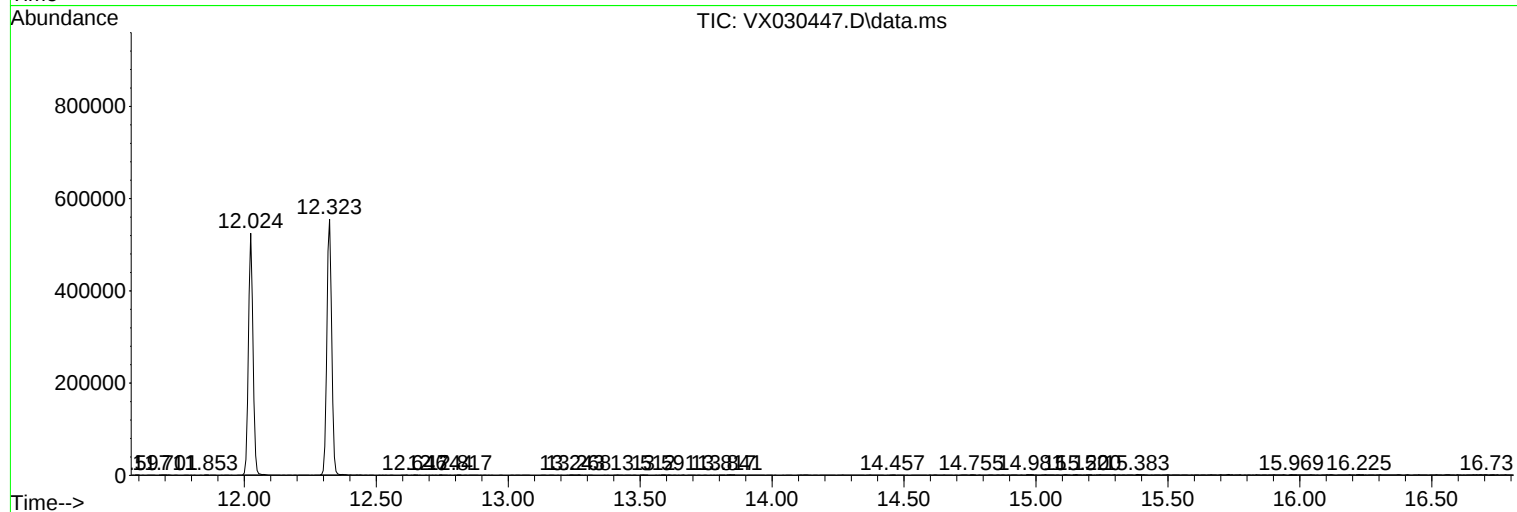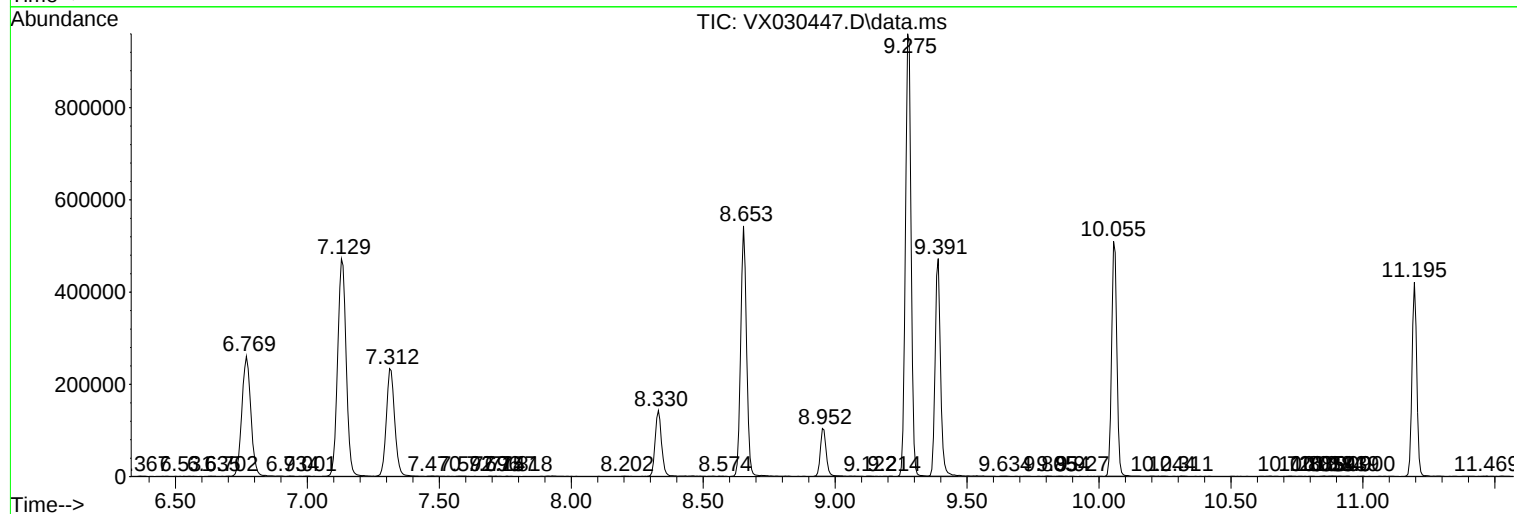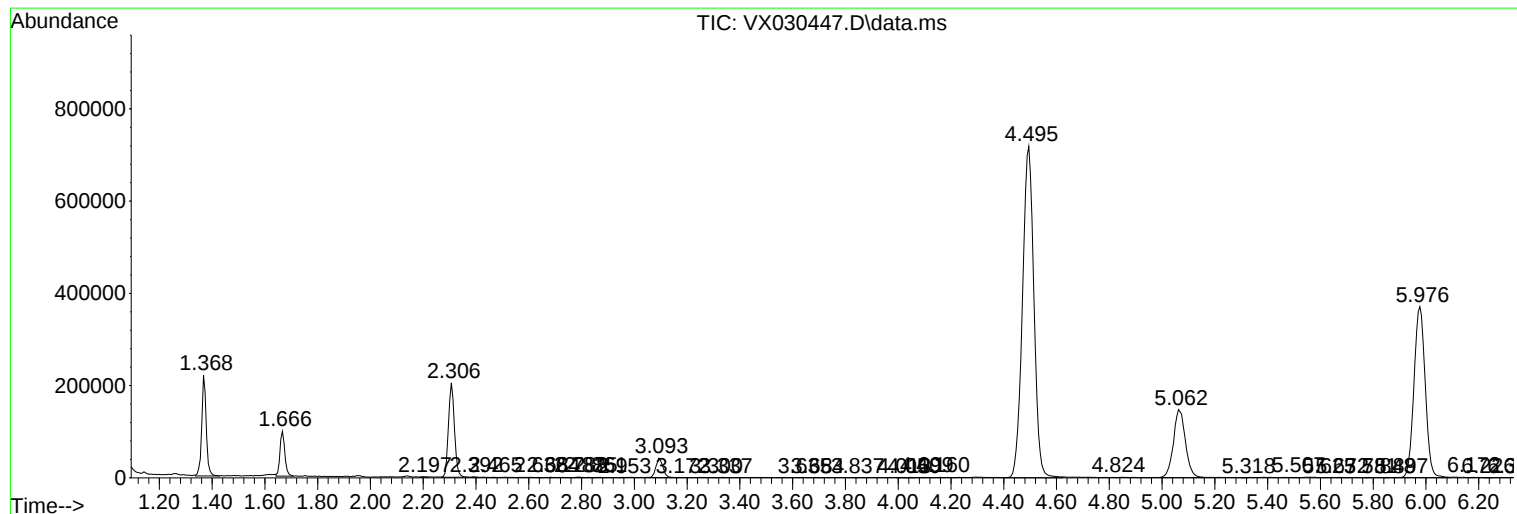

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030447.D
Acq On : 05 Aug 2022 22:49
Operator : JC/MD
Sample : N4066-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030447.D
Acq On : 05 Aug 2022 22:49
Operator : JC/MD
Sample : N4066-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc