

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030448.D
 Acq On : 05 Aug 2022 23:12
 Operator : JC/MD
 Sample : N4066-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030448.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	57	rVB2	332030	384464	2.84%	1.258%
2	1.666	91	95	105	rVB	104221	125355	0.93%	0.410%
3	2.184	178	180	181	rBV2	809	494	0.00%	0.002%
4	2.306	194	200	211	rVB	216829	344499	2.55%	1.127%
5	3.093	320	329	337	rVV	31871	61558	0.46%	0.201%
6	3.312	362	365	366	rBV2	456	418	0.00%	0.001%
7	3.477	390	392	393	rVV	640	434	0.00%	0.001%
8	3.599	410	412	414	rVB	554	389	0.00%	0.001%
9	4.007	477	479	484	rVV2	366	518	0.00%	0.002%
10	4.178	504	507	510	rBV	401	645	0.00%	0.002%
11	4.312	525	529	530	rBV2	546	503	0.00%	0.002%
12	4.495	544	559	583	rBV2	1655839	4559794	33.71%	14.916%
13	4.745	599	600	603	rBV2	724	628	0.00%	0.002%
14	4.964	633	636	637	rBV2	430	411	0.00%	0.001%
15	5.068	641	653	668	rVV	146670	453143	3.35%	1.482%
16	5.373	701	703	704	rVB	614	397	0.00%	0.001%
17	5.397	704	707	710	rBV3	735	1163	0.01%	0.004%
18	5.440	713	714	718	rBV	355	482	0.00%	0.002%
19	5.519	724	727	729	rBV	467	533	0.00%	0.002%
20	5.550	731	732	734	rBV	521	440	0.00%	0.001%
21	5.800	769	773	774	rBV2	502	559	0.00%	0.002%
22	5.885	785	787	789	rBV	569	390	0.00%	0.001%
23	5.976	789	802	819	rBV3	370851	1091188	8.07%	3.569%
24	6.233	842	844	845	rBV	390	375	0.00%	0.001%
25	6.275	848	851	852	rVB2	494	475	0.00%	0.002%
26	6.293	852	854	856	rBV2	382	435	0.00%	0.001%
27	6.348	861	863	866	rBV3	368	572	0.00%	0.002%
28	6.476	882	884	887	rVB2	503	654	0.00%	0.002%
29	6.507	887	889	890	rBV	632	465	0.00%	0.002%
30	6.568	898	899	901	rVV	829	371	0.00%	0.001%
31	6.708	919	922	923	rBV	427	447	0.00%	0.001%
32	6.769	923	932	949	rVV	259321	626844	4.63%	2.051%
33	7.007	969	971	973	rVB	473	364	0.00%	0.001%
34	7.135	981	992	1012	rBV	6252766	13528331	100.00%	44.253%
35	7.312	1014	1021	1037	rVB	230450	518299	3.83%	1.695%
36	7.531	1056	1057	1059	rVB2	932	534	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030448.D
 Acq On : 05 Aug 2022 23:12
 Operator : JC/MD
 Sample : N4066-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.629	1070	1073	1074	rBV	732	747	0.01%	0.002%
38	7.769	1094	1096	1097	rVB2	676	388	0.00%	0.001%
39	7.793	1099	1100	1103	rVV2	422	411	0.00%	0.001%
40	7.842	1107	1108	1110	rBV	631	377	0.00%	0.001%
41	7.940	1120	1124	1125	rVV3	860	1134	0.01%	0.004%
42	7.970	1127	1129	1130	rVB2	1084	575	0.00%	0.002%
43	8.049	1140	1142	1145	rVB3	463	497	0.00%	0.002%
44	8.080	1145	1147	1149	rBV	569	552	0.00%	0.002%
45	8.159	1156	1160	1161	rBV3	367	527	0.00%	0.002%
46	8.281	1176	1180	1182	rBV2	352	545	0.00%	0.002%
47	8.330	1182	1188	1196	rBV	148702	237202	1.75%	0.776%
48	8.476	1210	1212	1214	rVV2	753	601	0.00%	0.002%
49	8.586	1229	1230	1233	rBV	550	375	0.00%	0.001%
50	8.653	1234	1241	1253	rVV	543099	839886	6.21%	2.747%
51	8.830	1268	1270	1275	rVB3	726	735	0.01%	0.002%
52	8.878	1275	1278	1280	rBV2	548	624	0.00%	0.002%
53	8.952	1285	1290	1301	rBV	102592	157286	1.16%	0.515%
54	9.201	1328	1331	1332	rBV2	515	398	0.00%	0.001%
55	9.275	1337	1343	1356	rVV	2908317	4258684	31.48%	13.931%
56	9.390	1356	1362	1376	rVB	467171	679257	5.02%	2.222%
57	9.622	1398	1400	1402	rVB4	947	735	0.01%	0.002%
58	9.659	1402	1406	1408	rBV2	729	1163	0.01%	0.004%
59	9.939	1451	1452	1456	rBV	417	451	0.00%	0.001%
60	10.055	1466	1471	1479	rBV	539613	725351	5.36%	2.373%
61	10.220	1492	1498	1499	rBV4	504	881	0.01%	0.003%
62	10.421	1529	1531	1536	rVB3	397	474	0.00%	0.002%
63	10.476	1539	1540	1542	rBV2	530	418	0.00%	0.001%
64	10.537	1547	1550	1552	rBV	343	457	0.00%	0.001%
65	10.652	1567	1569	1572	rVB2	398	386	0.00%	0.001%
66	10.726	1578	1581	1582	rBV	400	379	0.00%	0.001%
67	11.195	1652	1658	1668	rBV	431212	538832	3.98%	1.763%
68	11.415	1689	1694	1696	rBV3	311	458	0.00%	0.001%
69	11.457	1698	1701	1702	rVV2	544	474	0.00%	0.002%
70	11.530	1711	1713	1715	rBV2	494	577	0.00%	0.002%
71	11.555	1715	1717	1720	rVB	712	504	0.00%	0.002%
72	11.677	1735	1737	1738	rBV2	437	429	0.00%	0.001%
73	11.762	1749	1751	1755	rBV2	579	641	0.00%	0.002%
74	11.799	1755	1757	1760	rBV2	363	379	0.00%	0.001%
75	12.024	1789	1794	1802	rBV	552486	664129	4.91%	2.172%
76	12.152	1814	1815	1819	rBV	744	602	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030448.D
 Acq On : 05 Aug 2022 23:12
 Operator : JC/MD
 Sample : N4066-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.183	1819	1820	1823	rVB2	678	364	0.00%	0.001%
78	12.262	1829	1833	1835	rBV2	453	372	0.00%	0.001%
79	12.323	1837	1843	1851	rVV	582045	731326	5.41%	2.392%
80	12.384	1851	1853	1858	rVB2	1062	1392	0.01%	0.005%
81	12.628	1891	1893	1895	rVV2	498	556	0.00%	0.002%
82	13.097	1969	1970	1972	rVB	760	399	0.00%	0.001%
83	13.304	2001	2004	2005	rBV2	550	385	0.00%	0.001%
84	13.457	2027	2029	2034	rVB3	412	731	0.01%	0.002%
85	13.719	2070	2072	2076	rVB2	429	478	0.00%	0.002%
86	13.774	2078	2081	2085	rVV4	605	1028	0.01%	0.003%
87	13.829	2088	2090	2092	rVB2	879	619	0.00%	0.002%
88	13.914	2101	2104	2105	rBV2	466	480	0.00%	0.002%
89	13.999	2114	2118	2122	rBV3	391	705	0.01%	0.002%
90	14.060	2125	2128	2132	rBV	451	818	0.01%	0.003%
91	14.219	2152	2154	2156	rBV	482	407	0.00%	0.001%
92	14.268	2159	2162	2164	rBV2	388	493	0.00%	0.002%
93	14.353	2174	2176	2177	rBV	697	381	0.00%	0.001%
94	14.444	2189	2191	2193	rBV2	543	482	0.00%	0.002%
95	14.914	2265	2268	2270	rBV3	648	710	0.01%	0.002%
96	14.938	2270	2272	2273	rVB2	607	360	0.00%	0.001%
97	15.091	2295	2297	2301	rBV4	895	1082	0.01%	0.004%
98	15.475	2358	2360	2362	rBV2	684	553	0.00%	0.002%
99	15.615	2381	2383	2384	rBV	645	467	0.00%	0.002%
100	16.761	2568	2571	2572	rBV2	584	614	0.00%	0.002%




Sum of corrected areas: 30570294

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030448.D
Acq On : 05 Aug 2022 23:12
Operator : JC/MD
Sample : N4066-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

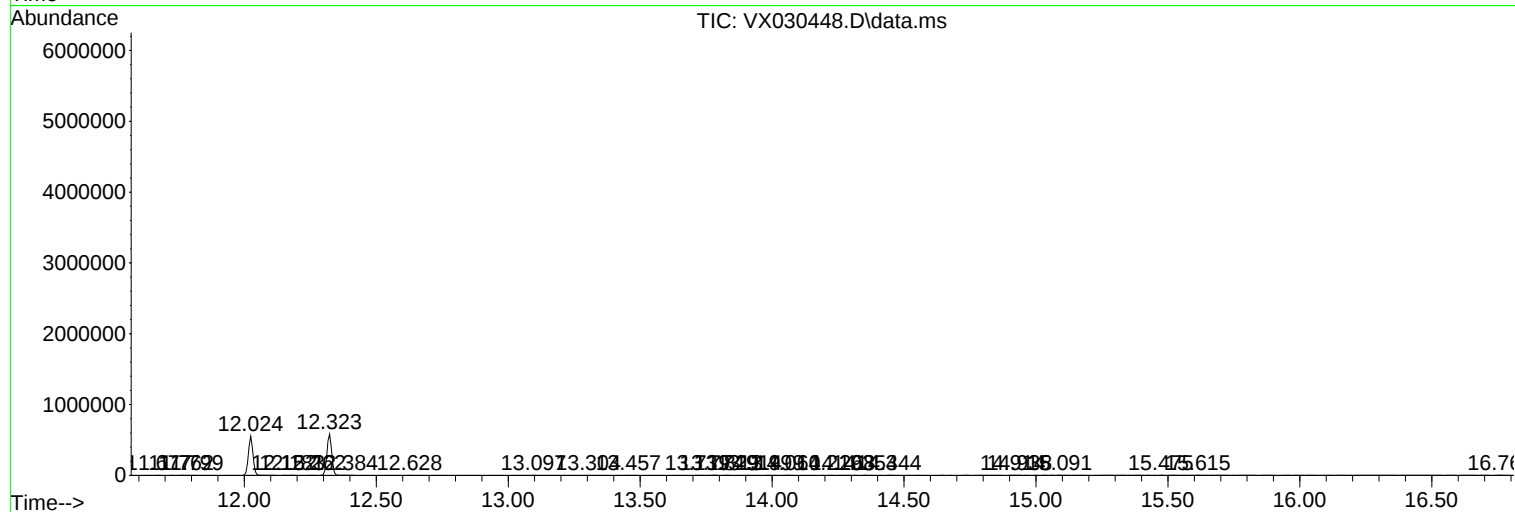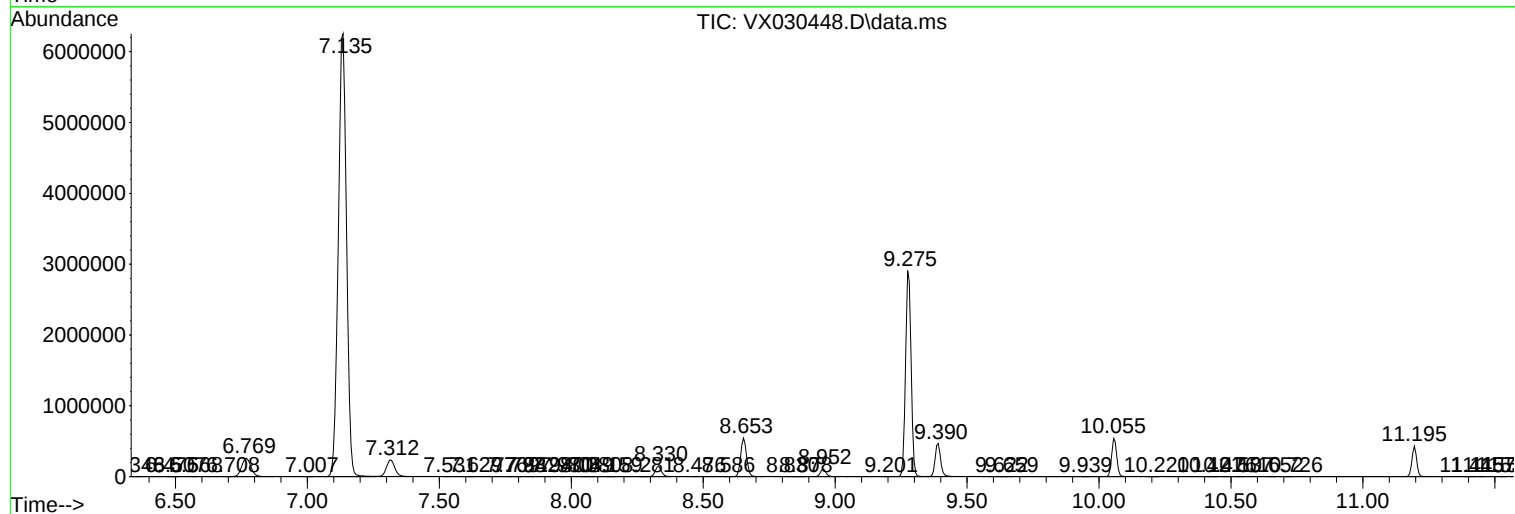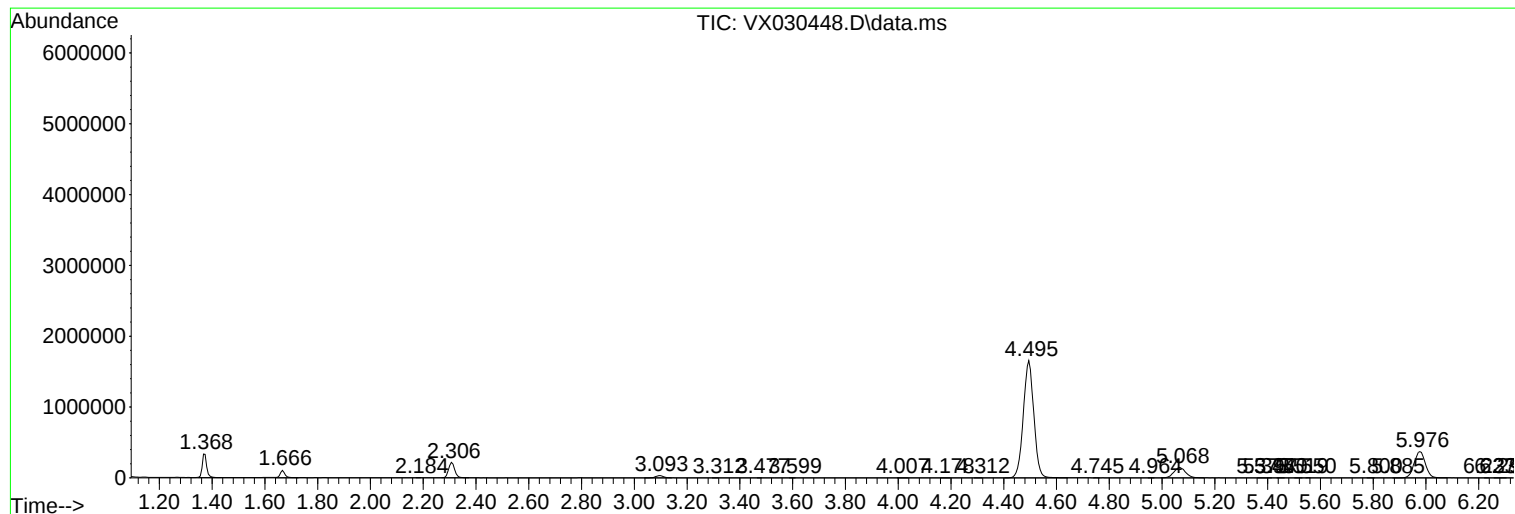

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030448.D
Acq On : 05 Aug 2022 23:12
Operator : JC/MD
Sample : N4066-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030448.D
Acq On : 05 Aug 2022 23:12
Operator : JC/MD
Sample : N4066-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------