

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030449.D
 Acq On : 05 Aug 2022 23:36
 Operator : JC/MD
 Sample : N4066-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030449.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	55	rVB2	307604	365050	2.70%	1.197%
2	1.666	91	95	106	rVB	105215	126284	0.93%	0.414%
3	2.306	194	200	212	rVB	202993	326395	2.41%	1.071%
4	2.459	223	225	227	rBV	512	449	0.00%	0.001%
5	2.532	236	237	239	rBV2	490	313	0.00%	0.001%
6	2.636	252	254	256	rBV	500	325	0.00%	0.001%
7	2.678	260	261	264	rBV2	501	359	0.00%	0.001%
8	2.782	276	278	283	rVB2	819	940	0.01%	0.003%
9	3.093	321	329	337	rBV	31998	59929	0.44%	0.197%
10	3.196	344	346	347	rVB	478	279	0.00%	0.001%
11	3.227	347	351	353	rBV2	430	523	0.00%	0.002%
12	3.410	378	381	385	rVB	400	391	0.00%	0.001%
13	3.471	389	391	394	rVB3	391	376	0.00%	0.001%
14	3.617	413	415	418	rBV	537	472	0.00%	0.002%
15	3.660	420	422	423	rVB	528	297	0.00%	0.001%
16	3.745	433	436	439	rBV2	343	356	0.00%	0.001%
17	3.794	443	444	448	rVB2	411	417	0.00%	0.001%
18	3.837	448	451	454	rBV	373	586	0.00%	0.002%
19	3.916	463	464	468	rVV2	339	378	0.00%	0.001%
20	3.995	475	477	478	rVB2	466	284	0.00%	0.001%
21	4.007	478	479	484	rBV2	379	484	0.00%	0.002%
22	4.044	484	485	488	rBV2	446	489	0.00%	0.002%
23	4.099	492	494	495	rBV	410	264	0.00%	0.001%
24	4.117	495	497	500	rVB2	377	349	0.00%	0.001%
25	4.495	546	559	576	rBV2	1551694	4407731	32.54%	14.459%
26	5.068	639	653	670	rBV	142338	452815	3.34%	1.485%
27	5.184	670	672	674	rVV2	692	494	0.00%	0.002%
28	5.221	676	678	681	rBV2	772	563	0.00%	0.002%
29	5.349	697	699	701	rBV2	322	346	0.00%	0.001%
30	5.495	718	723	726	rBV4	810	1097	0.01%	0.004%
31	5.562	729	734	739	rVV3	562	1431	0.01%	0.005%
32	5.659	748	750	753	rVB2	454	430	0.00%	0.001%
33	5.714	757	759	761	rBV2	563	554	0.00%	0.002%
34	5.848	777	781	782	rBV2	473	411	0.00%	0.001%
35	5.976	789	802	818	rBV2	370924	1084162	8.00%	3.556%
36	6.202	838	839	841	rBV	444	370	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030449.D
 Acq On : 05 Aug 2022 23:36
 Operator : JC/MD
 Sample : N4066-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.239	843	845	847	rVV	482	437	0.00%	0.001%
38	6.342	859	862	863	rBV	548	548	0.00%	0.002%
39	6.623	906	908	910	rVB	443	273	0.00%	0.001%
40	6.769	922	932	947	rBV	263240	630852	4.66%	2.069%
41	6.934	958	959	961	rBV2	349	277	0.00%	0.001%
42	7.037	972	976	981	rBV2	548	962	0.01%	0.003%
43	7.135	981	992	1012	rBV	6419915	13544102	100.00%	44.429%
44	7.318	1014	1022	1036	rVB	229360	511449	3.78%	1.678%
45	7.616	1069	1071	1072	rBV2	571	402	0.00%	0.001%
46	7.897	1115	1117	1119	rVV	311	285	0.00%	0.001%
47	8.001	1132	1134	1136	rBV2	322	357	0.00%	0.001%
48	8.330	1181	1188	1198	rVV	146326	239365	1.77%	0.785%
49	8.482	1210	1213	1215	rBV3	465	502	0.00%	0.002%
50	8.653	1234	1241	1250	rBV	547307	829205	6.12%	2.720%
51	8.854	1272	1274	1276	rBV2	431	398	0.00%	0.001%
52	8.952	1285	1290	1299	rBV	103702	157754	1.16%	0.517%
53	9.153	1322	1323	1325	rBV	485	304	0.00%	0.001%
54	9.275	1337	1343	1356	rBV	2938645	4340772	32.05%	14.239%
55	9.390	1356	1362	1375	rVB	470350	664983	4.91%	2.181%
56	9.762	1421	1423	1426	rVB2	594	553	0.00%	0.002%
57	9.939	1450	1452	1453	rBV2	606	482	0.00%	0.002%
58	10.000	1459	1462	1463	rVB	396	278	0.00%	0.001%
59	10.055	1465	1471	1486	rVV	548216	736145	5.44%	2.415%
60	10.445	1533	1535	1537	rBV	401	320	0.00%	0.001%
61	10.604	1559	1561	1564	rBV2	498	454	0.00%	0.001%
62	10.787	1589	1591	1592	rBV	586	428	0.00%	0.001%
63	10.829	1595	1598	1599	rBV2	595	546	0.00%	0.002%
64	11.085	1636	1640	1641	rBV	476	679	0.01%	0.002%
65	11.195	1652	1658	1671	rVB	424837	533747	3.94%	1.751%
66	11.427	1695	1696	1699	rVB2	360	316	0.00%	0.001%
67	11.469	1699	1703	1704	rBV2	435	588	0.00%	0.002%
68	11.530	1712	1713	1716	rVB2	478	352	0.00%	0.001%
69	11.683	1734	1738	1740	rBV	565	816	0.01%	0.003%
70	11.799	1754	1757	1760	rBV2	395	735	0.01%	0.002%
71	11.957	1781	1783	1786	rBV2	356	326	0.00%	0.001%
72	12.024	1789	1794	1804	rVB	560979	695560	5.14%	2.282%
73	12.207	1823	1824	1826	rBV2	664	392	0.00%	0.001%
74	12.323	1837	1843	1855	rBV	585459	739323	5.46%	2.425%
75	12.573	1882	1884	1885	rBV	414	297	0.00%	0.001%
76	12.664	1897	1899	1900	rBV	423	353	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030449.D
 Acq On : 05 Aug 2022 23:36
 Operator : JC/MD
 Sample : N4066-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	13.006	1951	1955	1958	rVB3	474	638	0.00%	0.002%
78	13.067	1963	1965	1967	rBV2	339	279	0.00%	0.001%
79	13.146	1976	1978	1979	rBV	389	276	0.00%	0.001%
80	13.457	2026	2029	2030	rBV	361	335	0.00%	0.001%
81	13.524	2039	2040	2043	rVB2	471	411	0.00%	0.001%
82	13.554	2043	2045	2048	rBV2	251	307	0.00%	0.001%
83	13.591	2050	2051	2053	rBV2	555	399	0.00%	0.001%
84	13.719	2070	2072	2075	rBV2	615	600	0.00%	0.002%
85	13.804	2084	2086	2087	rBV	521	329	0.00%	0.001%
86	13.847	2091	2093	2096	rVB	515	278	0.00%	0.001%
87	14.024	2120	2122	2124	rVB2	478	269	0.00%	0.001%
88	14.066	2127	2129	2132	rBV2	643	802	0.01%	0.003%
89	14.097	2132	2134	2137	rBV	374	507	0.00%	0.002%
90	14.140	2139	2141	2145	rVB2	428	333	0.00%	0.001%
91	14.170	2145	2146	2149	rVB2	561	364	0.00%	0.001%
92	14.213	2149	2153	2154	rBV3	647	635	0.00%	0.002%
93	14.457	2189	2193	2194	rBV2	660	658	0.00%	0.002%
94	14.694	2230	2232	2235	rBV3	718	838	0.01%	0.003%
95	14.890	2262	2264	2266	rBV3	609	669	0.00%	0.002%
96	15.280	2326	2328	2331	rBV4	535	634	0.00%	0.002%
97	15.389	2344	2346	2351	rBV3	642	993	0.01%	0.003%
98	15.487	2361	2362	2365	rBV2	931	915	0.01%	0.003%
99	15.883	2425	2427	2429	rVB	704	303	0.00%	0.001%
100	16.475	2522	2524	2527	rBV2	636	618	0.00%	0.002%




Sum of corrected areas: 30484700

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030449.D
Acq On : 05 Aug 2022 23:36
Operator : JC/MD
Sample : N4066-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

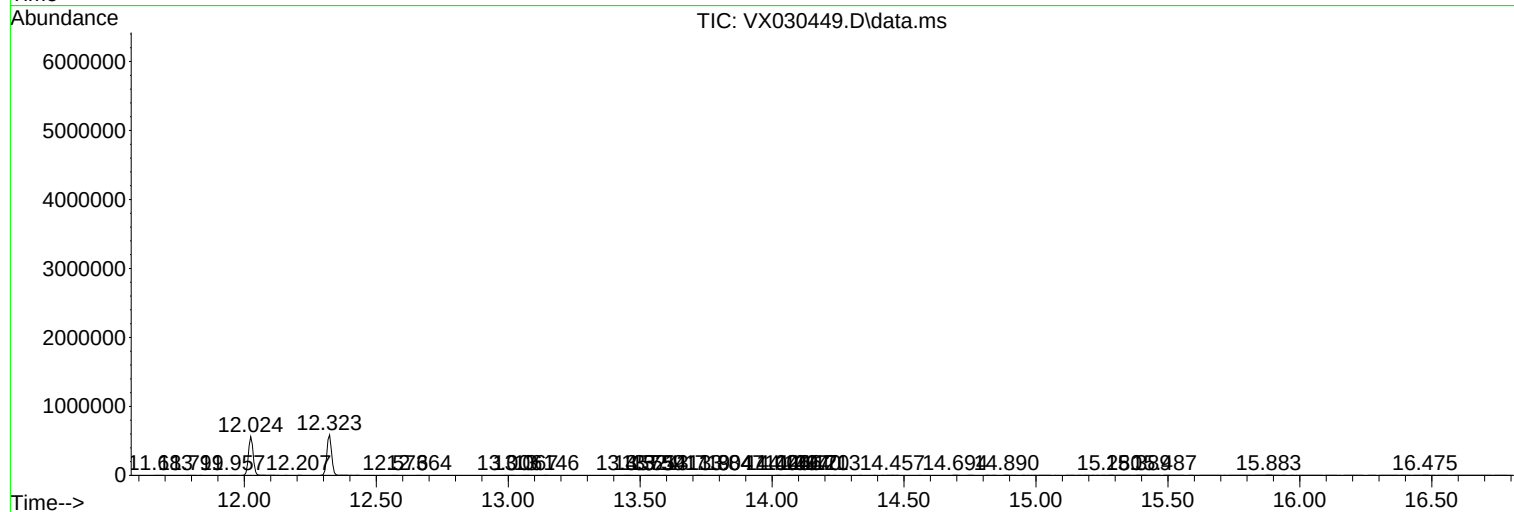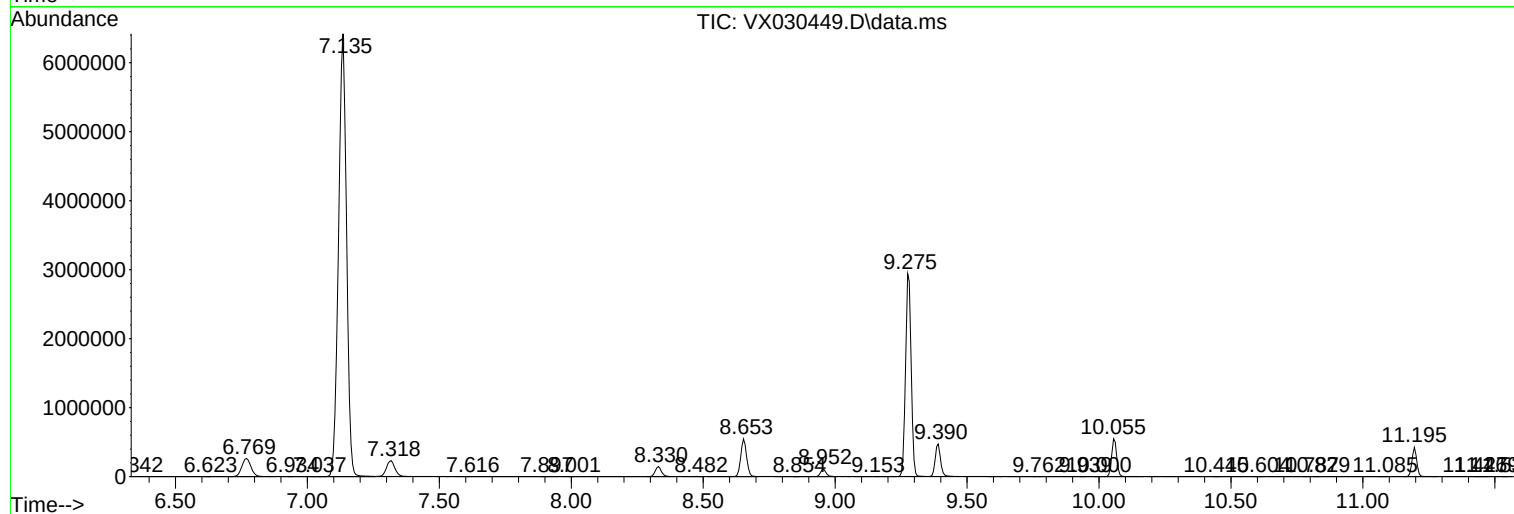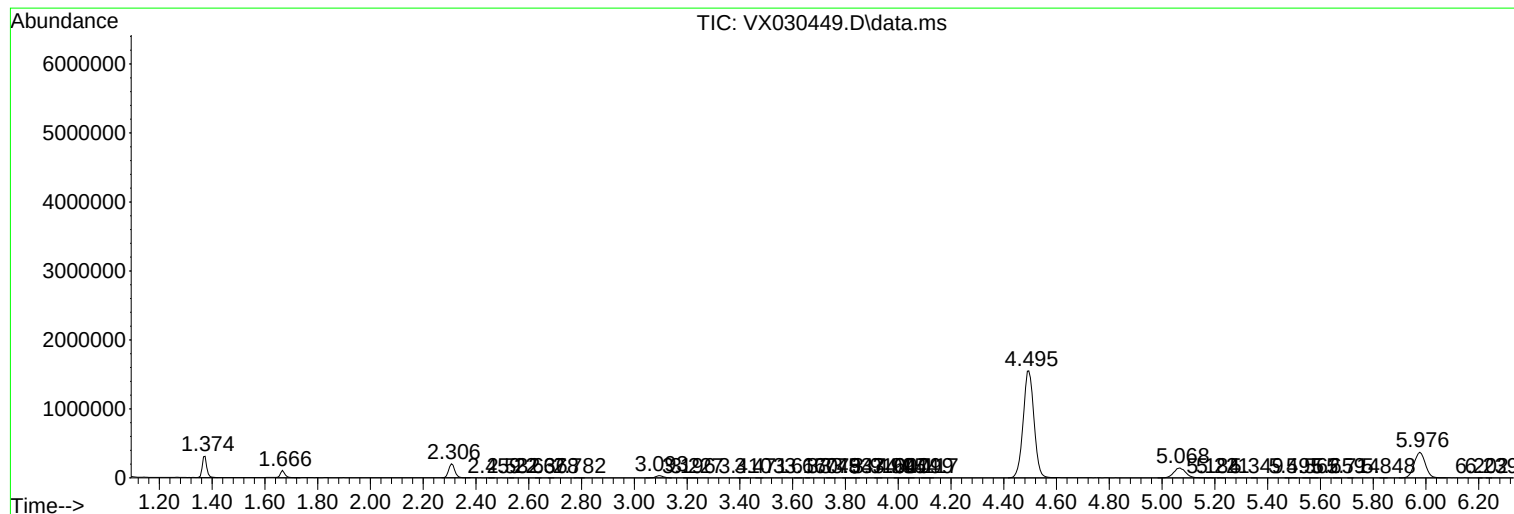

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030449.D
Acq On : 05 Aug 2022 23:36
Operator : JC/MD
Sample : N4066-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030449.D
Acq On : 05 Aug 2022 23:36
Operator : JC/MD
Sample : N4066-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc