


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030416.D
 Acq On : 05 Aug 2022 08:08
 Operator : JC/MD
 Sample : BFB671
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB671

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM080422WMA.M
 Title : VOC Analysis
 Last Update : Sat Aug 06 02:08:42 2022

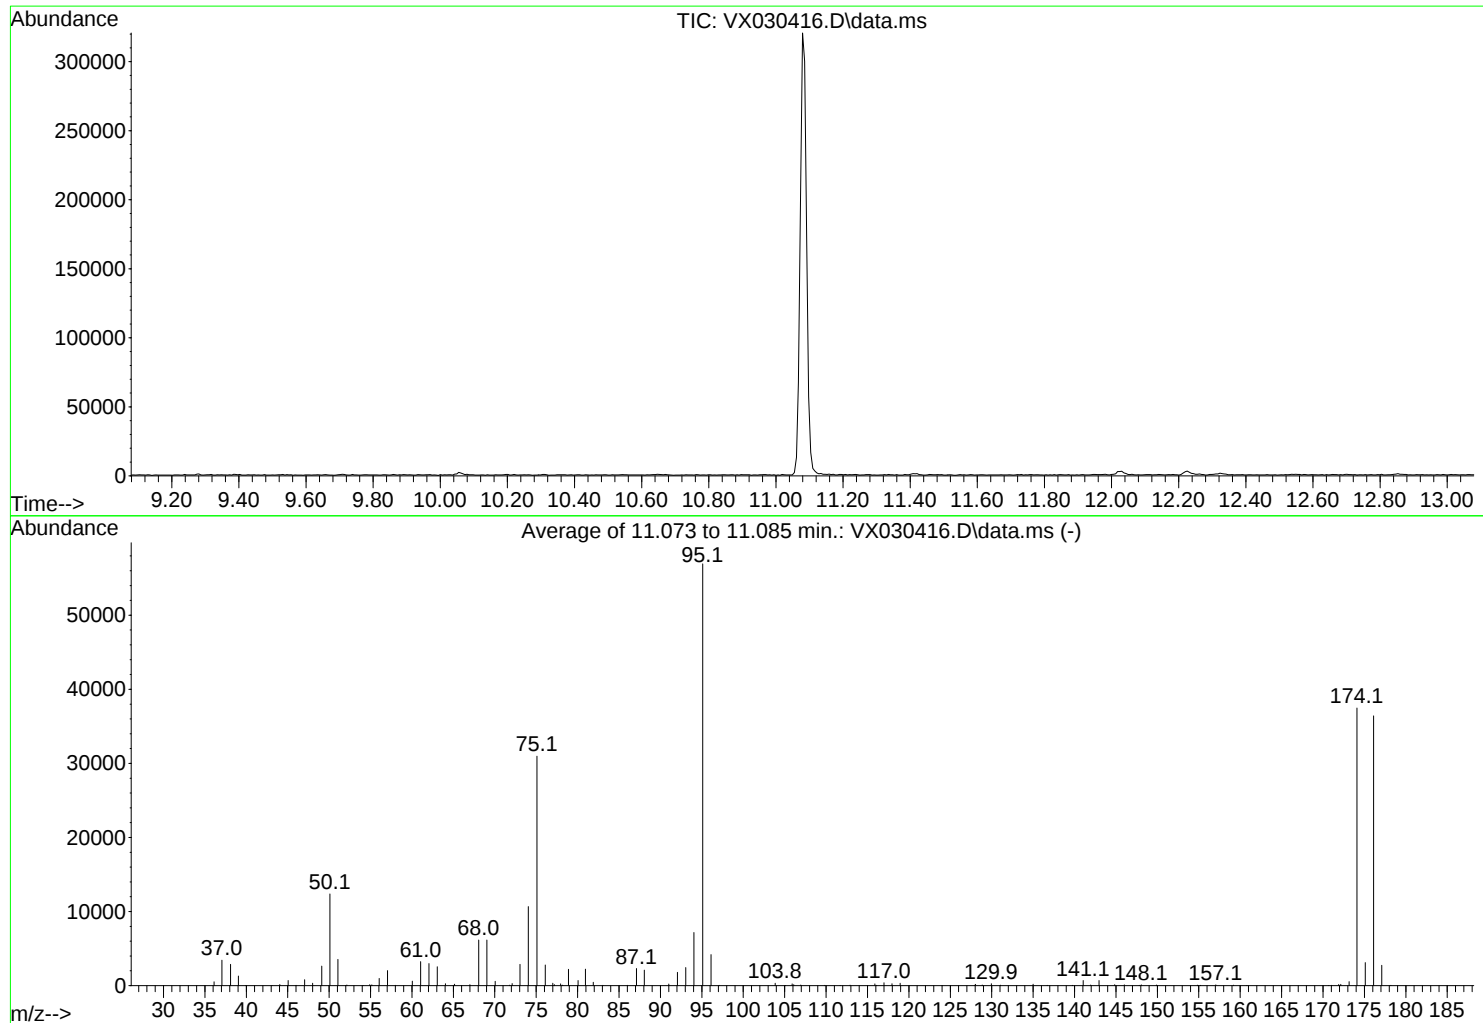

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	12366	PASS
75	95	30	80	54.4	30971	PASS
95	95	100	100	100.0	56933	PASS
96	95	5	9	7.3	4184	PASS
173	174	0.00	2	1.4	532	PASS
174	95	50	120	65.8	37464	PASS
175	174	5	9	8.3	3102	PASS
176	174	95	101	97.2	36419	PASS
177	176	5	9	7.5	2739	PASS

m/z	Abundance
39.90	331.0
44.00	367.0

Instrument :
MSVOA_X
ClientSampleId :
BFB671

m/z	Abundance
36.10	394.0
37.00	3206.0
38.10	2606.0
39.10	981.0
40.00	276.0
43.10	85.0
44.10	538.0
45.00	644.0
47.10	547.0
47.90	320.0
49.10	2341.0
50.10	9343.0
51.10	2666.0
52.00	85.0
55.20	86.0
56.00	814.0
57.00	1624.0
60.10	527.0
61.10	2938.0
62.10	2216.0
63.10	2188.0
64.00	189.0
65.00	130.0
68.10	4486.0
69.00	4417.0
70.10	487.0
71.80	203.0
72.20	186.0
73.10	2099.0
74.10	8733.0
75.10	23696.0
76.10	2197.0
77.00	435.0
78.00	270.0
78.90	1872.0
80.00	497.0
81.00	1639.0
81.90	371.0
86.00	68.0
87.10	1595.0
88.10	1497.0
91.00	217.0
92.00	1622.0
93.10	2081.0
94.00	5292.0
95.10	41624.0
96.10	3635.0
103.80	284.0
105.90	279.0
107.00	106.0
109.90	78.0
115.80	98.0
116.10	110.0
117.00	232.0
117.90	199.0
119.00	218.0
127.90	169.0
130.00	135.0
135.00	129.0
136.70	76.0
139.80	72.0
141.10	434.0
143.00	479.0
144.80	120.0
145.90	83.0
147.80	142.0
149.90	126.0
154.90	113.0
157.10	125.0
172.30	167.0
173.20	377.0
174.10	23296.0
175.10	1770.0
176.10	23312.0
177.10	1668.0

Instrument :
MSVOA_X
ClientSampleId :
BFB671

m/z	Abundance
36.00	531.0
37.10	3899.0
38.10	3271.0
39.10	1692.0
40.10	416.0
44.00	628.0
45.00	740.0
46.10	58.0
47.00	962.0
48.00	371.0
49.10	2799.0
50.10	14829.0
51.00	4554.0
52.20	147.0
54.10	51.0
54.90	360.0
56.10	1180.0
57.10	2391.0
60.00	566.0
61.10	3702.0
62.00	3593.0
63.10	2946.0
64.10	262.0
65.20	258.0
66.00	54.0
67.00	93.0
68.00	7719.0
69.10	8215.0
70.00	865.0
72.10	292.0
73.00	3628.0
74.00	12467.0
75.10	36720.0
76.10	3220.0
77.00	540.0
77.90	432.0
78.90	2520.0
79.90	515.0
80.10	508.0
80.90	2485.0
81.80	521.0
83.00	59.0
86.00	97.0
87.10	2671.0
88.10	2763.0
90.90	185.0
92.10	2165.0
93.00	2604.0
94.10	8673.0
95.10	66440.0
96.10	4924.0
97.10	58.0
103.90	309.0
105.90	458.0
107.00	83.0
109.80	54.0
111.70	56.0
112.90	107.0
115.90	295.0
117.00	558.0
118.00	270.0
118.90	426.0
124.00	69.0
128.10	292.0
128.90	91.0
130.00	272.0
131.00	68.0
135.00	292.0
136.70	73.0
139.70	66.0
141.00	793.0
142.00	157.0
143.00	898.0
144.90	136.0
146.00	133.0
148.00	145.0
149.90	56.0
154.80	80.0
157.00	125.0
159.20	65.0
160.80	51.0
170.70	75.0
171.00	56.0
172.10	336.0
173.10	535.0
174.10	43680.0
175.10	3498.0
176.10	41096.0
177.10	3350.0

Instrument :
MSVOA_X
ClientSampleId :
BFB671

m/z	Abundance
36.20	610.0
37.10	3184.0
38.10	2733.0
39.00	1226.0
40.00	346.0
44.20	395.0
45.10	700.0
45.90	75.0
47.00	906.0
48.10	301.0
49.10	2745.0
50.10	12926.0
51.00	3431.0
52.10	144.0
55.10	254.0
56.10	940.0
57.10	2064.0
58.00	107.0
60.10	729.0
61.00	3100.0
62.10	3114.0
63.00	2524.0
64.10	360.0
65.10	349.0
67.00	290.0
68.00	6272.0
69.00	5849.0
70.00	394.0
72.00	340.0
73.00	2882.0
74.00	10783.0
75.10	32496.0
76.10	2950.0
77.20	418.0
78.20	223.0
78.90	2225.0
80.10	548.0
81.00	2552.0
82.00	467.0
83.10	58.0
87.10	2651.0
88.00	2048.0
91.10	217.0
92.10	1617.0
93.10	2653.0
94.00	7570.0
95.10	62736.0
96.10	3994.0
97.10	99.0
103.90	350.0
105.10	52.0
106.10	419.0
106.90	66.0
112.90	69.0
115.90	339.0
117.00	390.0
118.00	299.0
118.90	348.0
128.00	203.0
128.80	161.0
129.90	348.0
131.10	103.0
135.00	171.0
141.00	854.0
141.90	126.0
142.90	693.0
144.90	158.0
146.10	93.0
148.10	158.0
149.90	65.0
155.20	131.0
157.00	71.0
159.20	121.0
171.10	87.0
171.90	489.0
173.10	684.0
174.10	45416.0
175.10	4039.0
176.10	44848.0
177.10	3199.0
178.20	113.0

Instrument :
MSVOA_X
ClientSampleId :
BFB671