



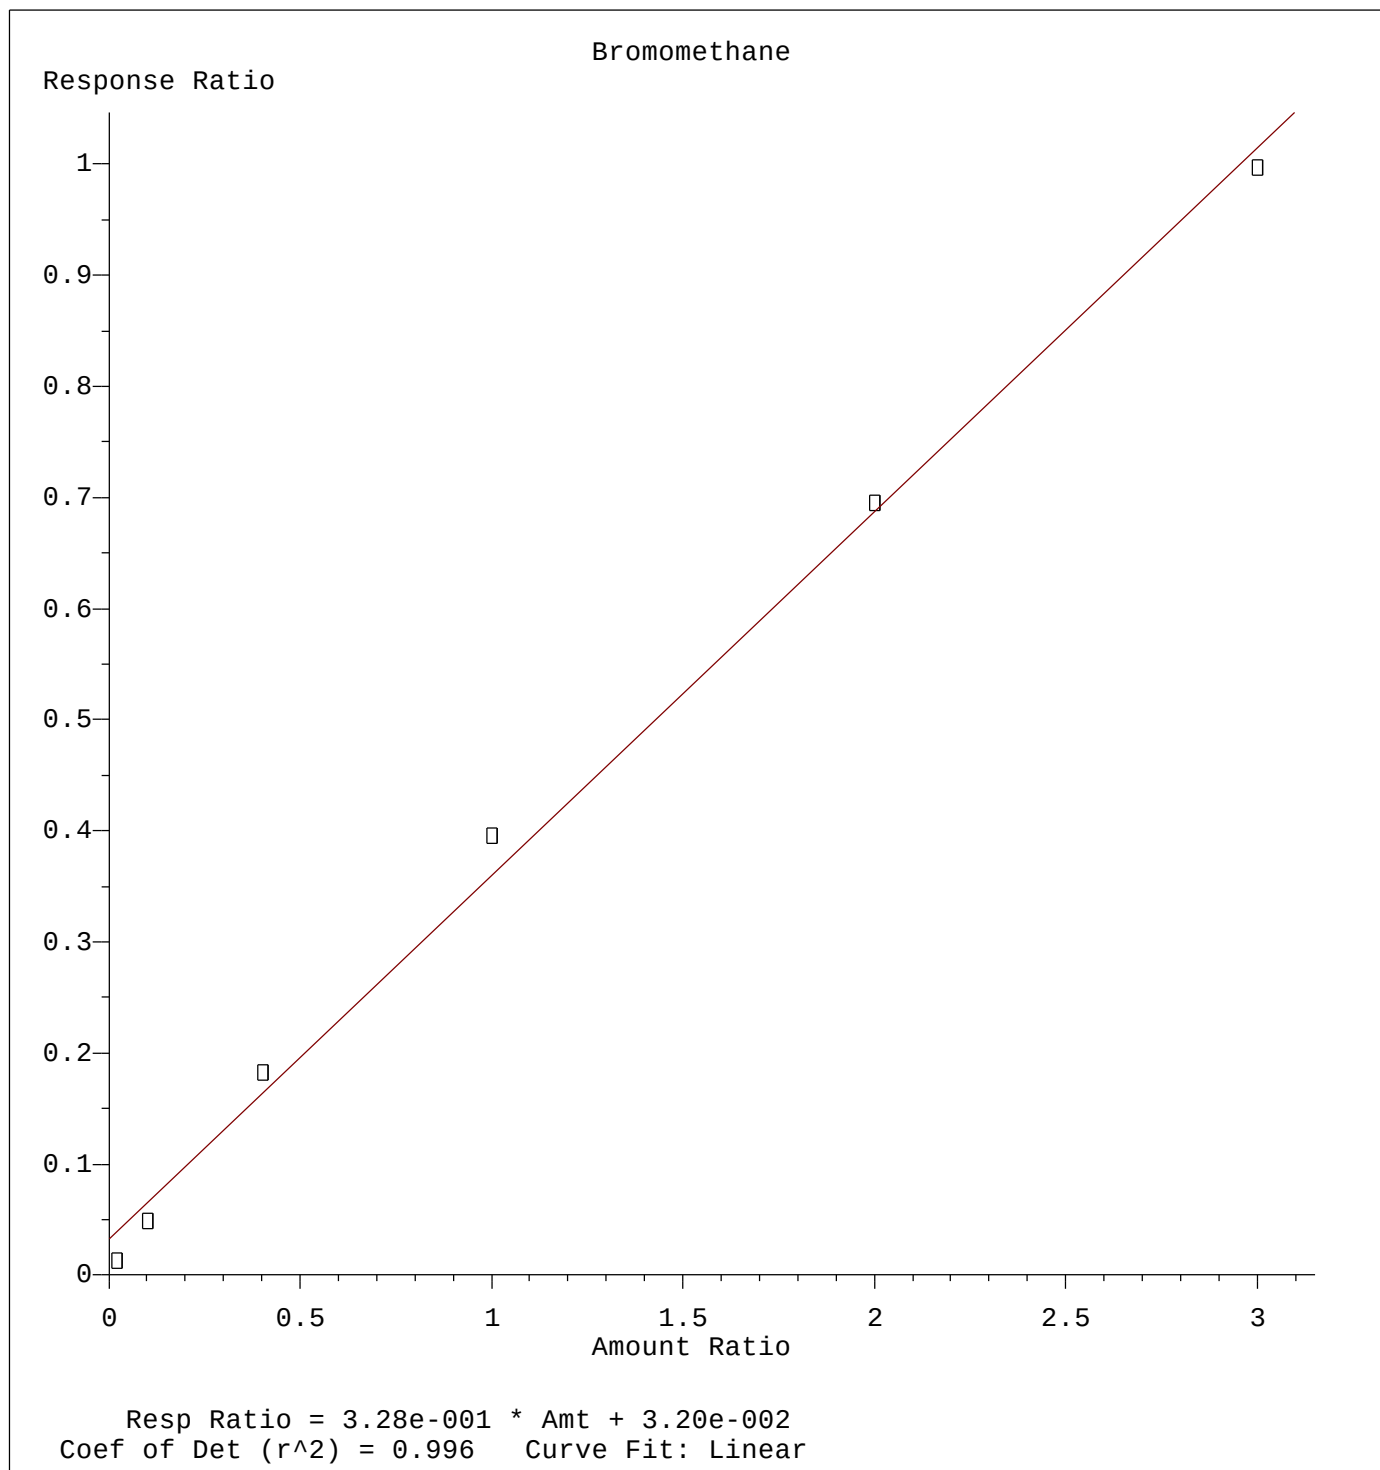

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080618W.M
Calibration Table Last Updated: Tue Aug 07 07:45:48 2018


Acrolein

Response Ratio

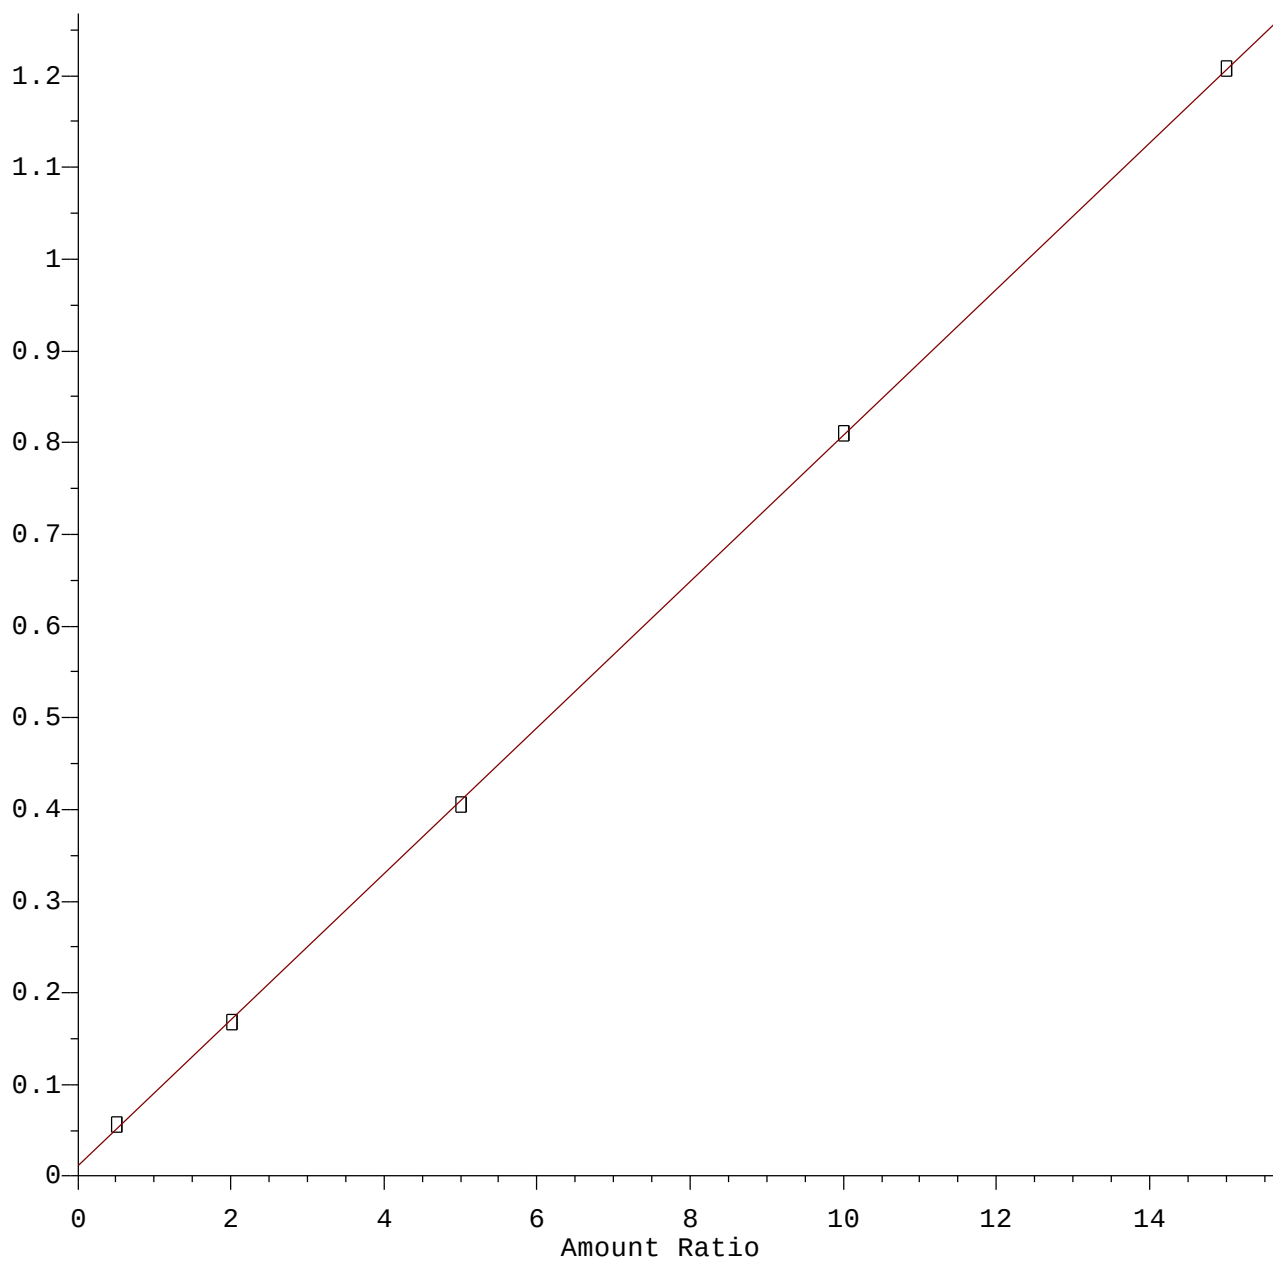


Resp Ratio = 7.97e-002 * Amt + 1.11e-002
Coef of Det (r²) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080618W.M
Calibration Table Last Updated: Tue Aug 07 07:45:48 2018

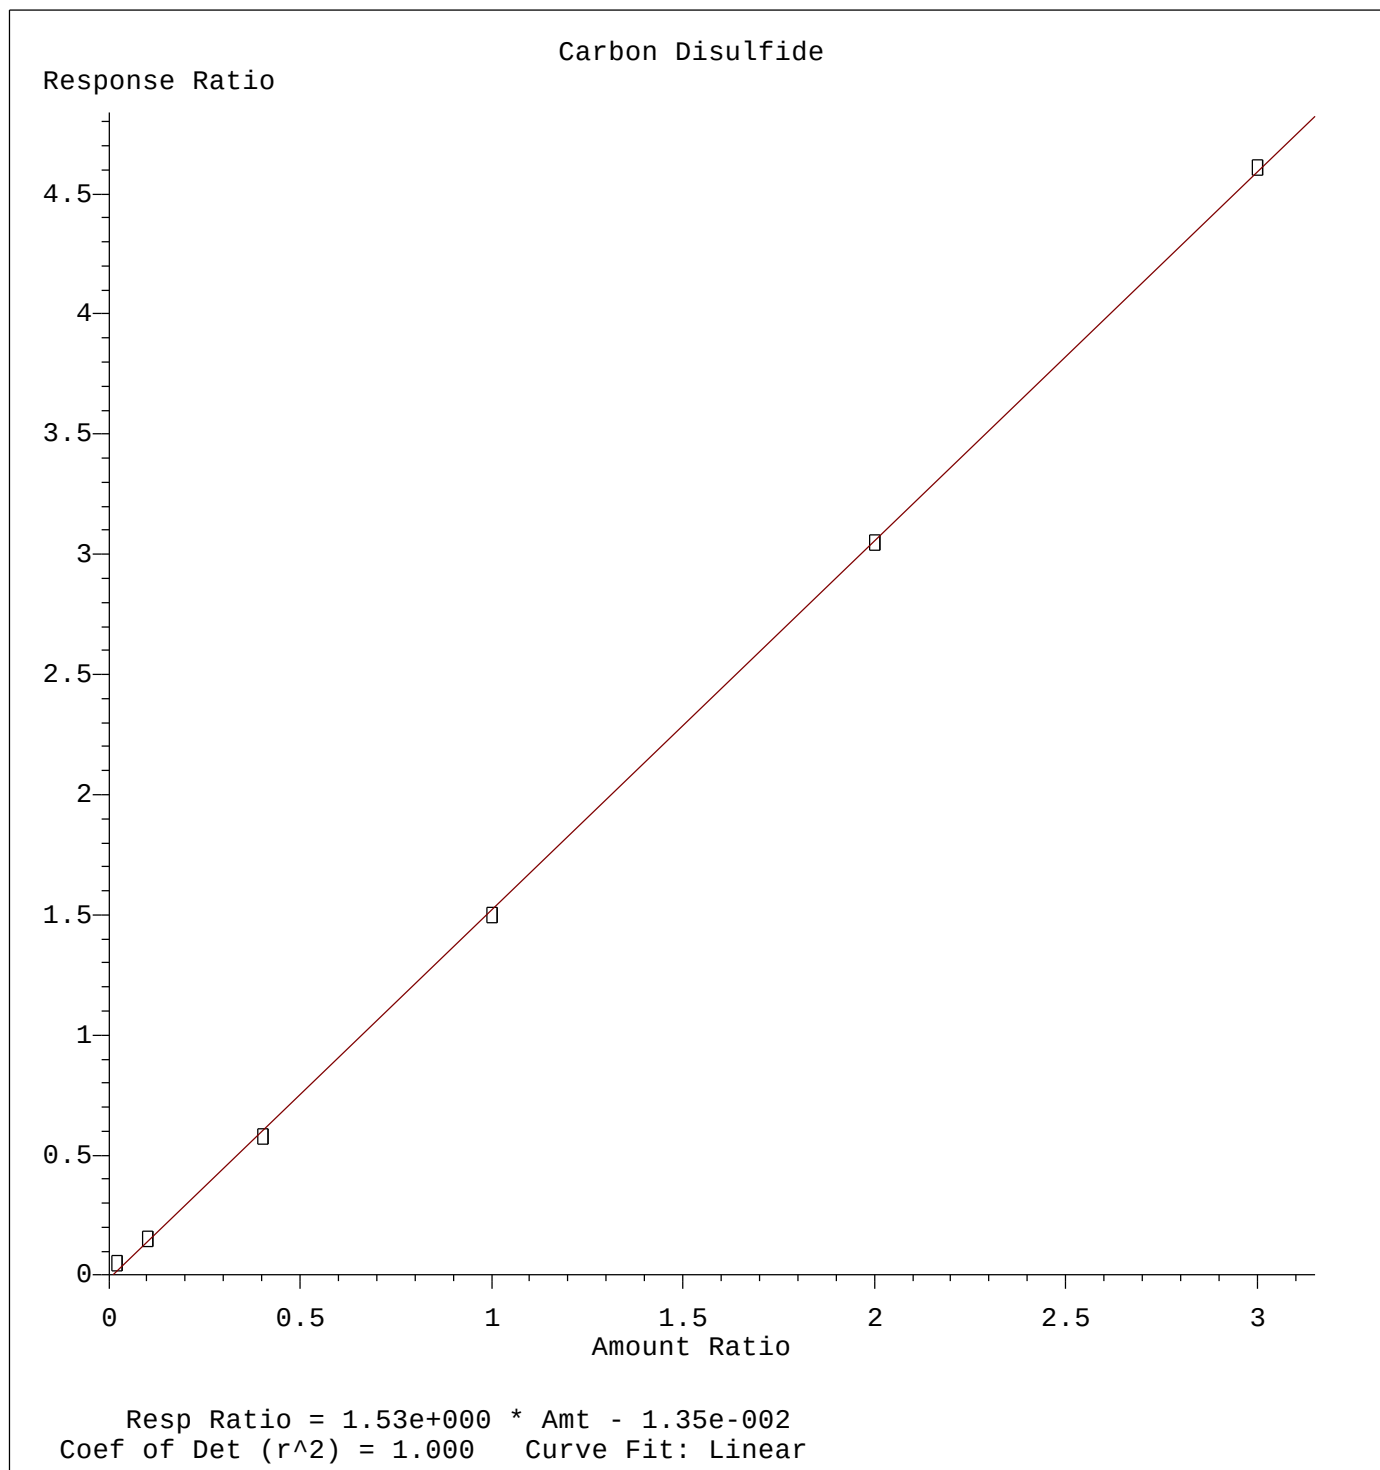

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080618W.M
Calibration Table Last Updated: Tue Aug 07 07:45:48 2018

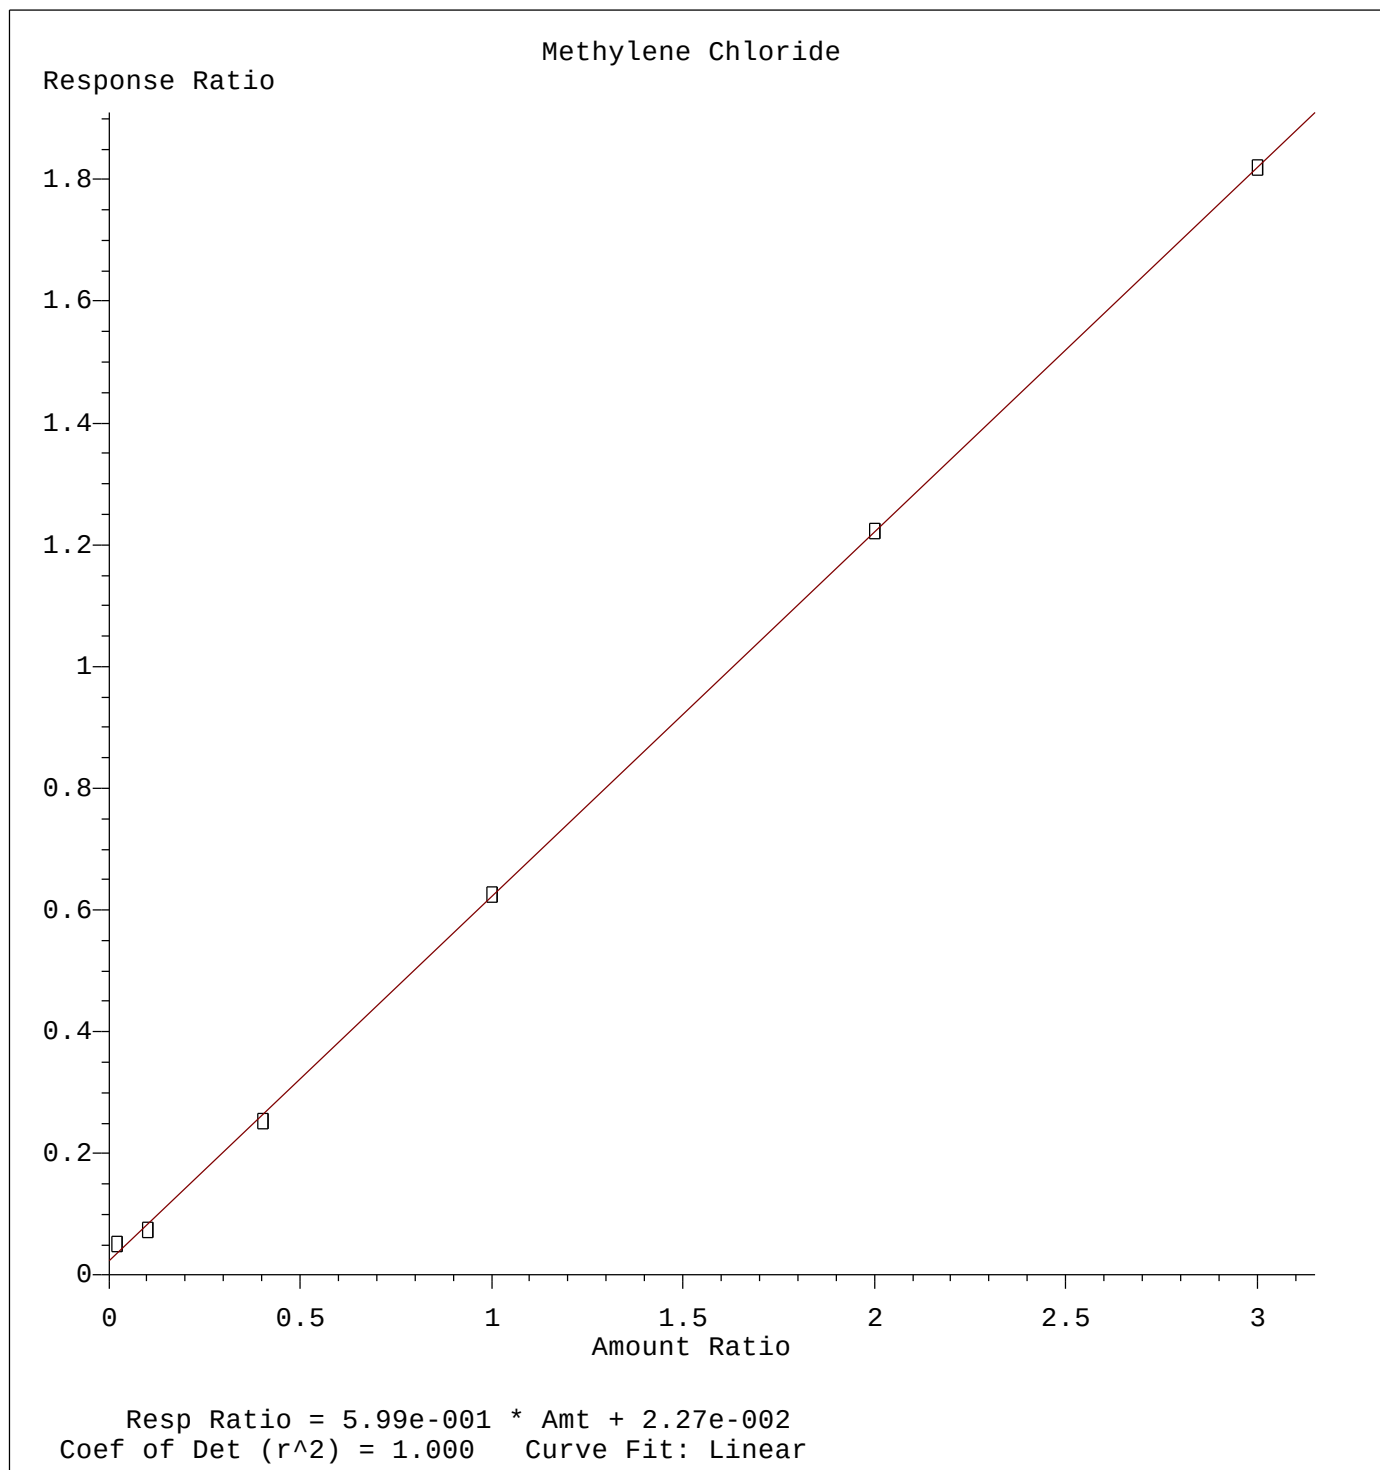


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080618W.M
Calibration Table Last Updated: Tue Aug 07 07:45:48 2018

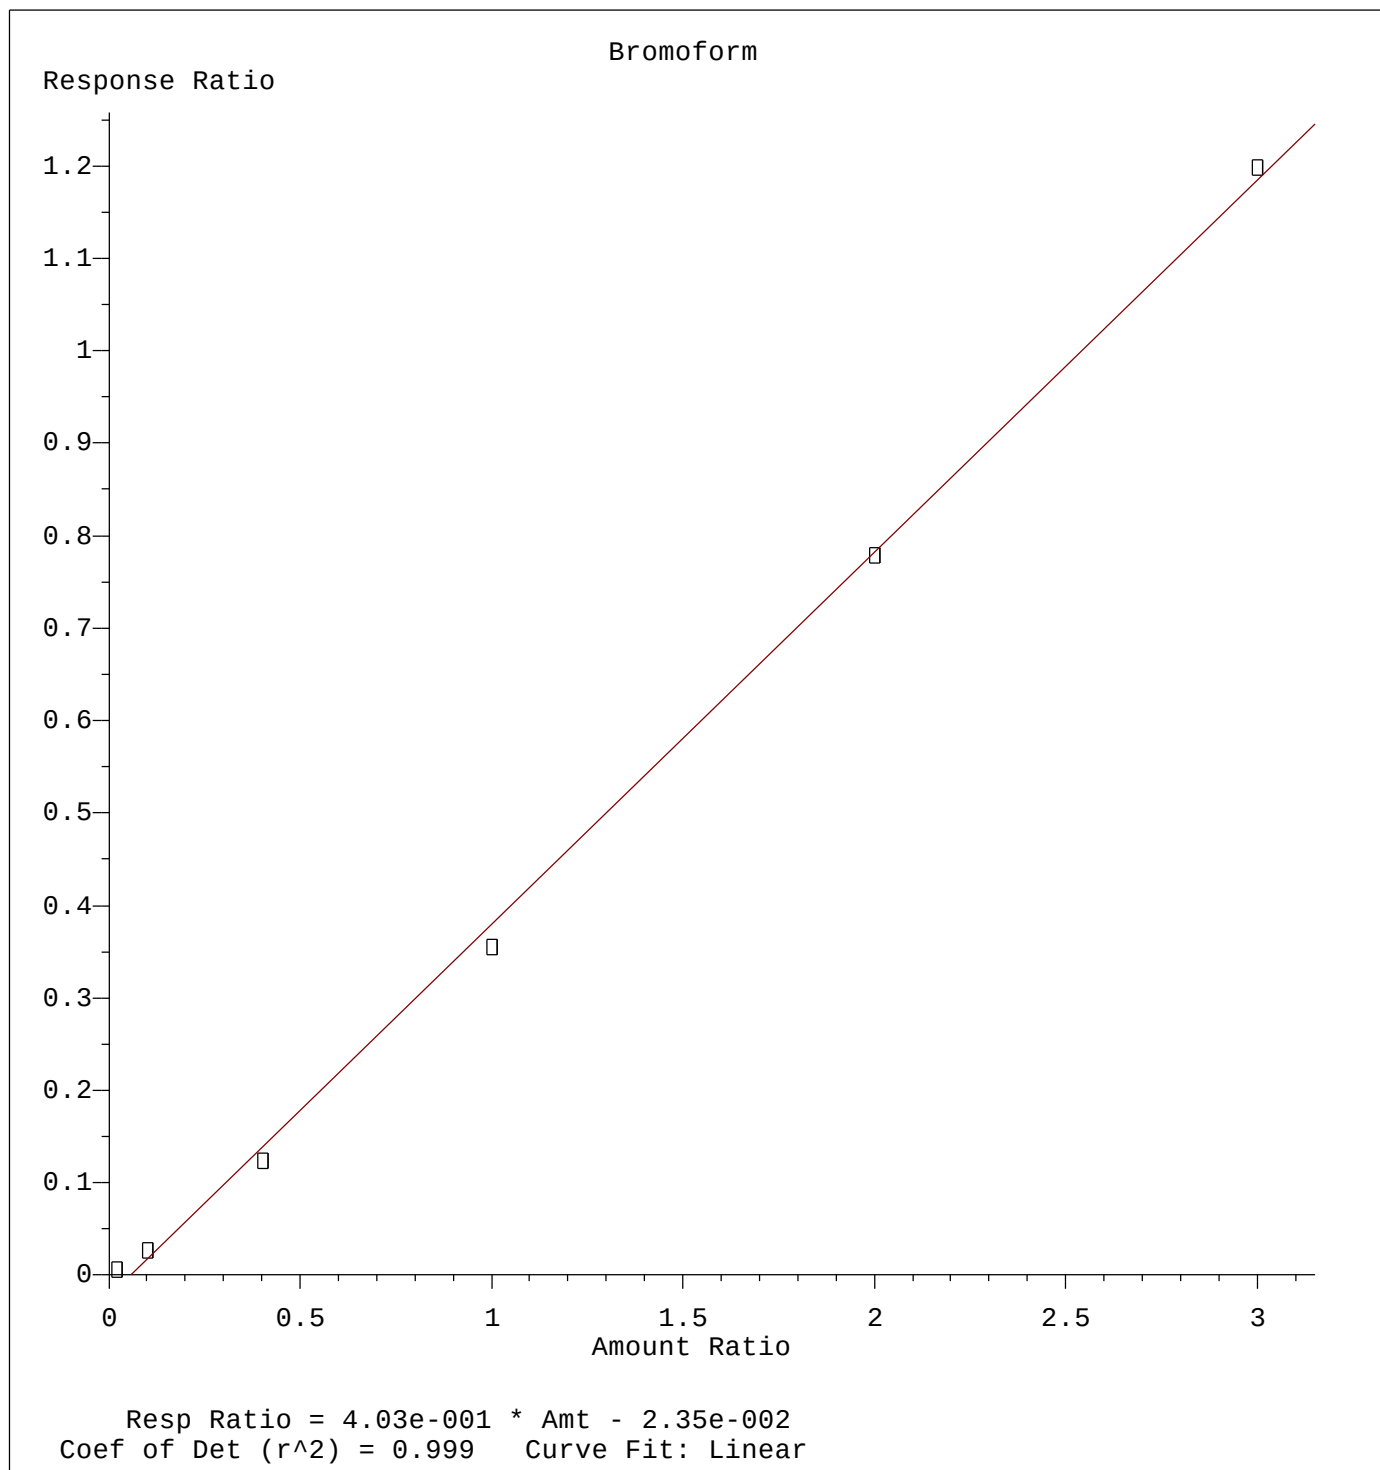

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080618W.M
Calibration Table Last Updated: Tue Aug 07 07:45:48 2018


trans-1,4-Dichloro-2-butene

Response Ratio

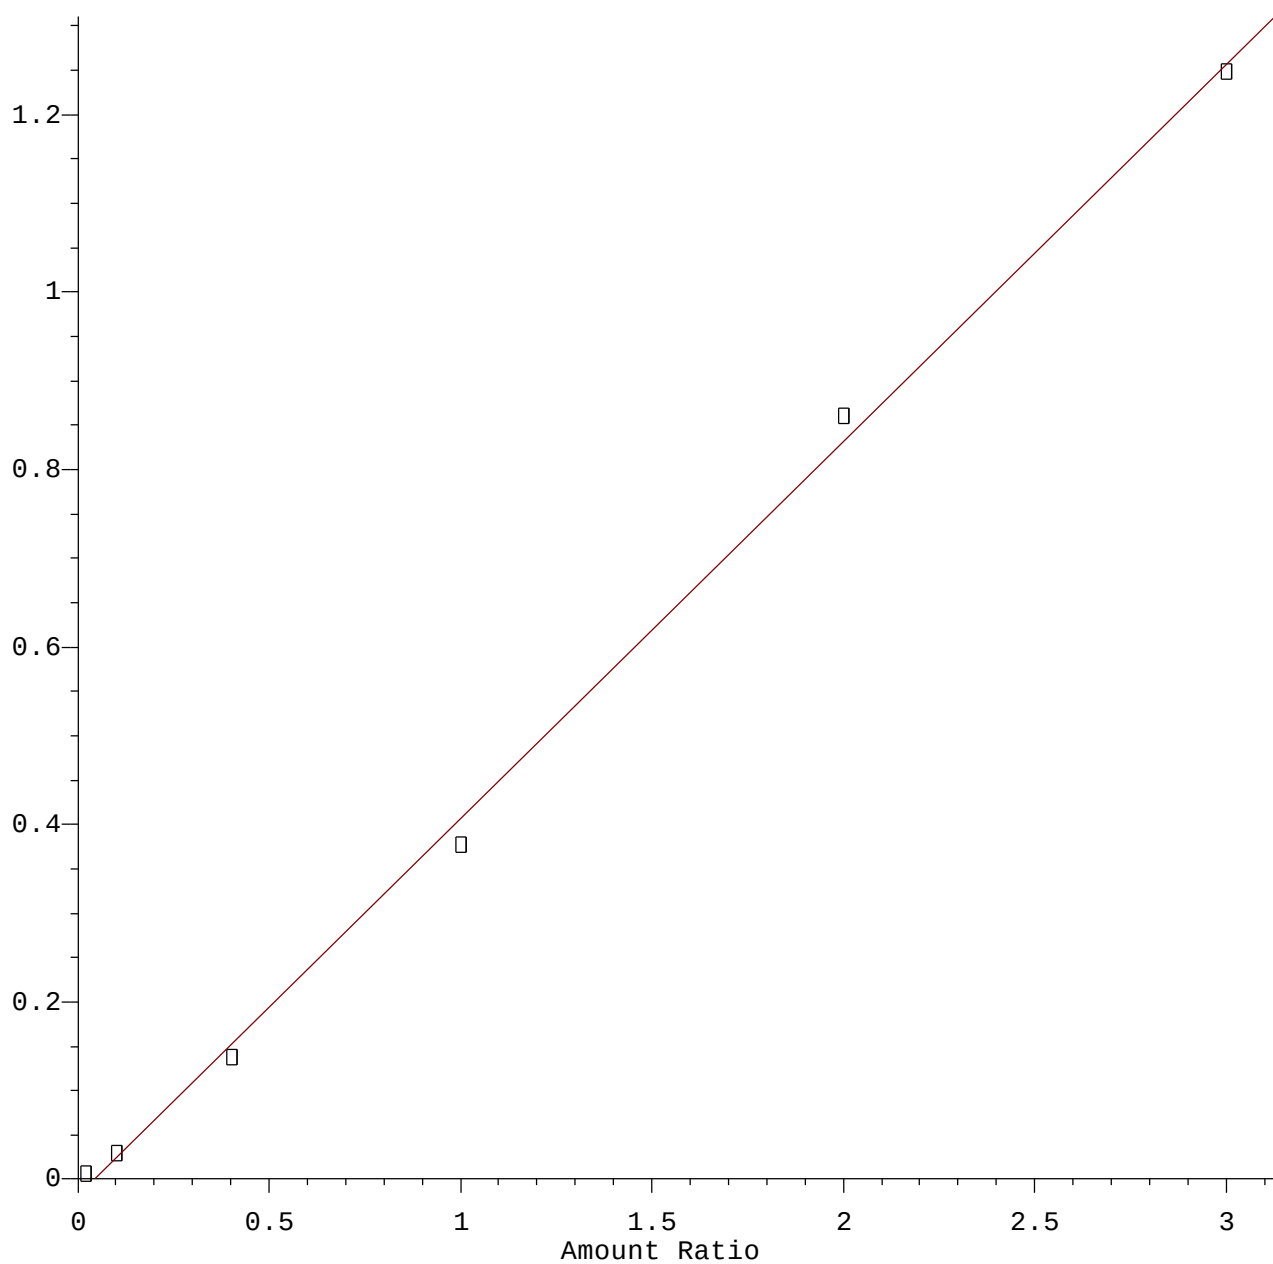


Resp Ratio = $4.25 \times 10^{-1} \times \text{Amt} - 1.88 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080618W.M
Calibration Table Last Updated: Tue Aug 07 07:45:48 2018

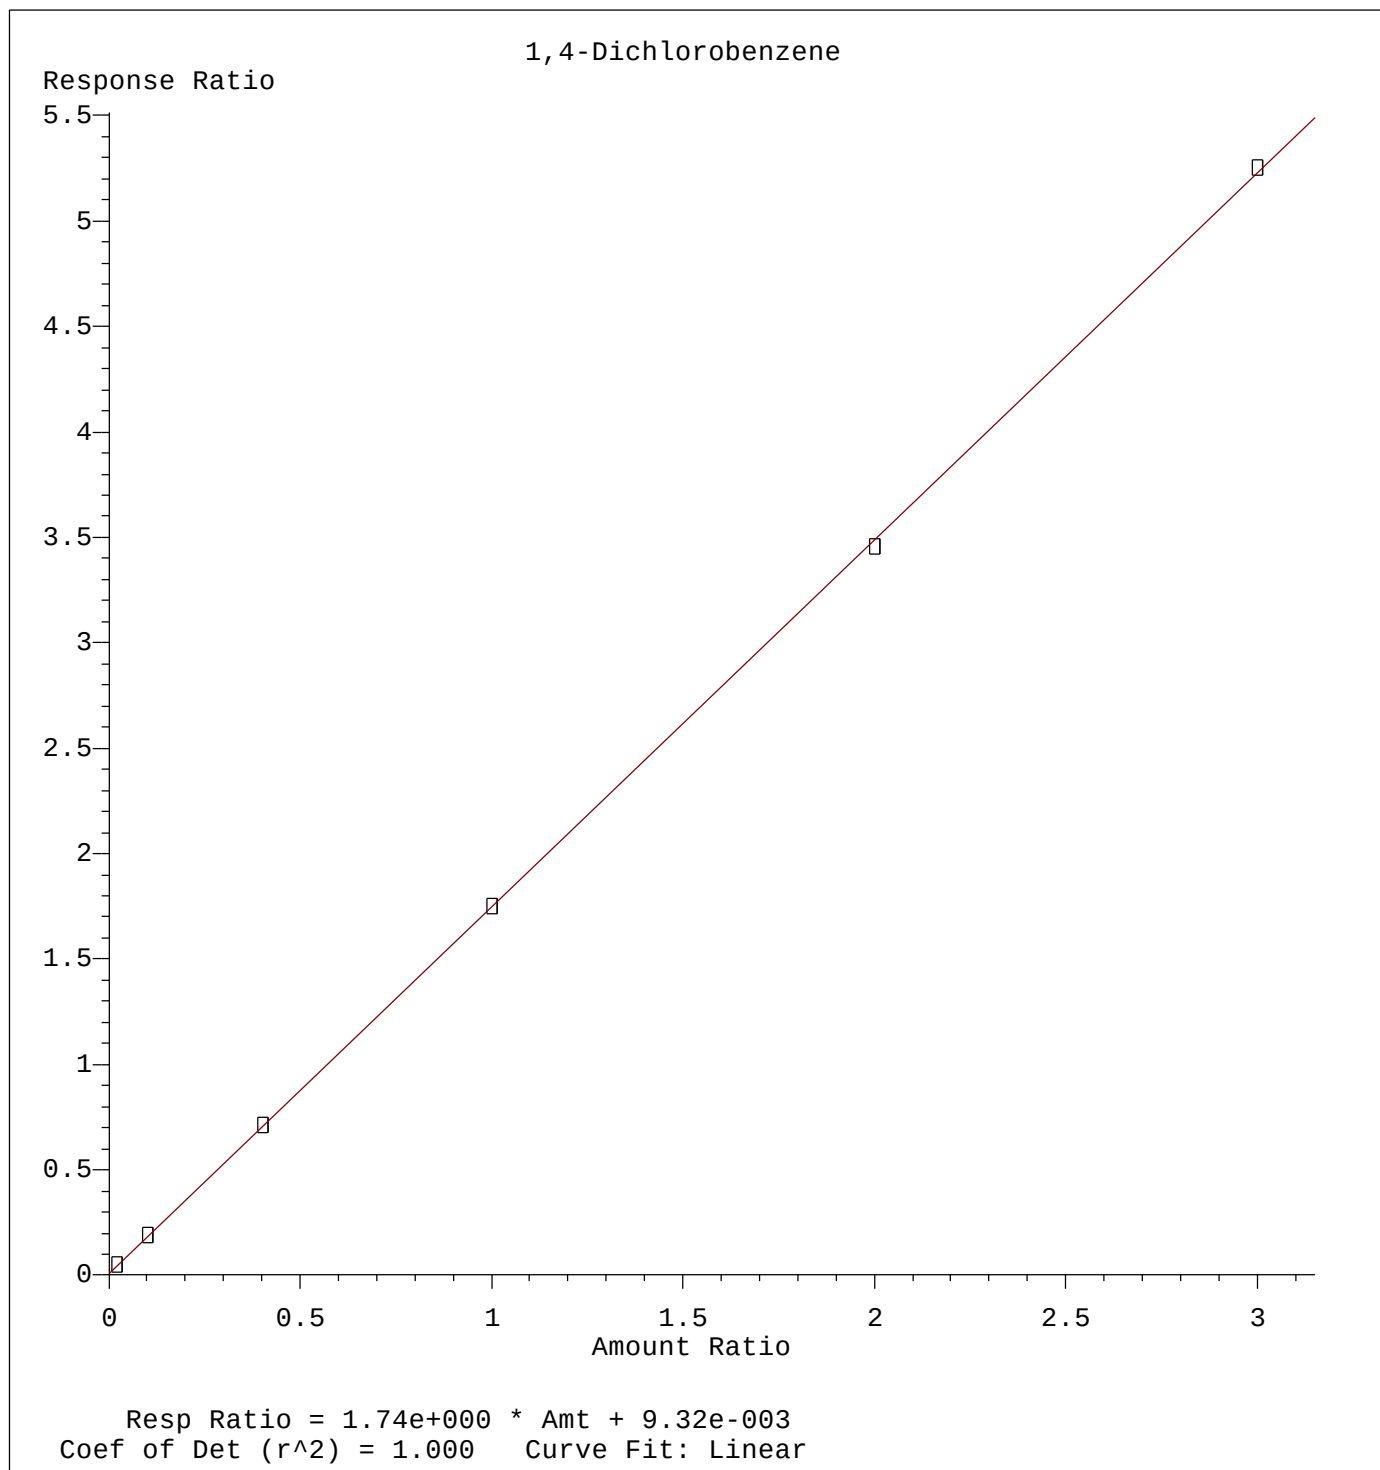

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080618W.M
Calibration Table Last Updated: Tue Aug 07 07:45:48 2018

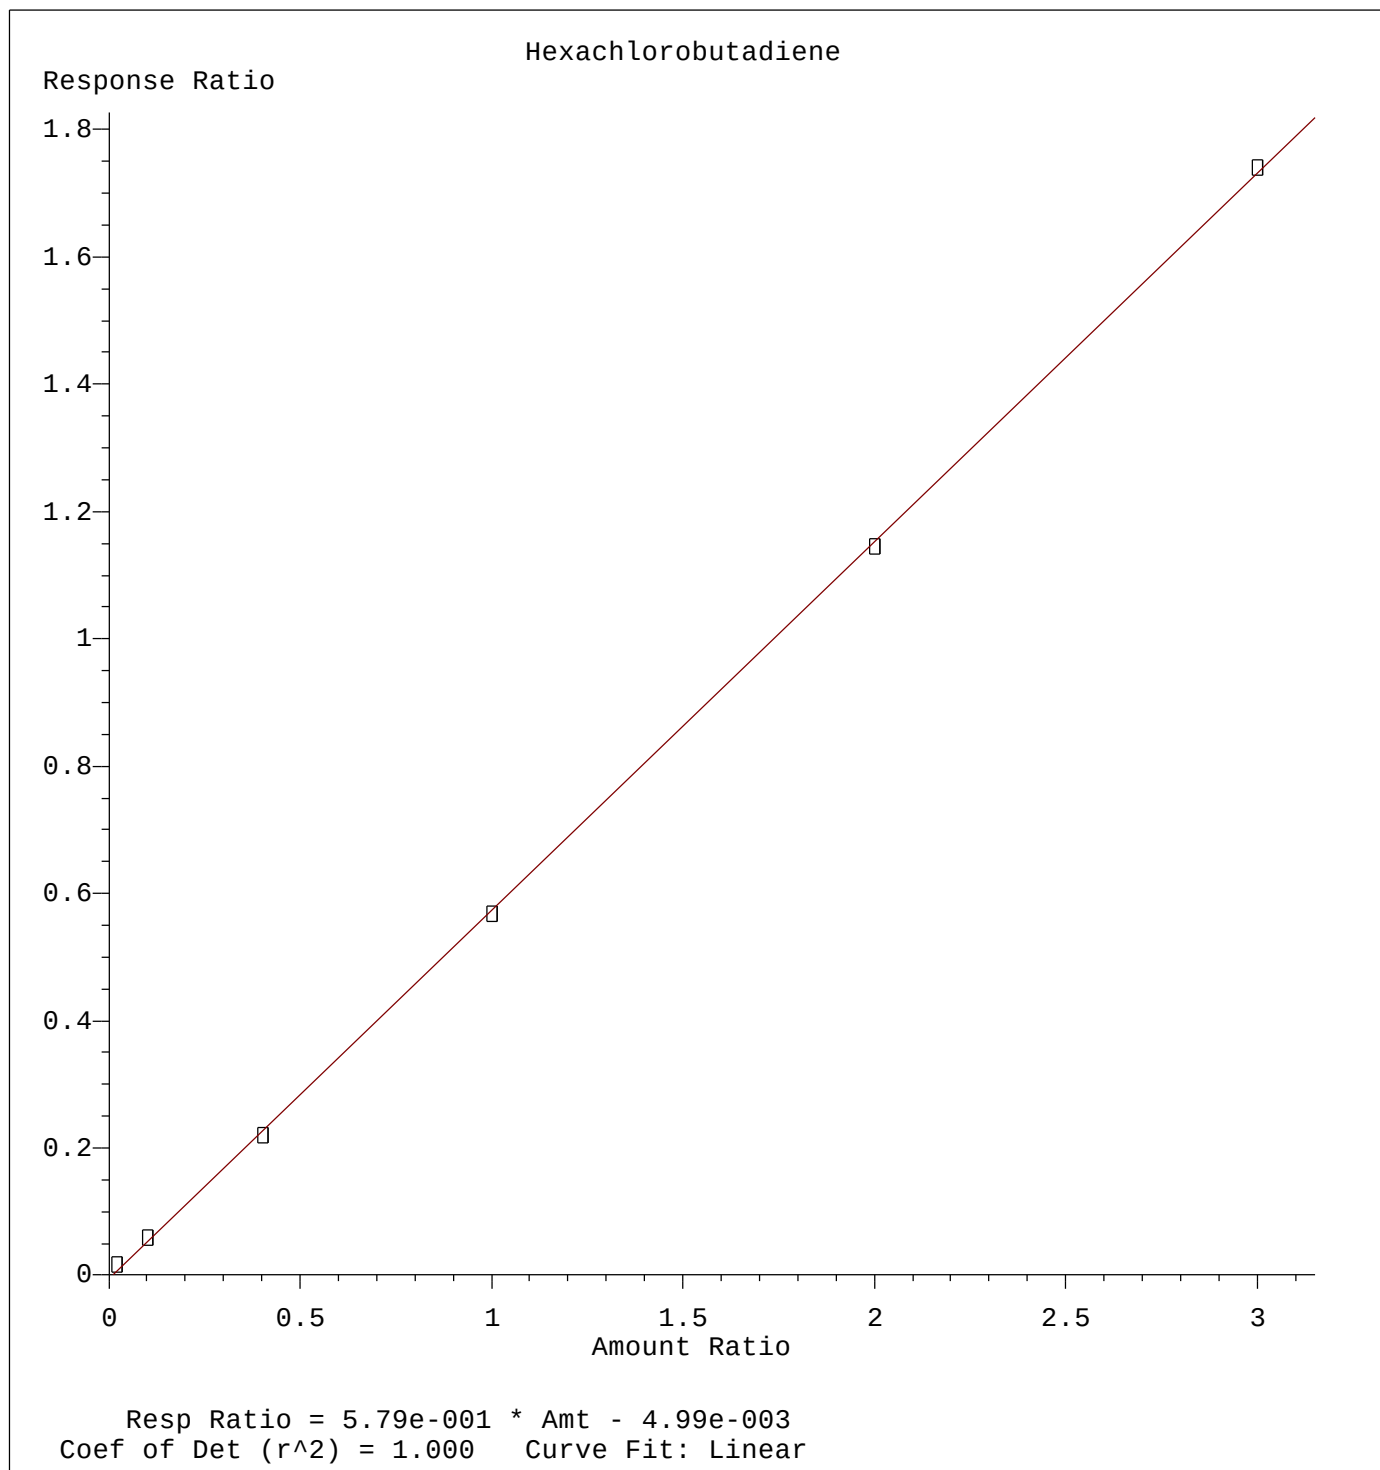

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080618W.M
Calibration Table Last Updated: Tue Aug 07 07:45:48 2018