


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX080618\
Data File : VX003863.D
Acq On : 06 Aug 2018 15:39
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080618W.M
Title : SW846 8260
Last Update : Tue Aug 07 07:45:48 2018

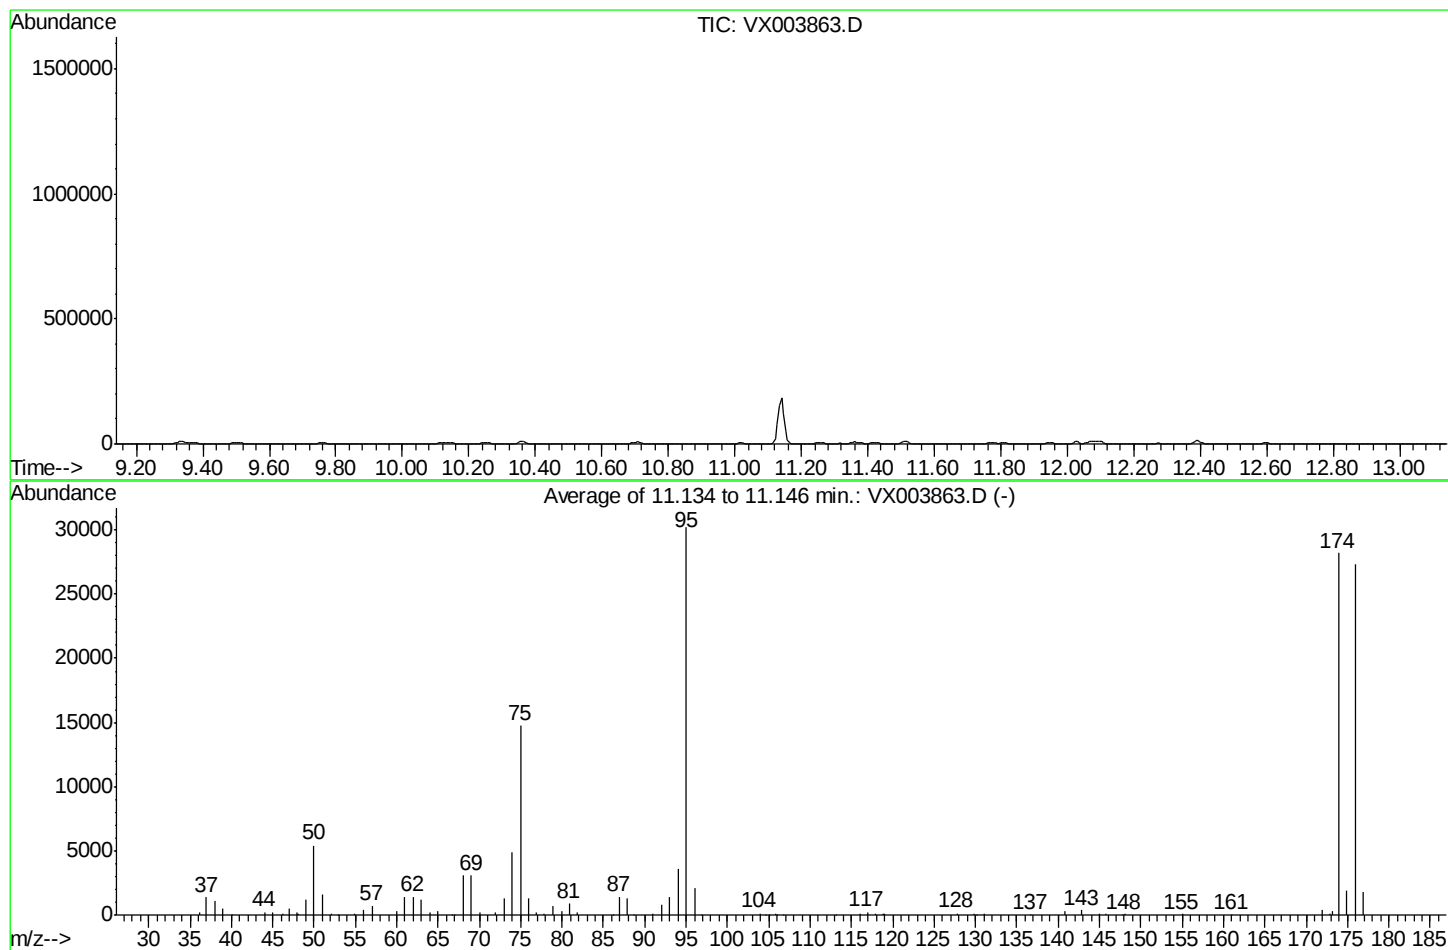

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	5405	PASS
75	95	30	60	48.8	14727	PASS
95	95	100	100	100.0	30205	PASS
96	95	5	9	7.1	2144	PASS
173	174	0.00	2	1.0	283	PASS
174	95	50	100	93.4	28210	PASS
175	174	5	9	6.9	1947	PASS
176	174	95	101	96.9	27328	PASS
177	176	5	9	6.6	1796	PASS