

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX080619\
 Data File : VX011346.D
 Acq On : 06 Aug 2019 12:17
 Operator : JC/SP
 Sample : K4153-01
 Misc : 5.99g/5mL/100uL/10mL/MSVOA_X/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RT-4221

Quant Time: Aug 07 01:36:25 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 02 01:55:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	191899	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	275222	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	224837	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	108916	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.06	65	93367	48.31	ug/l	0.00
Spiked Amount			Recovery	=	96.62%	
35) Dibromofluoromethane	5.49	113	77719	43.25	ug/l	0.00
Spiked Amount			Recovery	=	86.50%	
50) Toluene-d8	8.71	98	312457	46.07	ug/l	0.00
Spiked Amount			Recovery	=	92.14%	
62) 4-Bromofluorobenzene	11.13	95	96506	39.85	ug/l	0.00
Spiked Amount			Recovery	=	79.70%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX080619\
Data File : VX011346.D
Acq On : 06 Aug 2019 12:17
Operator : JC/SP
Sample : K4153-01
Misc : 5.99µ/5mL/100µL/10mL/MSVOA_X/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RT-4221

Quant Time: Aug 07 01:36:25 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 02 01:55:00 2019
Response via : Initial Calibration

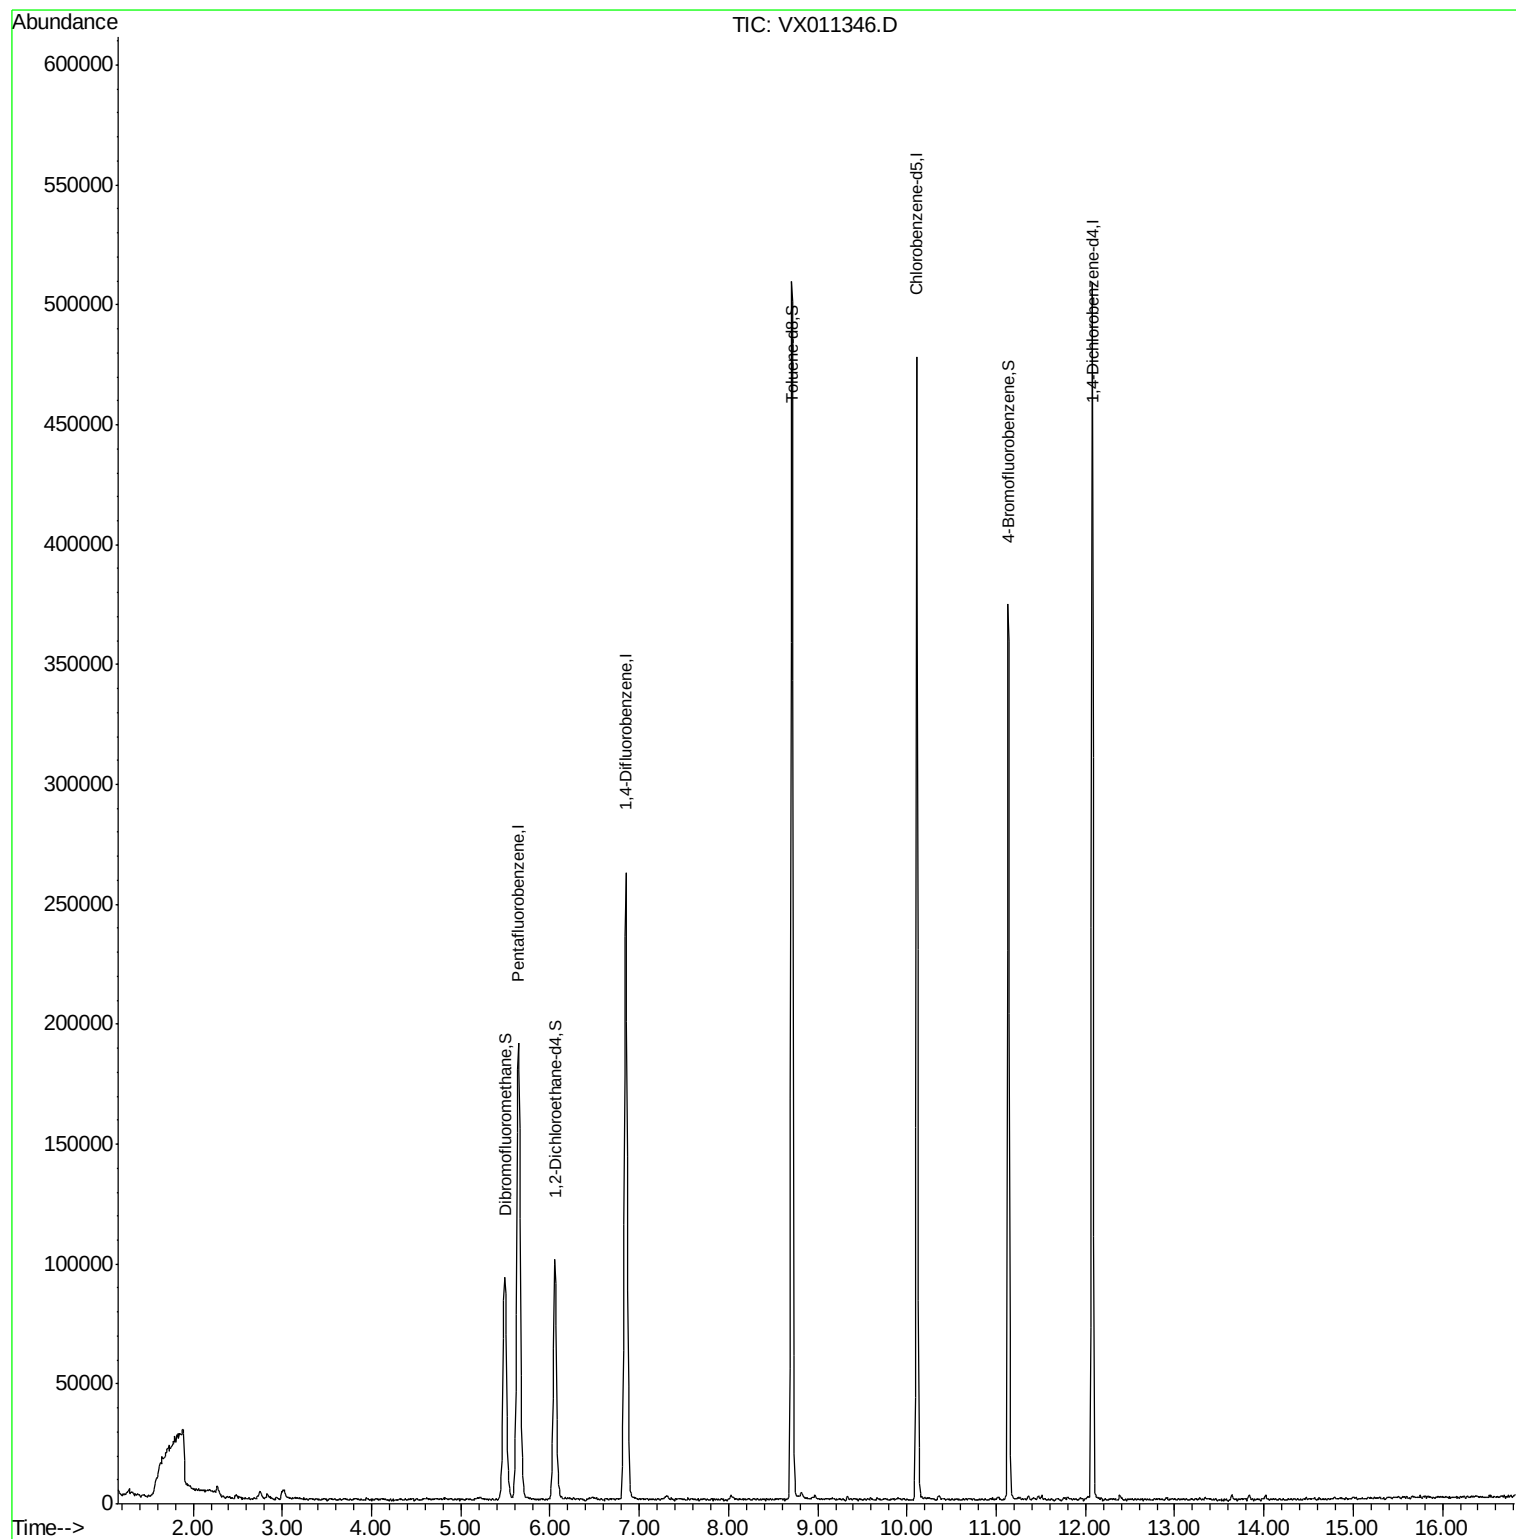

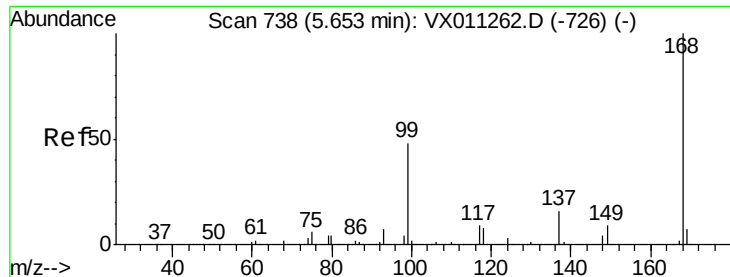

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 737

Delta R.T. -0.01 min

Lab File: VX011346.D

Acq: 06 Aug 2019 12:17

Instrument :

MSVOA_X

ClientSampleId :


RT-4221

Tot Ion:168 Resp: 191899

Ion Ratio Lower Upper

168 100

99 50.3 38.5 57.7

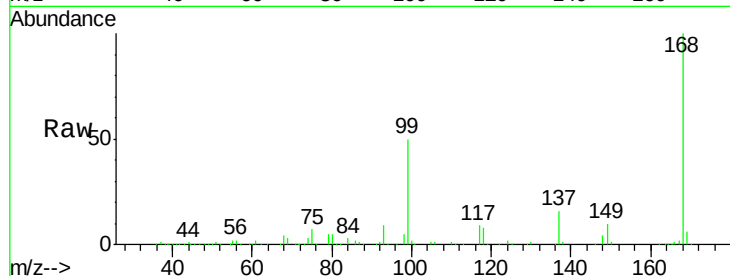

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.65

60000



40000

20000

0

Time-->

5.50 5.60 5.70 5.80

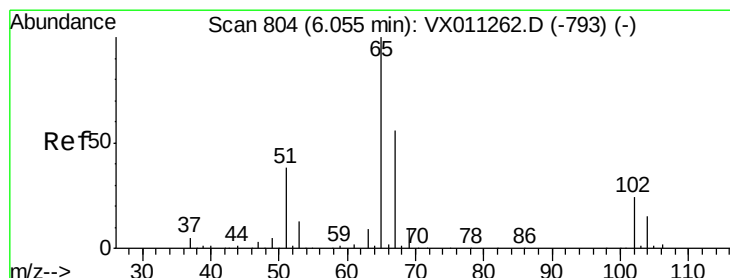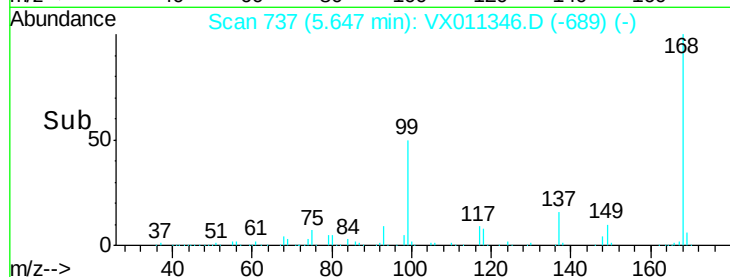

#33

1,2-Dichloroethane-d4

Concen: 48.313 ug/l

RT: 6.06 min Scan# 804

Delta R.T. 0.00 min

Lab File: VX011346.D


Acq: 06 Aug 2019 12:17

Tgt Ion: 65 Resp: 93367

Ion Ratio Lower Upper

65 100

67 53.3 0.0 110.6

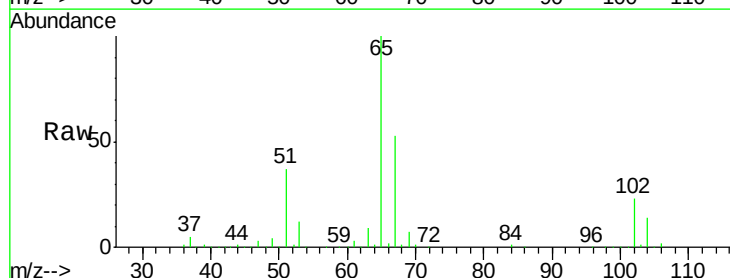

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.06

40000

30000


20000


10000

0

Time-->

5.90 6.00 6.10 6.20

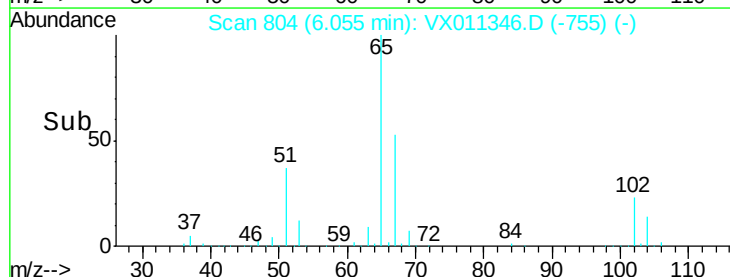


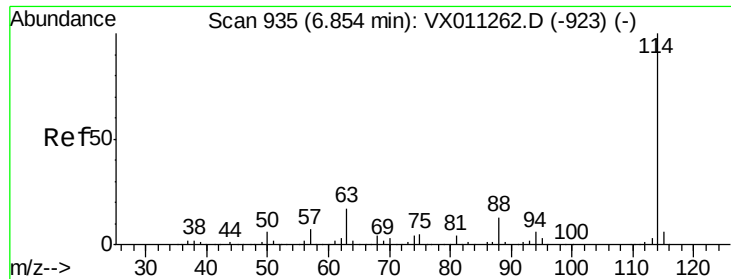




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.85 min Scan# 934
 Delta R.T. -0.01 min
 Lab File: VX011346.D
 Acq: 06 Aug 2019 12:17

Instrument :
 MSVOA_X
 ClientSampleId :
 RT-4221

Tot Ion:114 Resp: 275222
 Ion Ratio Lower Upper
 114 100
 63 17.5 0.0 34.0
 88 14.7 0.0 26.4

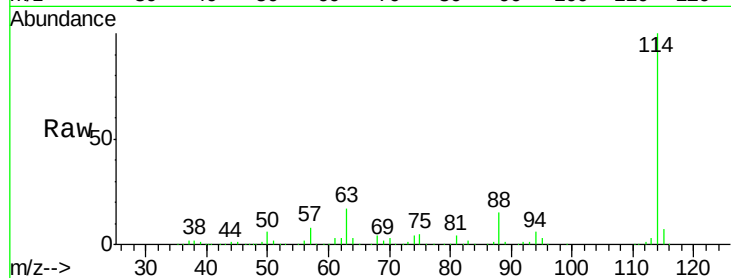


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VX0
 Ion 87.90 (87.60 to 88.60): VX0

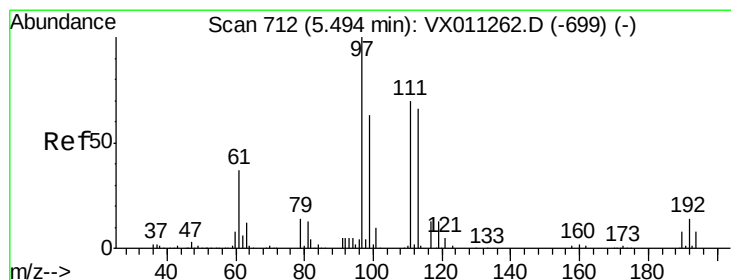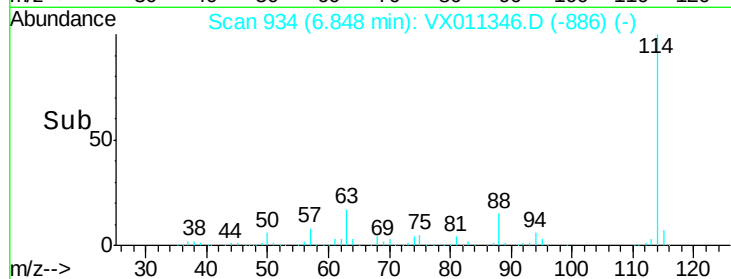
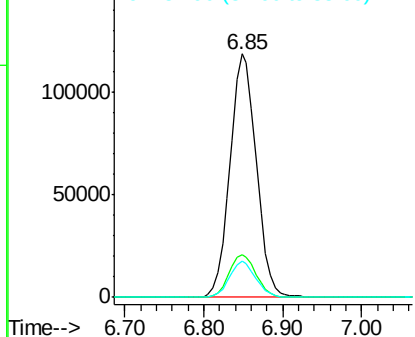



#35
 Dibromofluoromethane
 Concen: 43.253 ug/l
 RT: 5.49 min Scan# 712
 Delta R.T. 0.00 min
 Lab File: VX011346.D
 Acq: 06 Aug 2019 12:17

Tgt Ion:113 Resp: 77719
 Ion Ratio Lower Upper
 113 100
 111 103.5 81.9 122.9
 192 22.2 17.8 26.8

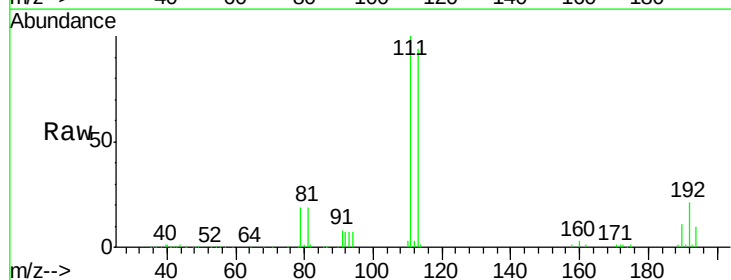

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V



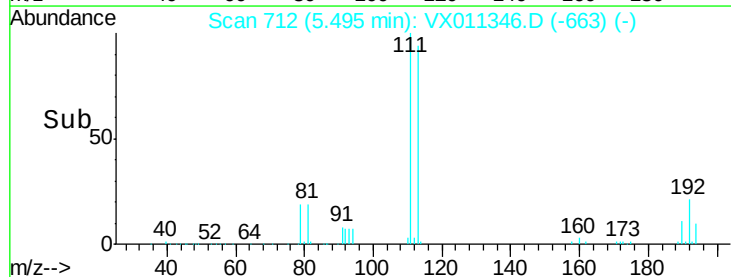
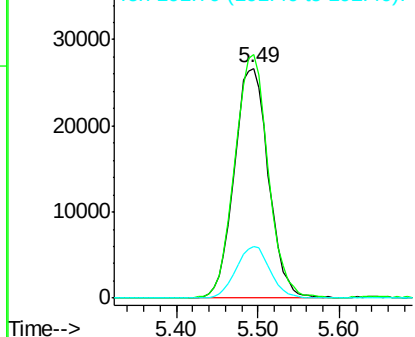


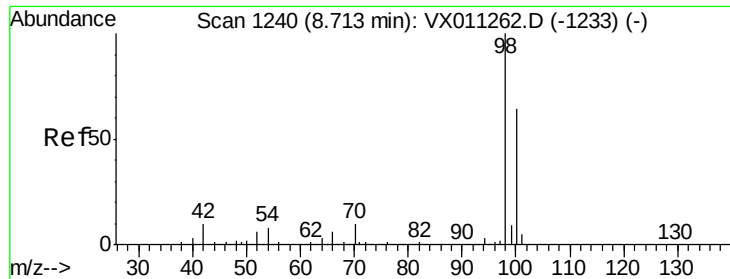

#50
Toluene-d8
Concen: 46.067 ug/l
RT: 8.71 min Scan# 1240
Delta R.T. 0.00 min
Lab File: VX011346.D
Acq: 06 Aug 2019 12:17




Instrument :
MSVOA_X
ClientSampled :
RT-4221


Tot Ion: 98 Resp: 312457
Ion Ratio Lower Upper
98 100
100 63.3 51.7 77.5

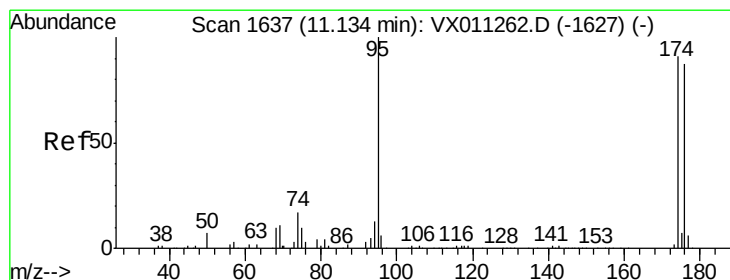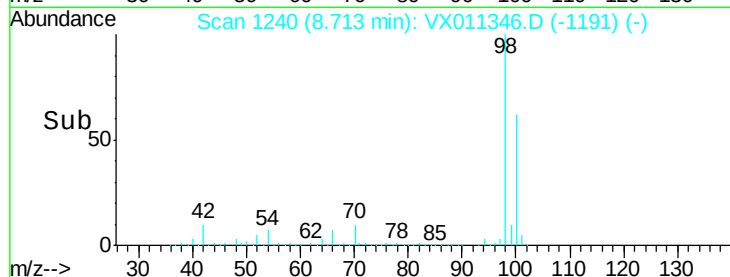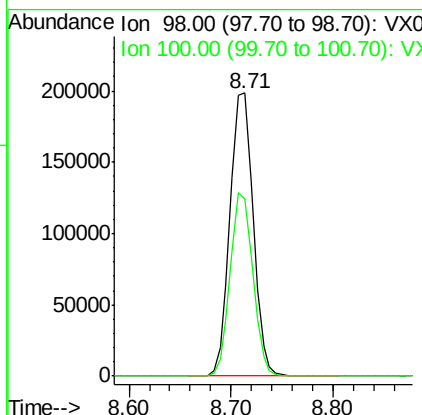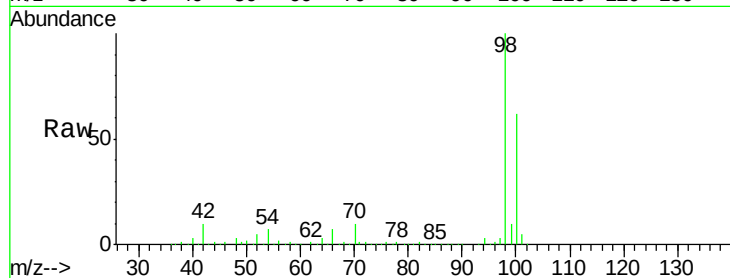

#62
4-Bromofluorobenzene
Concen: 39.852 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. 0.00 min
Lab File: VX011346.D
Acq: 06 Aug 2019 12:17

Tgt Ion: 95 Resp: 96506
Ion Ratio Lower Upper
95 100
174 93.2 0.0 191.2
176 88.0 0.0 184.8


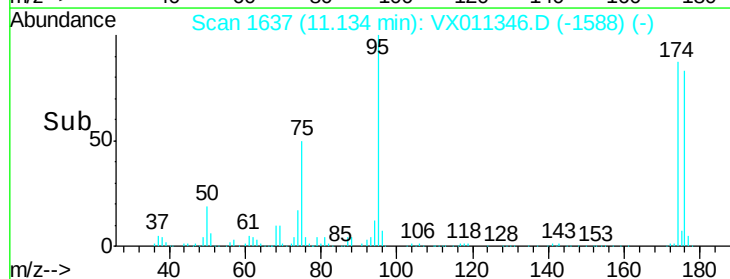
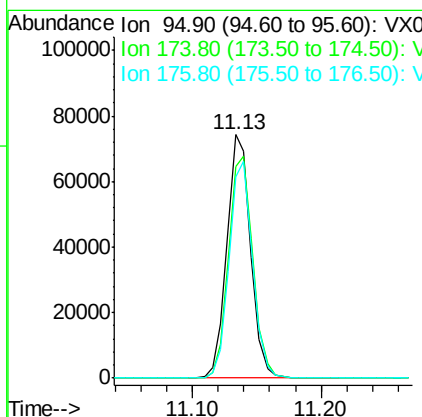
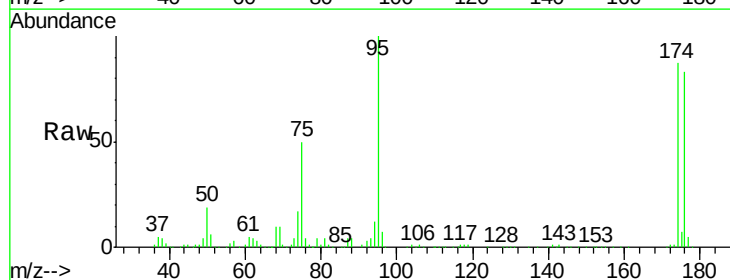


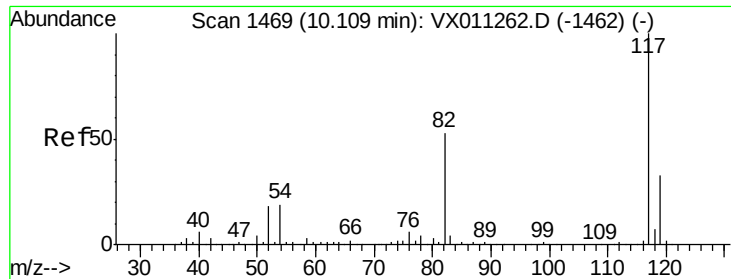

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. 0.00 min
Lab File: VX011346.D
Acq: 06 Aug 2019 12:17

Instrument :
MSVOA_X
ClientSampled :
RT-4221

Tot Ion:117 Resp: 224837
Ion Ratio Lower Upper
117 100
82 51.5 42.2 63.2
119 32.2 26.6 39.8

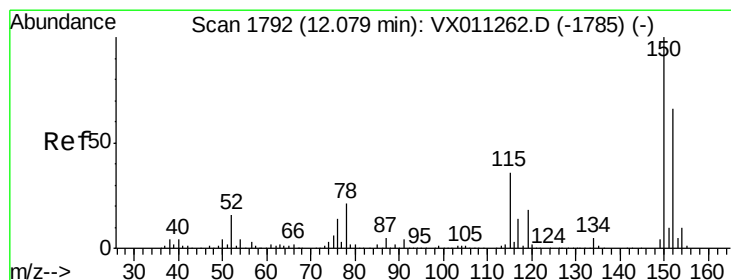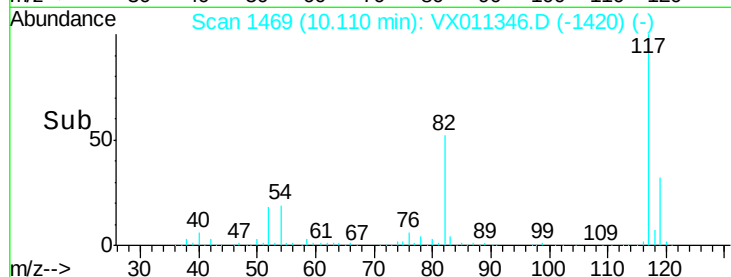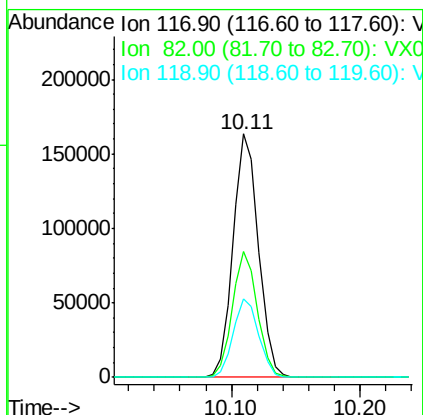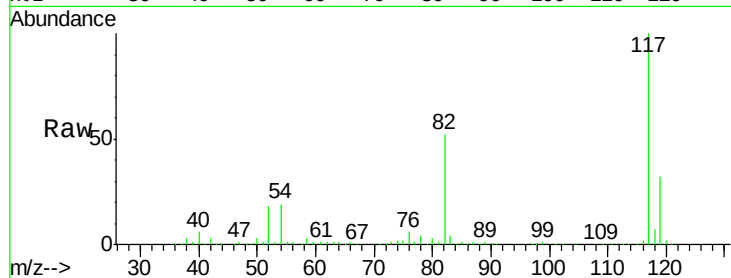

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. 0.00 min
Lab File: VX011346.D
Acq: 06 Aug 2019 12:17

Tgt Ion:152 Resp: 108916
Ion Ratio Lower Upper
152 100
115 55.6 40.0 119.9
150 156.3 0.0 350.4

