


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX080619\
Data File : VX011340.D
Acq On : 06 Aug 2019 09:08
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D072919S.M
Title : SW846 8260
Last Update : Tue Jul 30 03:04:50 2019

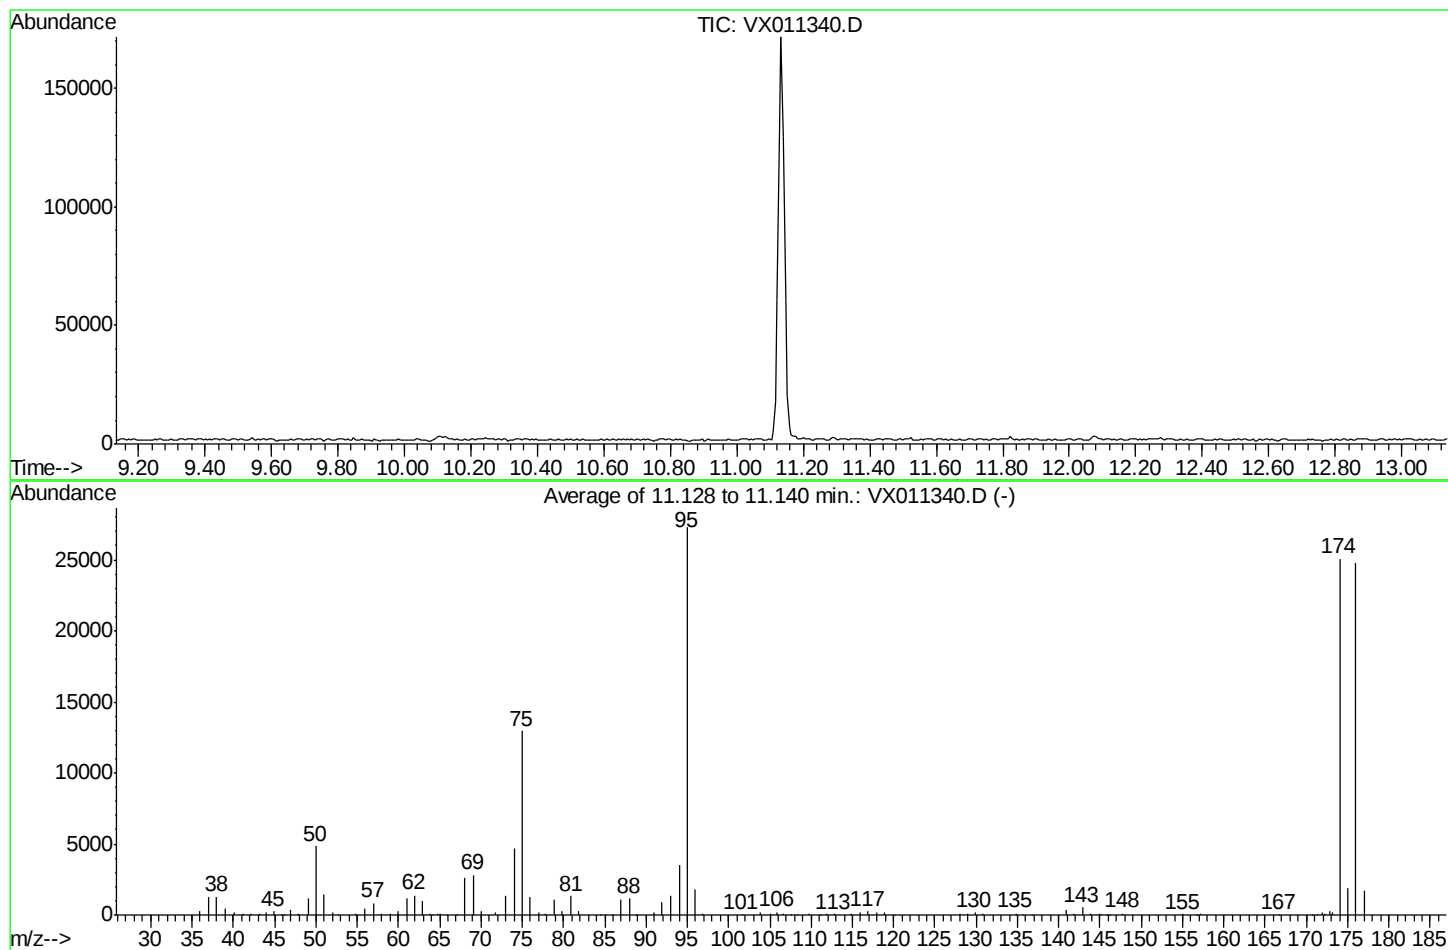

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	4852	PASS
75	95	30	60	47.4	12943	PASS
95	95	100	100	100.0	27290	PASS
96	95	5	9	6.7	1840	PASS
173	174	0.00	2	1.0	241	PASS
174	95	50	100	92.0	25098	PASS
175	174	5	9	7.5	1874	PASS
176	174	95	101	98.8	24800	PASS
177	176	5	9	6.8	1681	PASS