

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030454.D
 Acq On : 06 Aug 2022 11:13
 Operator : JC/MD
 Sample : VX0806WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Aug 07 00:16:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 06 02:08:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	290428	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	259561	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	114362	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	78199	41.928	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	83.860%
7) Chloroethane-d5	1.666	69	63426	48.241	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	96.480%
11) 1,1-Dichloroethene-d2	2.306	63	119669	33.920	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.840%
21) 2-Butanone-d5	4.458	46	190486	110.229	ug/L	-0.01
Spiked Amount	100.000	Range	40 - 130	Recovery	=	110.230%
24) Chloroform-d	5.062	84	175861	45.805	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.620%
26) 1,2-Dichloroethane-d4	5.964	65	124558	47.780	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.560%
32) Benzene-d6	5.976	84	331364	44.568	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.140%
36) 1,2-Dichloropropane-d6	7.312	67	113581	47.085	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.180%
41) Toluene-d8	8.653	98	291211	41.552	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.100%
43) trans-1,3-Dichloroprop...	8.952	79	50040	41.698	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.400%
47) 2-Hexanone-d5	9.384	63	124417	101.187	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	101.190%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	150508	47.495	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.000%
66) 1,2-Dichlorobenzene-d4	12.323	152	104899	47.291	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.580%
Target Compounds						
44) trans-1,3-Dichloropropene	8.952	75	2492	0.771	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030454.D
Acq On : 06 Aug 2022 11:13
Operator : JC/MD
Sample : VX0806WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Aug 07 00:16:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 06 02:08:42 2022
Response via : Initial Calibration

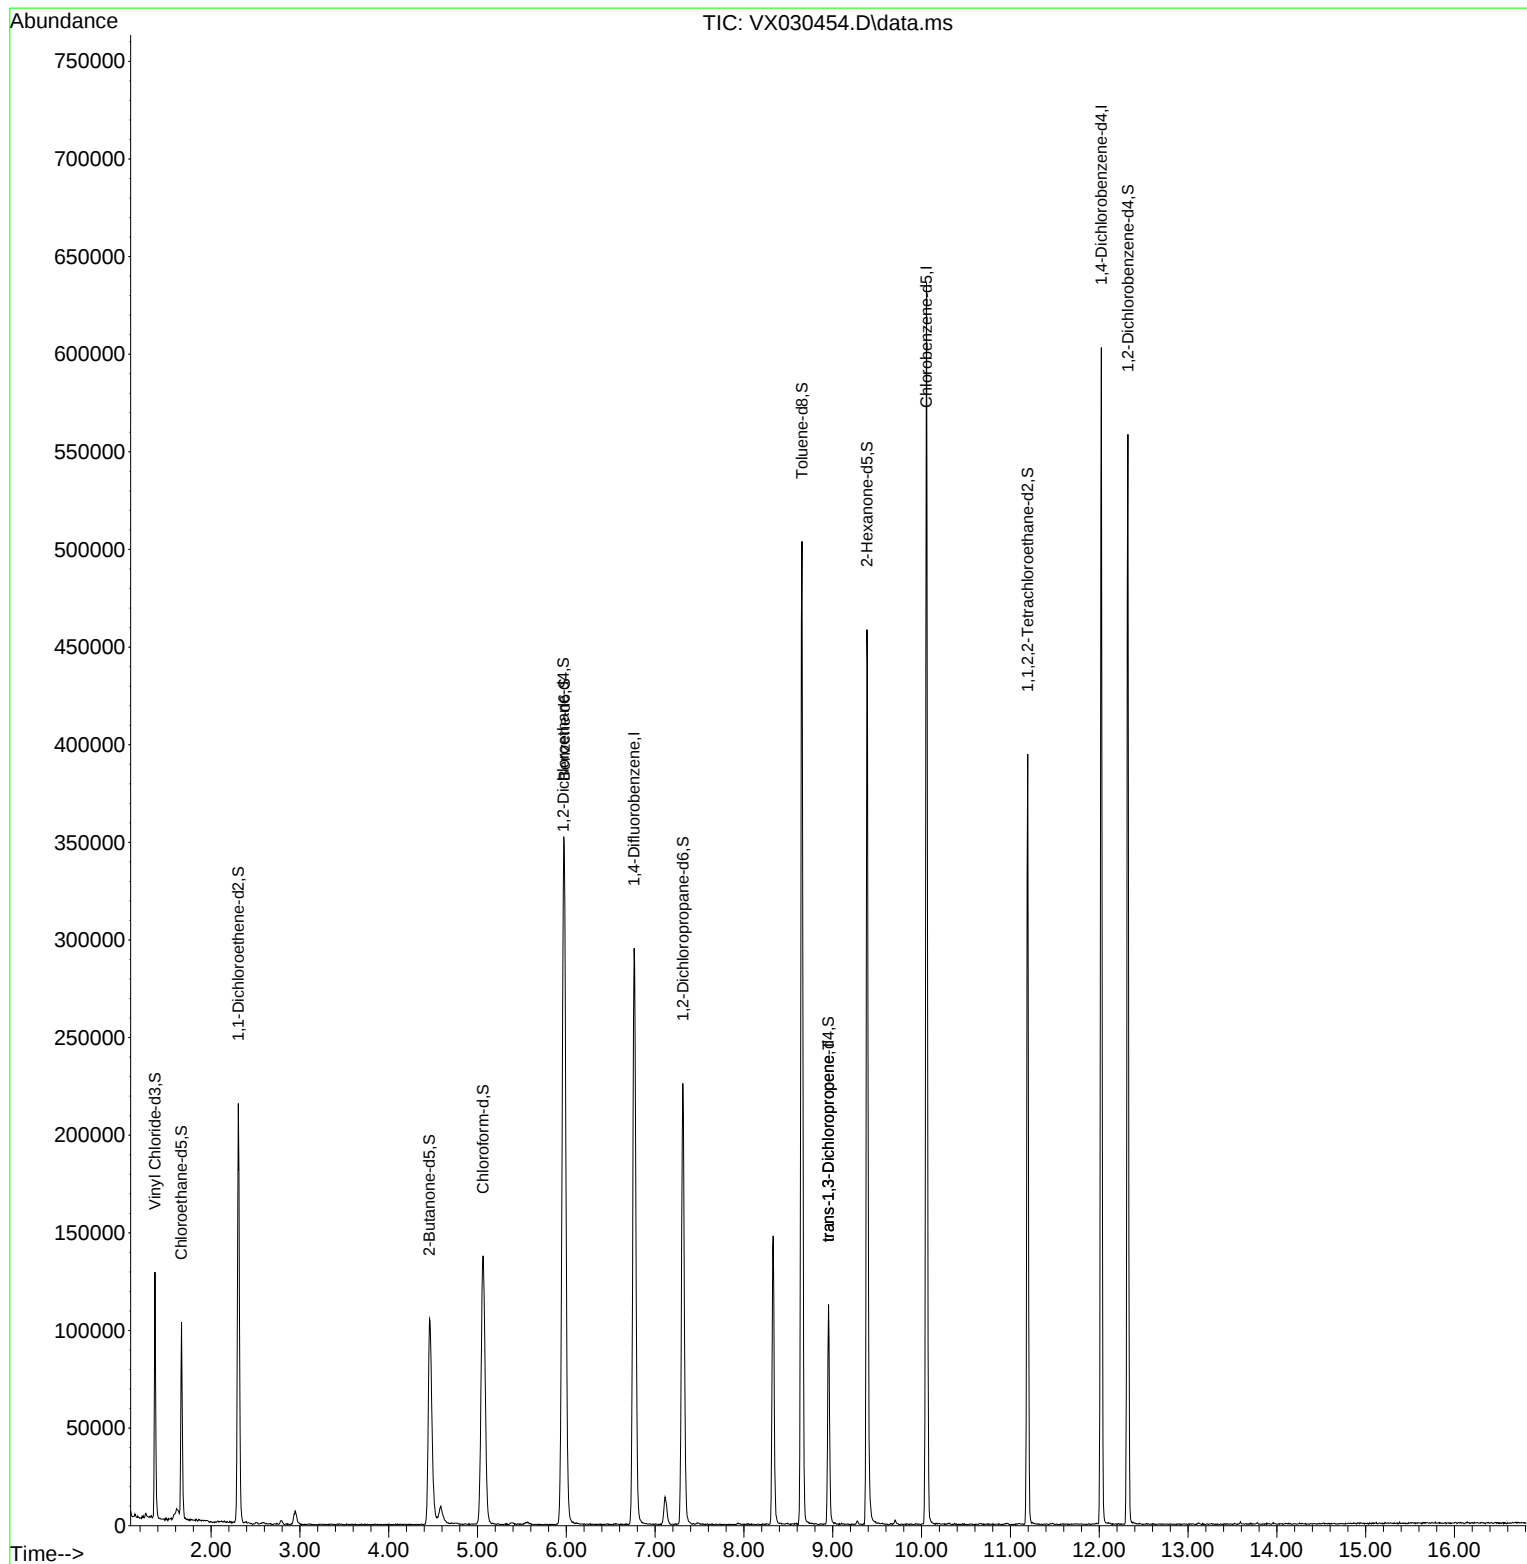

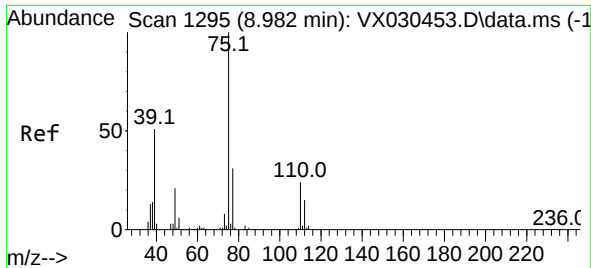

#44
 trans-1,3-Dichloropropene
 Concen: 0.771 ug/L
 RT: 8.952 min Scan# 11
 Delta R.T. -0.031 min
 Lab File: VX030454.D
 Acq: 06 Aug 2022 11:13

Instrument :
 MSVOA_X
 ClientSampleId :

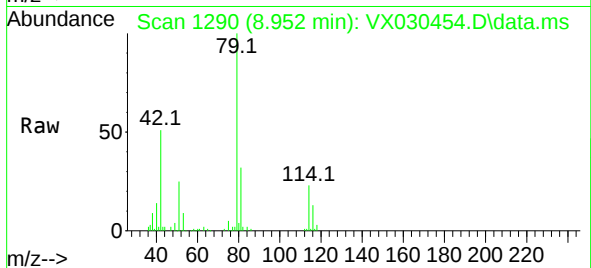

Tgt Ion: 75 Resp: 2492
 Ion Ratio Lower Upper
 75 100
 77 34.5 22.5 41.7

