

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030467.D
 Acq On : 06 Aug 2022 16:19
 Operator : JC/MD
 Sample : N4003-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Aug 07 00:18:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 06 02:08:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	294105	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	260843	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	119379	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	78552	41.591	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	83.180%
7) Chloroethane-d5	1.666	69	59319	44.553	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	89.100%
11) 1,1-Dichloroethene-d2	2.307	63	121502	34.009	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.020%
21) 2-Butanone-d5	4.471	46	166393	95.083	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	95.080%
24) Chloroform-d	5.068	84	162081	41.688	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.380%
26) 1,2-Dichloroethane-d4	5.964	65	116365	44.079	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.160%
32) Benzene-d6	5.983	84	324695	43.456	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.920%
36) 1,2-Dichloropropane-d6	7.312	67	108001	44.552	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	89.100%
41) Toluene-d8	8.653	98	293684	41.699	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.400%
43) trans-1,3-Dichloroprop...	8.958	79	44216	36.664	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	73.320%
47) 2-Hexanone-d5	9.391	63	109645	88.735	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	88.740%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	137031	43.030	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	86.060%
66) 1,2-Dichlorobenzene-d4	12.323	152	97046	41.912	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.820%
Target Compounds						
44) trans-1,3-Dichloropropene	8.952	75	2320	0.715	ug/L	Qvalue 99
61) 1,2,3-Trichloropropane	12.024	75	16133	6.293	ug/L	# 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030467.D
Acq On : 06 Aug 2022 16:19
Operator : JC/MD
Sample : N4003-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Aug 07 00:18:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 06 02:08:42 2022
Response via : Initial Calibration

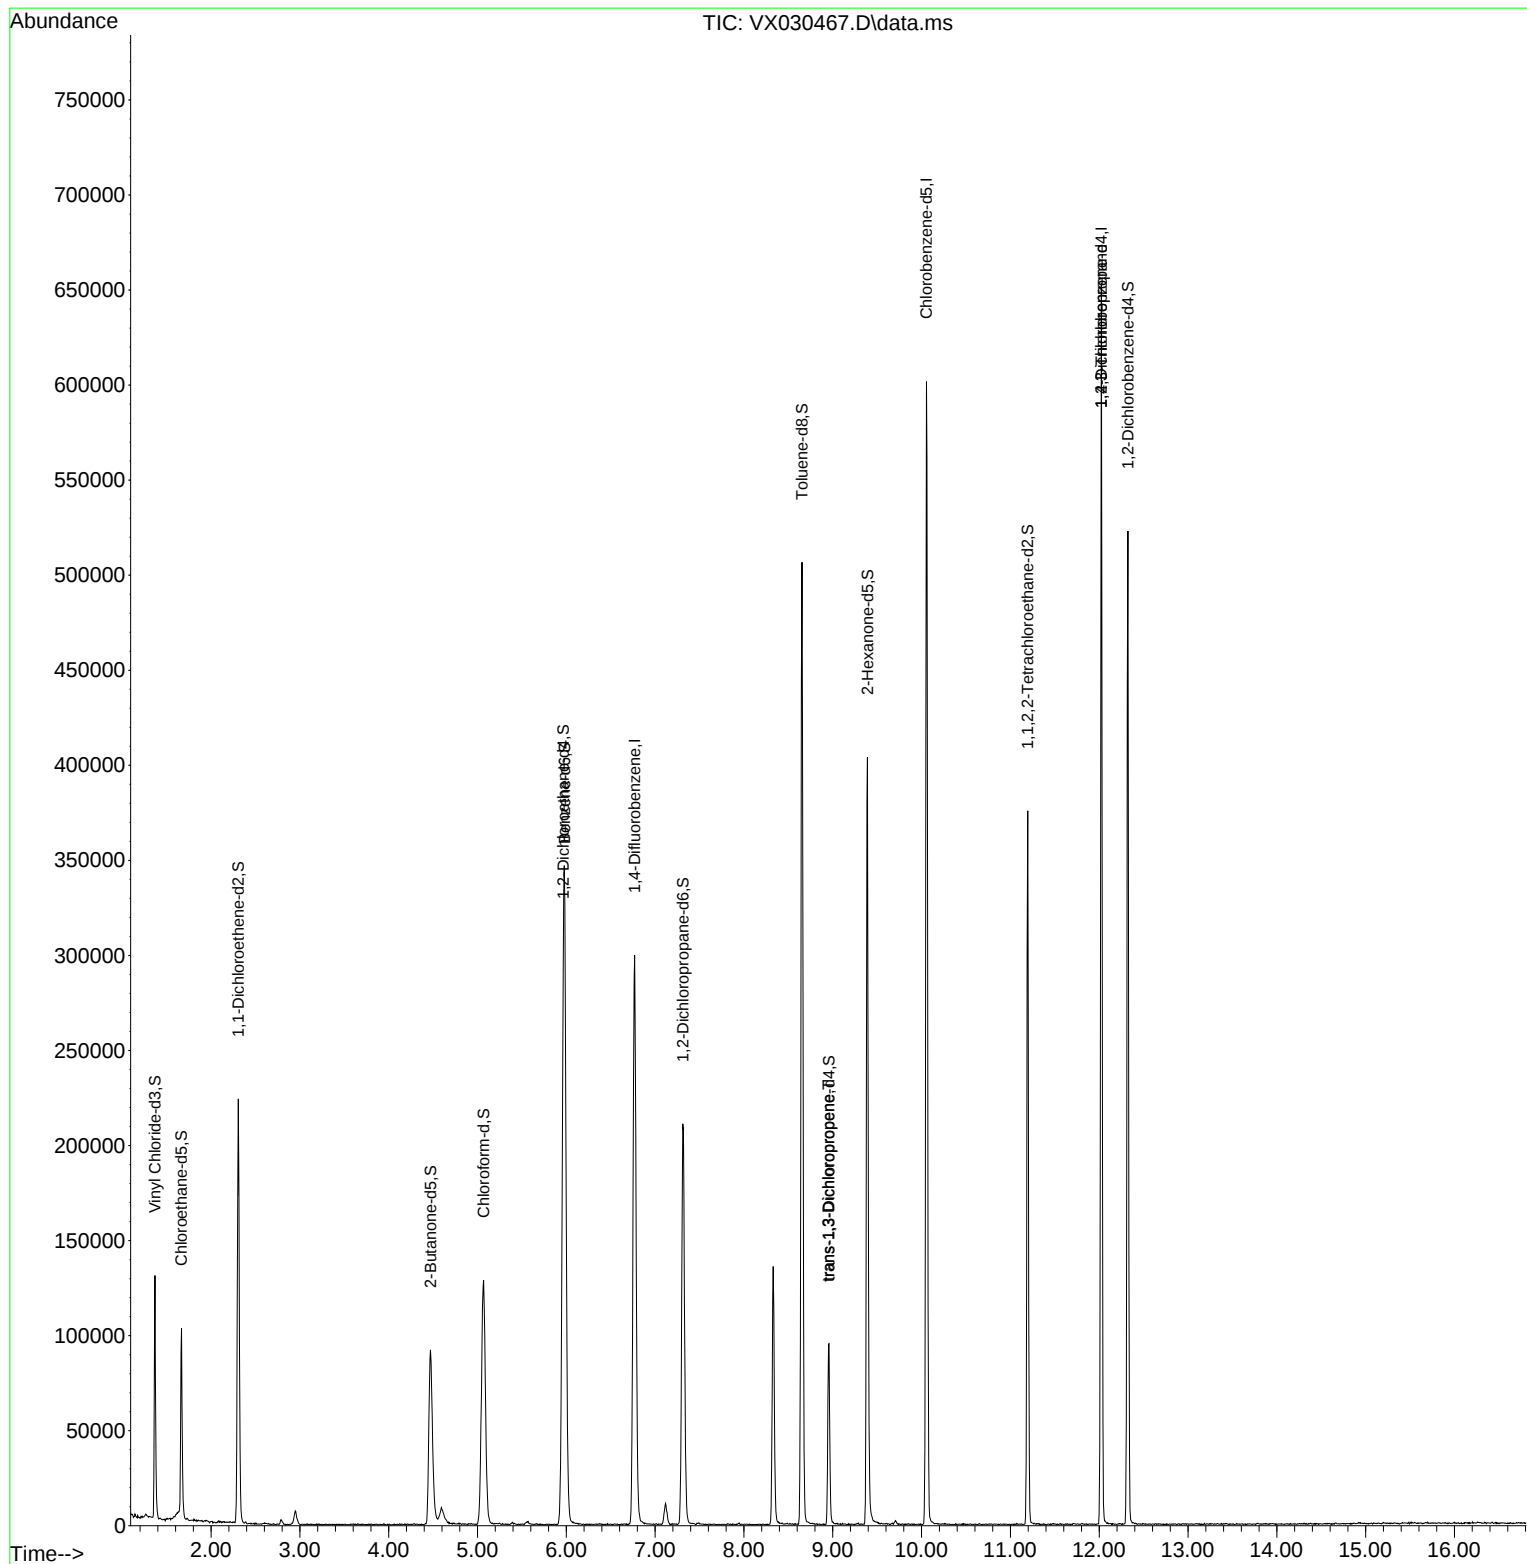



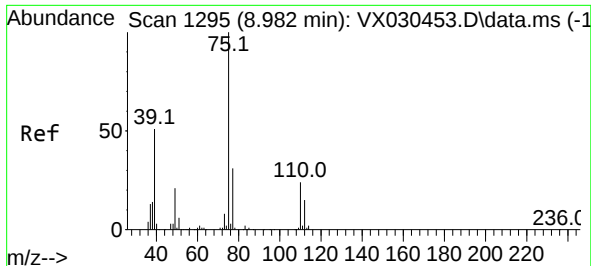


#44
trans-1,3-Dichloropropene
Concen: 0.715 ug/L
RT: 8.952 min Scan# 11
Delta R.T. -0.031 min
Lab File: VX030467.D
Acq: 06 Aug 2022 16:19

Instrument :
MSVOA_X
ClientSampleId :

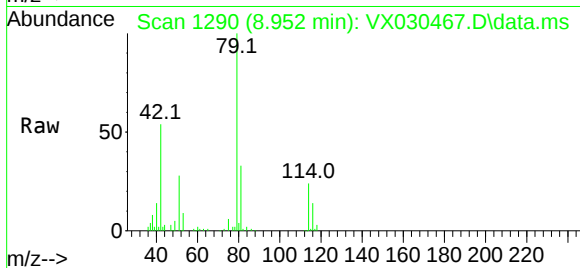

Tgt Ion: 75 Resp: 2320
Ion Ratio Lower Upper
75 100
77 32.5 22.5 41.7

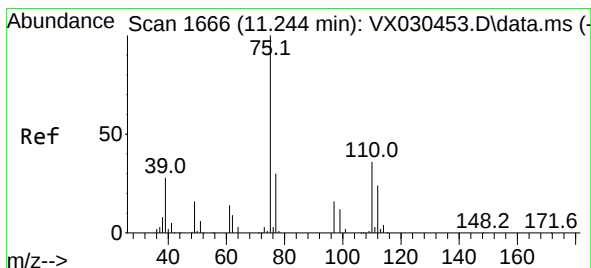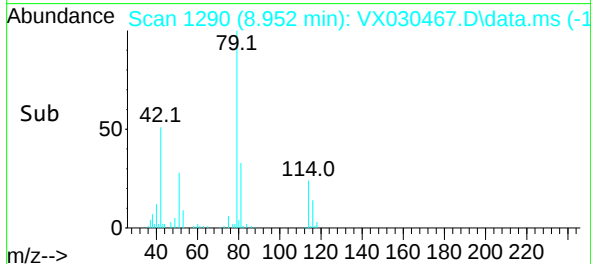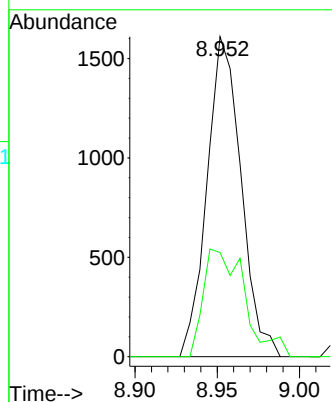

#61
1,2,3-Trichloropropane
Concen: 6.293 ug/L
RT: 12.024 min Scan# 1794
Delta R.T. 0.780 min
Lab File: VX030467.D
Acq: 06 Aug 2022 16:19

Tgt Ion: 75 Resp: 16133
Ion Ratio Lower Upper
75 100
77 33.0 26.1 39.1
110 3.4 30.5 45.7#

