

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030482.D
 Acq On : 06 Aug 2022 22:58
 Operator : JC/MD
 Sample : N4066-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E54

Quant Time: Aug 07 05:46:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 06 02:08:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	294996	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	262846	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	118614	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	70664	37.301	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	74.600%		
7) Chloroethane-d5	1.666	69	58885	44.093	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	88.180%		
11) 1,1-Dichloroethene-d2	2.307	63	109058	30.434	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	60.860%		
21) 2-Butanone-d5	4.471	46	163320	93.046	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	93.050%		
24) Chloroform-d	5.068	84	162038	41.551	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	83.100%		
26) 1,2-Dichloroethane-d4	5.964	65	113991	43.049	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.100%		
32) Benzene-d6	5.983	84	321283	42.672	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.340%		
36) 1,2-Dichloropropane-d6	7.312	67	108707	44.501	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	89.000%		
41) Toluene-d8	8.653	98	289872	40.844	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	81.680%		
43) trans-1,3-Dichloroprop...	8.952	79	41252	33.946	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	67.900%		
47) 2-Hexanone-d5	9.391	63	109828	88.206	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	88.210%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	133372	41.562	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	83.120%		
66) 1,2-Dichlorobenzene-d4	12.323	152	99241	43.136	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.280%		
Target Compounds					Qvalue	
13) Acetone	2.398	43	3105	2.414	ug/L	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030482.D
Acq On : 06 Aug 2022 22:58
Operator : JC/MD
Sample : N4066-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E54

Quant Time: Aug 07 05:46:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 06 02:08:42 2022
Response via : Initial Calibration

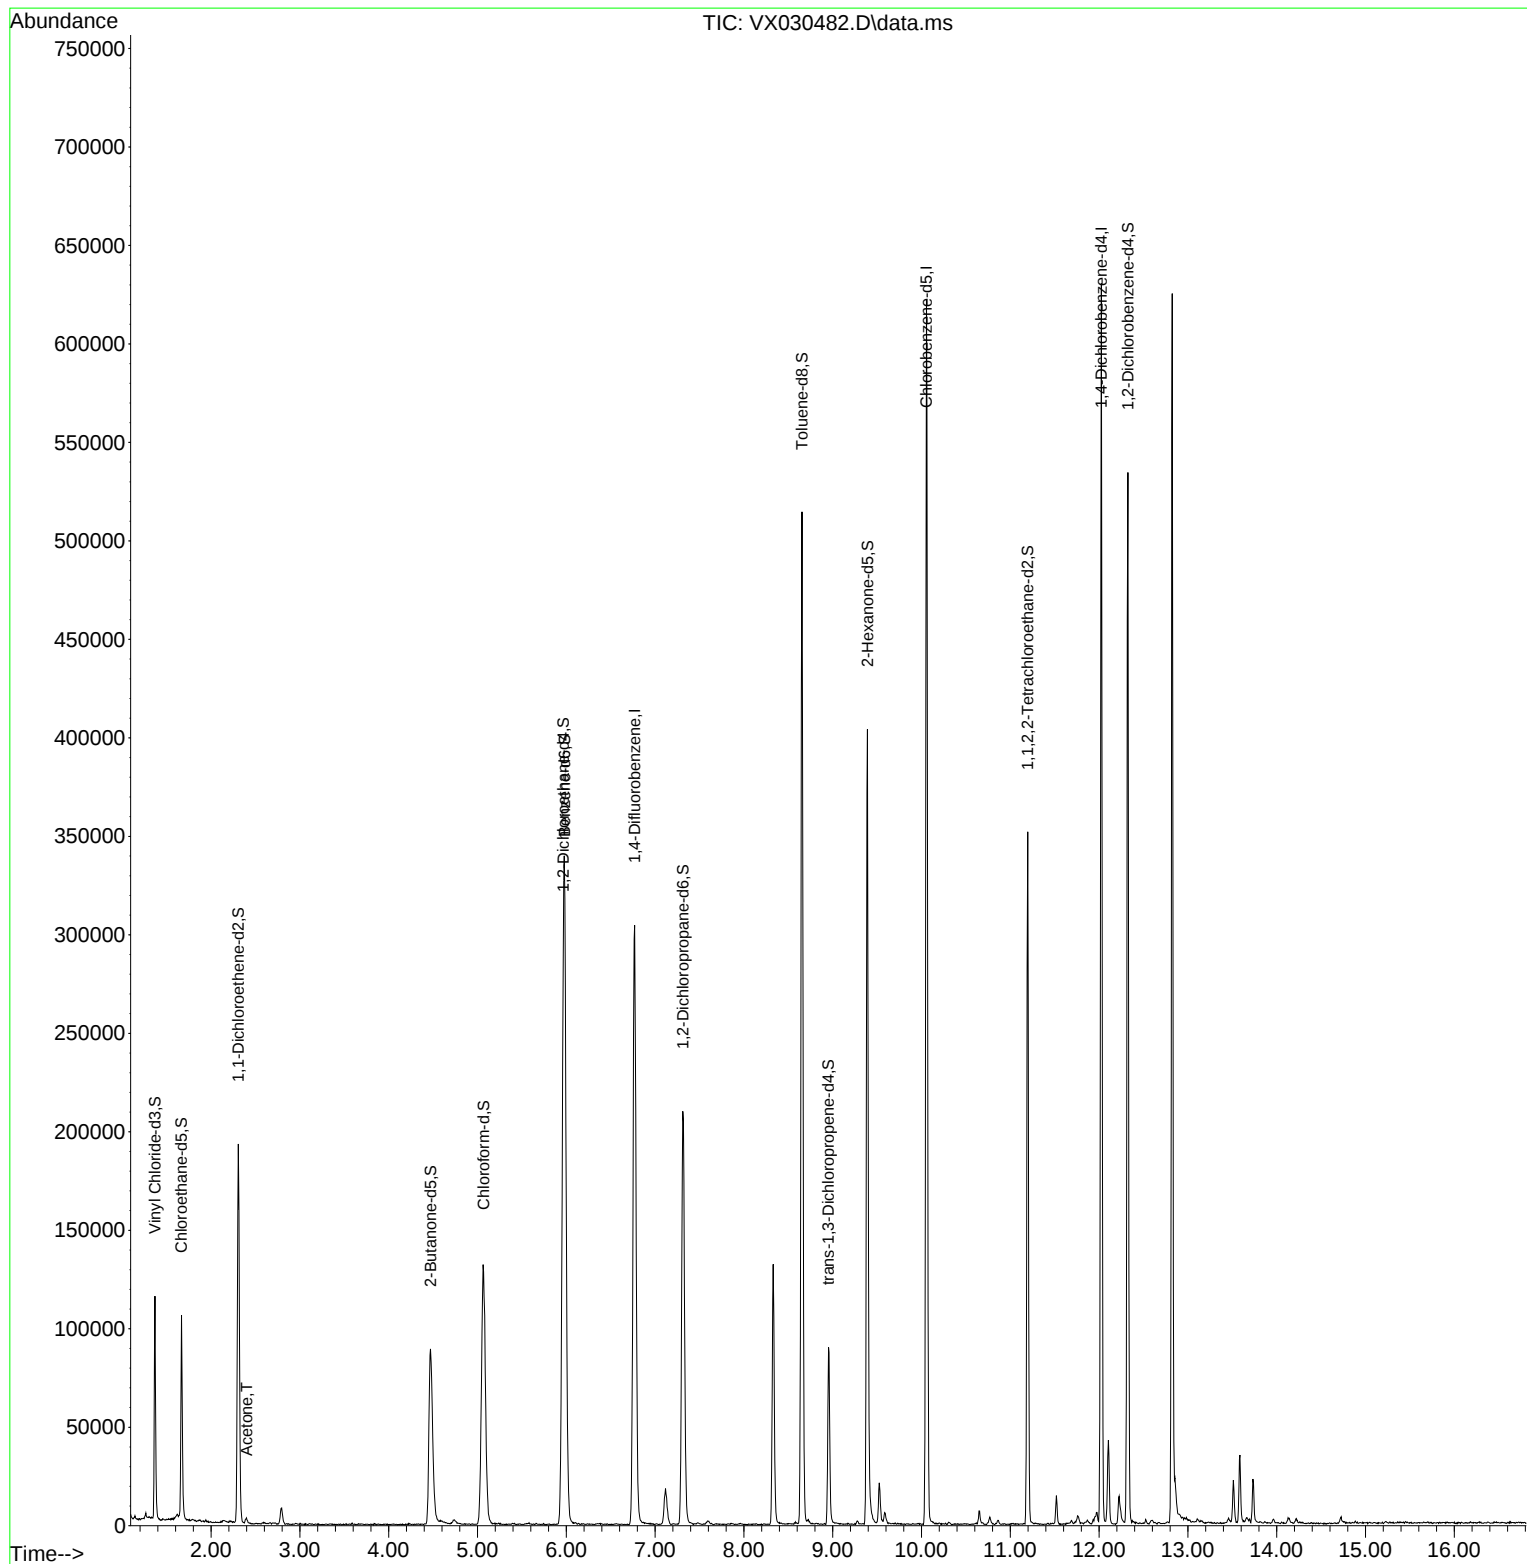

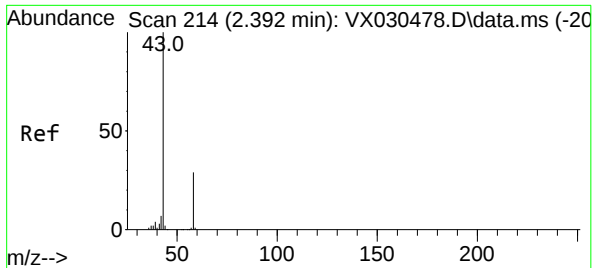

#13
Acetone
Concen: 2.414 ug/L
RT: 2.398 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX030482.D
Acq: 06 Aug 2022 22:58

Instrument :
MSVOA_X
ClientSampleId :
F5E54

Tgt Ion: 43	Resp: 3105
Ion Ratio	Lower Upper
43	100
58	13.9 0.0 57.8

