

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030454.D
 Acq On : 06 Aug 2022 11:13
 Operator : JC/MD
 Sample : VX0806WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK671

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030454.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB	126159	127992	12.18%	1.536%
2	1.666	91	95	101	rVB	100383	119469	11.37%	1.434%
3	2.306	194	200	210	rVB	214860	324770	30.92%	3.899%
4	2.502	230	232	233	rBV	785	659	0.06%	0.008%
5	2.721	264	268	270	rBV3	379	519	0.05%	0.006%
6	2.739	270	271	274	rVV	556	371	0.04%	0.004%
7	2.788	275	279	285	rVB4	2076	4047	0.39%	0.049%
8	2.855	286	290	291	rVB2	445	366	0.03%	0.004%
9	2.904	296	298	299	rBV	504	374	0.04%	0.004%
10	2.947	299	305	316	rVB2	6940	16628	1.58%	0.200%
11	3.099	326	330	332	rBV3	344	462	0.04%	0.006%
12	3.428	380	384	385	rBV2	489	632	0.06%	0.008%
13	3.526	397	400	402	rBV2	541	419	0.04%	0.005%
14	3.672	422	424	426	rBV2	352	343	0.03%	0.004%
15	3.849	449	453	455	rBV	365	396	0.04%	0.005%
16	4.001	477	478	482	rBV2	418	401	0.04%	0.005%
17	4.458	545	553	566	rBV	105392	303537	28.89%	3.644%
18	4.855	615	618	624	rBV3	438	964	0.09%	0.012%
19	4.940	627	632	635	rBV3	334	625	0.06%	0.008%
20	5.062	640	652	668	rVV	137472	435951	41.50%	5.233%
21	5.312	689	693	694	rVB	444	437	0.04%	0.005%
22	5.324	694	695	698	rBV3	562	451	0.04%	0.005%
23	5.379	700	704	705	rBV4	863	1254	0.12%	0.015%
24	5.452	714	716	719	rVB2	515	510	0.05%	0.006%
25	5.477	719	720	723	rBV	438	376	0.04%	0.005%
26	5.538	729	730	733	rBV2	583	681	0.06%	0.008%
27	5.623	742	744	747	rBV2	273	346	0.03%	0.004%
28	5.690	754	755	758	rBV2	371	393	0.04%	0.005%
29	5.763	764	767	769	rBV2	246	339	0.03%	0.004%
30	5.970	786	801	817	rBV2	352520	1050492	100.00%	12.611%
31	6.233	841	844	847	rVB2	341	365	0.03%	0.004%
32	6.458	878	881	882	rBV	473	441	0.04%	0.005%
33	6.531	890	893	894	rBV2	450	350	0.03%	0.004%
34	6.678	914	917	919	rVB2	437	485	0.05%	0.006%
35	6.763	921	931	946	rBV	295129	715842	68.14%	8.593%
36	7.110	981	988	999	rVV4	14152	33846	3.22%	0.406%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030454.D
 Acq On : 06 Aug 2022 11:13
 Operator : JC/MD
 Sample : VX0806WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK671

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.196	999	1002	1005	rVB2	280	395	0.04%	0.005%
38	7.226	1005	1007	1009	rBV	542	439	0.04%	0.005%
39	7.312	1012	1021	1038	rVB	225814	493386	46.97%	5.923%
40	7.592	1064	1067	1068	rVB2	497	397	0.04%	0.005%
41	7.683	1080	1082	1085	rBV2	430	439	0.04%	0.005%
42	7.787	1096	1099	1101	rVV2	315	375	0.04%	0.005%
43	7.830	1105	1106	1110	rBV2	342	395	0.04%	0.005%
44	7.933	1119	1123	1125	rBV2	855	1129	0.11%	0.014%
45	8.208	1167	1168	1170	rBV	517	390	0.04%	0.005%
46	8.257	1172	1176	1180	rBB	453	706	0.07%	0.008%
47	8.330	1181	1188	1199	rVV	147700	246872	23.50%	2.964%
48	8.488	1211	1214	1219	rVB3	670	956	0.09%	0.011%
49	8.653	1234	1241	1255	rBV	503584	794568	75.64%	9.538%
50	8.799	1263	1265	1271	rVB3	517	842	0.08%	0.010%
51	8.860	1273	1275	1277	rVV	474	378	0.04%	0.005%
52	8.903	1280	1282	1284	rBV2	408	451	0.04%	0.005%
53	8.952	1285	1290	1300	rVV	112656	164164	15.63%	1.971%
54	9.025	1300	1302	1305	rVV2	1025	1037	0.10%	0.012%
55	9.073	1309	1310	1312	rBV	690	466	0.04%	0.006%
56	9.098	1312	1314	1315	rVV2	651	386	0.04%	0.005%
57	9.275	1340	1343	1348	rVB4	1762	2085	0.20%	0.025%
58	9.348	1353	1355	1356	rBV	481	411	0.04%	0.005%
59	9.384	1356	1361	1374	rBV	458189	659762	62.81%	7.920%
60	9.659	1403	1406	1408	rVB3	505	518	0.05%	0.006%
61	9.701	1408	1413	1420	rBV5	2226	3522	0.34%	0.042%
62	9.775	1423	1425	1427	rBV	410	392	0.04%	0.005%
63	10.012	1460	1464	1465	rBV2	481	735	0.07%	0.009%
64	10.055	1465	1471	1483	rVV	635626	830843	79.09%	9.974%
65	10.171	1488	1490	1492	rBV	538	348	0.03%	0.004%
66	10.299	1509	1511	1513	rVV3	388	343	0.03%	0.004%
67	10.372	1520	1523	1525	rBV2	670	514	0.05%	0.006%
68	10.482	1539	1541	1544	rVB	543	383	0.04%	0.005%
69	10.652	1567	1569	1570	rBV	408	400	0.04%	0.005%
70	10.768	1586	1588	1590	rBV	335	354	0.03%	0.004%
71	10.835	1596	1599	1601	rBV2	252	353	0.03%	0.004%
72	10.945	1612	1617	1618	rBV2	548	654	0.06%	0.008%
73	11.195	1652	1658	1665	rBV	394492	503508	47.93%	6.044%
74	11.451	1697	1700	1702	rBV3	539	677	0.06%	0.008%
75	11.969	1781	1785	1786	rBV2	591	550	0.05%	0.007%
76	12.024	1788	1794	1803	rVV	602396	755622	71.93%	9.071%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030454.D
 Acq On : 06 Aug 2022 11:13
 Operator : JC/MD
 Sample : VX0806WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK671

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.152	1814	1815	1818	rBV2	474	435	0.04%	0.005%
78	12.183	1818	1820	1823	rVB2	443	480	0.05%	0.006%
79	12.323	1837	1843	1852	rBV	558010	701304	66.76%	8.419%
80	13.030	1957	1959	1961	rVV2	330	350	0.03%	0.004%
81	13.054	1961	1963	1966	rVV2	388	448	0.04%	0.005%
82	13.115	1971	1973	1979	rVV4	913	1282	0.12%	0.015%
83	13.365	2012	2014	2017	rBV	474	435	0.04%	0.005%
84	13.591	2048	2051	2056	rVV2	1162	1036	0.10%	0.012%
85	13.652	2058	2061	2063	rVB2	394	401	0.04%	0.005%
86	13.707	2068	2070	2072	rVB2	690	460	0.04%	0.006%
87	13.835	2089	2091	2095	rBV2	345	431	0.04%	0.005%
88	13.890	2099	2100	2101	rBV	754	376	0.04%	0.005%
89	13.963	2108	2112	2113	rBV	806	874	0.08%	0.010%
90	14.182	2146	2148	2151	rBV2	305	382	0.04%	0.005%
91	14.255	2158	2160	2163	rVB2	599	467	0.04%	0.006%
92	14.347	2172	2175	2178	rBV	340	499	0.05%	0.006%
93	14.377	2178	2180	2181	rBV	542	390	0.04%	0.005%
94	14.914	2266	2268	2271	rBV3	745	947	0.09%	0.011%
95	15.042	2287	2289	2290	rBV	750	478	0.05%	0.006%
96	15.219	2317	2318	2320	rBV2	749	500	0.05%	0.006%
97	15.383	2343	2345	2346	rVB	817	381	0.04%	0.005%
98	16.042	2451	2453	2456	rBV3	620	853	0.08%	0.010%
99	16.359	2503	2505	2508	rBV4	657	950	0.09%	0.011%
100	16.597	2542	2544	2545	rBV	595	364	0.03%	0.004%




Sum of corrected areas: 8330201

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030454.D
Acq On : 06 Aug 2022 11:13
Operator : JC/MD
Sample : VX0806WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK671

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

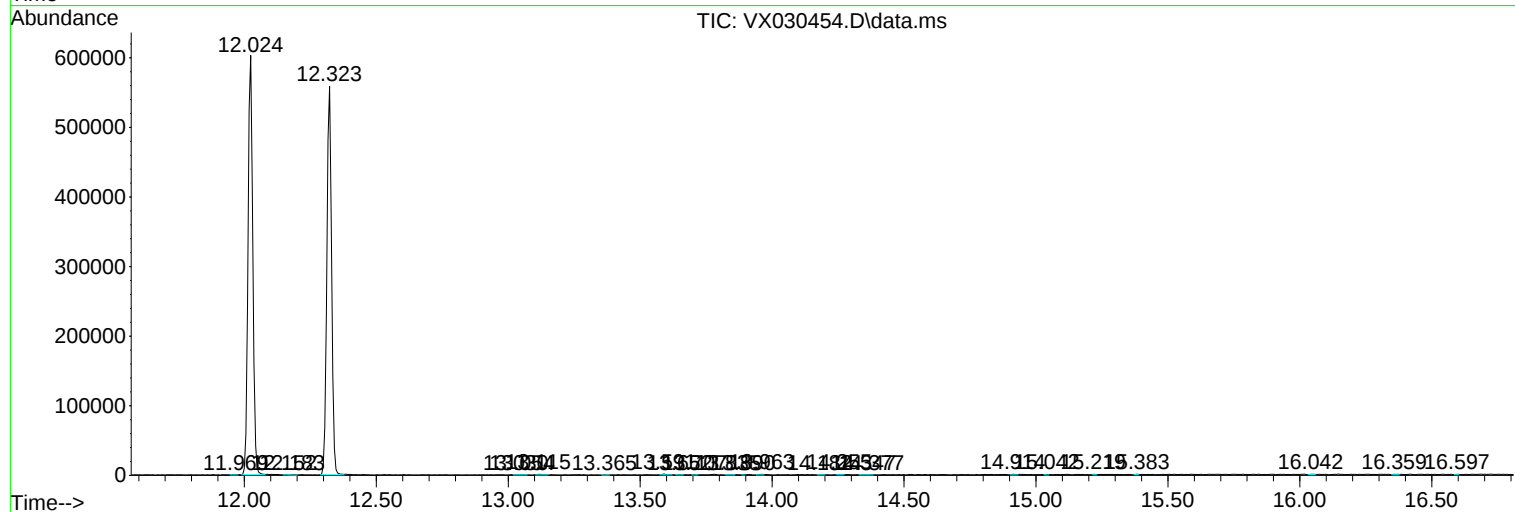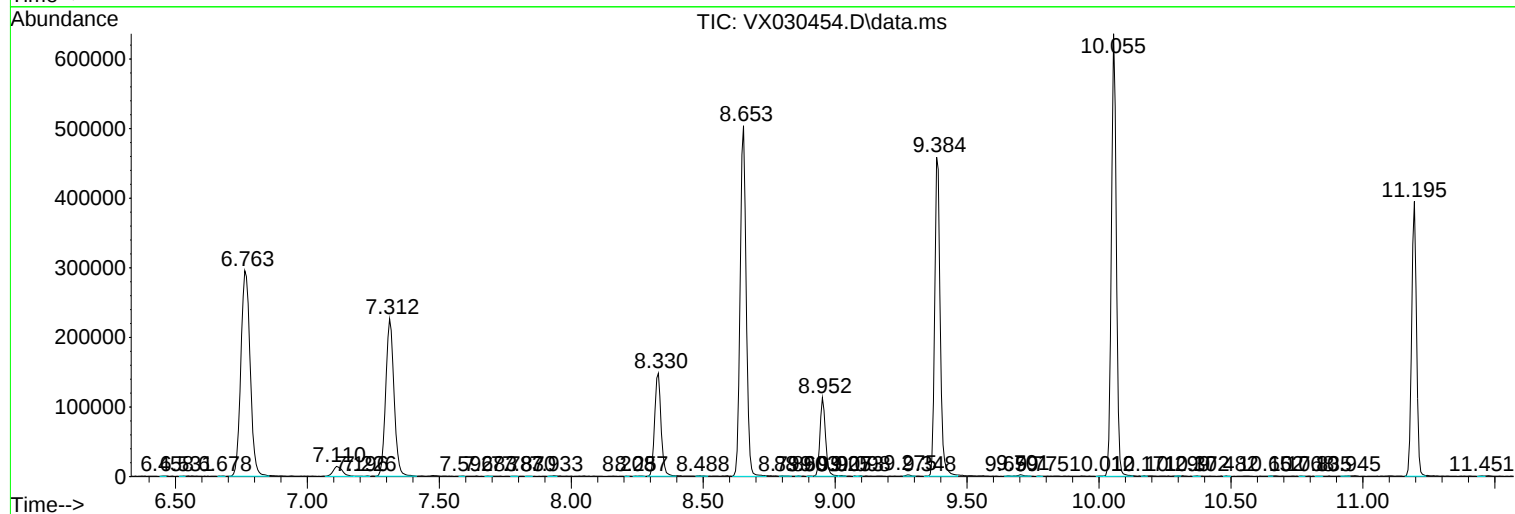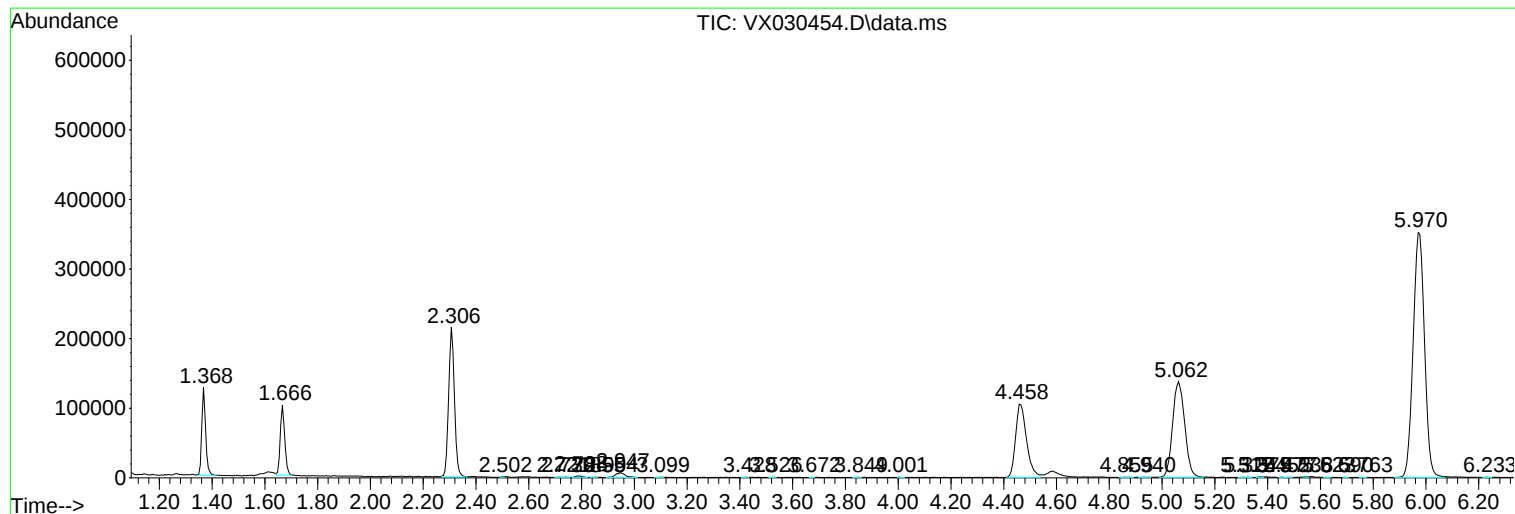

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030454.D
Acq On : 06 Aug 2022 11:13
Operator : JC/MD
Sample : VX0806WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK671

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030454.D
Acq On : 06 Aug 2022 11:13
Operator : JC/MD
Sample : VX0806WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK671

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc