

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030455.D
 Acq On : 06 Aug 2022 11:38
 Operator : JC/MD
 Sample : N4003-07DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D32DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030455.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB2	185990	200989	18.72%	2.217%
2	1.666	91	95	103	rVB	105649	128657	11.98%	1.419%
3	2.306	193	200	210	rVB	237618	363224	33.83%	4.006%
4	2.556	239	241	243	rBV	607	671	0.06%	0.007%
5	2.727	266	269	270	rBV	293	293	0.03%	0.003%
6	2.788	275	279	286	rVV4	2705	5474	0.51%	0.060%
7	2.861	290	291	294	rBV2	366	280	0.03%	0.003%
8	2.947	297	305	314	rBV2	9820	21455	2.00%	0.237%
9	3.093	323	329	337	rBV2	7783	15040	1.40%	0.166%
10	3.221	347	350	353	rVB2	298	412	0.04%	0.005%
11	3.245	353	354	359	rBV2	562	613	0.06%	0.007%
12	3.599	410	412	413	rVV	404	317	0.03%	0.003%
13	3.715	428	431	433	rBV2	414	496	0.05%	0.005%
14	3.788	440	443	447	rVB3	500	613	0.06%	0.007%
15	3.861	450	455	456	rBV2	385	444	0.04%	0.005%
16	3.898	460	461	463	rVB	590	280	0.03%	0.003%
17	3.922	463	465	467	rBV	457	384	0.04%	0.004%
18	3.952	467	470	472	rBV2	324	314	0.03%	0.003%
19	4.154	500	503	506	rBV2	397	459	0.04%	0.005%
20	4.202	508	511	512	rBV2	342	306	0.03%	0.003%
21	4.263	520	521	523	rBV2	425	294	0.03%	0.003%
22	4.489	545	558	570	rBV2	222055	748542	69.73%	8.256%
23	5.062	638	652	666	rBV	138287	435537	40.57%	4.804%
24	5.196	672	674	676	rBV3	588	530	0.05%	0.006%
25	5.306	688	692	693	rBV	412	421	0.04%	0.005%
26	5.391	701	706	710	rBV3	1089	2378	0.22%	0.026%
27	5.544	728	731	732	rBV2	1035	993	0.09%	0.011%
28	5.690	752	755	756	rBV	338	290	0.03%	0.003%
29	5.787	768	771	773	rVB2	496	563	0.05%	0.006%
30	5.970	789	801	820	rBV2	364635	1073536	100.00%	11.840%
31	6.464	879	882	885	rBV	397	556	0.05%	0.006%
32	6.550	893	896	897	rBV	387	374	0.03%	0.004%
33	6.598	902	904	907	rVB2	294	328	0.03%	0.004%
34	6.629	907	909	910	rBV	426	338	0.03%	0.004%
35	6.763	922	931	946	rBV	317706	756752	70.49%	8.346%
36	7.117	982	989	999	rVB5	14272	38936	3.63%	0.429%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030455.D
 Acq On : 06 Aug 2022 11:38
 Operator : JC/MD
 Sample : N4003-07DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D32DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.214	1002	1005	1007	rVB	359	409	0.04%	0.005%
38	7.238	1007	1009	1012	rVB2	386	328	0.03%	0.004%
39	7.312	1012	1021	1041	rBV	223471	489445	45.59%	5.398%
40	7.446	1041	1043	1044	rBV	531	521	0.05%	0.006%
41	7.543	1058	1059	1062	rBV	437	322	0.03%	0.004%
42	7.635	1072	1074	1078	rVV	466	449	0.04%	0.005%
43	7.696	1082	1084	1087	rBV	437	427	0.04%	0.005%
44	7.738	1089	1091	1094	rVB	332	273	0.03%	0.003%
45	7.799	1098	1101	1102	rBV	353	274	0.03%	0.003%
46	7.946	1124	1125	1128	rVV2	391	313	0.03%	0.003%
47	8.043	1137	1141	1143	rVB	449	512	0.05%	0.006%
48	8.080	1145	1147	1151	rBV	431	447	0.04%	0.005%
49	8.330	1181	1188	1199	rBV	147794	250208	23.31%	2.760%
50	8.653	1234	1241	1250	rVV	543253	846642	78.86%	9.338%
51	8.952	1284	1290	1300	rBV	112734	167761	15.63%	1.850%
52	9.092	1311	1313	1315	rBV	536	469	0.04%	0.005%
53	9.226	1333	1335	1337	rBV2	542	389	0.04%	0.004%
54	9.275	1337	1343	1347	rBV4	4525	6323	0.59%	0.070%
55	9.342	1351	1354	1355	rBV	349	370	0.03%	0.004%
56	9.384	1356	1361	1376	rBV	415325	596889	55.60%	6.583%
57	9.701	1409	1413	1419	rVB3	1614	2286	0.21%	0.025%
58	9.848	1435	1437	1438	rBV2	769	438	0.04%	0.005%
59	9.994	1459	1461	1463	rBV	388	265	0.02%	0.003%
60	10.055	1465	1471	1482	rBV	657620	887958	82.71%	9.793%
61	10.165	1487	1489	1491	rVB3	763	648	0.06%	0.007%
62	10.195	1491	1494	1496	rVB2	738	562	0.05%	0.006%
63	10.238	1496	1501	1505	rBV3	618	1162	0.11%	0.013%
64	10.299	1507	1511	1512	rBV2	629	582	0.05%	0.006%
65	10.372	1520	1523	1525	rBV3	569	646	0.06%	0.007%
66	10.500	1542	1544	1548	rBV2	449	460	0.04%	0.005%
67	10.622	1562	1564	1567	rVB2	362	303	0.03%	0.003%
68	10.665	1570	1571	1573	rBV2	337	301	0.03%	0.003%
69	10.811	1593	1595	1599	rBV2	270	359	0.03%	0.004%
70	10.939	1613	1616	1619	rBV2	350	552	0.05%	0.006%
71	10.963	1619	1620	1624	rVB	445	288	0.03%	0.003%
72	11.195	1652	1658	1669	rBV	372085	479792	44.69%	5.292%
73	11.372	1682	1687	1689	rBV2	458	622	0.06%	0.007%
74	11.439	1697	1698	1700	rBV	364	290	0.03%	0.003%
75	11.664	1734	1735	1737	rVB	576	322	0.03%	0.004%
76	11.713	1742	1743	1746	rVB	493	318	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030455.D
 Acq On : 06 Aug 2022 11:38
 Operator : JC/MD
 Sample : N4003-07DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D32DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.975	1784	1786	1788	rBV2	485	515	0.05%	0.006%
78	12.024	1789	1794	1803	rVV	683288	814356	75.86%	8.982%
79	12.177	1817	1819	1823	rBV	443	459	0.04%	0.005%
80	12.323	1837	1843	1849	rBV	557515	700717	65.27%	7.728%
81	12.481	1867	1869	1870	rBV2	379	295	0.03%	0.003%
82	12.628	1890	1893	1895	rBV3	482	493	0.05%	0.005%
83	12.719	1906	1908	1911	rVB2	490	374	0.03%	0.004%
84	12.750	1911	1913	1916	rBV2	395	436	0.04%	0.005%
85	12.792	1916	1920	1922	rVB2	335	356	0.03%	0.004%
86	12.859	1929	1931	1933	rBV2	359	305	0.03%	0.003%
87	13.079	1965	1967	1970	rBV2	592	833	0.08%	0.009%
88	13.201	1986	1987	1989	rBV	610	265	0.02%	0.003%
89	13.219	1989	1990	1993	rBV	365	396	0.04%	0.004%
90	13.530	2036	2041	2043	rBV2	600	667	0.06%	0.007%
91	13.560	2043	2046	2048	rBV2	465	510	0.05%	0.006%
92	13.591	2050	2051	2054	rBV2	597	619	0.06%	0.007%
93	14.030	2122	2123	2125	rBV	405	322	0.03%	0.004%
94	14.140	2139	2141	2144	rBV2	584	584	0.05%	0.006%
95	14.341	2172	2174	2176	rBV	407	422	0.04%	0.005%
96	14.524	2202	2204	2205	rBV	420	264	0.02%	0.003%
97	14.701	2231	2233	2234	rVB	703	373	0.03%	0.004%
98	15.146	2305	2306	2307	rBV	709	350	0.03%	0.004%
99	15.975	2439	2442	2443	rBV2	702	684	0.06%	0.008%
100	16.755	2568	2570	2571	rBV	597	296	0.03%	0.003%




Sum of corrected areas: 9066905

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030455.D
Acq On : 06 Aug 2022 11:38
Operator : JC/MD
Sample : N4003-07DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D32DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

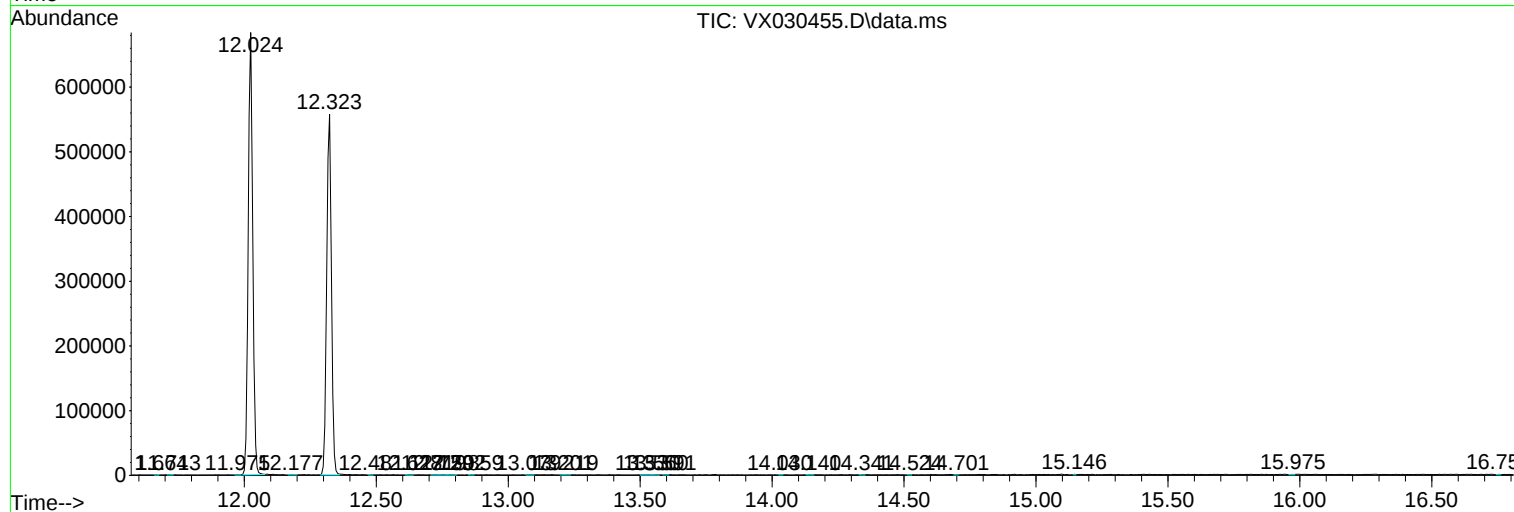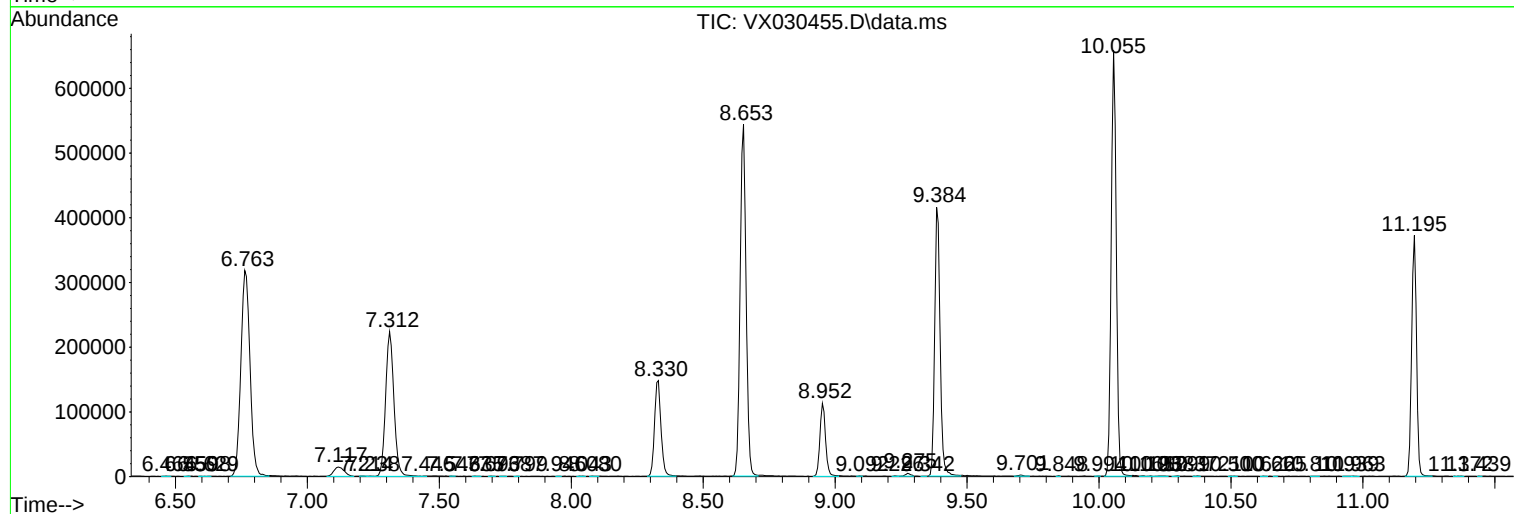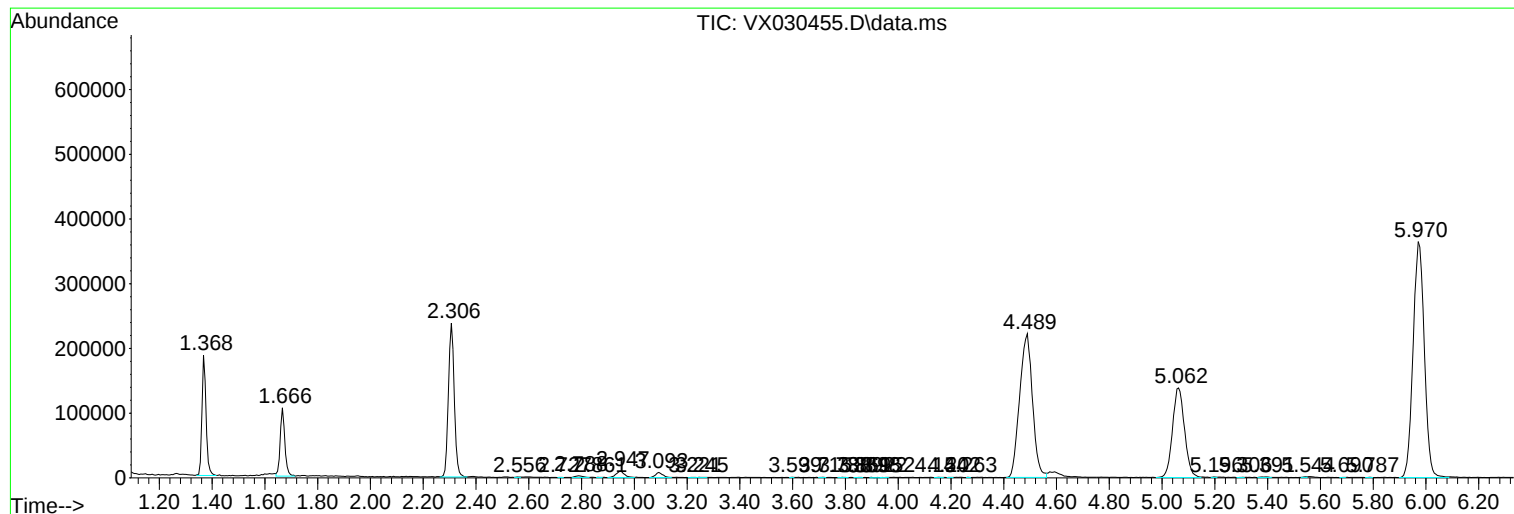

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030455.D
Acq On : 06 Aug 2022 11:38
Operator : JC/MD
Sample : N4003-07DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D32DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030455.D
Acq On : 06 Aug 2022 11:38
Operator : JC/MD
Sample : N4003-07DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D32DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------