

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030456.D
 Acq On : 06 Aug 2022 12:02
 Operator : JC/MD
 Sample : N4003-09DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D34DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030456.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB2	147434	161670	15.04%	1.717%
2	1.660	90	94	102	rBV	81131	97878	9.11%	1.040%
3	2.069	160	161	162	rBV	883	418	0.04%	0.004%
4	2.300	193	199	209	rVB	230492	348999	32.48%	3.707%
5	2.386	211	213	214	rBV	904	647	0.06%	0.007%
6	2.465	225	226	227	rBV	612	346	0.03%	0.004%
7	2.697	263	264	267	rBV2	784	517	0.05%	0.005%
8	2.788	274	279	286	rVB3	5426	10151	0.94%	0.108%
9	2.886	292	295	296	rBV2	512	549	0.05%	0.006%
10	2.947	296	305	316	rBV	21183	49213	4.58%	0.523%
11	3.093	323	329	336	rBV2	9017	17338	1.61%	0.184%
12	3.282	357	360	361	rBV2	395	339	0.03%	0.004%
13	3.434	380	385	388	rBV4	612	1033	0.10%	0.011%
14	3.544	400	403	405	rBV2	448	539	0.05%	0.006%
15	3.770	437	440	441	rBV2	461	396	0.04%	0.004%
16	3.800	443	445	449	rVB2	467	524	0.05%	0.006%
17	3.867	454	456	458	rVB2	359	368	0.03%	0.004%
18	3.891	458	460	462	rBV2	395	462	0.04%	0.005%
19	4.026	480	482	484	rBV	458	340	0.03%	0.004%
20	4.117	496	497	501	rVB2	394	416	0.04%	0.004%
21	4.489	544	558	570	rBV2	291519	902479	83.98%	9.585%
22	4.824	611	613	616	rVB2	445	478	0.04%	0.005%
23	4.903	624	626	628	rVB2	500	364	0.03%	0.004%
24	5.062	638	652	667	rBV	138638	437057	40.67%	4.642%
25	5.190	672	673	675	rBV2	437	402	0.04%	0.004%
26	5.214	675	677	681	rVV3	695	792	0.07%	0.008%
27	5.300	689	691	694	rBV2	290	342	0.03%	0.004%
28	5.385	700	705	708	rBV4	767	1410	0.13%	0.015%
29	5.477	718	720	721	rBV2	507	369	0.03%	0.004%
30	5.531	727	729	730	rBV	776	520	0.05%	0.006%
31	5.550	730	732	738	rVV4	1459	2716	0.25%	0.029%
32	5.672	749	752	754	rBV3	667	539	0.05%	0.006%
33	5.733	758	762	763	rBV2	537	547	0.05%	0.006%
34	5.970	790	801	818	rBV2	371509	1074609	100.00%	11.413%
35	6.354	858	864	865	rBV3	2090	3007	0.28%	0.032%
36	6.464	880	882	884	rBV	456	461	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030456.D
 Acq On : 06 Aug 2022 12:02
 Operator : JC/MD
 Sample : N4003-09DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D34DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.543	890	895	898	rBV2	480	748	0.07%	0.008%
38	6.763	922	931	946	rBV	310306	743661	69.20%	7.898%
39	6.885	949	951	953	rVB2	639	488	0.05%	0.005%
40	7.129	982	991	1002	rBV2	135979	312753	29.10%	3.322%
41	7.312	1012	1021	1039	rBV	224959	494437	46.01%	5.251%
42	7.476	1045	1048	1049	rBV2	852	771	0.07%	0.008%
43	7.751	1092	1093	1097	rBV2	511	570	0.05%	0.006%
44	7.830	1103	1106	1108	rVV2	651	547	0.05%	0.006%
45	7.909	1116	1119	1123	rBV2	430	638	0.06%	0.007%
46	7.958	1123	1127	1134	rVB6	1144	2396	0.22%	0.025%
47	8.171	1159	1162	1164	rBV2	314	406	0.04%	0.004%
48	8.250	1171	1175	1176	rBV	408	408	0.04%	0.004%
49	8.269	1176	1178	1180	rVB2	578	380	0.04%	0.004%
50	8.330	1180	1188	1202	rBV	154247	253520	23.59%	2.693%
51	8.586	1226	1230	1234	rBV4	1548	2150	0.20%	0.023%
52	8.653	1234	1241	1251	rBV	547914	851709	79.26%	9.046%
53	8.884	1277	1279	1281	rVB	591	433	0.04%	0.005%
54	8.952	1283	1290	1305	rBV	111938	166127	15.46%	1.764%
55	9.104	1311	1315	1316	rBV4	542	616	0.06%	0.007%
56	9.214	1329	1333	1335	rVB	633	533	0.05%	0.006%
57	9.275	1338	1343	1351	rVB	22594	31883	2.97%	0.339%
58	9.390	1356	1362	1375	rBV	367765	578778	53.86%	6.147%
59	9.604	1395	1397	1401	rBV2	611	860	0.08%	0.009%
60	9.665	1405	1407	1410	rVV2	372	425	0.04%	0.005%
61	9.707	1410	1414	1421	rVB5	1758	3391	0.32%	0.036%
62	9.775	1423	1425	1428	rVB	465	500	0.05%	0.005%
63	9.811	1428	1431	1435	rVB	405	569	0.05%	0.006%
64	10.055	1466	1471	1484	rVB	658751	876408	81.56%	9.308%
65	10.201	1493	1495	1499	rVB4	1514	1226	0.11%	0.013%
66	10.305	1509	1512	1521	rBV3	1361	2477	0.23%	0.026%
67	10.549	1549	1552	1554	rBV2	408	438	0.04%	0.005%
68	10.640	1565	1567	1570	rBV3	1197	1544	0.14%	0.016%
69	10.969	1617	1621	1623	rVB2	989	1103	0.10%	0.012%
70	11.049	1631	1634	1637	rBV2	294	385	0.04%	0.004%
71	11.079	1637	1639	1641	rBV2	303	365	0.03%	0.004%
72	11.195	1653	1658	1665	rBV	366507	466386	43.40%	4.953%
73	11.341	1680	1682	1685	rBV	560	384	0.04%	0.004%
74	11.671	1733	1736	1741	rBV2	507	1083	0.10%	0.012%
75	11.719	1741	1744	1745	rVV	716	649	0.06%	0.007%
76	11.756	1747	1750	1753	rVV3	1111	1141	0.11%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030456.D
 Acq On : 06 Aug 2022 12:02
 Operator : JC/MD
 Sample : N4003-09DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D34DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.969	1784	1785	1789	rVV2	615	666	0.06%	0.007%
78	12.024	1789	1794	1803	rBV	639499	780531	72.63%	8.290%
79	12.146	1811	1814	1816	rVB2	453	512	0.05%	0.005%
80	12.170	1816	1818	1822	rBV3	467	458	0.04%	0.005%
81	12.323	1835	1843	1849	rBV	576156	698491	65.00%	7.418%
82	12.689	1902	1903	1907	rBV3	428	612	0.06%	0.006%
83	12.725	1907	1909	1912	rVV2	458	471	0.04%	0.005%
84	13.042	1959	1961	1962	rBV	411	363	0.03%	0.004%
85	13.115	1971	1973	1976	rVB2	1292	1199	0.11%	0.013%
86	13.536	2039	2042	2045	rVB2	732	773	0.07%	0.008%
87	13.591	2045	2051	2054	rBV3	868	1689	0.16%	0.018%
88	13.737	2073	2075	2078	rBV	585	505	0.05%	0.005%
89	13.780	2080	2082	2087	rBB	1410	1616	0.15%	0.017%
90	13.969	2111	2113	2116	rVB2	973	854	0.08%	0.009%
91	14.194	2147	2150	2153	rVV	513	709	0.07%	0.008%
92	14.335	2171	2173	2176	rVB2	614	582	0.05%	0.006%
93	14.493	2198	2199	2202	rBV	614	510	0.05%	0.005%
94	14.701	2231	2233	2234	rBV	887	538	0.05%	0.006%
95	14.810	2249	2251	2254	rVB2	603	539	0.05%	0.006%
96	14.944	2271	2273	2275	rVB	812	616	0.06%	0.007%
97	15.085	2294	2296	2298	rBV	529	458	0.04%	0.005%
98	16.078	2458	2459	2460	rBV	924	469	0.04%	0.005%
99	16.170	2472	2474	2475	rBV	613	487	0.05%	0.005%
100	16.712	2562	2563	2566	rVB	964	539	0.05%	0.006%


Sum of corrected areas: 9415708

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030456.D
Acq On : 06 Aug 2022 12:02
Operator : JC/MD
Sample : N4003-09DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D34DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

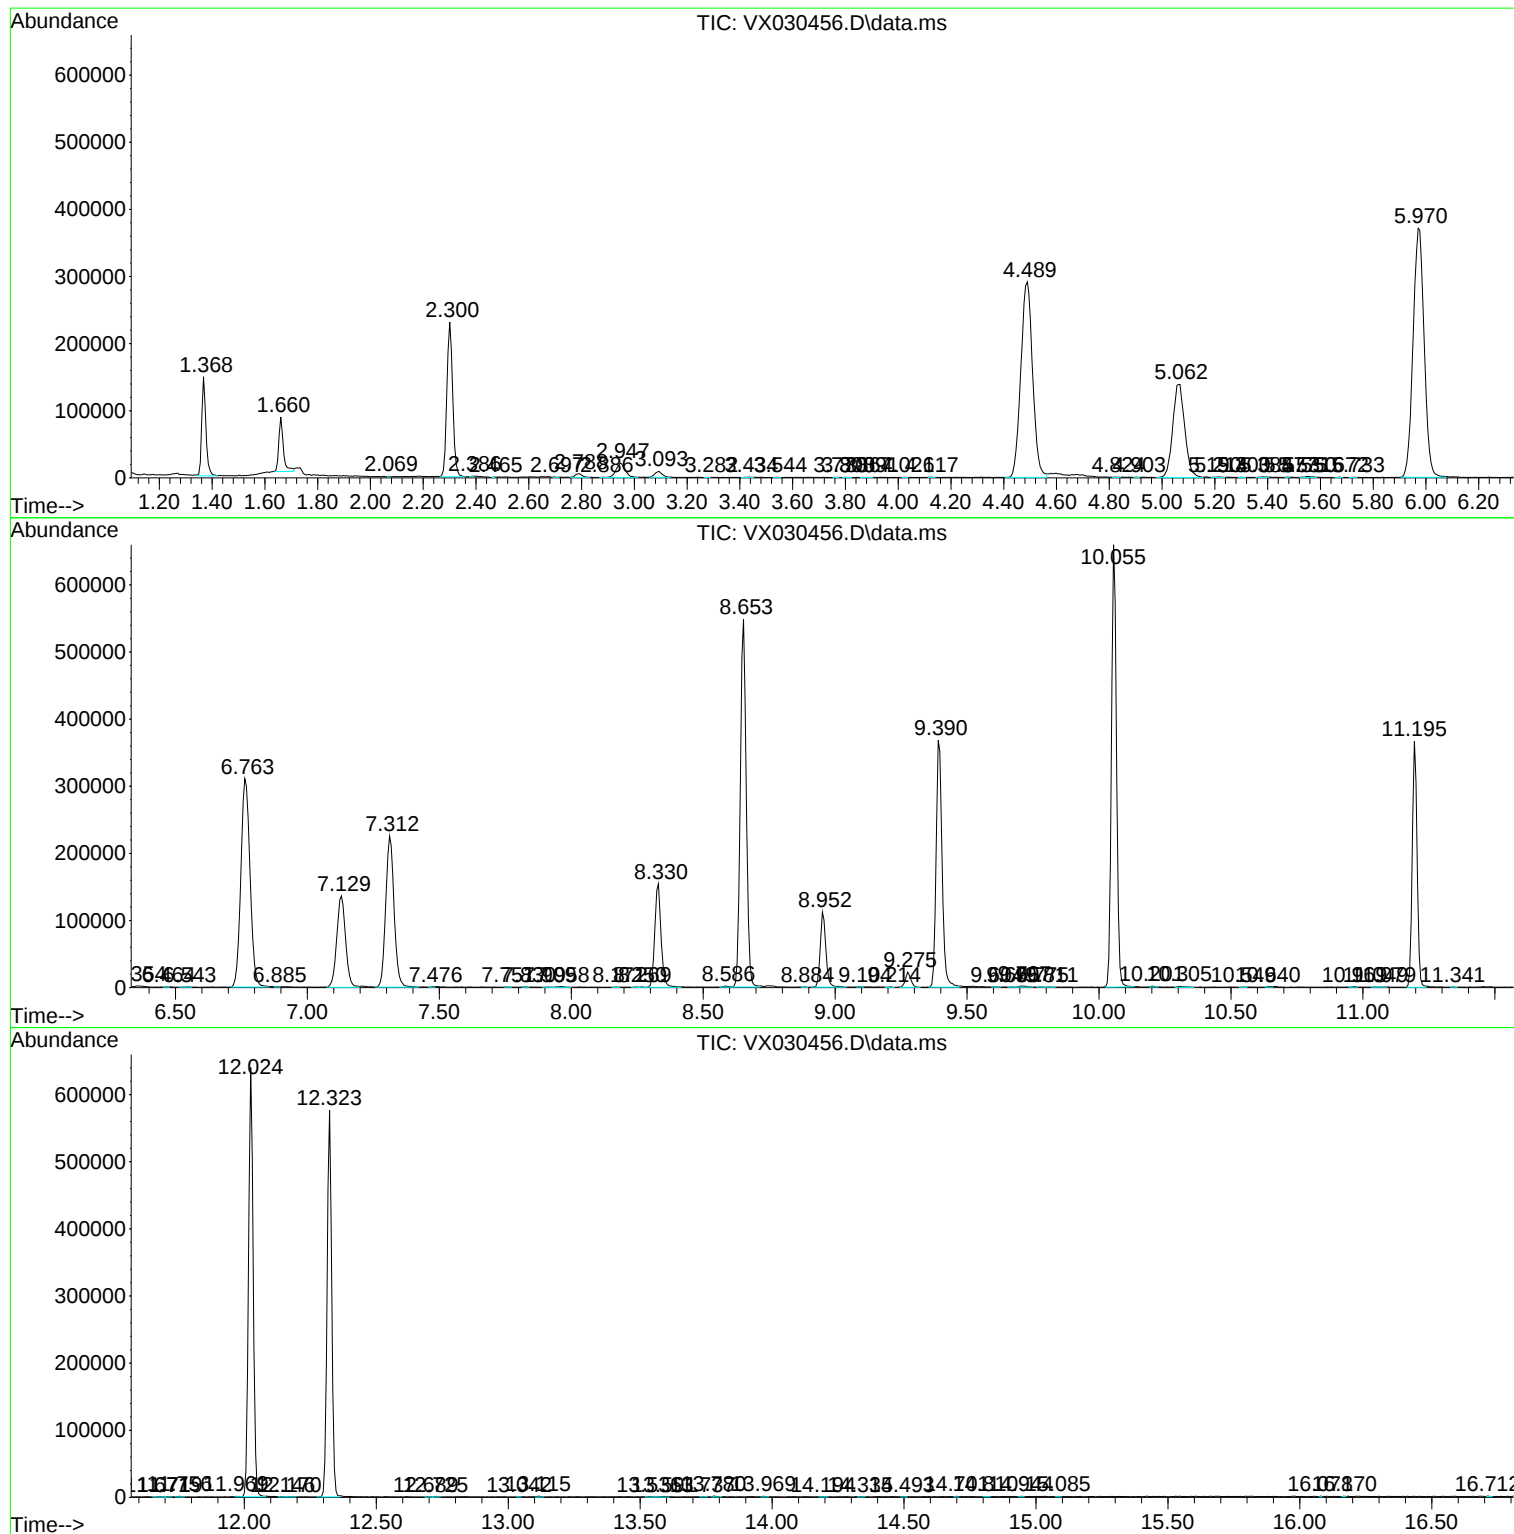

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030456.D
Acq On : 06 Aug 2022 12:02
Operator : JC/MD
Sample : N4003-09DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D34DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030456.D
Acq On : 06 Aug 2022 12:02
Operator : JC/MD
Sample : N4003-09DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D34DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------