

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030457.D
 Acq On : 06 Aug 2022 12:25
 Operator : JC/MD
 Sample : N4003-11DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D58DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030457.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB2	159972	178584	16.15%	1.947%
2	1.660	91	94	102	rVB	76130	84820	7.67%	0.925%
3	2.300	192	199	209	rVB	232957	357919	32.36%	3.902%
4	2.508	231	233	241	rVB3	1080	1570	0.14%	0.017%
5	2.569	241	243	244	rBV2	553	432	0.04%	0.005%
6	2.654	253	257	258	rBV2	1069	1040	0.09%	0.011%
7	2.788	273	279	286	rVB2	6755	11189	1.01%	0.122%
8	2.947	297	305	321	rVV	27387	65629	5.93%	0.716%
9	3.093	321	329	340	rVB3	6112	12906	1.17%	0.141%
10	3.203	345	347	349	rBV	418	342	0.03%	0.004%
11	3.434	382	385	390	rVB5	795	1382	0.12%	0.015%
12	3.587	409	410	413	rBV2	573	501	0.05%	0.005%
13	3.757	437	438	444	rVB2	357	509	0.05%	0.006%
14	3.849	450	453	455	rVB2	390	367	0.03%	0.004%
15	3.910	459	463	465	rVB2	301	427	0.04%	0.005%
16	4.208	510	512	515	rBV2	397	418	0.04%	0.005%
17	4.373	536	539	543	rBV2	387	454	0.04%	0.005%
18	4.489	546	558	570	rBV2	269278	824209	74.53%	8.986%
19	5.062	640	652	670	rVB2	146955	442856	40.04%	4.829%
20	5.385	700	705	707	rBV2	1436	2314	0.21%	0.025%
21	5.519	724	727	728	rBV2	416	496	0.04%	0.005%
22	5.538	728	730	731	rVV	751	699	0.06%	0.008%
23	5.556	731	733	737	rVB3	1402	1712	0.15%	0.019%
24	5.739	761	763	766	rBV3	418	552	0.05%	0.006%
25	5.787	766	771	772	rBV3	361	563	0.05%	0.006%
26	5.885	785	787	790	rBV2	309	360	0.03%	0.004%
27	5.970	790	801	819	rBV2	377019	1105937	100.00%	12.058%
28	6.251	846	847	848	rBV	651	345	0.03%	0.004%
29	6.367	858	866	874	rBV5	2395	7315	0.66%	0.080%
30	6.428	874	876	878	rVB	591	443	0.04%	0.005%
31	6.519	888	891	893	rBV2	277	352	0.03%	0.004%
32	6.623	906	908	910	rBV	581	342	0.03%	0.004%
33	6.659	912	914	918	rVB3	326	400	0.04%	0.004%
34	6.702	918	921	922	rBV	426	372	0.03%	0.004%
35	6.763	922	931	943	rBV	315170	761236	68.83%	8.300%
36	7.007	969	971	973	rVB2	468	351	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030457.D
 Acq On : 06 Aug 2022 12:25
 Operator : JC/MD
 Sample : N4003-11DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D58DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.117	979	989	998	rBV7	12928	33985	3.07%	0.371%
38	7.202	1001	1003	1005	rBV2	599	578	0.05%	0.006%
39	7.312	1013	1021	1037	rVB2	226340	494789	44.74%	5.395%
40	7.830	1104	1106	1110	rVB3	744	871	0.08%	0.009%
41	7.921	1115	1121	1122	rBV	618	998	0.09%	0.011%
42	8.104	1148	1151	1155	rBV	465	526	0.05%	0.006%
43	8.226	1167	1171	1175	rBV2	302	547	0.05%	0.006%
44	8.330	1181	1188	1200	rBV	151202	251218	22.72%	2.739%
45	8.488	1213	1214	1218	rVB2	783	723	0.07%	0.008%
46	8.537	1218	1222	1223	rBV2	408	393	0.04%	0.004%
47	8.592	1227	1231	1234	rBV4	1960	2384	0.22%	0.026%
48	8.653	1234	1241	1249	rBV	570337	875170	79.13%	9.542%
49	8.952	1285	1290	1303	rBV	106138	165509	14.97%	1.805%
50	9.086	1308	1312	1314	rBV3	469	717	0.06%	0.008%
51	9.159	1322	1324	1332	rVB4	926	1486	0.13%	0.016%
52	9.275	1340	1343	1348	rVB4	1757	2844	0.26%	0.031%
53	9.397	1356	1363	1378	rBV	365816	581519	52.58%	6.340%
54	9.610	1395	1398	1399	rBV2	799	729	0.07%	0.008%
55	9.714	1412	1415	1420	rVV6	2972	4373	0.40%	0.048%
56	9.836	1433	1435	1438	rVV2	532	505	0.05%	0.006%
57	9.903	1444	1446	1450	rVB3	425	450	0.04%	0.005%
58	10.055	1465	1471	1487	rBV	660903	895328	80.96%	9.762%
59	10.195	1491	1494	1500	rVB3	1835	2724	0.25%	0.030%
60	10.311	1508	1513	1519	rVB5	1527	2831	0.26%	0.031%
61	10.366	1520	1522	1526	rBV2	472	555	0.05%	0.006%
62	10.433	1529	1533	1534	rBV2	547	448	0.04%	0.005%
63	10.652	1564	1569	1576	rVB5	2188	4436	0.40%	0.048%
64	10.756	1584	1586	1590	rBV2	415	386	0.03%	0.004%
65	10.811	1592	1595	1597	rBV3	830	921	0.08%	0.010%
66	10.854	1600	1602	1605	rVB2	470	442	0.04%	0.005%
67	10.969	1616	1621	1625	rVB2	1789	2712	0.25%	0.030%
68	11.006	1625	1627	1629	rBV	491	352	0.03%	0.004%
69	11.195	1653	1658	1665	rBV	366735	468166	42.33%	5.104%
70	11.378	1684	1688	1689	rBV2	425	423	0.04%	0.005%
71	11.457	1697	1701	1704	rBV3	1913	2790	0.25%	0.030%
72	11.573	1719	1720	1723	rBV2	499	430	0.04%	0.005%
73	11.756	1747	1750	1754	rVB	1469	2119	0.19%	0.023%
74	11.866	1765	1768	1771	rVB3	661	537	0.05%	0.006%
75	11.963	1782	1784	1785	rBV	1379	1130	0.10%	0.012%
76	12.024	1789	1794	1802	rBV	641884	784538	70.94%	8.554%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030457.D
 Acq On : 06 Aug 2022 12:25
 Operator : JC/MD
 Sample : N4003-11DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D58DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.238	1827	1829	1831	rVB2	573	530	0.05%	0.006%
78	12.323	1837	1843	1852	rBV	549763	692023	62.57%	7.545%
79	12.616	1889	1891	1892	rVB	609	397	0.04%	0.004%
80	12.859	1929	1931	1933	rVV2	660	546	0.05%	0.006%
81	12.902	1936	1938	1941	rVV2	371	404	0.04%	0.004%
82	13.012	1954	1956	1958	rVB	479	354	0.03%	0.004%
83	13.109	1970	1972	1979	rVB3	1253	1681	0.15%	0.018%
84	13.182	1982	1984	1986	rBV2	469	434	0.04%	0.005%
85	13.274	1998	1999	2003	rBV2	369	364	0.03%	0.004%
86	13.451	2026	2028	2030	rVB	454	347	0.03%	0.004%
87	13.536	2041	2042	2047	rVB2	484	526	0.05%	0.006%
88	13.597	2047	2052	2056	rBV3	1068	2280	0.21%	0.025%
89	13.780	2079	2082	2086	rVB3	1601	1798	0.16%	0.020%
90	13.969	2110	2113	2117	rBV2	1188	1499	0.14%	0.016%
91	14.585	2212	2214	2216	rBV	642	723	0.07%	0.008%
92	14.725	2235	2237	2240	rBV2	543	718	0.06%	0.008%
93	14.944	2271	2273	2275	rBV	531	465	0.04%	0.005%
94	15.383	2343	2345	2348	rVV2	718	525	0.05%	0.006%
95	15.560	2371	2374	2376	rVB2	736	710	0.06%	0.008%
96	15.694	2393	2396	2398	rBV	869	1178	0.11%	0.013%
97	15.737	2401	2403	2407	rVB	981	857	0.08%	0.009%
98	16.066	2454	2457	2460	rBV2	737	930	0.08%	0.010%
99	16.151	2470	2471	2474	rBV	981	625	0.06%	0.007%
100	16.615	2546	2547	2549	rBV	1016	837	0.08%	0.009%




Sum of corrected areas: 9171676

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030457.D
Acq On : 06 Aug 2022 12:25
Operator : JC/MD
Sample : N4003-11DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D58DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

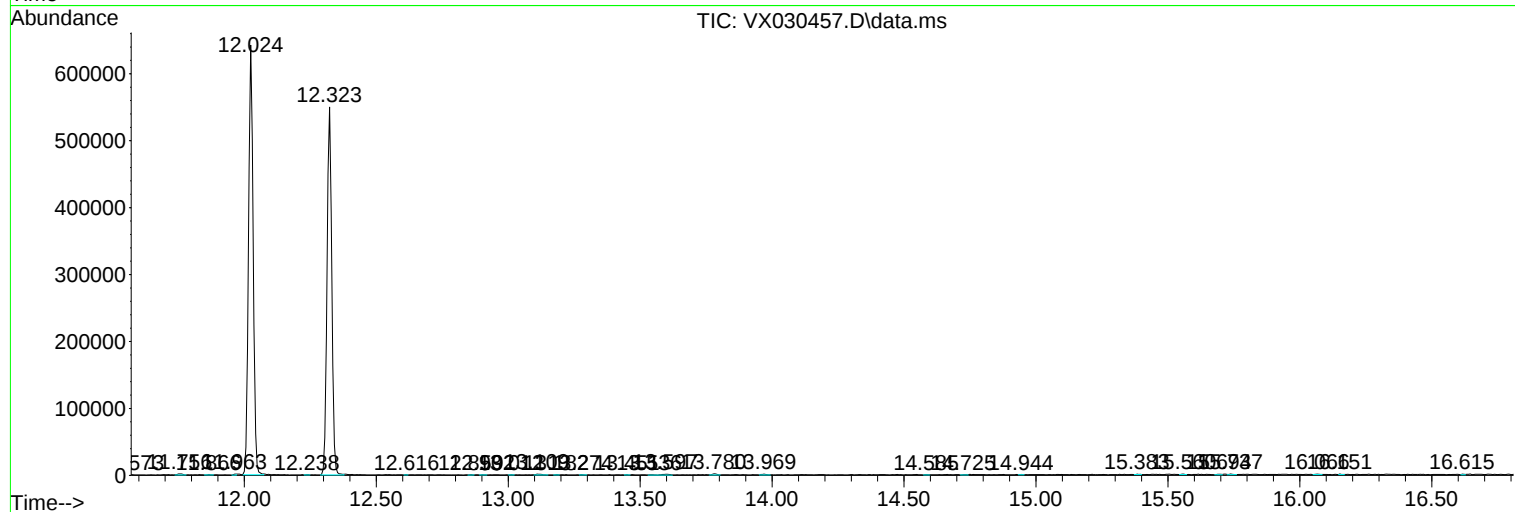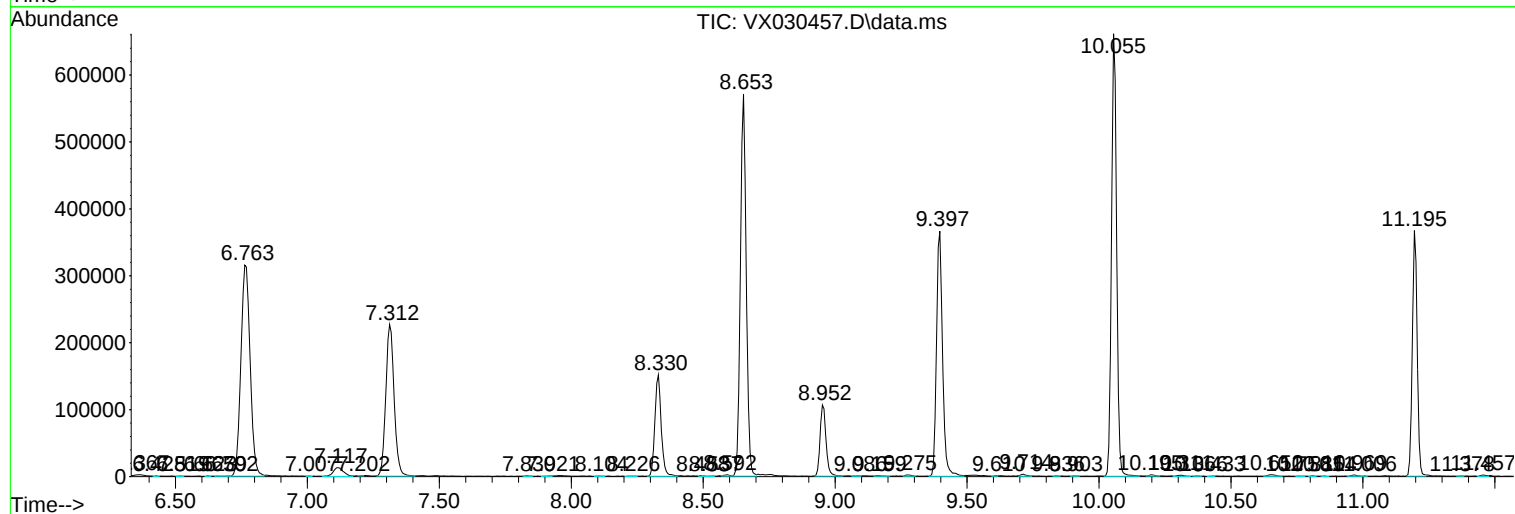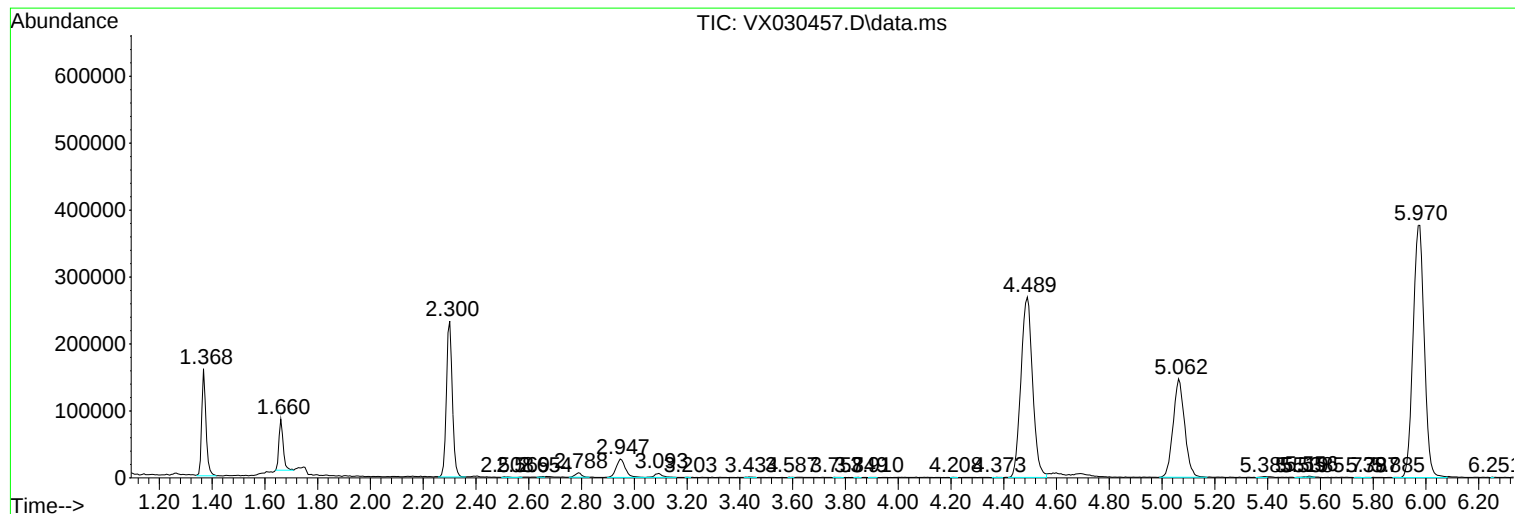

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030457.D
Acq On : 06 Aug 2022 12:25
Operator : JC/MD
Sample : N4003-11DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D58DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030457.D
Acq On : 06 Aug 2022 12:25
Operator : JC/MD
Sample : N4003-11DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D58DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc