

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030458.D
 Acq On : 06 Aug 2022 12:48
 Operator : JC/MD
 Sample : N4003-19DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D89DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030458.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	57	rVB2	248965	313705	28.64%	3.426%
2	1.660	90	94	100	rBV	80691	96616	8.82%	1.055%
3	2.300	193	199	210	rVB	220665	350508	32.00%	3.828%
4	2.501	229	232	234	rBV3	781	1147	0.10%	0.013%
5	2.788	274	279	290	rBV5	5352	14273	1.30%	0.156%
6	2.946	296	305	318	rBV	22954	53544	4.89%	0.585%
7	3.093	322	329	340	rVB4	13662	29904	2.73%	0.327%
8	3.251	353	355	357	rVB2	390	304	0.03%	0.003%
9	3.282	357	360	363	rBV3	244	390	0.04%	0.004%
10	3.330	365	368	370	rBV2	389	494	0.05%	0.005%
11	3.623	414	416	419	rVB	472	602	0.05%	0.007%
12	3.654	419	421	423	rVB2	462	370	0.03%	0.004%
13	3.751	435	437	438	rVB	587	320	0.03%	0.003%
14	3.830	448	450	453	rVB	479	372	0.03%	0.004%
15	3.885	457	459	462	rBV	268	281	0.03%	0.003%
16	3.971	472	473	475	rBV	453	383	0.03%	0.004%
17	4.147	499	502	505	rVB2	470	723	0.07%	0.008%
18	4.184	505	508	511	rBV2	546	848	0.08%	0.009%
19	4.227	513	515	518	rVB	481	420	0.04%	0.005%
20	4.306	520	528	533	rBV4	1919	4776	0.44%	0.052%
21	4.489	546	558	571	rBV2	202128	650089	59.36%	7.099%
22	4.909	626	627	629	rBV2	466	282	0.03%	0.003%
23	4.970	636	637	639	rBV2	530	452	0.04%	0.005%
24	5.068	641	653	669	rVB	144202	445761	40.70%	4.868%
25	5.281	685	688	689	rBV3	440	495	0.05%	0.005%
26	5.385	702	705	706	rBV2	725	943	0.09%	0.010%
27	5.671	751	752	757	rVB3	423	429	0.04%	0.005%
28	5.787	769	771	773	rBV2	359	273	0.02%	0.003%
29	5.970	789	801	819	rBV2	378128	1095216	100.00%	11.960%
30	6.141	828	829	832	rVB2	517	356	0.03%	0.004%
31	6.354	859	864	871	rVV6	2657	6418	0.59%	0.070%
32	6.555	890	897	898	rBV3	568	964	0.09%	0.011%
33	6.763	922	931	944	rVV	324109	764699	69.82%	8.350%
34	7.055	977	979	982	rBV2	366	325	0.03%	0.004%
35	7.116	982	989	999	rVB4	10341	26380	2.41%	0.288%
36	7.214	999	1005	1010	rBV3	1108	2776	0.25%	0.030%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030458.D
 Acq On : 06 Aug 2022 12:48
 Operator : JC/MD
 Sample : N4003-19DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D89DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.311	1013	1021	1041	rVB	224647	508400	46.42%	5.552%
38	7.464	1044	1046	1047	rBV2	573	355	0.03%	0.004%
39	7.720	1086	1088	1090	rVB	500	361	0.03%	0.004%
40	7.958	1122	1127	1132	rBV5	1230	2481	0.23%	0.027%
41	8.049	1139	1142	1144	rBV2	431	370	0.03%	0.004%
42	8.067	1144	1145	1147	rVV	349	333	0.03%	0.004%
43	8.110	1150	1152	1155	rVB2	399	404	0.04%	0.004%
44	8.141	1155	1157	1158	rBV	364	274	0.03%	0.003%
45	8.232	1169	1172	1175	rBV	393	494	0.05%	0.005%
46	8.330	1181	1188	1200	rBV	151842	250423	22.87%	2.735%
47	8.458	1207	1209	1211	rBV	447	367	0.03%	0.004%
48	8.586	1226	1230	1234	rBV4	1308	2297	0.21%	0.025%
49	8.653	1234	1241	1250	rBV	557894	866995	79.16%	9.467%
50	8.817	1267	1268	1271	rBV2	592	348	0.03%	0.004%
51	8.909	1281	1283	1284	rBV2	535	354	0.03%	0.004%
52	8.951	1285	1290	1300	rVV	109646	164835	15.05%	1.800%
53	9.055	1305	1307	1308	rBV2	420	276	0.03%	0.003%
54	9.110	1313	1316	1319	rBV2	754	813	0.07%	0.009%
55	9.274	1340	1343	1348	rVV5	1549	2332	0.21%	0.025%
56	9.396	1357	1363	1376	rBV	361561	577513	52.73%	6.306%
57	9.713	1410	1415	1419	rBV5	2188	3825	0.35%	0.042%
58	9.829	1432	1434	1436	rBV2	324	332	0.03%	0.004%
59	10.055	1466	1471	1479	rBV	659512	893658	81.60%	9.759%
60	10.165	1488	1489	1492	rBV3	760	735	0.07%	0.008%
61	10.195	1492	1494	1501	rVB3	1679	2269	0.21%	0.025%
62	10.305	1509	1512	1517	rVB3	1248	1954	0.18%	0.021%
63	10.390	1524	1526	1528	rBV2	525	388	0.04%	0.004%
64	10.408	1528	1529	1532	rVB	427	302	0.03%	0.003%
65	10.494	1540	1543	1544	rBV	429	343	0.03%	0.004%
66	10.652	1564	1569	1573	rBV5	1539	3118	0.28%	0.034%
67	10.762	1584	1587	1589	rBV	560	524	0.05%	0.006%
68	10.811	1593	1595	1598	rVB2	415	399	0.04%	0.004%
69	10.933	1612	1615	1616	rBV	311	278	0.03%	0.003%
70	10.969	1616	1621	1626	rBV3	1030	1824	0.17%	0.020%
71	11.061	1635	1636	1638	rVB	410	272	0.02%	0.003%
72	11.195	1652	1658	1665	rBV	368970	475286	43.40%	5.190%
73	11.335	1679	1681	1683	rVB	685	331	0.03%	0.004%
74	11.353	1683	1684	1687	rBV	492	392	0.04%	0.004%
75	11.457	1697	1701	1703	rBV2	1088	1507	0.14%	0.016%
76	11.542	1714	1715	1719	rVB2	532	345	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030458.D
 Acq On : 06 Aug 2022 12:48
 Operator : JC/MD
 Sample : N4003-19DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D89DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.756	1747	1750	1755	rVB3	939	1389	0.13%	0.015%
78	11.878	1768	1770	1771	rBV	357	274	0.03%	0.003%
79	12.024	1789	1794	1807	rBV	672683	806858	73.67%	8.811%
80	12.170	1817	1818	1819	rBV	608	309	0.03%	0.003%
81	12.213	1822	1825	1827	rBV	315	420	0.04%	0.005%
82	12.323	1837	1843	1854	rBV	589707	704274	64.30%	7.691%
83	12.451	1862	1864	1866	rBV2	400	398	0.04%	0.004%
84	12.792	1915	1920	1923	rBV2	403	702	0.06%	0.008%
85	13.115	1970	1973	1974	rBV2	535	443	0.04%	0.005%
86	13.207	1986	1988	1990	rBV	433	346	0.03%	0.004%
87	13.249	1994	1995	2000	rBV2	723	740	0.07%	0.008%
88	13.286	2000	2001	2007	rBV2	390	697	0.06%	0.008%
89	13.469	2029	2031	2034	rVB2	435	340	0.03%	0.004%
90	13.530	2039	2041	2044	rBV2	404	339	0.03%	0.004%
91	13.786	2079	2083	2084	rBV2	879	1148	0.10%	0.013%
92	13.969	2110	2113	2116	rBV	790	965	0.09%	0.011%
93	14.115	2136	2137	2138	rBV	606	343	0.03%	0.004%
94	14.292	2164	2166	2167	rBV2	615	459	0.04%	0.005%
95	14.463	2192	2194	2196	rVB	550	338	0.03%	0.004%
96	14.542	2205	2207	2210	rVB3	521	421	0.04%	0.005%
97	15.328	2333	2336	2337	rBV3	819	913	0.08%	0.010%
98	15.462	2357	2358	2360	rBV	874	541	0.05%	0.006%
99	15.932	2433	2435	2437	rVB	890	455	0.04%	0.005%
100	16.292	2492	2494	2495	rBV2	762	539	0.05%	0.006%


Sum of corrected areas: 9157596

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030458.D
Acq On : 06 Aug 2022 12:48
Operator : JC/MD
Sample : N4003-19DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D89DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

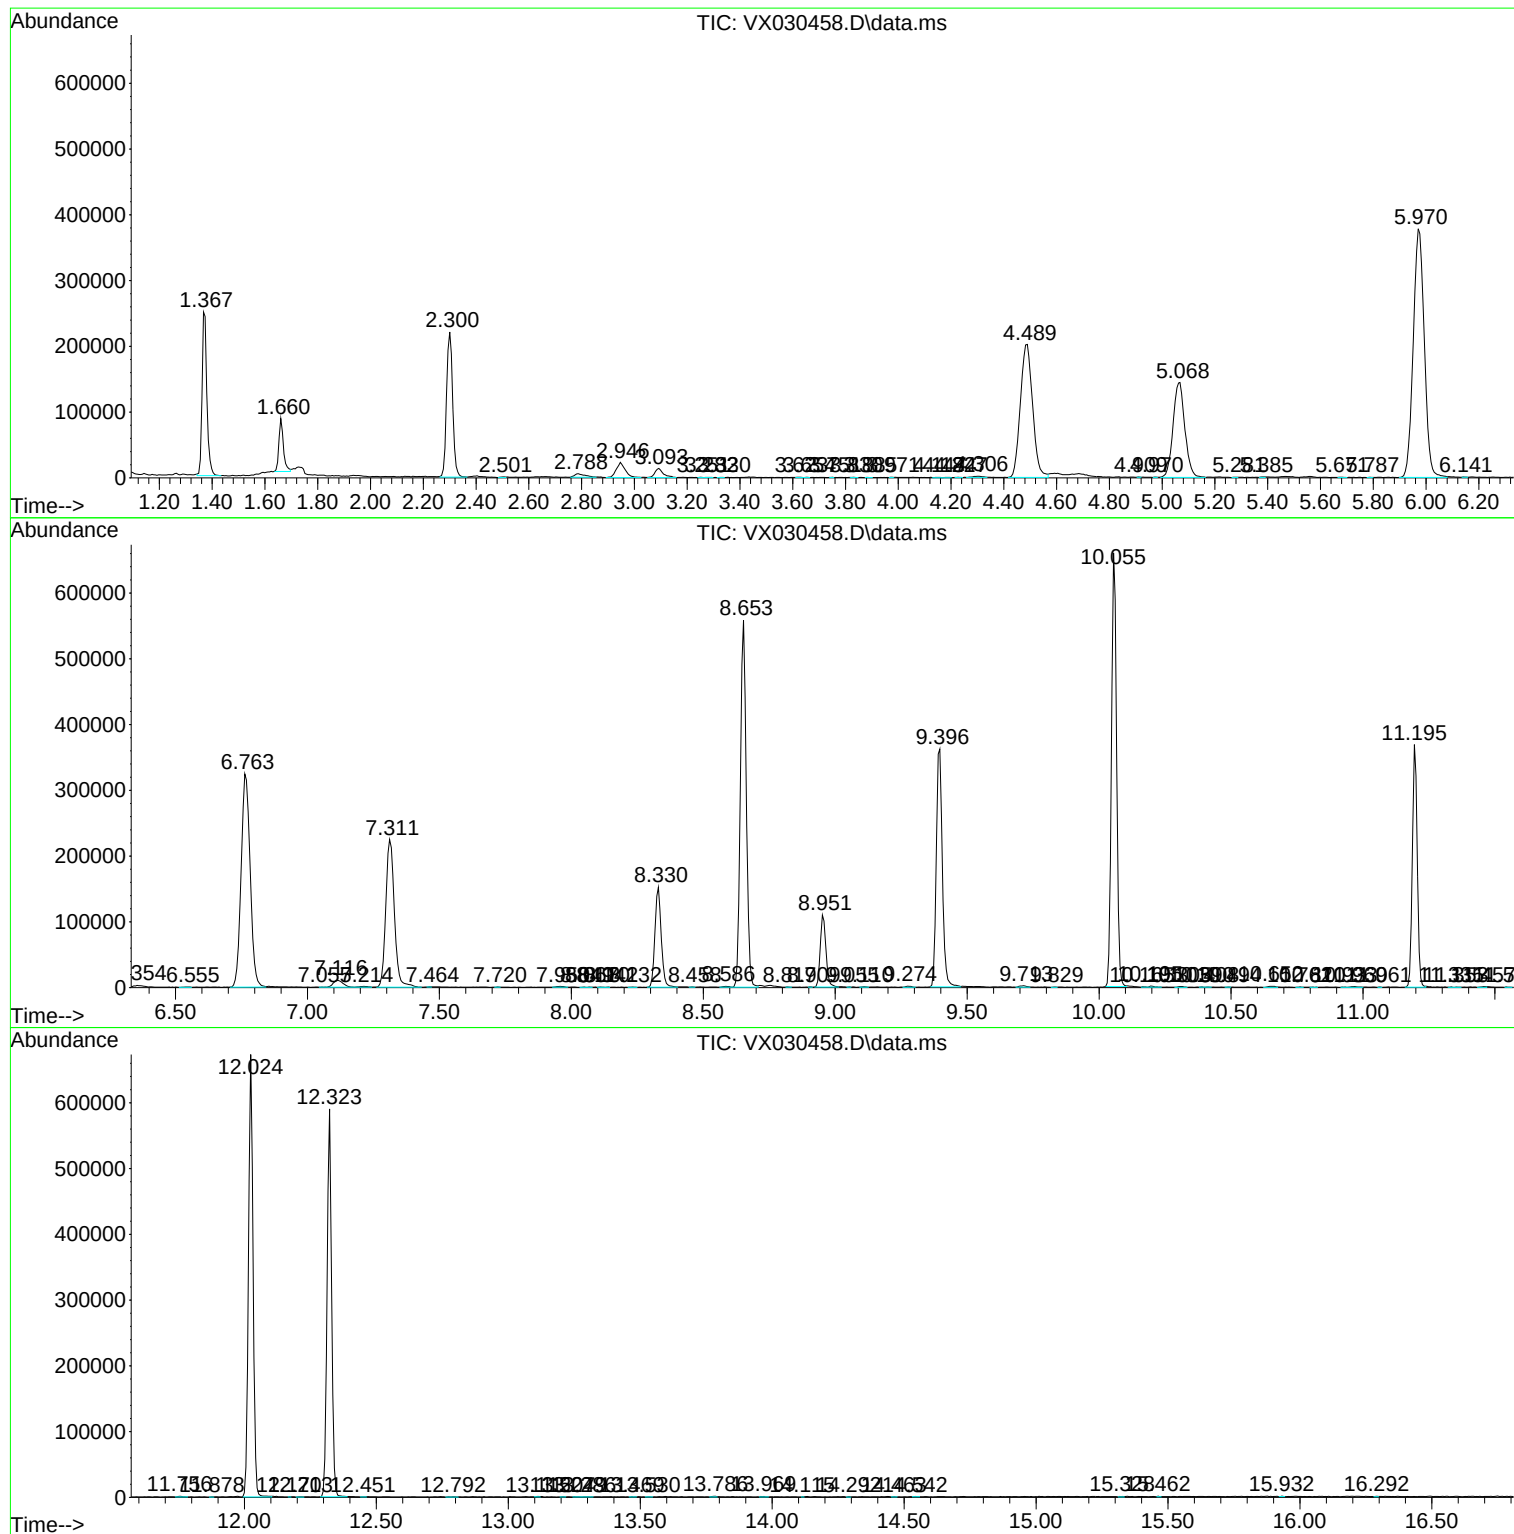

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030458.D
Acq On : 06 Aug 2022 12:48
Operator : JC/MD
Sample : N4003-19DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D89DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030458.D
Acq On : 06 Aug 2022 12:48
Operator : JC/MD
Sample : N4003-19DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D89DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc