

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030459.D
 Acq On : 06 Aug 2022 13:12
 Operator : JC/MD
 Sample : N4003-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030459.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	55	rVB2	448200	517878	8.14%	3.483%
2	1.666	91	95	102	rVB	97875	128128	2.01%	0.862%
3	2.306	194	200	212	rVB	242054	361950	5.69%	2.434%
4	2.800	277	281	283	rBV4	769	1107	0.02%	0.007%
5	2.934	301	303	305	rVB2	482	352	0.01%	0.002%
6	3.014	314	316	318	rVB2	613	481	0.01%	0.003%
7	3.093	322	329	339	rVV	54482	103150	1.62%	0.694%
8	3.190	343	345	347	rBV2	349	360	0.01%	0.002%
9	3.440	385	386	391	rVB2	600	617	0.01%	0.004%
10	3.678	423	425	426	rVV2	525	341	0.01%	0.002%
11	3.763	437	439	441	rBV2	478	477	0.01%	0.003%
12	3.843	449	452	453	rBV	351	335	0.01%	0.002%
13	3.855	453	454	457	rVV2	380	333	0.01%	0.002%
14	3.977	468	474	476	rBV3	271	535	0.01%	0.004%
15	4.099	492	494	496	rVB	391	338	0.01%	0.002%
16	4.123	496	498	501	rVB2	493	495	0.01%	0.003%
17	4.166	501	505	506	rBV	408	495	0.01%	0.003%
18	4.489	545	558	579	rBV	2282762	6359321	100.00%	42.768%
19	4.897	622	625	627	rBV2	520	528	0.01%	0.004%
20	4.989	636	640	641	rBV2	587	855	0.01%	0.006%
21	5.068	641	653	669	rVB	138474	425814	6.70%	2.864%
22	5.227	677	679	680	rVB	710	393	0.01%	0.003%
23	5.306	691	692	695	rBV2	394	334	0.01%	0.002%
24	5.355	698	700	702	rVV3	554	475	0.01%	0.003%
25	5.477	717	720	723	rBV2	467	714	0.01%	0.005%
26	5.556	727	733	741	rVV4	1884	4344	0.07%	0.029%
27	5.739	761	763	765	rBV2	437	350	0.01%	0.002%
28	5.976	789	802	816	rBV2	362226	1065967	16.76%	7.169%
29	6.397	869	871	874	rVV3	460	364	0.01%	0.002%
30	6.507	887	889	892	rBV	295	359	0.01%	0.002%
31	6.653	911	913	917	rVB3	552	552	0.01%	0.004%
32	6.769	922	932	950	rBV	299871	728612	11.46%	4.900%
33	6.976	964	966	968	rVB	494	346	0.01%	0.002%
34	6.995	968	969	971	rBV	458	351	0.01%	0.002%
35	7.019	971	973	978	rVB2	487	587	0.01%	0.004%
36	7.123	980	990	1003	rBV6	15999	42091	0.66%	0.283%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030459.D
 Acq On : 06 Aug 2022 13:12
 Operator : JC/MD
 Sample : N4003-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.312	1012	1021	1036	rBV	220074	484882	7.62%	3.261%
38	7.440	1041	1042	1045	rBV2	482	389	0.01%	0.003%
39	7.476	1045	1048	1049	rBV2	666	601	0.01%	0.004%
40	7.696	1082	1084	1087	rVB	490	619	0.01%	0.004%
41	7.793	1098	1100	1104	rBV	315	403	0.01%	0.003%
42	7.842	1106	1108	1111	rVB	490	521	0.01%	0.004%
43	7.879	1111	1114	1115	rBV2	392	357	0.01%	0.002%
44	8.104	1149	1151	1154	rVB2	396	404	0.01%	0.003%
45	8.171	1159	1162	1164	rBV	383	394	0.01%	0.003%
46	8.208	1167	1168	1170	rBV	595	447	0.01%	0.003%
47	8.330	1181	1188	1198	rBV	148150	242488	3.81%	1.631%
48	8.574	1224	1228	1231	rVB2	458	545	0.01%	0.004%
49	8.653	1231	1241	1255	rBV	541463	839178	13.20%	5.644%
50	8.952	1285	1290	1300	rBV	110033	158918	2.50%	1.069%
51	9.122	1312	1318	1319	rBV2	508	995	0.02%	0.007%
52	9.171	1324	1326	1330	rVV2	357	403	0.01%	0.003%
53	9.281	1340	1344	1349	rVV4	2130	2828	0.04%	0.019%
54	9.390	1356	1362	1375	rBV	397672	581350	9.14%	3.910%
55	9.628	1399	1401	1404	rVB2	439	360	0.01%	0.002%
56	9.732	1417	1418	1421	rVB	698	458	0.01%	0.003%
57	9.762	1421	1423	1426	rBV2	318	411	0.01%	0.003%
58	9.793	1426	1428	1432	rVB2	412	422	0.01%	0.003%
59	9.860	1438	1439	1441	rBV	370	361	0.01%	0.002%
60	9.878	1441	1442	1445	rVB	540	420	0.01%	0.003%
61	10.055	1465	1471	1481	rBV	631235	847794	13.33%	5.702%
62	10.256	1502	1504	1506	rBV2	413	421	0.01%	0.003%
63	10.372	1519	1523	1525	rVV2	440	510	0.01%	0.003%
64	10.433	1531	1533	1536	rVB2	520	391	0.01%	0.003%
65	10.659	1568	1570	1572	rVB3	639	372	0.01%	0.003%
66	10.915	1608	1612	1615	rBV2	370	602	0.01%	0.004%
67	11.018	1627	1629	1632	rBV3	288	370	0.01%	0.002%
68	11.195	1652	1658	1664	rBV	380144	480086	7.55%	3.229%
69	11.293	1672	1674	1676	rBV2	399	421	0.01%	0.003%
70	11.433	1693	1697	1698	rBV2	525	525	0.01%	0.004%
71	11.482	1703	1705	1708	rBV3	654	674	0.01%	0.005%
72	11.506	1708	1709	1714	rVB2	753	660	0.01%	0.004%
73	11.555	1714	1717	1720	rBV2	600	740	0.01%	0.005%
74	11.585	1720	1722	1725	rVB2	547	341	0.01%	0.002%
75	11.719	1743	1744	1747	rVB2	360	345	0.01%	0.002%
76	11.744	1747	1748	1750	rBV	721	557	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030459.D
 Acq On : 06 Aug 2022 13:12
 Operator : JC/MD
 Sample : N4003-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.951	1780	1782	1785	rBV2	322	469	0.01%	0.003%
78	12.024	1788	1794	1804	rVV	635687	766314	12.05%	5.154%
79	12.323	1837	1843	1853	rBV	542433	687727	10.81%	4.625%
80	12.567	1881	1883	1885	rBV	697	427	0.01%	0.003%
81	12.628	1890	1893	1896	rVB	712	658	0.01%	0.004%
82	12.652	1896	1897	1900	rBV2	543	450	0.01%	0.003%
83	13.463	2028	2030	2031	rBV2	559	358	0.01%	0.002%
84	13.567	2044	2047	2048	rBV	397	349	0.01%	0.002%
85	13.585	2048	2050	2053	rVB	367	425	0.01%	0.003%
86	13.695	2065	2068	2069	rBV	409	362	0.01%	0.002%
87	13.743	2072	2076	2077	rVB2	397	435	0.01%	0.003%
88	13.780	2080	2082	2085	rVB2	606	458	0.01%	0.003%
89	14.152	2139	2143	2146	rVB2	563	757	0.01%	0.005%
90	14.237	2155	2157	2158	rBV	549	370	0.01%	0.002%
91	14.347	2174	2175	2178	rBV2	582	442	0.01%	0.003%
92	14.444	2188	2191	2194	rVB3	559	676	0.01%	0.005%
93	14.481	2194	2197	2202	rBV2	691	1345	0.02%	0.009%
94	14.786	2245	2247	2250	rVB2	692	594	0.01%	0.004%
95	15.048	2288	2290	2291	rBV	566	444	0.01%	0.003%
96	15.420	2349	2351	2353	rBV2	680	552	0.01%	0.004%
97	15.798	2411	2413	2414	rBV	715	551	0.01%	0.004%
98	16.383	2507	2509	2510	rBV2	673	482	0.01%	0.003%
99	16.676	2553	2557	2558	rBV3	799	1103	0.02%	0.007%
100	16.712	2561	2563	2566	rBV2	832	799	0.01%	0.005%




Sum of corrected areas: 14869239

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030459.D
Acq On : 06 Aug 2022 13:12
Operator : JC/MD
Sample : N4003-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

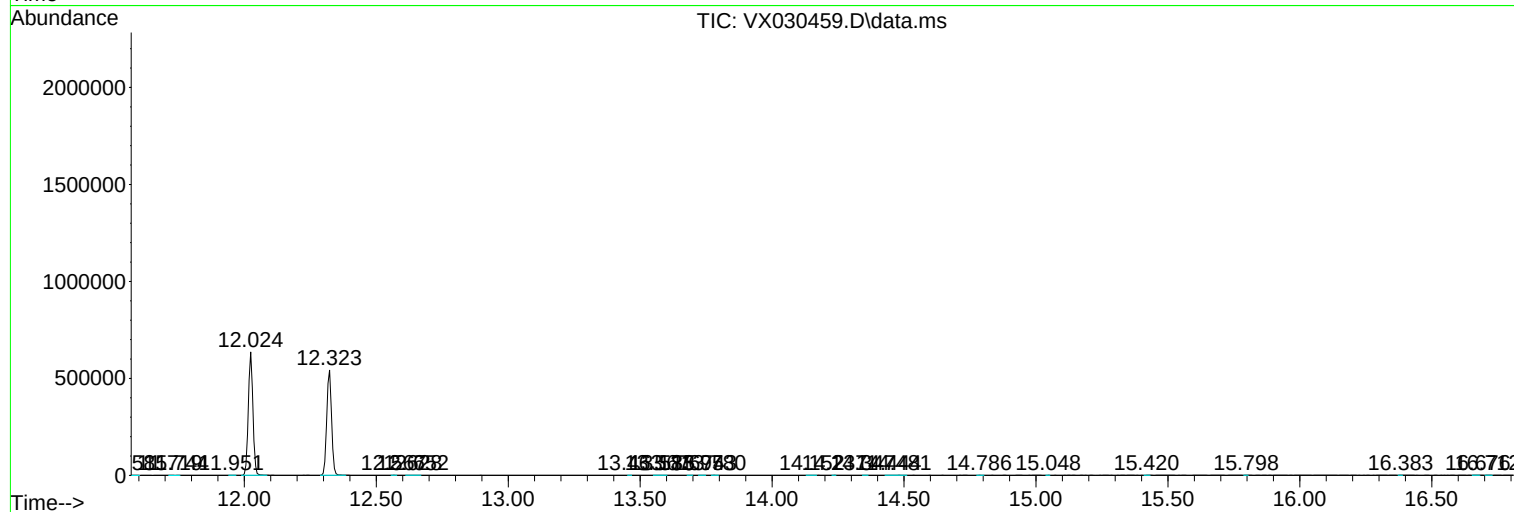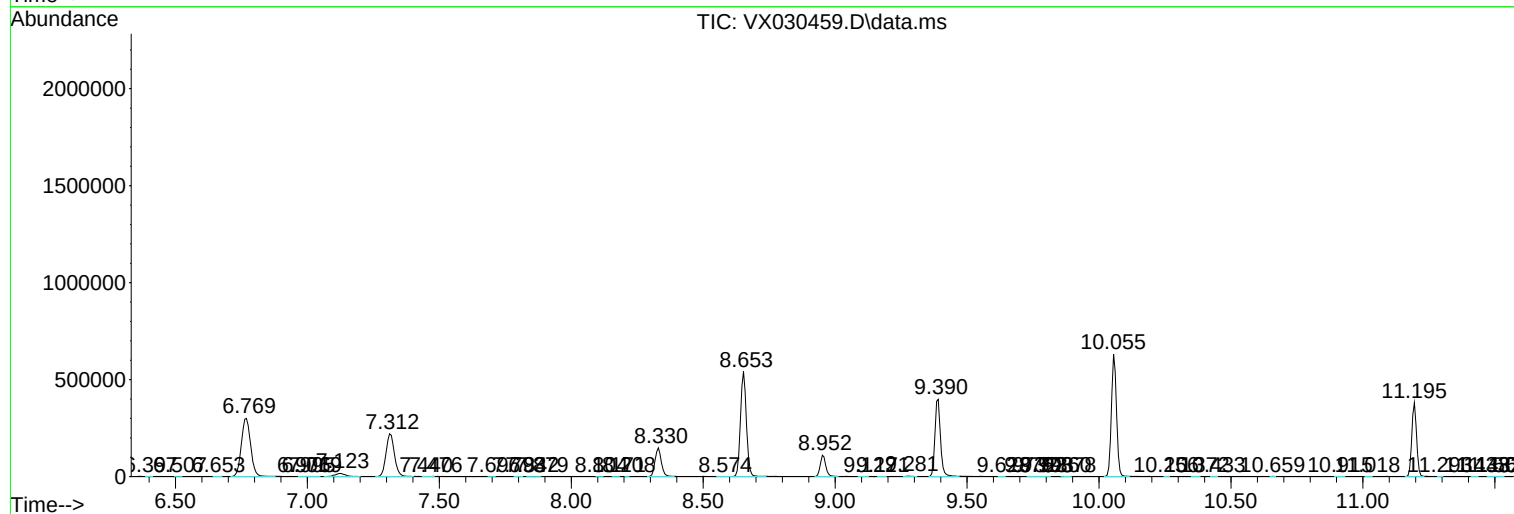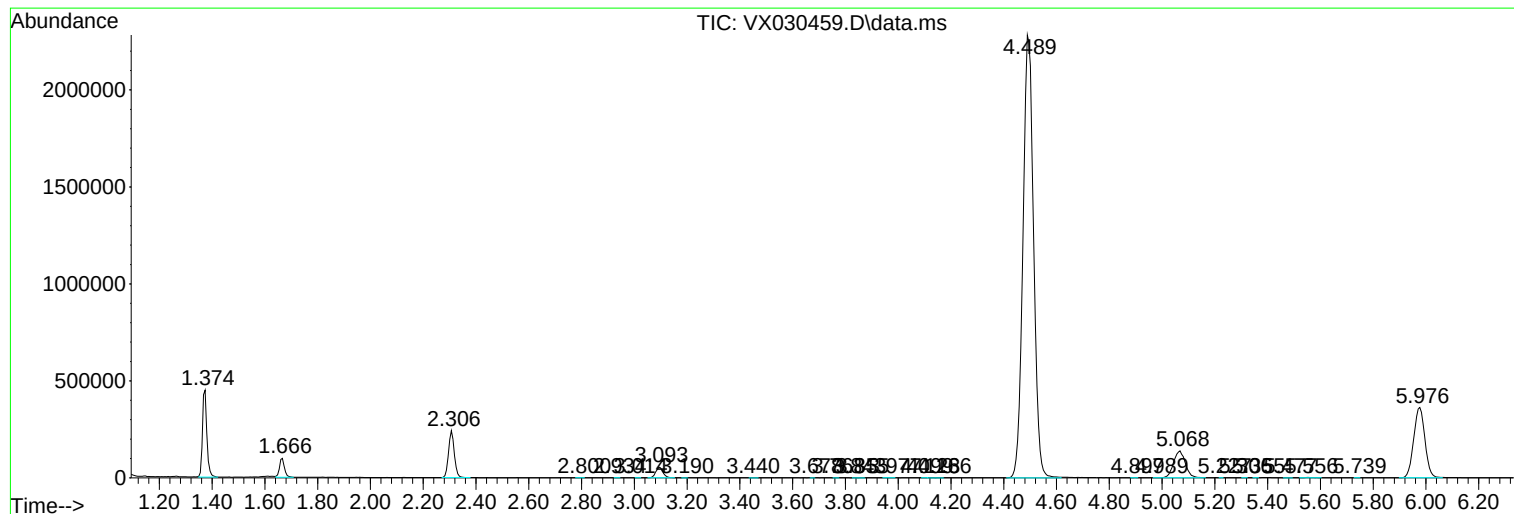

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030459.D
Acq On : 06 Aug 2022 13:12
Operator : JC/MD
Sample : N4003-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030459.D
Acq On : 06 Aug 2022 13:12
Operator : JC/MD
Sample : N4003-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc