

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030460.D
 Acq On : 06 Aug 2022 13:35
 Operator : JC/MD
 Sample : VIBLK650
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK650

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030460.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	57	rVB	140599	141134	13.14%	1.653%
2	1.666	91	95	105	rVB	105567	129164	12.03%	1.513%
3	2.307	194	200	211	rVB	241832	359219	33.45%	4.207%
4	2.502	230	232	237	rBV4	754	1233	0.11%	0.014%
5	2.648	254	256	259	rVB	734	616	0.06%	0.007%
6	2.678	259	261	262	rBV	716	429	0.04%	0.005%
7	2.721	265	268	269	rBV	507	462	0.04%	0.005%
8	2.794	275	280	285	rVB5	2477	4309	0.40%	0.050%
9	2.953	298	306	312	rBV2	6139	14335	1.33%	0.168%
10	3.093	326	329	330	rBV2	530	492	0.05%	0.006%
11	3.111	330	332	334	rBV2	381	407	0.04%	0.005%
12	3.251	353	355	360	rBV2	250	410	0.04%	0.005%
13	3.398	377	379	385	rVV2	253	327	0.03%	0.004%
14	3.440	385	386	389	rVB2	705	526	0.05%	0.006%
15	3.471	389	391	395	rBV2	496	539	0.05%	0.006%
16	3.818	446	448	452	rBV3	293	402	0.04%	0.005%
17	4.032	481	483	486	rBV	305	373	0.03%	0.004%
18	4.318	527	530	531	rVB2	417	385	0.04%	0.005%
19	4.385	539	541	544	rBV2	464	670	0.06%	0.008%
20	4.471	544	555	568	rBV	95077	287118	26.73%	3.362%
21	4.818	610	612	617	rBV2	452	883	0.08%	0.010%
22	4.977	635	638	640	rBV2	553	564	0.05%	0.007%
23	5.068	640	653	670	rVV	139313	432678	40.29%	5.067%
24	5.294	686	690	691	rVB	486	446	0.04%	0.005%
25	5.385	696	705	706	rBV3	952	1443	0.13%	0.017%
26	5.464	716	718	720	rBV2	498	527	0.05%	0.006%
27	5.489	720	722	726	rVV2	671	731	0.07%	0.009%
28	5.525	726	728	729	rVV2	630	505	0.05%	0.006%
29	5.568	729	735	738	rVV6	1624	3586	0.33%	0.042%
30	5.617	742	743	746	rBV2	452	392	0.04%	0.005%
31	5.751	762	765	767	rBV2	576	755	0.07%	0.009%
32	5.806	772	774	775	rVV	386	386	0.04%	0.005%
33	5.977	790	802	818	rBV2	364249	1074003	100.00%	12.578%
34	6.117	824	825	827	rVB	760	438	0.04%	0.005%
35	6.348	861	863	864	rVV2	494	387	0.04%	0.005%
36	6.367	864	866	868	rVV2	556	478	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030460.D
 Acq On : 06 Aug 2022 13:35
 Operator : JC/MD
 Sample : VIBLK650
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK650

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
 Title : VOC Analysis

37	6.391	868	870	873	rVB2	382	402	0.04%	0.005%
38	6.458	878	881	884	rVB	459	642	0.06%	0.008%
39	6.519	889	891	893	rBV	426	396	0.04%	0.005%
40	6.769	922	932	949	rBV	315083	758913	70.66%	8.888%
41	6.885	949	951	952	rVB	822	355	0.03%	0.004%
42	6.958	961	963	968	rVB2	603	630	0.06%	0.007%
43	7.001	968	970	972	rVB2	477	338	0.03%	0.004%
44	7.037	972	976	977	rVB	522	628	0.06%	0.007%
45	7.117	982	989	996	rBV5	12092	26647	2.48%	0.312%
46	7.312	1012	1021	1032	rBV	219509	491483	45.76%	5.756%
47	7.720	1085	1088	1091	rBV2	317	436	0.04%	0.005%
48	7.891	1112	1116	1118	rBV2	375	483	0.04%	0.006%
49	7.934	1121	1123	1127	rBV2	543	574	0.05%	0.007%
50	7.970	1127	1129	1133	rVB2	588	494	0.05%	0.006%
51	8.330	1181	1188	1196	rBV	151920	248090	23.10%	2.905%
52	8.653	1234	1241	1254	rBV	543539	852938	79.42%	9.989%
53	8.818	1265	1268	1272	rVB3	520	676	0.06%	0.008%
54	8.952	1283	1290	1301	rBV	111303	165092	15.37%	1.933%
55	9.086	1310	1312	1313	rBV	430	331	0.03%	0.004%
56	9.171	1322	1326	1328	rBV2	544	513	0.05%	0.006%
57	9.275	1338	1343	1345	rBV2	1228	1345	0.13%	0.016%
58	9.391	1356	1362	1379	rBV	403507	603792	56.22%	7.071%
59	9.604	1395	1397	1398	rBV2	405	377	0.04%	0.004%
60	9.702	1407	1413	1418	rVV5	1514	3139	0.29%	0.037%
61	9.836	1433	1435	1437	rVV	530	377	0.04%	0.004%
62	10.006	1461	1463	1465	rBV	384	332	0.03%	0.004%
63	10.055	1465	1471	1480	rBV	684452	886511	82.54%	10.382%
64	10.208	1493	1496	1500	rBV3	525	713	0.07%	0.008%
65	10.287	1506	1509	1510	rBV	533	539	0.05%	0.006%
66	10.537	1548	1550	1554	rBV3	542	659	0.06%	0.008%
67	10.787	1589	1591	1596	rVV2	401	627	0.06%	0.007%
68	10.848	1598	1601	1603	rBV2	451	609	0.06%	0.007%
69	10.878	1603	1606	1607	rBV	466	311	0.03%	0.004%
70	11.098	1638	1642	1643	rBV2	636	793	0.07%	0.009%
71	11.195	1652	1658	1671	rBV	375469	490589	45.68%	5.745%
72	11.299	1674	1675	1678	rVV3	426	342	0.03%	0.004%
73	11.335	1678	1681	1685	rVB3	340	425	0.04%	0.005%
74	11.476	1701	1704	1706	rBV2	574	635	0.06%	0.007%
75	11.665	1733	1735	1739	rVB2	342	336	0.03%	0.004%
76	11.701	1739	1741	1744	rVV2	371	461	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030460.D
 Acq On : 06 Aug 2022 13:35
 Operator : JC/MD
 Sample : VIBLK650
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK650

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
 Title : VOC Analysis

77	11.750	1747	1749	1752	rVB	564	499	0.05%	0.006%
78	11.799	1754	1757	1759	rBV	520	607	0.06%	0.007%
79	11.847	1763	1765	1767	rVB	565	327	0.03%	0.004%
80	11.951	1779	1782	1783	rBV	394	504	0.05%	0.006%
81	12.024	1789	1794	1804	rBV	694010	819536	76.31%	9.598%
82	12.323	1837	1843	1854	rBV	572077	704336	65.58%	8.249%
83	12.469	1865	1867	1869	rBV	695	660	0.06%	0.008%
84	12.677	1898	1901	1902	rBV2	276	343	0.03%	0.004%
85	12.780	1917	1918	1921	rVV2	702	688	0.06%	0.008%
86	13.298	2001	2003	2004	rBV	480	367	0.03%	0.004%
87	13.530	2039	2041	2043	rBV	564	462	0.04%	0.005%
88	13.780	2080	2082	2085	rVB	633	444	0.04%	0.005%
89	13.811	2085	2087	2089	rBV2	340	311	0.03%	0.004%
90	13.945	2107	2109	2112	rVB2	638	586	0.05%	0.007%
91	13.993	2113	2117	2118	rVV2	557	502	0.05%	0.006%
92	14.103	2132	2135	2137	rBV2	582	570	0.05%	0.007%
93	14.341	2173	2174	2176	rBV2	447	362	0.03%	0.004%
94	14.566	2209	2211	2212	rBV	787	603	0.06%	0.007%
95	14.701	2230	2233	2237	rBV2	588	1021	0.10%	0.012%
96	14.993	2279	2281	2283	rBV2	681	621	0.06%	0.007%
97	15.103	2297	2299	2300	rBV	617	543	0.05%	0.006%
98	15.524	2366	2368	2370	rVB	673	374	0.03%	0.004%
99	15.658	2389	2390	2391	rBV	979	489	0.05%	0.006%
100	16.158	2471	2472	2474	rBV	759	406	0.04%	0.005%

Sum of corrected areas: 8538886




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030460.D
Acq On : 06 Aug 2022 13:35
Operator : JC/MD
Sample : VIBLK650
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK650

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXL080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

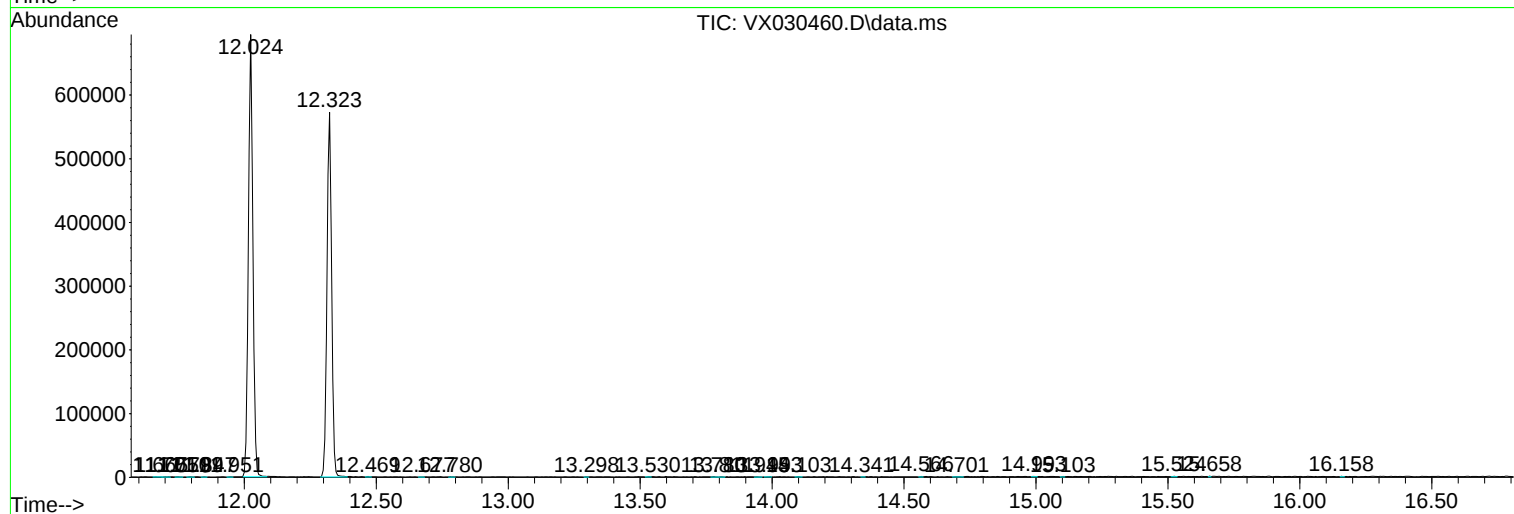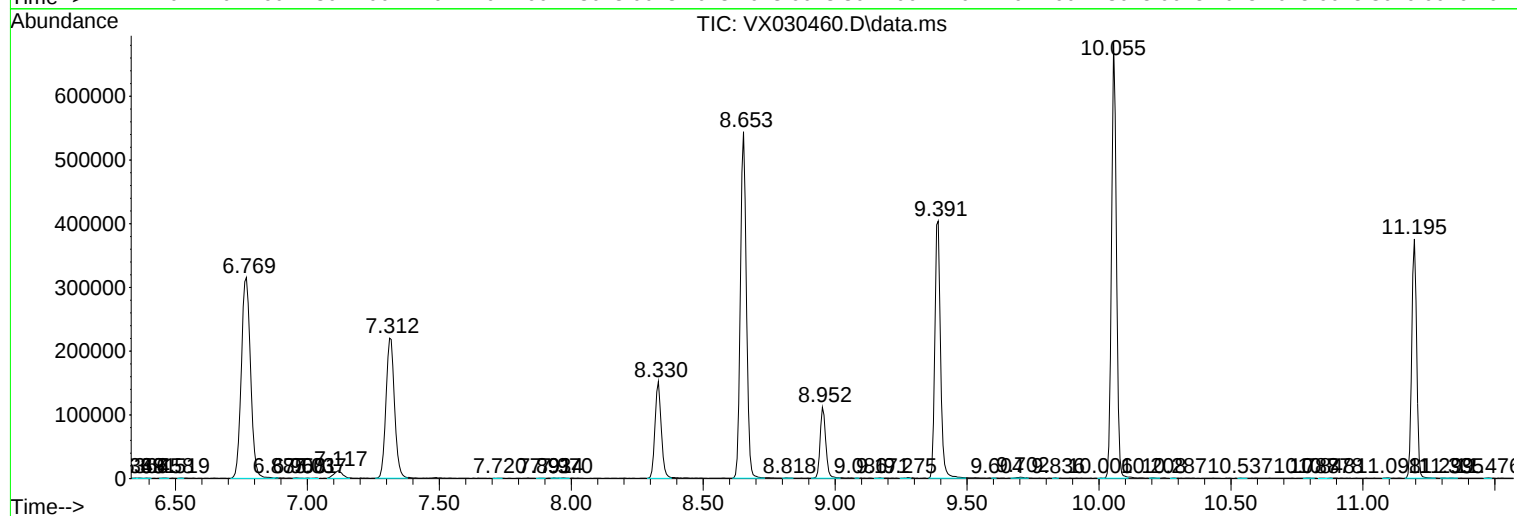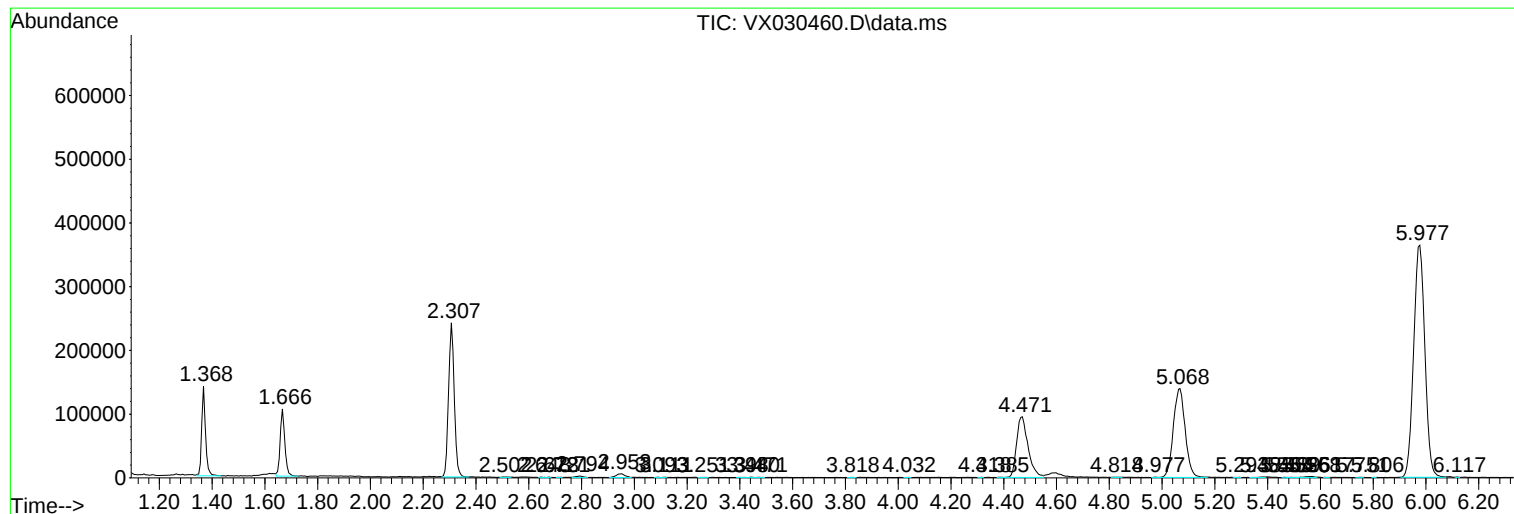

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030460.D
Acq On : 06 Aug 2022 13:35
Operator : JC/MD
Sample : VIBLK650
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK650

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030460.D
Acq On : 06 Aug 2022 13:35
Operator : JC/MD
Sample : VIBLK650
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK650

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc