

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030461.D
 Acq On : 06 Aug 2022 13:59
 Operator : JC/MD
 Sample : N4003-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030461.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.373	43	47	56	rVB2	436088	501210	8.03%	3.418%
2	1.666	91	95	105	rVB	103437	128111	2.05%	0.874%
3	2.056	157	159	162	rBV2	818	819	0.01%	0.006%
4	2.306	194	200	210	rVB	215159	335146	5.37%	2.286%
5	2.794	276	280	284	rVB4	992	1671	0.03%	0.011%
6	2.916	299	300	306	rVB2	472	552	0.01%	0.004%
7	2.989	310	312	313	rVV	468	327	0.01%	0.002%
8	3.093	323	329	340	rVB	51714	101220	1.62%	0.690%
9	3.623	415	416	423	rBV2	326	491	0.01%	0.003%
10	3.721	429	432	434	rVB2	469	450	0.01%	0.003%
11	3.757	436	438	443	rVB	616	550	0.01%	0.004%
12	3.806	445	446	449	rBV2	400	327	0.01%	0.002%
13	3.940	465	468	471	rBV2	514	484	0.01%	0.003%
14	4.275	522	523	525	rBV	530	348	0.01%	0.002%
15	4.495	543	559	581	rBV	2270763	6240197	100.00%	42.561%
16	5.062	640	652	669	rVV	138344	420999	6.75%	2.871%
17	5.239	679	681	688	rVB4	931	1428	0.02%	0.010%
18	5.367	699	702	703	rBV3	545	568	0.01%	0.004%
19	5.549	729	732	734	rBV2	1225	1514	0.02%	0.010%
20	5.799	770	773	775	rBV3	437	333	0.01%	0.002%
21	5.976	789	802	822	rBV2	357701	1056916	16.94%	7.209%
22	6.196	835	838	839	rVB2	743	683	0.01%	0.005%
23	6.214	839	841	842	rBV2	411	444	0.01%	0.003%
24	6.360	861	865	867	rVV2	507	673	0.01%	0.005%
25	6.385	867	869	872	rVV4	646	663	0.01%	0.005%
26	6.555	894	897	902	rVB3	410	609	0.01%	0.004%
27	6.622	902	908	911	rVB2	369	590	0.01%	0.004%
28	6.690	915	919	920	rBV	224	335	0.01%	0.002%
29	6.769	922	932	947	rBV	299023	715054	11.46%	4.877%
30	7.128	982	991	1001	rBV5	14755	38661	0.62%	0.264%
31	7.311	1012	1021	1034	rBV	215714	478616	7.67%	3.264%
32	7.543	1057	1059	1061	rBV2	387	364	0.01%	0.002%
33	7.750	1090	1093	1097	rVB2	396	359	0.01%	0.002%
34	7.891	1114	1116	1119	rBV2	438	477	0.01%	0.003%
35	7.994	1128	1133	1134	rBV2	413	549	0.01%	0.004%
36	8.049	1140	1142	1146	rBV2	402	617	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030461.D
 Acq On : 06 Aug 2022 13:59
 Operator : JC/MD
 Sample : N4003-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	8.140	1154	1157	1158	rBV	314	321	0.01%	0.002%
38	8.329	1181	1188	1203	rBV	150471	242484	3.89%	1.654%
39	8.506	1215	1217	1220	rVB2	436	434	0.01%	0.003%
40	8.537	1220	1222	1224	rBV3	348	353	0.01%	0.002%
41	8.653	1234	1241	1254	rBV	541506	838582	13.44%	5.720%
42	8.951	1282	1290	1299	rBV	101248	158895	2.55%	1.084%
43	9.244	1335	1338	1340	rBV	322	342	0.01%	0.002%
44	9.274	1340	1343	1348	rBV4	1227	1715	0.03%	0.012%
45	9.348	1354	1355	1356	rBV4	460	320	0.01%	0.002%
46	9.390	1356	1362	1376	rBV	412661	582716	9.34%	3.974%
47	9.634	1399	1402	1405	rBV2	642	589	0.01%	0.004%
48	9.756	1420	1422	1425	rBV2	496	458	0.01%	0.003%
49	9.811	1429	1431	1433	rBV2	369	340	0.01%	0.002%
50	9.878	1440	1442	1443	rBV	432	333	0.01%	0.002%
51	9.939	1451	1452	1455	rBV2	533	386	0.01%	0.003%
52	10.006	1461	1463	1465	rBV	430	358	0.01%	0.002%
53	10.055	1466	1471	1480	rBV	626117	834921	13.38%	5.695%
54	10.171	1488	1490	1494	rVB2	756	666	0.01%	0.005%
55	10.250	1500	1503	1504	rBV	381	395	0.01%	0.003%
56	10.402	1526	1528	1531	rVB2	554	609	0.01%	0.004%
57	10.616	1561	1563	1566	rBV2	413	443	0.01%	0.003%
58	10.841	1597	1600	1603	rBV2	420	705	0.01%	0.005%
59	10.981	1618	1623	1624	rBV2	563	684	0.01%	0.005%
60	11.061	1632	1636	1637	rBV2	377	569	0.01%	0.004%
61	11.195	1652	1658	1665	rBV	379859	479895	7.69%	3.273%
62	11.347	1682	1683	1686	rBV	434	317	0.01%	0.002%
63	11.475	1701	1704	1707	rBV3	489	690	0.01%	0.005%
64	11.652	1730	1733	1735	rVB2	565	568	0.01%	0.004%
65	11.670	1735	1736	1739	rBV2	440	330	0.01%	0.002%
66	11.707	1739	1742	1746	rVB2	472	747	0.01%	0.005%
67	11.756	1748	1750	1753	rVB	559	445	0.01%	0.003%
68	11.792	1753	1756	1759	rVB2	697	777	0.01%	0.005%
69	12.024	1788	1794	1805	rBV	640266	763913	12.24%	5.210%
70	12.323	1837	1843	1855	rVV	555981	700745	11.23%	4.779%
71	12.579	1883	1885	1887	rBV	427	500	0.01%	0.003%
72	12.725	1907	1909	1910	rBV2	412	312	0.00%	0.002%
73	12.743	1910	1912	1915	rVV3	298	362	0.01%	0.002%
74	12.914	1939	1940	1943	rBV	553	501	0.01%	0.003%
75	13.024	1957	1958	1960	rBV	499	348	0.01%	0.002%
76	13.091	1968	1969	1971	rBV2	453	378	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030461.D
 Acq On : 06 Aug 2022 13:59
 Operator : JC/MD
 Sample : N4003-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	13.133	1975	1976	1978	rVB	658	302	0.00%	0.002%
78	13.371	2013	2015	2016	rBV	576	400	0.01%	0.003%
79	13.774	2080	2081	2084	rBV2	340	326	0.01%	0.002%
80	13.920	2103	2105	2106	rBV	454	460	0.01%	0.003%
81	13.993	2112	2117	2118	rBV3	303	468	0.01%	0.003%
82	14.078	2129	2131	2134	rBV3	349	369	0.01%	0.003%
83	14.145	2140	2142	2145	rVB2	426	401	0.01%	0.003%
84	14.194	2148	2150	2152	rBV2	372	395	0.01%	0.003%
85	14.274	2162	2163	2165	rBV2	446	356	0.01%	0.002%
86	14.414	2184	2186	2188	rBV	618	403	0.01%	0.003%
87	14.481	2195	2197	2198	rBV2	352	301	0.00%	0.002%
88	14.682	2229	2230	2232	rVB	561	370	0.01%	0.003%
89	14.706	2232	2234	2235	rBV2	518	407	0.01%	0.003%
90	14.908	2265	2267	2268	rVB	741	345	0.01%	0.002%
91	14.975	2276	2278	2279	rBV	661	623	0.01%	0.004%
92	15.109	2298	2300	2303	rBV2	372	335	0.01%	0.002%
93	15.194	2312	2314	2315	rBV2	733	511	0.01%	0.003%
94	15.316	2331	2334	2335	rBV	480	519	0.01%	0.004%
95	15.359	2339	2341	2342	rVB	860	557	0.01%	0.004%
96	15.407	2348	2349	2352	rBV2	692	746	0.01%	0.005%
97	15.456	2355	2357	2358	rBV	796	516	0.01%	0.004%
98	15.670	2390	2392	2393	rVB	817	437	0.01%	0.003%
99	16.249	2485	2487	2490	rBV2	706	838	0.01%	0.006%
100	16.688	2558	2559	2562	rVB	998	569	0.01%	0.004%

Sum of corrected areas: 14661755




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030461.D
Acq On : 06 Aug 2022 13:59
Operator : JC/MD
Sample : N4003-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

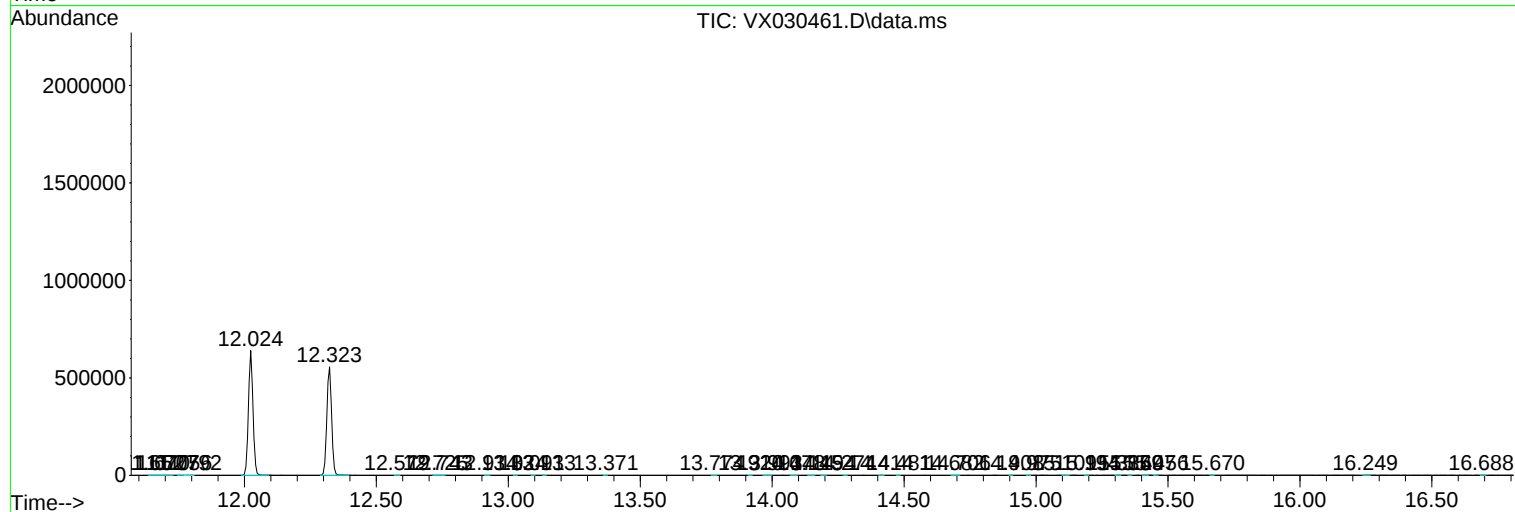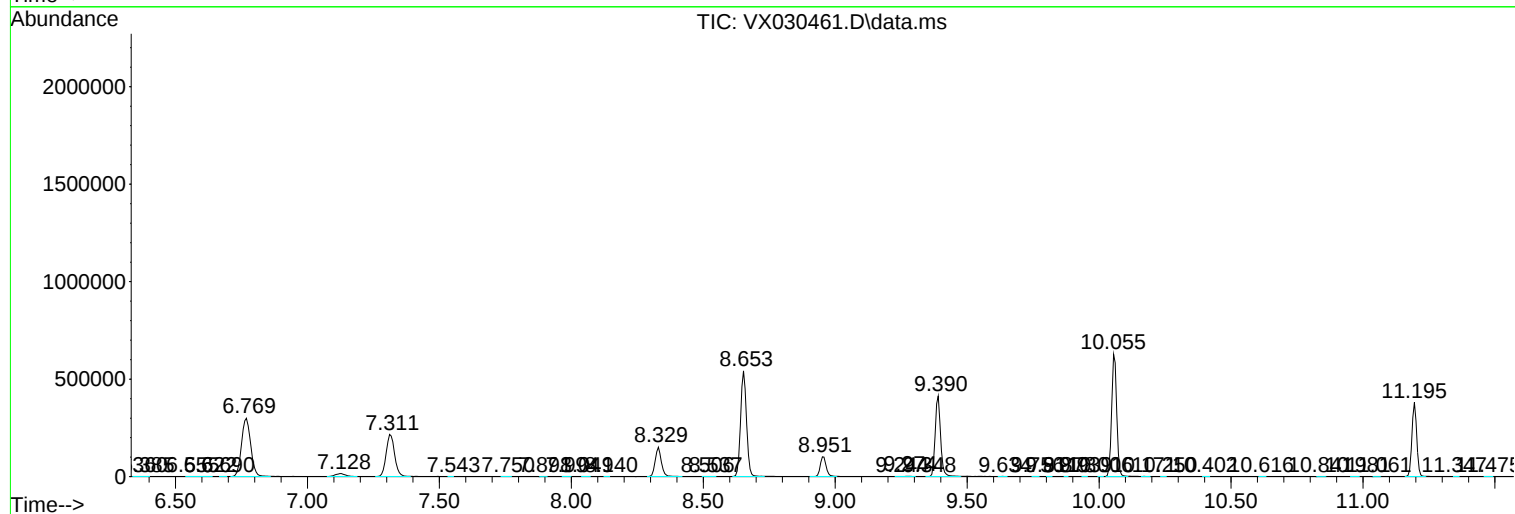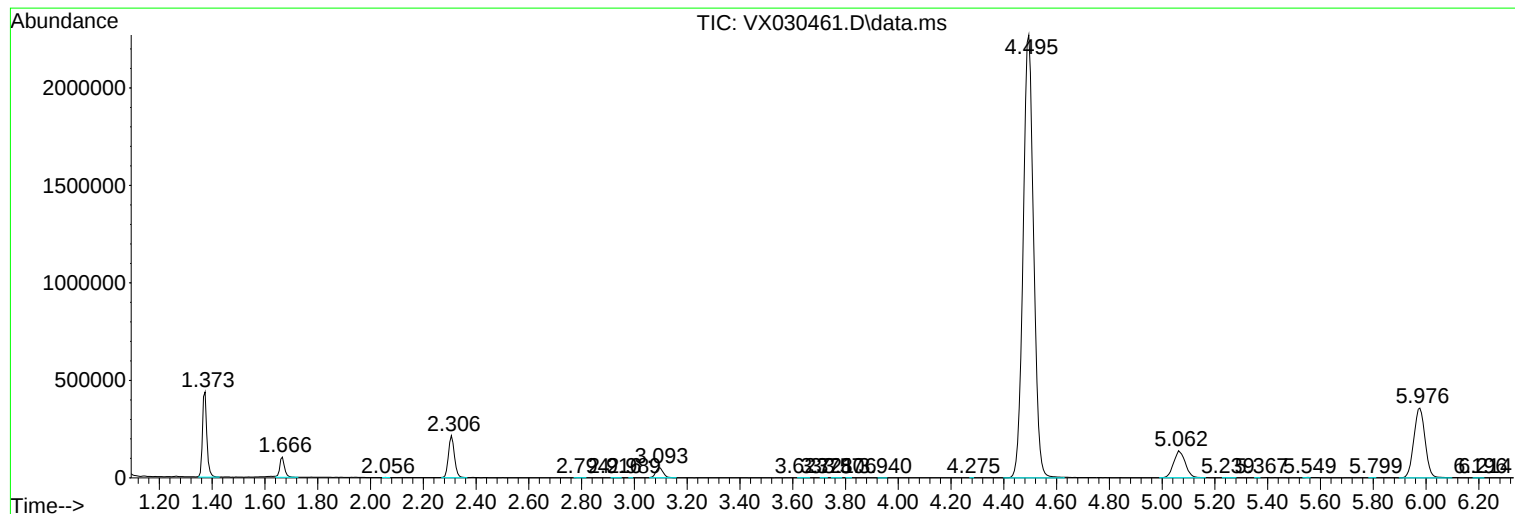

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030461.D
Acq On : 06 Aug 2022 13:59
Operator : JC/MD
Sample : N4003-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030461.D
Acq On : 06 Aug 2022 13:59
Operator : JC/MD
Sample : N4003-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc