

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030462.D
 Acq On : 06 Aug 2022 14:22
 Operator : JC/MD
 Sample : VIBLK651
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK651

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030462.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rVB	136167	137245	12.94%	1.635%
2	1.666	91	95	104	rVB	109731	131066	12.36%	1.561%
3	2.306	194	200	211	rVB	240366	363094	34.23%	4.325%
4	2.502	230	232	234	rBV2	557	489	0.05%	0.006%
5	2.575	242	244	245	rBV	494	340	0.03%	0.004%
6	2.794	275	280	287	rVB4	2710	5350	0.50%	0.064%
7	2.947	299	305	314	rVB	7950	18702	1.76%	0.223%
8	3.099	328	330	331	rVB2	478	308	0.03%	0.004%
9	3.184	341	344	346	rBV2	402	599	0.06%	0.007%
10	3.343	368	370	373	rBV2	346	375	0.04%	0.004%
11	3.398	378	379	382	rVB2	406	375	0.04%	0.004%
12	3.453	387	388	391	rBV	468	312	0.03%	0.004%
13	3.532	398	401	403	rBV	407	524	0.05%	0.006%
14	3.678	422	425	426	rBV2	378	364	0.03%	0.004%
15	3.885	457	459	460	rVV2	427	308	0.03%	0.004%
16	3.922	462	465	466	rVV	444	408	0.04%	0.005%
17	3.959	469	471	474	rBV2	324	373	0.04%	0.004%
18	4.160	503	504	506	rBV	337	305	0.03%	0.004%
19	4.471	545	555	567	rBV	92720	282675	26.65%	3.367%
20	4.757	600	602	607	rBV4	356	522	0.05%	0.006%
21	5.068	640	653	668	rBV	142391	430539	40.59%	5.128%
22	5.233	678	680	681	rVV2	428	423	0.04%	0.005%
23	5.275	684	687	691	rBV2	612	1146	0.11%	0.014%
24	5.391	703	706	707	rBV2	702	697	0.07%	0.008%
25	5.471	716	719	720	rBV2	277	316	0.03%	0.004%
26	5.568	726	735	736	rBV4	1629	3681	0.35%	0.044%
27	5.617	741	743	747	rBV2	599	532	0.05%	0.006%
28	5.867	782	784	787	rVB	521	330	0.03%	0.004%
29	5.977	790	802	817	rBV2	364053	1060832	100.00%	12.635%
30	6.111	823	824	830	rVV4	749	888	0.08%	0.011%
31	6.178	833	835	838	rVB	666	460	0.04%	0.005%
32	6.452	877	880	881	rVV2	300	362	0.03%	0.004%
33	6.513	889	890	895	rBV2	522	588	0.06%	0.007%
34	6.556	895	897	904	rVB3	654	1326	0.12%	0.016%
35	6.617	904	907	911	rBV2	631	1020	0.10%	0.012%
36	6.769	922	932	944	rBV	308754	737213	69.49%	8.781%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030462.D
 Acq On : 06 Aug 2022 14:22
 Operator : JC/MD
 Sample : VIBLK651
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK651

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.909	953	955	957	rVB2	645	440	0.04%	0.005%
38	7.013	970	972	974	rVB	589	523	0.05%	0.006%
39	7.117	982	989	997	rVV4	12846	29488	2.78%	0.351%
40	7.312	1013	1021	1033	rVV	220320	490626	46.25%	5.844%
41	7.482	1048	1049	1053	rVB2	748	424	0.04%	0.005%
42	7.562	1060	1062	1065	rVB2	417	487	0.05%	0.006%
43	7.604	1065	1069	1071	rBV2	469	624	0.06%	0.007%
44	7.696	1080	1084	1085	rBV2	251	339	0.03%	0.004%
45	7.824	1102	1105	1107	rBV2	457	518	0.05%	0.006%
46	8.086	1147	1148	1151	rBV2	522	573	0.05%	0.007%
47	8.141	1155	1157	1160	rVV2	497	644	0.06%	0.008%
48	8.330	1181	1188	1198	rBV	146831	240228	22.65%	2.861%
49	8.476	1209	1212	1214	rVV3	605	490	0.05%	0.006%
50	8.513	1214	1218	1219	rVB2	570	664	0.06%	0.008%
51	8.580	1226	1229	1232	rBV	479	610	0.06%	0.007%
52	8.653	1234	1241	1255	rBV	540165	833180	78.54%	9.924%
53	8.952	1282	1290	1298	rBV	103871	158728	14.96%	1.891%
54	9.049	1304	1306	1308	rVB2	411	343	0.03%	0.004%
55	9.281	1341	1344	1347	rVB3	1147	1257	0.12%	0.015%
56	9.342	1352	1354	1356	rBV2	487	323	0.03%	0.004%
57	9.391	1356	1362	1376	rBV	408000	599345	56.50%	7.138%
58	9.567	1389	1391	1393	rVV3	662	389	0.04%	0.005%
59	9.671	1405	1408	1409	rBV	384	408	0.04%	0.005%
60	9.701	1410	1413	1420	rVV3	2788	4565	0.43%	0.054%
61	9.781	1422	1426	1429	rVB2	536	781	0.07%	0.009%
62	10.055	1465	1471	1481	rBV	640166	872383	82.24%	10.391%
63	10.189	1490	1493	1495	rBV2	536	459	0.04%	0.005%
64	10.299	1509	1511	1512	rBV	415	400	0.04%	0.005%
65	10.360	1520	1521	1524	rBV2	360	329	0.03%	0.004%
66	10.500	1542	1544	1547	rBV2	435	509	0.05%	0.006%
67	10.531	1547	1549	1552	rVB2	418	364	0.03%	0.004%
68	10.640	1566	1567	1570	rBV2	416	415	0.04%	0.005%
69	10.683	1572	1574	1577	rVB	475	578	0.05%	0.007%
70	10.720	1577	1580	1581	rBV	378	364	0.03%	0.004%
71	10.787	1589	1591	1594	rVB	410	316	0.03%	0.004%
72	10.945	1614	1617	1620	rVB2	366	544	0.05%	0.006%
73	11.031	1627	1631	1632	rBV2	357	368	0.03%	0.004%
74	11.079	1635	1639	1642	rBV2	566	658	0.06%	0.008%
75	11.195	1652	1658	1666	rBV	371849	473160	44.60%	5.636%
76	11.415	1693	1694	1697	rVB	466	325	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030462.D
 Acq On : 06 Aug 2022 14:22
 Operator : JC/MD
 Sample : VIBLK651
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK651

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
 Title : VOC Analysis

77	11.451	1697	1700	1701	rBV	486	452	0.04%	0.005%
78	11.537	1711	1714	1717	rBV2	569	822	0.08%	0.010%
79	11.652	1732	1733	1735	rBV	347	338	0.03%	0.004%
80	11.823	1759	1761	1764	rBV2	387	406	0.04%	0.005%
81	11.914	1772	1776	1778	rVB2	303	454	0.04%	0.005%
82	12.024	1788	1794	1804	rBV	634553	786002	74.09%	9.362%
83	12.262	1830	1833	1834	rBV	505	369	0.03%	0.004%
84	12.323	1837	1843	1850	rBV	541027	695957	65.60%	8.289%
85	12.646	1892	1896	1897	rBV	383	477	0.04%	0.006%
86	12.750	1910	1913	1914	rBV	471	366	0.03%	0.004%
87	12.975	1947	1950	1951	rBV2	560	618	0.06%	0.007%
88	13.103	1968	1971	1974	rBV2	443	664	0.06%	0.008%
89	13.170	1979	1982	1984	rBV3	689	849	0.08%	0.010%
90	13.195	1984	1986	1988	rVV2	445	321	0.03%	0.004%
91	13.823	2087	2089	2091	rBV	521	624	0.06%	0.007%
92	13.871	2093	2097	2101	rBV	733	1357	0.13%	0.016%
93	14.073	2128	2130	2133	rBV2	722	770	0.07%	0.009%
94	14.408	2183	2185	2187	rBV	392	420	0.04%	0.005%
95	14.816	2250	2252	2255	rBV2	666	703	0.07%	0.008%
96	15.011	2282	2284	2285	rBV2	616	394	0.04%	0.005%
97	15.329	2334	2336	2337	rBV2	664	374	0.04%	0.004%
98	15.347	2337	2339	2345	rBV3	721	1073	0.10%	0.013%
99	15.536	2369	2370	2371	rBV	563	361	0.03%	0.004%
100	15.920	2431	2433	2434	rBV2	805	536	0.05%	0.006%




Sum of corrected areas: 8395963

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030462.D
Acq On : 06 Aug 2022 14:22
Operator : JC/MD
Sample : VIBLK651
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK651

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

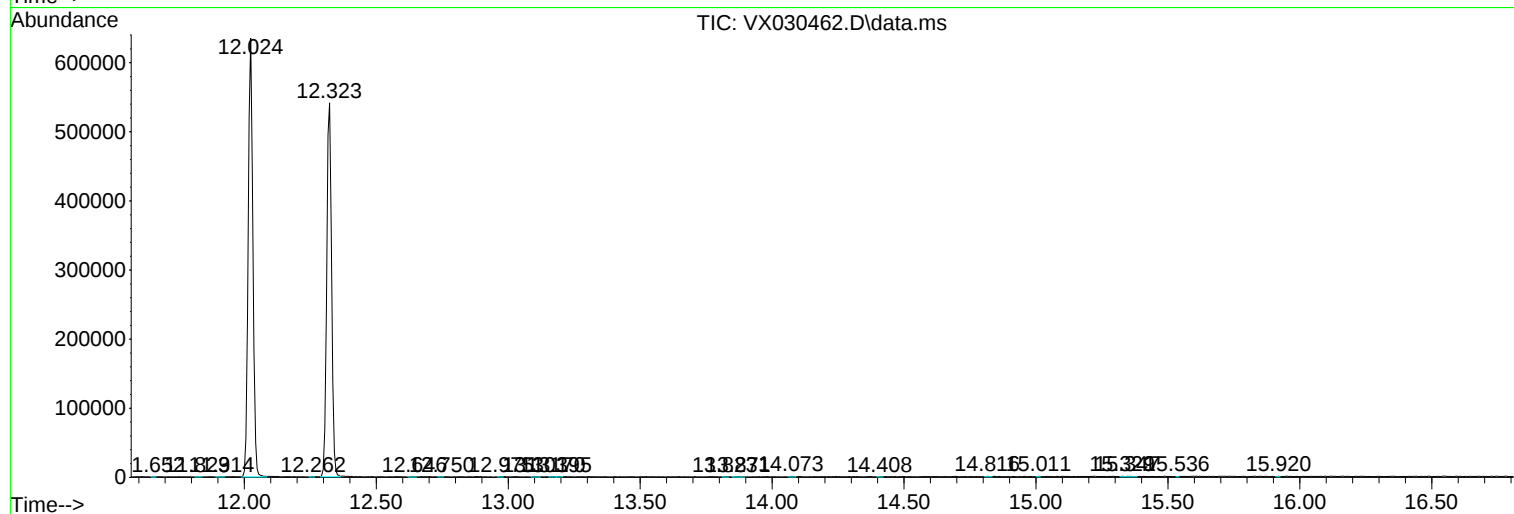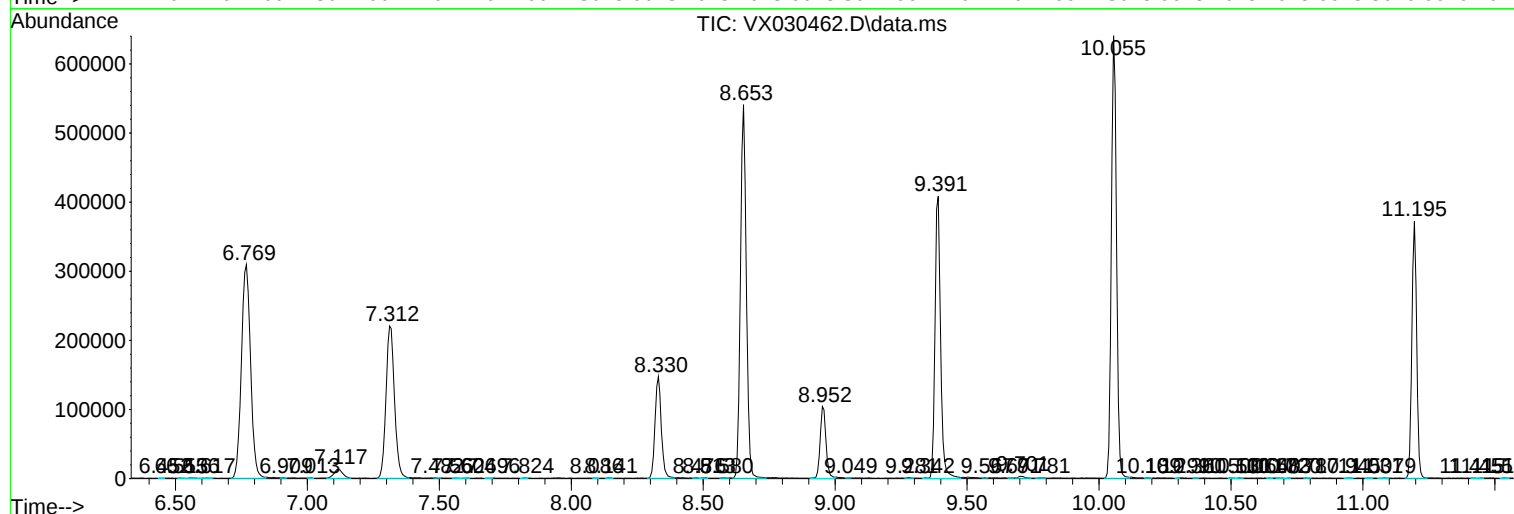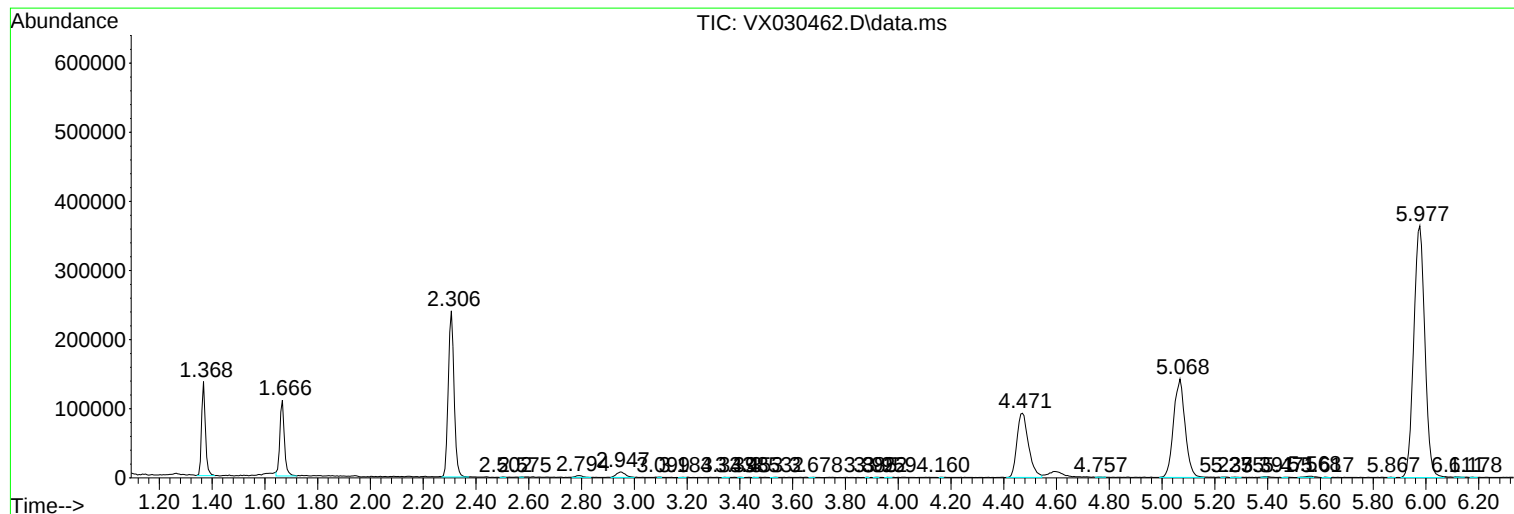

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030462.D
Acq On : 06 Aug 2022 14:22
Operator : JC/MD
Sample : VIBLK651
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK651

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030462.D
Acq On : 06 Aug 2022 14:22
Operator : JC/MD
Sample : VIBLK651
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK651

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc