

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030464.D
 Acq On : 06 Aug 2022 15:09
 Operator : JC/MD
 Sample : VIBLK652
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK652

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030464.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	56	rVB	143650	143598	13.43%	1.701%
2	1.666	91	95	104	rVB	107865	132655	12.41%	1.571%
3	2.306	194	200	211	rVB	226010	344953	32.27%	4.086%
4	2.556	239	241	242	rBV2	406	355	0.03%	0.004%
5	2.678	259	261	264	rVB2	356	345	0.03%	0.004%
6	2.715	264	267	269	rBV2	568	765	0.07%	0.009%
7	2.788	274	279	285	rBV4	2657	5269	0.49%	0.062%
8	2.886	292	295	297	rBV	344	395	0.04%	0.005%
9	2.946	297	305	316	rVB3	7400	18492	1.73%	0.219%
10	3.038	316	320	321	rBV	455	500	0.05%	0.006%
11	3.075	322	326	328	rBV2	336	471	0.04%	0.006%
12	3.605	409	413	414	rVB	439	523	0.05%	0.006%
13	3.635	414	418	419	rBV2	396	446	0.04%	0.005%
14	3.879	455	458	463	rVB	409	744	0.07%	0.009%
15	3.922	463	465	469	rBV	470	539	0.05%	0.006%
16	4.001	474	478	480	rBV2	375	491	0.05%	0.006%
17	4.111	495	496	501	rBV	507	473	0.04%	0.006%
18	4.190	505	509	512	rVB	362	455	0.04%	0.005%
19	4.233	515	516	518	rBV	310	288	0.03%	0.003%
20	4.471	546	555	568	rBV	94395	283044	26.48%	3.352%
21	5.068	641	653	669	rBV	141492	426090	39.86%	5.047%
22	5.239	680	681	683	rVV2	405	291	0.03%	0.003%
23	5.263	683	685	688	rVB2	562	640	0.06%	0.008%
24	5.367	700	702	704	rBV2	556	454	0.04%	0.005%
25	5.391	704	706	707	rBV	727	646	0.06%	0.008%
26	5.562	726	734	736	rBV4	1633	3179	0.30%	0.038%
27	5.976	790	802	821	rBV2	361619	1068959	100.00%	12.661%
28	6.165	832	833	836	rBV	356	314	0.03%	0.004%
29	6.190	836	837	841	rVB2	534	379	0.04%	0.004%
30	6.379	866	868	870	rVB2	687	469	0.04%	0.006%
31	6.403	870	872	875	rBV2	345	348	0.03%	0.004%
32	6.446	877	879	882	rVB2	378	282	0.03%	0.003%
33	6.513	888	890	891	rBV	471	301	0.03%	0.004%
34	6.574	898	900	903	rVB2	654	434	0.04%	0.005%
35	6.769	922	932	949	rVV	309255	732565	68.53%	8.676%
36	7.116	981	989	1000	rBV2	12286	27542	2.58%	0.326%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030464.D
 Acq On : 06 Aug 2022 15:09
 Operator : JC/MD
 Sample : VIBLK652
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK652

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.226	1004	1007	1009	rBV3	430	550	0.05%	0.007%
38	7.312	1013	1021	1035	rBV2	231335	495285	46.33%	5.866%
39	7.476	1045	1048	1049	rBV2	599	635	0.06%	0.008%
40	7.568	1062	1063	1066	rBV	463	274	0.03%	0.003%
41	7.811	1098	1103	1107	rVB2	486	870	0.08%	0.010%
42	7.866	1109	1112	1117	rVB	565	686	0.06%	0.008%
43	7.909	1117	1119	1121	rBV	324	305	0.03%	0.004%
44	7.939	1121	1124	1125	rBV2	338	343	0.03%	0.004%
45	8.013	1133	1136	1137	rBV	336	301	0.03%	0.004%
46	8.171	1158	1162	1163	rBV2	480	560	0.05%	0.007%
47	8.220	1168	1170	1171	rVB2	465	286	0.03%	0.003%
48	8.244	1171	1174	1175	rBV2	461	477	0.04%	0.006%
49	8.330	1182	1188	1200	rBV	147024	242085	22.65%	2.867%
50	8.653	1234	1241	1251	rBV	555067	849527	79.47%	10.062%
51	8.769	1258	1260	1267	rVB3	830	1239	0.12%	0.015%
52	8.951	1285	1290	1301	rVV	106360	159067	14.88%	1.884%
53	9.134	1318	1320	1323	rVB2	705	519	0.05%	0.006%
54	9.165	1323	1325	1328	rBV3	460	464	0.04%	0.005%
55	9.281	1342	1344	1348	rVB3	974	803	0.08%	0.010%
56	9.390	1356	1362	1384	rVV	415077	607495	56.83%	7.195%
57	9.537	1384	1386	1391	rVB4	1188	1613	0.15%	0.019%
58	9.579	1391	1393	1396	rVB2	700	785	0.07%	0.009%
59	9.610	1396	1398	1399	rBV2	497	328	0.03%	0.004%
60	9.707	1408	1414	1419	rBV	3090	5157	0.48%	0.061%
61	9.787	1425	1427	1429	rVB2	548	416	0.04%	0.005%
62	9.811	1429	1431	1432	rBV2	307	270	0.03%	0.003%
63	9.896	1444	1445	1447	rBV	593	446	0.04%	0.005%
64	9.988	1459	1460	1463	rBV2	392	435	0.04%	0.005%
65	10.055	1465	1471	1486	rVV	626118	863185	80.75%	10.223%
66	10.189	1492	1493	1494	rBV	419	287	0.03%	0.003%
67	10.293	1508	1510	1512	rBV	322	347	0.03%	0.004%
68	10.335	1515	1517	1518	rBV	618	440	0.04%	0.005%
69	10.537	1546	1550	1551	rBV2	343	447	0.04%	0.005%
70	10.969	1620	1621	1627	rVV	424	449	0.04%	0.005%
71	11.024	1627	1630	1632	rVV2	330	299	0.03%	0.004%
72	11.104	1641	1643	1646	rBV	421	328	0.03%	0.004%
73	11.195	1652	1658	1671	rBV	389343	483942	45.27%	5.732%
74	11.427	1694	1696	1699	rVB	514	283	0.03%	0.003%
75	11.451	1699	1700	1703	rBV2	279	308	0.03%	0.004%
76	11.622	1726	1728	1730	rBV2	280	277	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030464.D
 Acq On : 06 Aug 2022 15:09
 Operator : JC/MD
 Sample : VIBLK652
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK652

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.677	1735	1737	1738	rBV	586	332	0.03%	0.004%
78	11.774	1751	1753	1754	rBV	800	467	0.04%	0.006%
79	12.024	1789	1794	1802	rBV	677246	794343	74.31%	9.408%
80	12.213	1824	1825	1827	rBV2	441	336	0.03%	0.004%
81	12.323	1837	1843	1851	rBV	570831	718251	67.19%	8.507%
82	12.615	1888	1891	1894	rVB	518	523	0.05%	0.006%
83	12.951	1944	1946	1947	rVB	502	332	0.03%	0.004%
84	13.091	1967	1969	1972	rVB	417	341	0.03%	0.004%
85	13.152	1977	1979	1980	rBV2	390	363	0.03%	0.004%
86	13.170	1980	1982	1984	rBV	539	463	0.04%	0.005%
87	13.262	1994	1997	1998	rBV2	405	338	0.03%	0.004%
88	13.487	2032	2034	2035	rVB	621	297	0.03%	0.004%
89	13.762	2077	2079	2083	rBV2	687	960	0.09%	0.011%
90	13.877	2094	2098	2100	rBV2	436	617	0.06%	0.007%
91	14.048	2124	2126	2128	rBV	385	342	0.03%	0.004%
92	14.073	2128	2130	2131	rBV2	666	468	0.04%	0.006%
93	14.152	2142	2143	2145	rBV2	396	284	0.03%	0.003%
94	14.554	2206	2209	2211	rVB	628	547	0.05%	0.006%
95	14.603	2215	2217	2218	rBV2	662	450	0.04%	0.005%
96	14.816	2250	2252	2253	rBV	535	368	0.03%	0.004%
97	15.408	2347	2349	2350	rBV2	611	378	0.04%	0.004%
98	15.469	2356	2359	2362	rBV3	743	1083	0.10%	0.013%
99	16.426	2514	2516	2521	rBV4	648	877	0.08%	0.010%
100	16.639	2549	2551	2553	rBV3	1107	955	0.09%	0.011%




Sum of corrected areas: 8443222

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030464.D
Acq On : 06 Aug 2022 15:09
Operator : JC/MD
Sample : VIBLK652
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK652

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXL080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

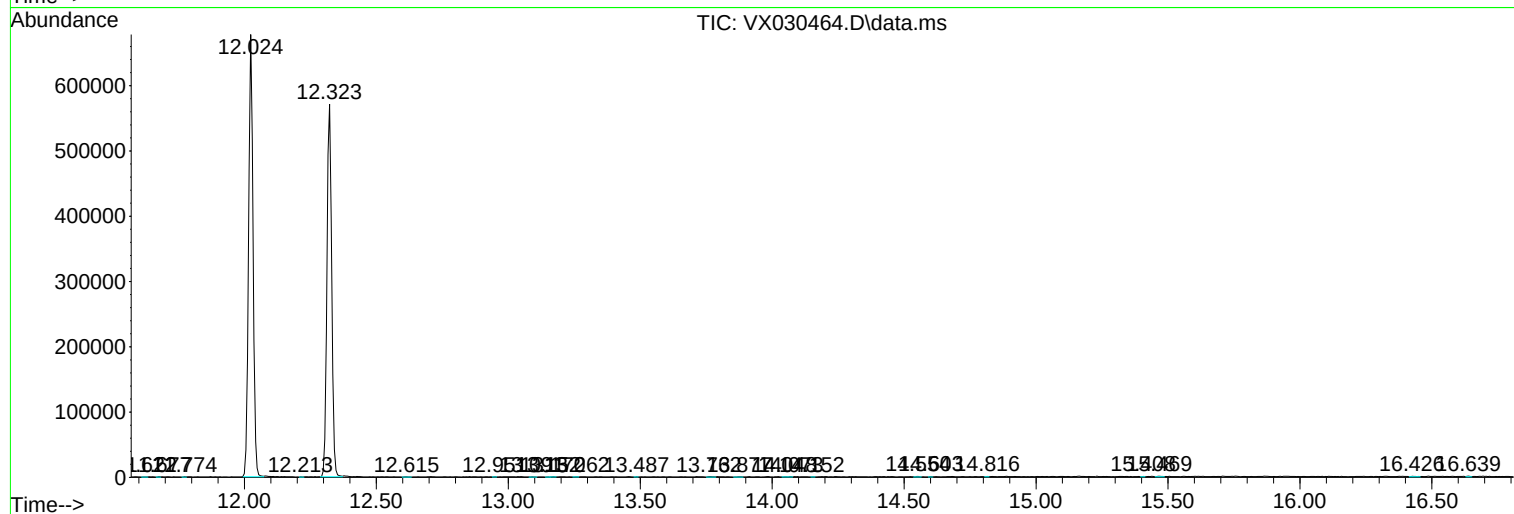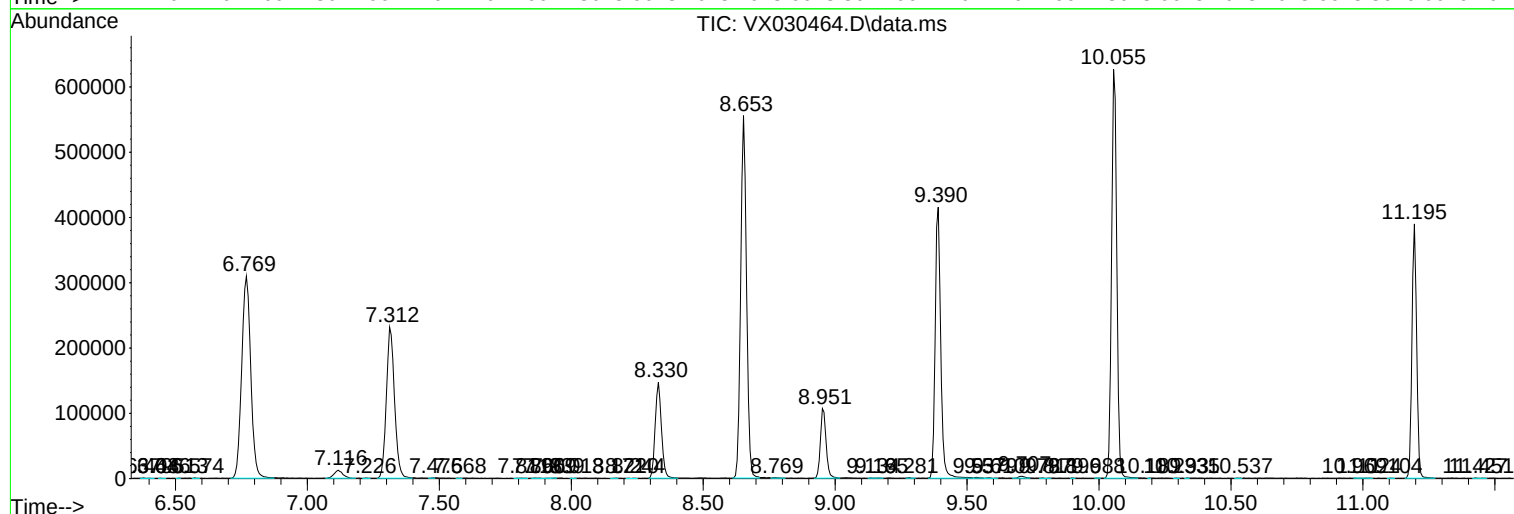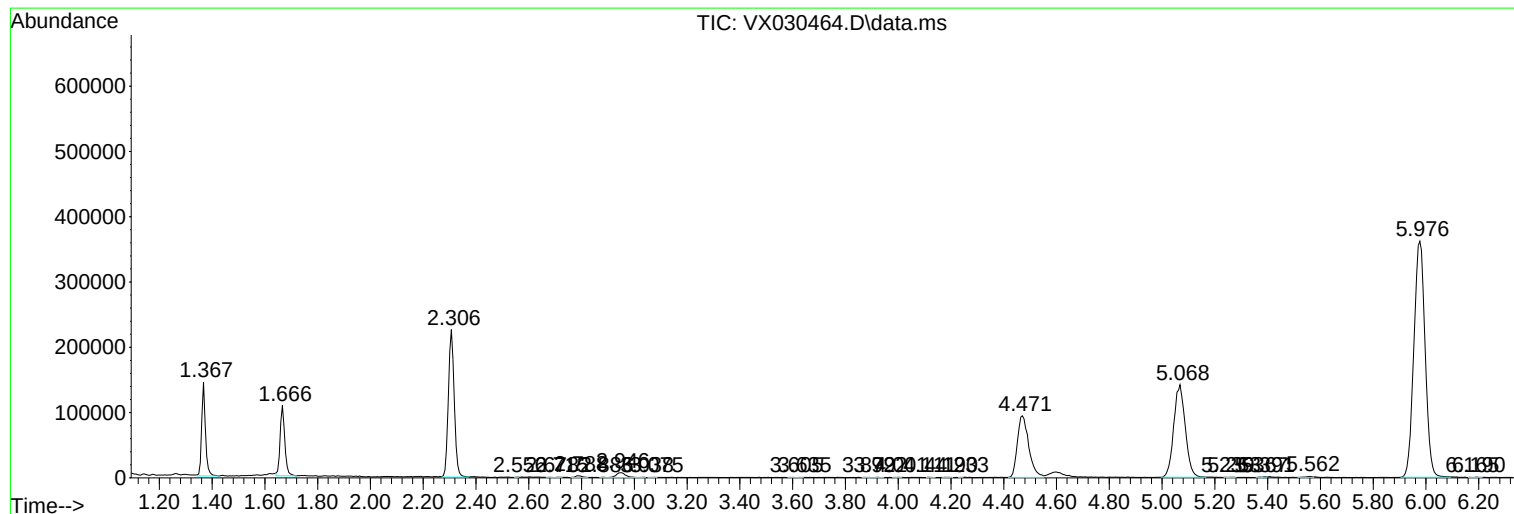

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030464.D
Acq On : 06 Aug 2022 15:09
Operator : JC/MD
Sample : VIBLK652
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK652

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030464.D
Acq On : 06 Aug 2022 15:09
Operator : JC/MD
Sample : VIBLK652
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK652

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc