

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030465.D
 Acq On : 06 Aug 2022 15:32
 Operator : JC/MD
 Sample : N4003-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030465.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	59	rVB	2114390	2292046	100.00%	21.064%
2	1.666	91	95	103	rVB	104533	125531	5.48%	1.154%
3	2.142	162	173	182	rBV5	4784	19567	0.85%	0.180%
4	2.306	194	200	210	rVV	241621	370887	16.18%	3.409%
5	2.392	210	214	219	rVB	5894	9091	0.40%	0.084%
6	2.495	229	231	236	rBV4	590	783	0.03%	0.007%
7	2.745	270	272	274	rVV	542	316	0.01%	0.003%
8	2.770	274	276	277	rVV3	443	486	0.02%	0.004%
9	2.788	277	279	285	rVV3	1262	1782	0.08%	0.016%
10	2.855	288	290	292	rBV	406	358	0.02%	0.003%
11	2.904	296	298	301	rVB2	539	540	0.02%	0.005%
12	3.093	322	329	339	rBV2	33092	67276	2.94%	0.618%
13	3.733	433	434	437	rBV2	475	486	0.02%	0.004%
14	3.989	474	476	478	rBV	373	306	0.01%	0.003%
15	4.020	478	481	483	rBV	420	332	0.01%	0.003%
16	4.257	519	520	524	rVV	419	444	0.02%	0.004%
17	4.367	536	538	541	rBV2	486	509	0.02%	0.005%
18	4.489	545	558	582	rBV3	196671	685819	29.92%	6.303%
19	4.769	602	604	608	rVB3	299	438	0.02%	0.004%
20	5.068	641	653	667	rVV	139124	413168	18.03%	3.797%
21	5.336	695	697	699	rBV2	314	312	0.01%	0.003%
22	5.385	699	705	709	rBV5	1062	2474	0.11%	0.023%
23	5.525	724	728	729	rVV2	422	519	0.02%	0.005%
24	5.556	729	733	737	rVV4	1624	3475	0.15%	0.032%
25	5.611	740	742	744	rVB2	650	535	0.02%	0.005%
26	5.660	747	750	753	rBV2	253	312	0.01%	0.003%
27	5.690	753	755	757	rVB2	434	429	0.02%	0.004%
28	5.800	772	773	775	rBV	411	322	0.01%	0.003%
29	5.977	790	802	818	rBV2	354222	1039908	45.37%	9.557%
30	6.111	822	824	828	rVB4	726	697	0.03%	0.006%
31	6.361	863	865	866	rBV	422	447	0.02%	0.004%
32	6.507	888	889	892	rBV	392	379	0.02%	0.003%
33	6.562	895	898	899	rBV	519	427	0.02%	0.004%
34	6.678	915	917	920	rVB2	325	341	0.01%	0.003%
35	6.769	922	932	945	rBV	300634	720259	31.42%	6.619%
36	7.117	980	989	996	rBV4	12130	27861	1.22%	0.256%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030465.D
 Acq On : 06 Aug 2022 15:32
 Operator : JC/MD
 Sample : N4003-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.312	1012	1021	1039	rVV	216742	476741	20.80%	4.381%
38	7.580	1062	1065	1066	rVB2	480	388	0.02%	0.004%
39	7.623	1066	1072	1073	rVB2	293	395	0.02%	0.004%
40	7.677	1077	1081	1083	rBV2	328	464	0.02%	0.004%
41	7.757	1092	1094	1098	rVB	286	313	0.01%	0.003%
42	7.812	1100	1103	1104	rBV2	373	398	0.02%	0.004%
43	7.885	1113	1115	1117	rBV2	444	306	0.01%	0.003%
44	7.903	1117	1118	1120	rBV	560	352	0.02%	0.003%
45	7.927	1120	1122	1123	rVB	754	398	0.02%	0.004%
46	7.946	1123	1125	1128	rBV2	704	891	0.04%	0.008%
47	8.031	1136	1139	1140	rVB2	421	312	0.01%	0.003%
48	8.129	1153	1155	1157	rBV	438	311	0.01%	0.003%
49	8.330	1181	1188	1197	rBV	145081	233217	10.18%	2.143%
50	8.500	1214	1216	1220	rBV2	594	602	0.03%	0.006%
51	8.653	1234	1241	1250	rBV	539586	817348	35.66%	7.512%
52	8.848	1271	1273	1274	rBV2	629	582	0.03%	0.005%
53	8.958	1284	1291	1299	rBV	102396	157027	6.85%	1.443%
54	9.074	1308	1310	1311	rBV	521	313	0.01%	0.003%
55	9.275	1341	1343	1347	rVB4	829	941	0.04%	0.009%
56	9.391	1356	1362	1380	rBV	411278	594467	25.94%	5.463%
57	9.848	1436	1437	1440	rVB	477	354	0.02%	0.003%
58	9.982	1457	1459	1461	rBV	397	399	0.02%	0.004%
59	10.055	1465	1471	1482	rBV	614720	846423	36.93%	7.779%
60	10.305	1511	1512	1517	rVB3	872	758	0.03%	0.007%
61	10.537	1548	1550	1552	rBV2	342	380	0.02%	0.003%
62	10.921	1609	1613	1617	rVB2	377	658	0.03%	0.006%
63	10.957	1617	1619	1620	rBV2	437	352	0.02%	0.003%
64	10.994	1623	1625	1626	rBV	545	445	0.02%	0.004%
65	11.195	1653	1658	1666	rBV	368655	462515	20.18%	4.251%
66	11.409	1691	1693	1695	rBV2	277	330	0.01%	0.003%
67	11.439	1695	1698	1702	rVB2	529	721	0.03%	0.007%
68	11.469	1702	1703	1706	rBV3	707	717	0.03%	0.007%
69	11.573	1718	1720	1724	rBV2	396	495	0.02%	0.005%
70	11.695	1738	1740	1741	rBV2	721	482	0.02%	0.004%
71	11.719	1741	1744	1745	rVV	365	373	0.02%	0.003%
72	12.024	1788	1794	1803	rBV	665124	779465	34.01%	7.163%
73	12.207	1822	1824	1826	rBV2	687	573	0.02%	0.005%
74	12.232	1826	1828	1831	rVB2	683	681	0.03%	0.006%
75	12.323	1837	1843	1854	rBV	559261	697099	30.41%	6.406%
76	12.561	1879	1882	1883	rBV2	568	685	0.03%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030465.D
 Acq On : 06 Aug 2022 15:32
 Operator : JC/MD
 Sample : N4003-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.658	1896	1898	1899	rVB2	547	315	0.01%	0.003%
78	12.683	1899	1902	1904	rBV2	317	414	0.02%	0.004%
79	12.799	1919	1921	1924	rBV	281	450	0.02%	0.004%
80	12.847	1927	1929	1931	rBV2	315	324	0.01%	0.003%
81	12.908	1937	1939	1941	rBV	298	318	0.01%	0.003%
82	13.152	1975	1979	1980	rBV2	342	366	0.02%	0.003%
83	13.183	1982	1984	1986	rVV	535	373	0.02%	0.003%
84	13.280	1998	2000	2004	rBV	379	553	0.02%	0.005%
85	13.378	2014	2016	2018	rBV	538	488	0.02%	0.004%
86	13.414	2018	2022	2025	rVB2	449	572	0.02%	0.005%
87	13.591	2047	2051	2055	rBV2	575	919	0.04%	0.008%
88	13.926	2105	2106	2110	rVB	515	361	0.02%	0.003%
89	14.073	2127	2130	2133	rBV2	546	906	0.04%	0.008%
90	14.225	2152	2155	2156	rBV2	626	584	0.03%	0.005%
91	14.274	2159	2163	2167	rBV3	559	1155	0.05%	0.011%
92	14.493	2197	2199	2200	rBV	525	356	0.02%	0.003%
93	14.865	2258	2260	2263	rBV2	514	618	0.03%	0.006%
94	14.896	2263	2265	2268	rVV2	629	575	0.03%	0.005%
95	15.060	2291	2292	2294	rBV	794	500	0.02%	0.005%
96	15.554	2371	2373	2376	rVB3	831	858	0.04%	0.008%
97	15.585	2376	2378	2379	rBV2	452	399	0.02%	0.004%
98	15.731	2401	2402	2403	rBV	608	321	0.01%	0.003%
99	15.847	2419	2421	2423	rBV2	556	498	0.02%	0.005%
100	15.981	2441	2443	2444	rBV2	708	474	0.02%	0.004%




Sum of corrected areas: 10881230

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030465.D
Acq On : 06 Aug 2022 15:32
Operator : JC/MD
Sample : N4003-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

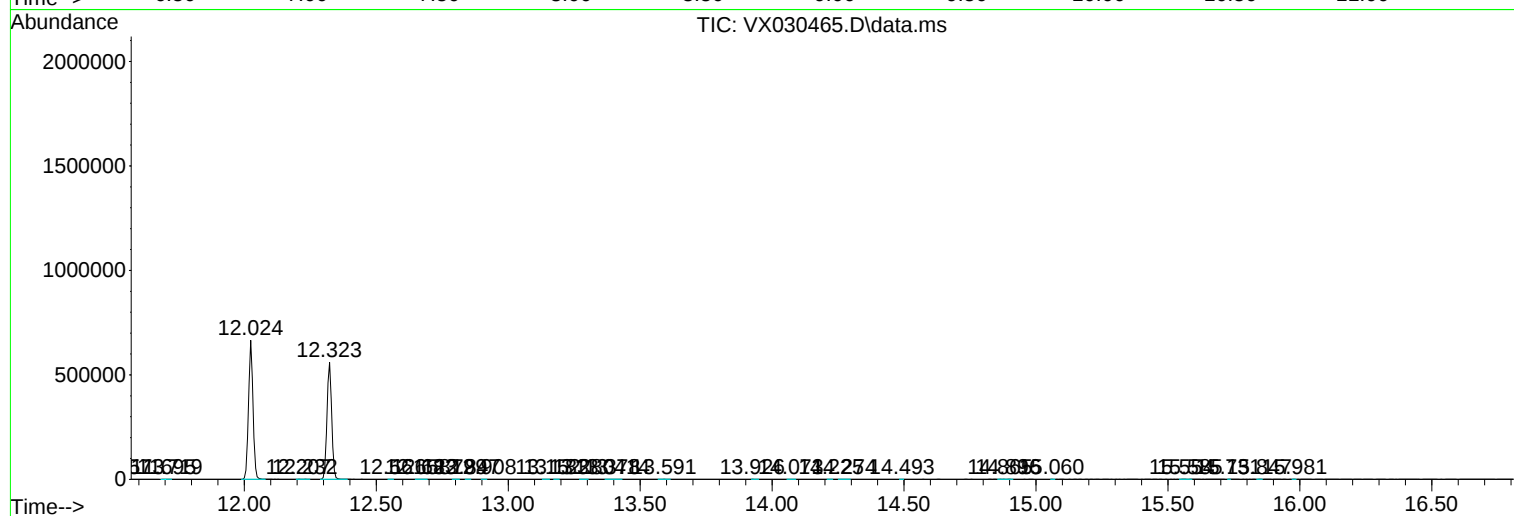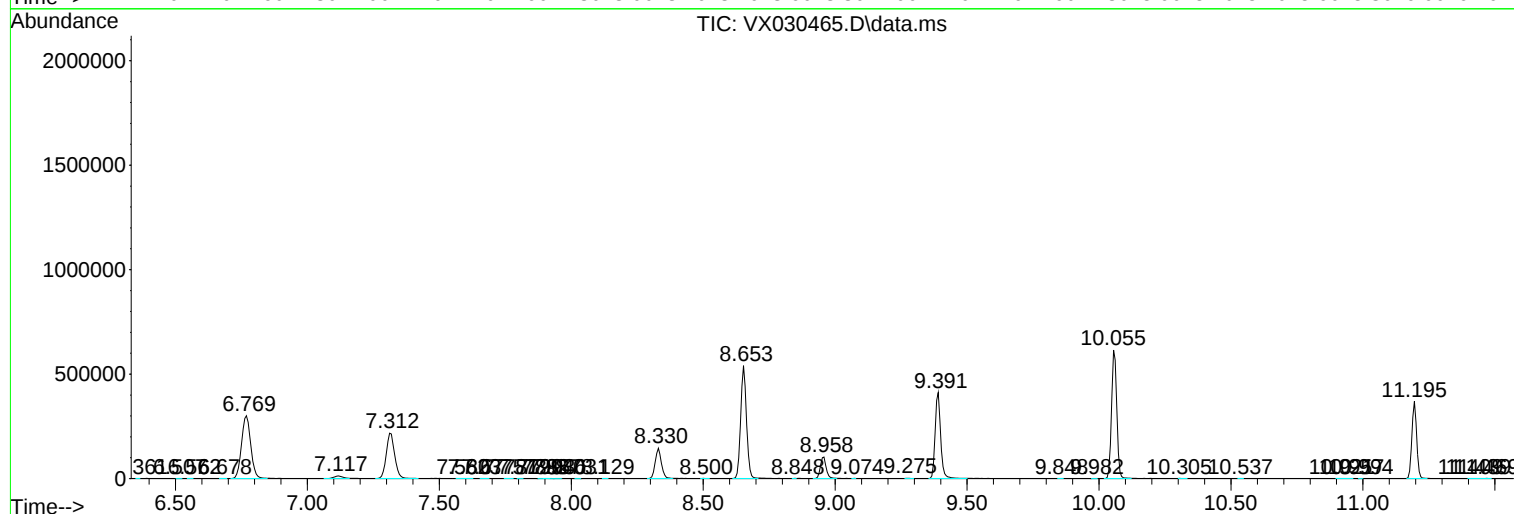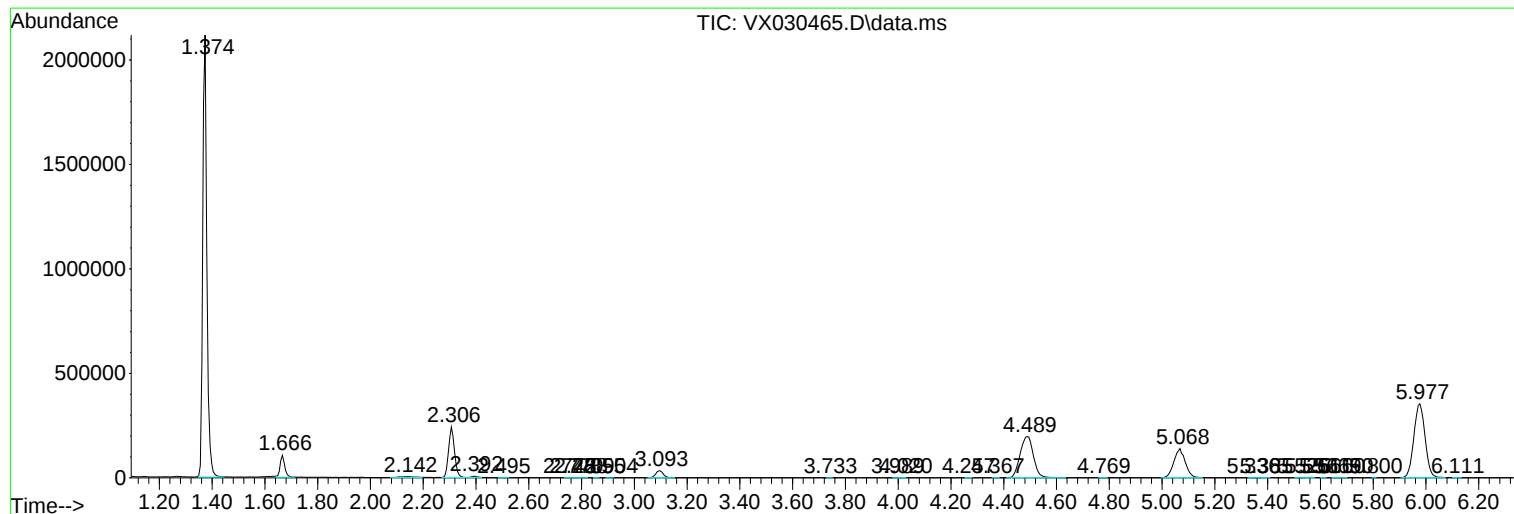

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030465.D
Acq On : 06 Aug 2022 15:32
Operator : JC/MD
Sample : N4003-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030465.D
Acq On : 06 Aug 2022 15:32
Operator : JC/MD
Sample : N4003-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc