

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030468.D
 Acq On : 06 Aug 2022 16:42
 Operator : JC/MD
 Sample : N4021-10DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D66DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030468.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	56	rVB	117634	134670	12.92%	1.565%
2	1.660	91	94	100	rBV	74892	87703	8.41%	1.019%
3	2.300	193	199	210	rVB	212832	331370	31.78%	3.852%
4	2.489	227	230	231	rBV3	556	461	0.04%	0.005%
5	2.550	239	240	244	rBV2	458	372	0.04%	0.004%
6	2.782	274	278	290	rVB2	4436	9257	0.89%	0.108%
7	2.873	290	293	294	rBV2	515	438	0.04%	0.005%
8	2.947	297	305	315	rVV	18076	43662	4.19%	0.508%
9	3.093	323	329	338	rVB3	6580	13690	1.31%	0.159%
10	3.325	364	367	369	rBV	848	609	0.06%	0.007%
11	3.440	383	386	389	rBV2	447	654	0.06%	0.008%
12	3.672	421	424	425	rBV2	397	495	0.05%	0.006%
13	3.812	444	447	450	rBV2	328	413	0.04%	0.005%
14	4.038	481	484	487	rVV	578	656	0.06%	0.008%
15	4.184	506	508	511	rBV2	306	371	0.04%	0.004%
16	4.215	511	513	516	rVV2	486	377	0.04%	0.004%
17	4.483	544	557	571	rBV2	215796	662133	63.51%	7.697%
18	4.824	611	613	614	rBV2	551	393	0.04%	0.005%
19	5.068	640	653	670	rVB	137669	417742	40.07%	4.856%
20	5.349	695	699	701	rBV3	420	633	0.06%	0.007%
21	5.391	704	706	708	rBV3	808	726	0.07%	0.008%
22	5.538	728	730	732	rBV	1150	1150	0.11%	0.013%
23	5.702	753	757	758	rBV	344	423	0.04%	0.005%
24	5.788	770	771	774	rBV2	468	465	0.04%	0.005%
25	5.818	774	776	781	rVB2	390	432	0.04%	0.005%
26	5.977	790	802	819	rBV2	358047	1042636	100.00%	12.120%
27	6.105	821	823	828	rBV4	958	1283	0.12%	0.015%
28	6.281	850	852	855	rBV2	819	884	0.08%	0.010%
29	6.354	859	864	866	rBV4	2176	3439	0.33%	0.040%
30	6.489	883	886	889	rVB3	605	733	0.07%	0.009%
31	6.531	889	893	894	rBV2	333	372	0.04%	0.004%
32	6.550	894	896	902	rVB2	672	683	0.07%	0.008%
33	6.653	909	913	916	rBV2	424	572	0.05%	0.007%
34	6.763	921	931	948	rBV	303741	740599	71.03%	8.609%
35	6.946	960	961	965	rVB2	597	522	0.05%	0.006%
36	6.976	965	966	971	rVB2	574	772	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030468.D
 Acq On : 06 Aug 2022 16:42
 Operator : JC/MD
 Sample : N4021-10DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D66DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.129	982	991	1003	rBV4	41667	104819	10.05%	1.218%
38	7.214	1003	1005	1010	rVB4	1508	1991	0.19%	0.023%
39	7.312	1010	1021	1033	rBV	216071	472893	45.36%	5.497%
40	7.751	1089	1093	1096	rVB2	435	555	0.05%	0.006%
41	7.909	1117	1119	1120	rBV	470	358	0.03%	0.004%
42	8.062	1141	1144	1145	rVB2	631	472	0.05%	0.005%
43	8.092	1145	1149	1151	rVB2	474	597	0.06%	0.007%
44	8.330	1182	1188	1203	rBV	134946	231579	22.21%	2.692%
45	8.653	1234	1241	1252	rBV	532060	824235	79.05%	9.581%
46	8.763	1255	1259	1264	rVV3	2524	4731	0.45%	0.055%
47	8.830	1268	1270	1272	rBV2	487	490	0.05%	0.006%
48	8.958	1285	1291	1303	rBV	97229	152143	14.59%	1.769%
49	9.092	1312	1313	1315	rBV	437	451	0.04%	0.005%
50	9.275	1338	1343	1348	rBV5	2461	4009	0.38%	0.047%
51	9.397	1356	1363	1376	rBV	337769	555250	53.25%	6.454%
52	9.708	1409	1414	1419	rBV4	1666	3127	0.30%	0.036%
53	9.836	1432	1435	1437	rBV2	303	351	0.03%	0.004%
54	10.055	1466	1471	1489	rVB	635807	867583	83.21%	10.085%
55	10.445	1533	1535	1538	rVB2	535	564	0.05%	0.007%
56	10.585	1556	1558	1560	rVB	552	392	0.04%	0.005%
57	10.628	1563	1565	1567	rBV2	332	353	0.03%	0.004%
58	10.829	1593	1598	1599	rBV	466	613	0.06%	0.007%
59	10.945	1616	1617	1619	rBV	612	542	0.05%	0.006%
60	11.195	1652	1658	1671	rBV	347142	449846	43.15%	5.229%
61	11.408	1691	1693	1698	rBV2	432	693	0.07%	0.008%
62	11.457	1698	1701	1702	rBV2	496	485	0.05%	0.006%
63	11.677	1736	1737	1740	rBV2	408	366	0.04%	0.004%
64	11.707	1740	1742	1746	rVB2	589	615	0.06%	0.007%
65	11.756	1749	1750	1753	rBV	650	443	0.04%	0.005%
66	11.878	1769	1770	1775	rBV2	263	375	0.04%	0.004%
67	11.951	1779	1782	1785	rBV3	593	688	0.07%	0.008%
68	11.988	1785	1788	1789	rBV2	410	512	0.05%	0.006%
69	12.024	1789	1794	1804	rBV	627712	754087	72.33%	8.766%
70	12.323	1837	1843	1851	rBV	530769	648770	62.22%	7.541%
71	12.451	1862	1864	1865	rVB	730	347	0.03%	0.004%
72	12.481	1865	1869	1873	rBV2	325	473	0.05%	0.005%
73	12.658	1894	1898	1900	rVB2	388	425	0.04%	0.005%
74	12.689	1900	1903	1904	rBV	390	392	0.04%	0.005%
75	12.872	1930	1933	1936	rVV3	454	614	0.06%	0.007%
76	12.987	1948	1952	1956	rBV2	406	730	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030468.D
 Acq On : 06 Aug 2022 16:42
 Operator : JC/MD
 Sample : N4021-10DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D66DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	13.109	1970	1972	1973	rBV2	486	407	0.04%	0.005%
78	13.475	2029	2032	2034	rBV2	470	549	0.05%	0.006%
79	13.603	2048	2053	2055	rBV2	497	723	0.07%	0.008%
80	13.689	2066	2067	2070	rBV2	407	477	0.05%	0.006%
81	13.835	2089	2091	2094	rBV	354	355	0.03%	0.004%
82	13.865	2094	2096	2099	rVV2	426	373	0.04%	0.004%
83	14.079	2128	2131	2132	rVB	513	415	0.04%	0.005%
84	14.103	2132	2135	2136	rBV	476	352	0.03%	0.004%
85	14.134	2139	2140	2142	rVB	624	419	0.04%	0.005%
86	14.274	2158	2163	2165	rBV2	470	746	0.07%	0.009%
87	14.676	2227	2229	2235	rBV2	354	522	0.05%	0.006%
88	14.780	2244	2246	2249	rVB	661	677	0.06%	0.008%
89	14.810	2249	2251	2252	rBV	546	376	0.04%	0.004%
90	15.121	2300	2302	2305	rBV2	753	727	0.07%	0.008%
91	15.188	2311	2313	2315	rBV2	584	356	0.03%	0.004%
92	15.542	2370	2371	2373	rBV2	741	414	0.04%	0.005%
93	15.731	2400	2402	2404	rBV2	867	718	0.07%	0.008%
94	15.987	2442	2444	2446	rVB2	792	484	0.05%	0.006%
95	16.048	2451	2454	2456	rBV2	795	886	0.08%	0.010%
96	16.072	2456	2458	2459	rBV	646	356	0.03%	0.004%
97	16.152	2469	2471	2473	rVB	669	403	0.04%	0.005%
98	16.420	2512	2515	2518	rBV3	709	1230	0.12%	0.014%
99	16.542	2533	2535	2537	rBV2	668	627	0.06%	0.007%
100	16.755	2568	2570	2571	rBV	897	511	0.05%	0.006%




Sum of corrected areas: 8602852

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030468.D
Acq On : 06 Aug 2022 16:42
Operator : JC/MD
Sample : N4021-10DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D66DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

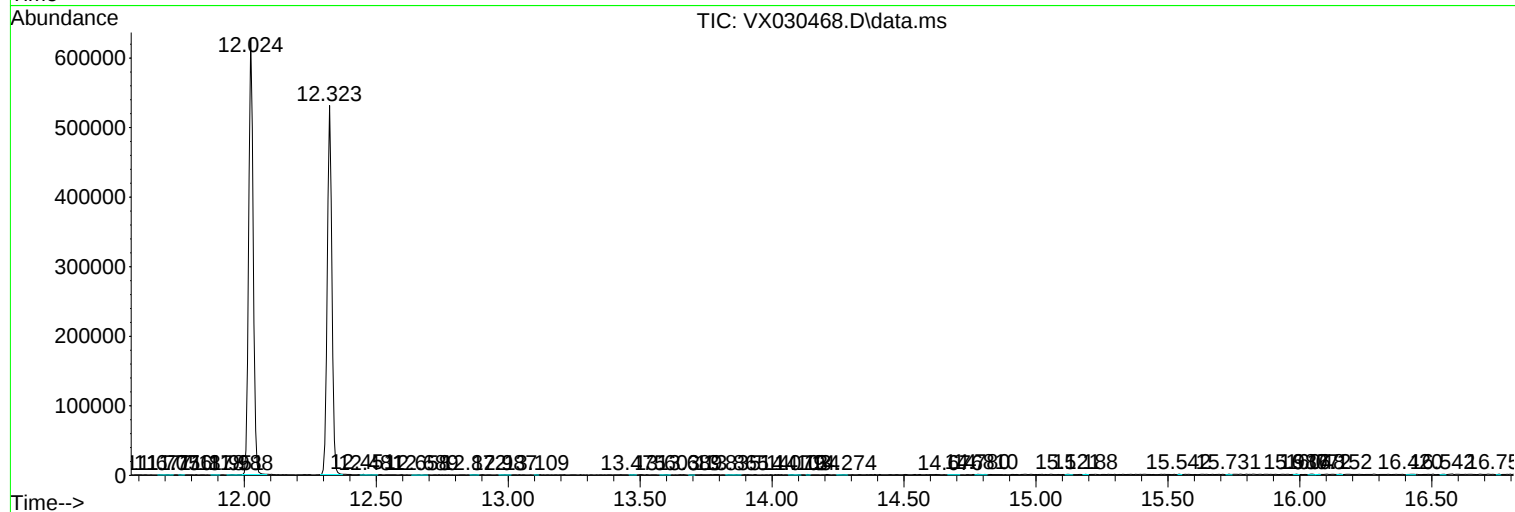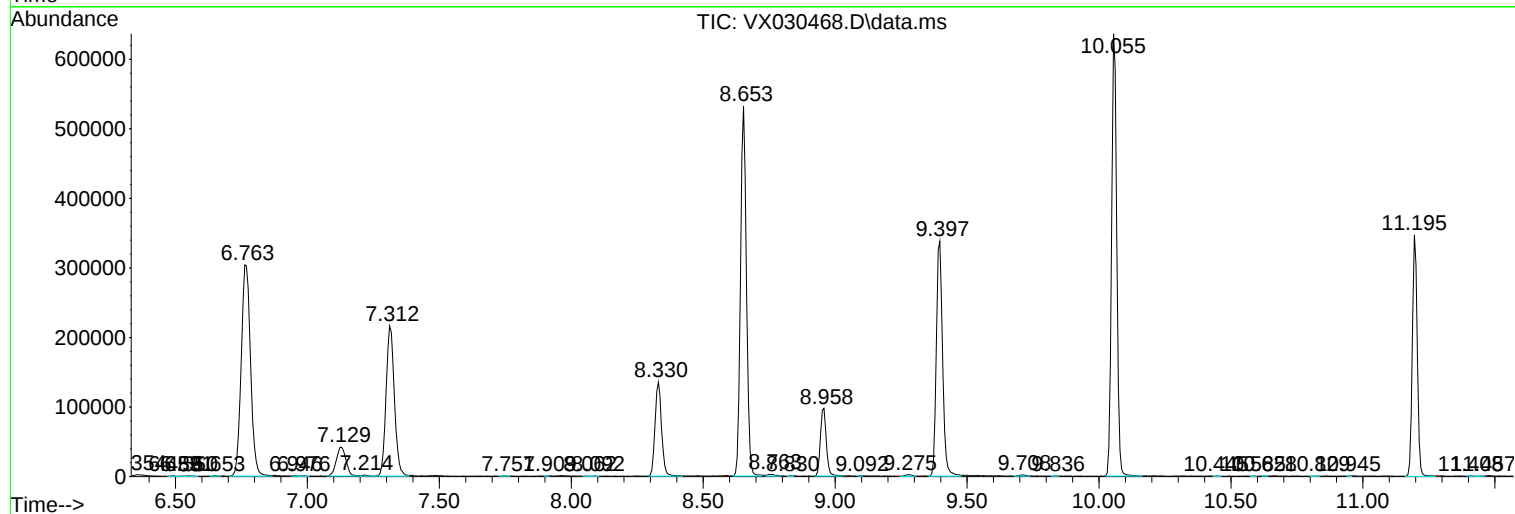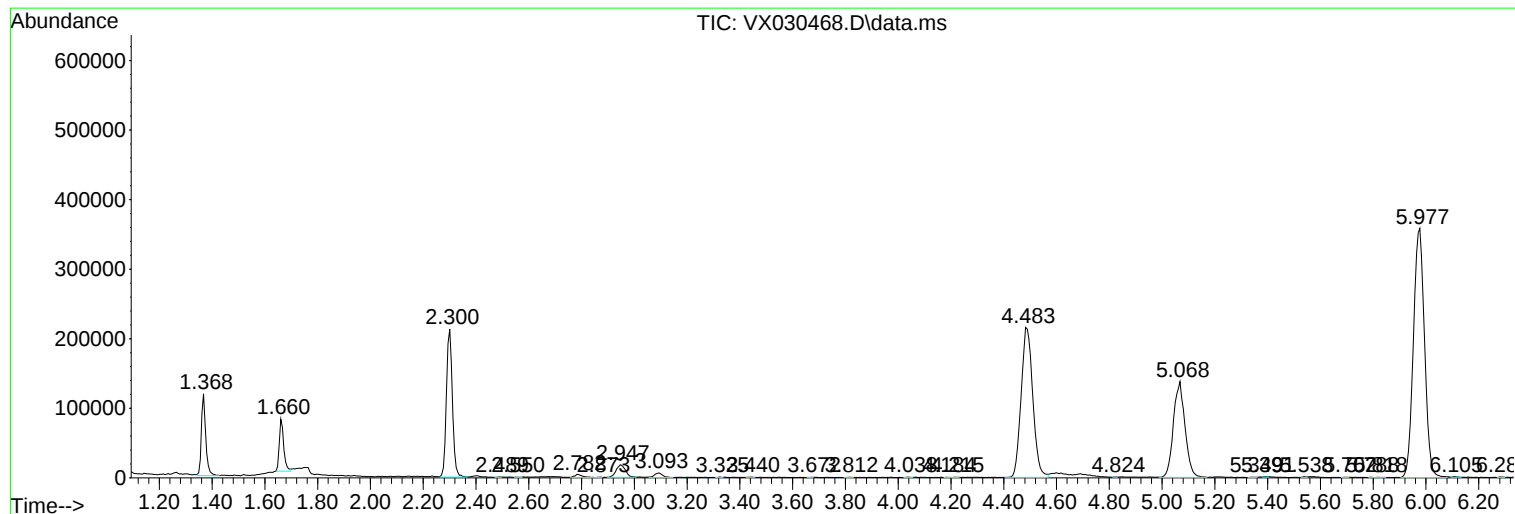

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030468.D
Acq On : 06 Aug 2022 16:42
Operator : JC/MD
Sample : N4021-10DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D66DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030468.D
Acq On : 06 Aug 2022 16:42
Operator : JC/MD
Sample : N4021-10DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D66DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc