

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030469.D
 Acq On : 06 Aug 2022 17:06
 Operator : JC/MD
 Sample : N4021-11DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D67DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030469.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	57	rVB2	311717	362974	33.84%	4.126%
2	1.660	91	94	102	rBV	74675	86751	8.09%	0.986%
3	2.300	193	199	210	rVB	212629	336962	31.41%	3.830%
4	2.404	210	216	225	rVB2	1982	4951	0.46%	0.056%
5	2.599	244	248	251	rBV2	794	1507	0.14%	0.017%
6	2.782	274	278	282	rBV6	3804	7900	0.74%	0.090%
7	2.953	298	306	318	rVB	18753	45407	4.23%	0.516%
8	3.087	323	328	337	rVB2	12759	24612	2.29%	0.280%
9	3.318	362	366	367	rBV3	346	389	0.04%	0.004%
10	3.440	379	386	392	rBV5	1059	2885	0.27%	0.033%
11	3.532	400	401	405	rBV	290	381	0.04%	0.004%
12	3.623	414	416	420	rVB2	494	602	0.06%	0.007%
13	3.684	420	426	428	rBV2	428	794	0.07%	0.009%
14	3.715	428	431	433	rVV2	484	519	0.05%	0.006%
15	3.739	433	435	439	rVV	349	404	0.04%	0.005%
16	3.837	448	451	453	rBV3	554	845	0.08%	0.010%
17	3.952	469	470	474	rBV	276	401	0.04%	0.005%
18	4.074	489	490	493	rVB	466	384	0.04%	0.004%
19	4.209	507	512	517	rBV5	975	1669	0.16%	0.019%
20	4.294	520	526	535	rVB3	5571	14960	1.39%	0.170%
21	4.373	537	539	543	rVB2	398	368	0.03%	0.004%
22	4.483	547	557	573	rBV3	163734	515147	48.02%	5.856%
23	4.873	620	621	624	rVB3	790	457	0.04%	0.005%
24	5.068	641	653	673	rVB	137950	425718	39.69%	4.839%
25	5.342	695	698	700	rBV2	517	557	0.05%	0.006%
26	5.367	700	702	704	rVV2	737	625	0.06%	0.007%
27	5.391	704	706	711	rVV3	997	1526	0.14%	0.017%
28	5.464	713	718	730	rVB5	5008	14295	1.33%	0.162%
29	5.684	753	754	757	rVB2	447	379	0.04%	0.004%
30	5.751	763	765	767	rBV2	383	417	0.04%	0.005%
31	5.830	773	778	784	rVB4	1716	4148	0.39%	0.047%
32	5.977	787	802	821	rBV2	371271	1072669	100.00%	12.193%
33	6.147	829	830	832	rBV	686	577	0.05%	0.007%
34	6.361	859	865	875	rVB8	3390	9553	0.89%	0.109%
35	6.769	922	932	949	rBV	305161	739714	68.96%	8.408%
36	7.025	971	974	976	rVV3	322	422	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030469.D
 Acq On : 06 Aug 2022 17:06
 Operator : JC/MD
 Sample : N4021-11DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D67DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.117	981	989	999	rVB6	12183	30843	2.88%	0.351%
38	7.190	999	1001	1002	rBV	405	363	0.03%	0.004%
39	7.220	1002	1006	1011	rVB5	1117	2145	0.20%	0.024%
40	7.312	1011	1021	1031	rBV	223008	488736	45.56%	5.556%
41	7.482	1047	1049	1054	rVB4	853	1223	0.11%	0.014%
42	7.531	1054	1057	1061	rVB	645	899	0.08%	0.010%
43	7.562	1061	1062	1067	rBV2	509	570	0.05%	0.006%
44	7.653	1074	1077	1078	rBV2	783	814	0.08%	0.009%
45	7.708	1085	1086	1088	rVB	752	431	0.04%	0.005%
46	7.830	1101	1106	1108	rBV2	565	926	0.09%	0.011%
47	7.854	1108	1110	1118	rVB4	721	1098	0.10%	0.012%
48	7.915	1118	1120	1122	rBV2	486	404	0.04%	0.005%
49	7.970	1123	1129	1132	rVB4	1318	2369	0.22%	0.027%
50	8.074	1144	1146	1149	rBV2	501	466	0.04%	0.005%
51	8.110	1149	1152	1154	rVV2	606	640	0.06%	0.007%
52	8.330	1181	1188	1198	rBV	144045	237972	22.19%	2.705%
53	8.586	1226	1230	1233	rBV4	915	1121	0.10%	0.013%
54	8.653	1234	1241	1252	rVV	537052	835519	77.89%	9.498%
55	8.952	1285	1290	1302	rBV	99266	155931	14.54%	1.773%
56	9.281	1341	1344	1349	rVB3	1133	1693	0.16%	0.019%
57	9.336	1349	1353	1356	rBV2	336	518	0.05%	0.006%
58	9.397	1357	1363	1376	rBV	351683	576811	53.77%	6.557%
59	9.714	1409	1415	1420	rBV4	2236	3594	0.34%	0.041%
60	9.909	1446	1447	1451	rBV	297	383	0.04%	0.004%
61	10.055	1465	1471	1486	rVB	650557	863615	80.51%	9.817%
62	10.159	1486	1488	1489	rVV2	597	455	0.04%	0.005%
63	10.195	1490	1494	1499	rVV3	1100	2319	0.22%	0.026%
64	10.256	1502	1504	1508	rVV2	553	595	0.06%	0.007%
65	10.305	1508	1512	1515	rVB2	1512	1662	0.15%	0.019%
66	10.646	1567	1568	1572	rVB3	802	794	0.07%	0.009%
67	10.713	1577	1579	1581	rVB3	435	451	0.04%	0.005%
68	10.823	1595	1597	1599	rBV	346	356	0.03%	0.004%
69	11.104	1642	1643	1646	rVV2	537	411	0.04%	0.005%
70	11.195	1653	1658	1667	rBV	355862	456310	42.54%	5.187%
71	11.354	1680	1684	1686	rVB2	691	767	0.07%	0.009%
72	11.451	1696	1700	1703	rBV2	522	880	0.08%	0.010%
73	11.488	1703	1706	1707	rVV2	891	767	0.07%	0.009%
74	11.634	1728	1730	1734	rVB4	653	731	0.07%	0.008%
75	12.024	1788	1794	1802	rBV	613959	753812	70.27%	8.569%
76	12.152	1813	1815	1817	rVB2	390	358	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030469.D
 Acq On : 06 Aug 2022 17:06
 Operator : JC/MD
 Sample : N4021-11DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D67DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.225	1825	1827	1830	rVB2	483	424	0.04%	0.005%
78	12.323	1837	1843	1851	rBV	548664	673844	62.82%	7.660%
79	12.439	1859	1862	1863	rBV2	388	338	0.03%	0.004%
80	12.701	1903	1905	1910	rBV2	377	677	0.06%	0.008%
81	13.030	1956	1959	1960	rBV	530	546	0.05%	0.006%
82	13.152	1977	1979	1982	rBV2	387	410	0.04%	0.005%
83	13.481	2032	2033	2036	rBV2	380	366	0.03%	0.004%
84	13.621	2055	2056	2058	rVB2	560	349	0.03%	0.004%
85	13.640	2058	2059	2061	rBV	542	359	0.03%	0.004%
86	13.670	2061	2064	2065	rVB2	612	467	0.04%	0.005%
87	13.780	2078	2082	2083	rBV2	733	940	0.09%	0.011%
88	13.810	2085	2087	2091	rBV2	546	632	0.06%	0.007%
89	14.079	2130	2131	2133	rBV	427	351	0.03%	0.004%
90	14.152	2141	2143	2145	rBV2	647	369	0.03%	0.004%
91	14.249	2156	2159	2163	rBV2	456	667	0.06%	0.008%
92	14.566	2208	2211	2213	rBV2	451	552	0.05%	0.006%
93	14.627	2219	2221	2223	rBV2	493	369	0.03%	0.004%
94	14.762	2242	2243	2245	rBV	492	497	0.05%	0.006%
95	14.993	2280	2281	2283	rBV2	461	355	0.03%	0.004%
96	15.176	2308	2311	2312	rBV2	473	458	0.04%	0.005%
97	15.261	2322	2325	2326	rBV2	770	748	0.07%	0.009%
98	15.359	2339	2341	2342	rBV	586	482	0.04%	0.005%
99	15.603	2379	2381	2386	rBV	540	682	0.06%	0.008%
100	16.609	2544	2546	2548	rBV2	763	725	0.07%	0.008%


Sum of corrected areas: 8797228

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030469.D
Acq On : 06 Aug 2022 17:06
Operator : JC/MD
Sample : N4021-11DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D67DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

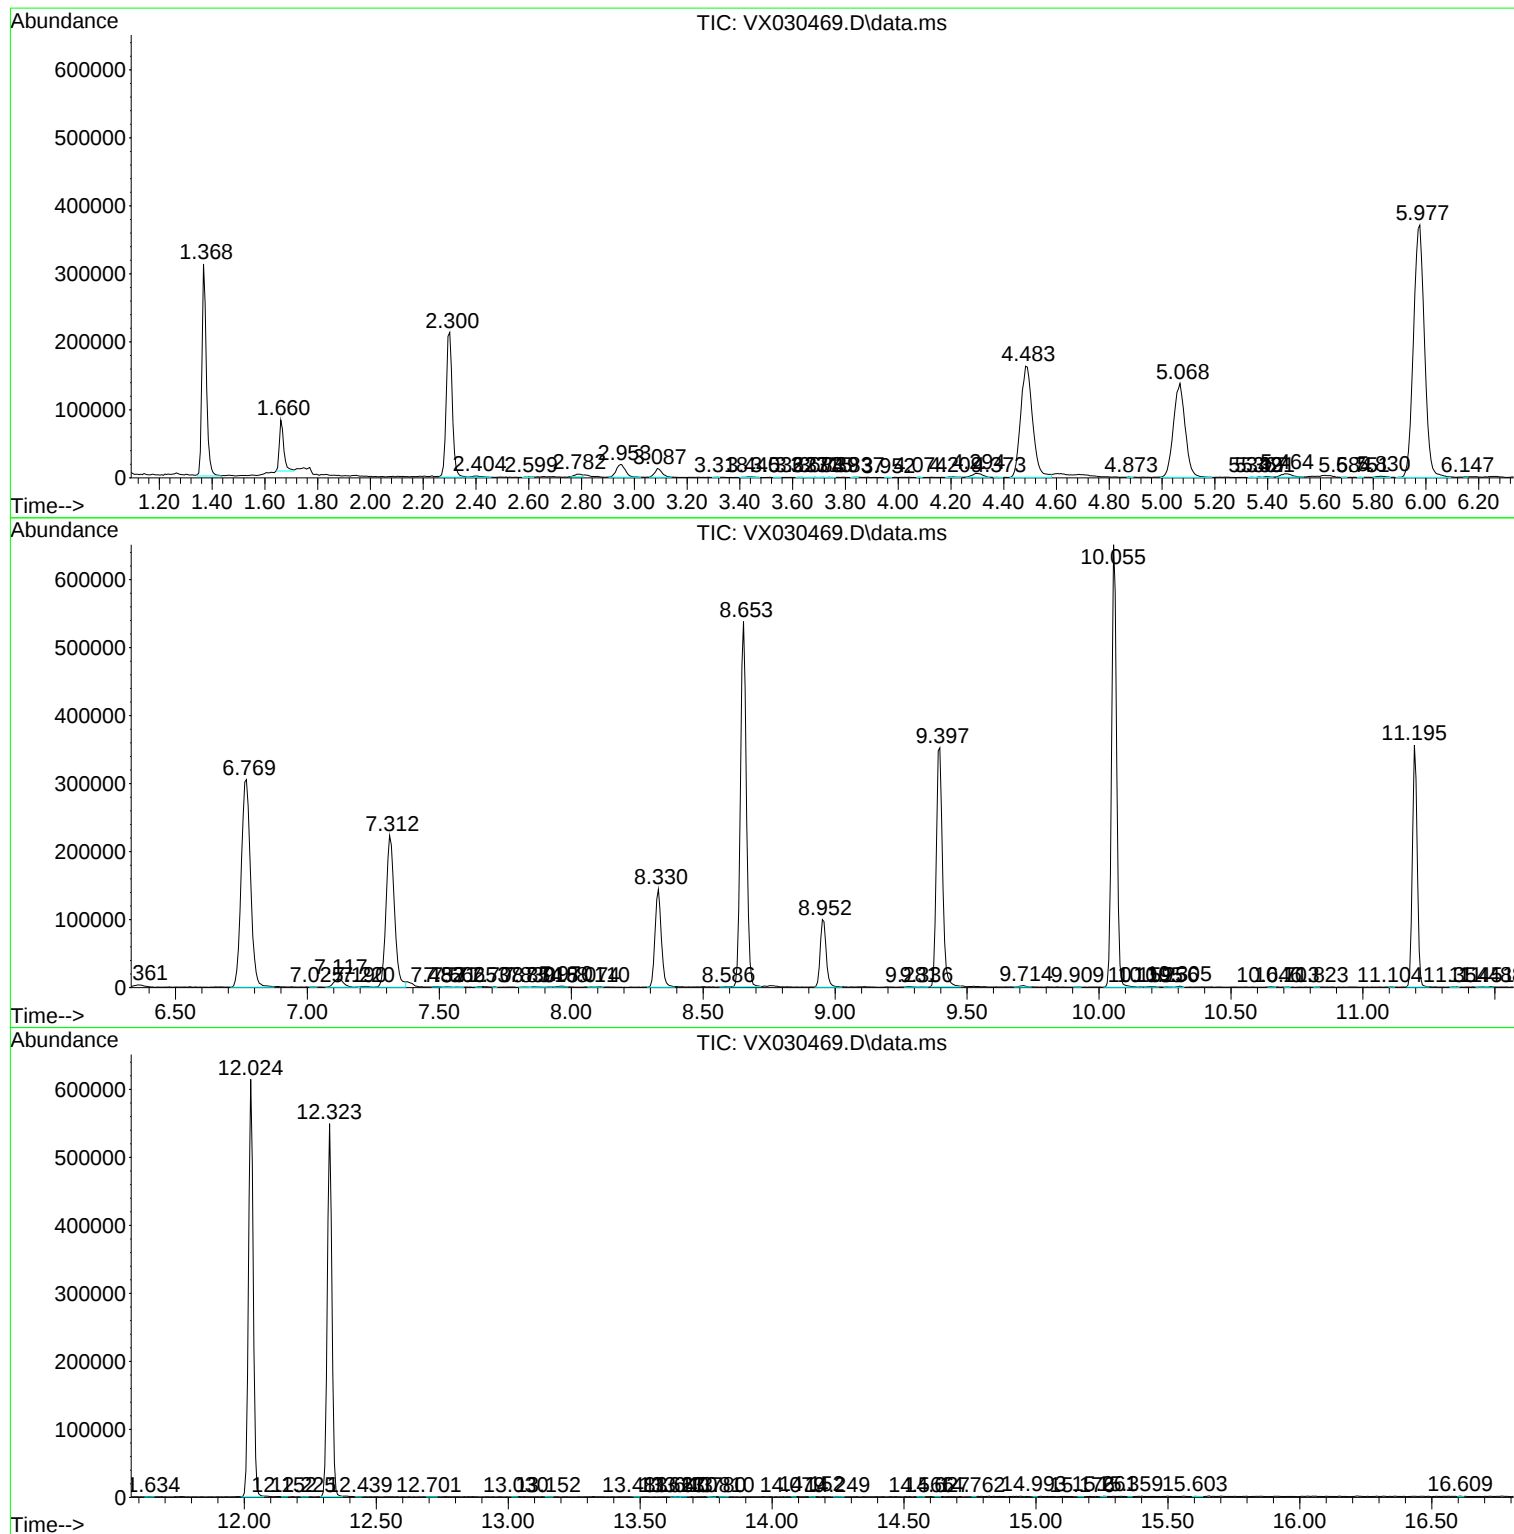

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030469.D
Acq On : 06 Aug 2022 17:06
Operator : JC/MD
Sample : N4021-11DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D67DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030469.D
Acq On : 06 Aug 2022 17:06
Operator : JC/MD
Sample : N4021-11DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D67DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc