

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030471.D
 Acq On : 06 Aug 2022 17:53
 Operator : JC/MD
 Sample : N4021-16DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E22DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030471.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB2	152668	168504	15.86%	1.712%
2	1.660	91	94	101	rBV	75171	91986	8.66%	0.934%
3	2.300	193	199	210	rVB	220947	344194	32.39%	3.496%
4	2.392	212	214	215	rBV3	856	578	0.05%	0.006%
5	2.733	268	270	273	rVB3	416	353	0.03%	0.004%
6	2.788	274	279	284	rVB4	3451	6551	0.62%	0.067%
7	2.947	296	305	316	rBV	16281	37438	3.52%	0.380%
8	3.093	324	329	337	rVB2	5896	11472	1.08%	0.117%
9	3.178	341	343	347	rVB2	391	458	0.04%	0.005%
10	3.239	351	353	355	rVV	378	407	0.04%	0.004%
11	3.410	379	381	383	rBV2	314	337	0.03%	0.003%
12	3.434	383	385	386	rBV	583	440	0.04%	0.004%
13	3.581	407	409	411	rBV	429	468	0.04%	0.005%
14	3.611	411	414	415	rVB	371	347	0.03%	0.004%
15	3.666	421	423	425	rBV2	409	330	0.03%	0.003%
16	3.763	435	439	440	rBV2	382	386	0.04%	0.004%
17	3.843	449	452	454	rBV2	582	620	0.06%	0.006%
18	4.032	482	483	487	rVB2	329	328	0.03%	0.003%
19	4.074	487	490	491	rBV	313	342	0.03%	0.003%
20	4.184	507	508	512	rVB	333	322	0.03%	0.003%
21	4.489	547	558	571	rBV2	248979	739281	69.56%	7.510%
22	4.818	611	612	616	rVB2	847	642	0.06%	0.007%
23	4.855	616	618	621	rBV2	362	327	0.03%	0.003%
24	4.928	628	630	634	rVB3	511	532	0.05%	0.005%
25	5.062	640	652	669	rBV	135104	433010	40.74%	4.399%
26	5.245	680	682	685	rBV2	546	553	0.05%	0.006%
27	5.312	690	693	695	rBV2	411	443	0.04%	0.005%
28	5.336	695	697	700	rBV2	326	442	0.04%	0.004%
29	5.659	747	750	752	rBV2	713	901	0.08%	0.009%
30	5.678	752	753	755	rVV	635	457	0.04%	0.005%
31	5.720	757	760	762	rBV2	358	553	0.05%	0.006%
32	5.775	767	769	771	rBV2	473	435	0.04%	0.004%
33	5.855	781	782	785	rVB	470	330	0.03%	0.003%
34	5.976	788	802	818	rBV2	369968	1062758	100.00%	10.796%
35	6.281	849	852	853	rBV2	387	388	0.04%	0.004%
36	6.361	858	865	874	rVB6	2113	5686	0.54%	0.058%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030471.D
 Acq On : 06 Aug 2022 17:53
 Operator : JC/MD
 Sample : N4021-16DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E22DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.629	905	909	910	rBV	354	308	0.03%	0.003%
38	6.690	918	919	921	rBV	316	318	0.03%	0.003%
39	6.769	921	932	947	rVV	310469	749036	70.48%	7.609%
40	7.129	982	991	1001	rBV2	180859	399917	37.63%	4.062%
41	7.312	1013	1021	1036	rBV	223481	484767	45.61%	4.924%
42	7.482	1047	1049	1054	rVB4	775	1289	0.12%	0.013%
43	7.629	1071	1073	1076	rBV2	437	429	0.04%	0.004%
44	7.732	1087	1090	1092	rBV2	235	308	0.03%	0.003%
45	7.781	1095	1098	1099	rVV2	770	668	0.06%	0.007%
46	7.842	1103	1108	1109	rVV2	495	622	0.06%	0.006%
47	7.952	1122	1126	1131	rBB6	1006	1911	0.18%	0.019%
48	8.074	1145	1146	1148	rBV2	511	432	0.04%	0.004%
49	8.257	1174	1176	1180	rVB3	391	468	0.04%	0.005%
50	8.330	1182	1188	1205	rVV	140710	234393	22.06%	2.381%
51	8.653	1235	1241	1250	rBV	551178	852006	80.17%	8.655%
52	8.952	1285	1290	1304	rVB	98161	150758	14.19%	1.531%
53	9.049	1304	1306	1308	rBV3	635	672	0.06%	0.007%
54	9.165	1323	1325	1326	rBV	566	432	0.04%	0.004%
55	9.275	1336	1343	1354	rBV	451832	657181	61.84%	6.676%
56	9.397	1357	1363	1378	rBV	358944	574661	54.07%	5.837%
57	9.622	1398	1400	1402	rBV3	492	326	0.03%	0.003%
58	9.750	1420	1421	1426	rVB2	402	419	0.04%	0.004%
59	9.793	1426	1428	1430	rBV3	421	413	0.04%	0.004%
60	9.945	1452	1453	1455	rBV2	536	313	0.03%	0.003%
61	10.055	1466	1471	1481	rBV	626899	873530	82.19%	8.873%
62	10.189	1492	1493	1496	rBV	787	813	0.08%	0.008%
63	10.305	1509	1512	1515	rBV4	875	1110	0.10%	0.011%
64	10.488	1540	1542	1548	rBV2	521	949	0.09%	0.010%
65	10.659	1565	1570	1576	rVV3	746	1635	0.15%	0.017%
66	10.750	1582	1585	1586	rBV	559	575	0.05%	0.006%
67	10.957	1614	1619	1622	rVB3	522	878	0.08%	0.009%
68	11.091	1639	1641	1643	rVB2	403	338	0.03%	0.003%
69	11.122	1644	1646	1650	rVB	645	625	0.06%	0.006%
70	11.195	1653	1658	1665	rBV	377710	466142	43.86%	4.735%
71	11.335	1679	1681	1683	rBV2	380	345	0.03%	0.004%
72	11.482	1703	1705	1710	rVB3	826	949	0.09%	0.010%
73	11.640	1728	1731	1736	rVB2	361	462	0.04%	0.005%
74	11.683	1736	1738	1741	rBV3	593	572	0.05%	0.006%
75	11.756	1748	1750	1751	rVV2	500	310	0.03%	0.003%
76	11.792	1755	1756	1758	rVB2	572	396	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030471.D
 Acq On : 06 Aug 2022 17:53
 Operator : JC/MD
 Sample : N4021-16DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E22DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.817	1758	1760	1761	rBV	488	313	0.03%	0.003%
78	11.902	1771	1774	1777	rBV2	251	331	0.03%	0.003%
79	11.951	1780	1782	1783	rBV2	495	334	0.03%	0.003%
80	12.024	1789	1794	1804	rBV	639002	770345	72.49%	7.825%
81	12.183	1818	1820	1823	rVB2	781	675	0.06%	0.007%
82	12.323	1838	1843	1851	rBV	558211	688025	64.74%	6.989%
83	12.597	1885	1888	1889	rBV2	373	366	0.03%	0.004%
84	12.878	1932	1934	1935	rBV2	487	387	0.04%	0.004%
85	12.987	1951	1952	1955	rBV	700	407	0.04%	0.004%
86	13.054	1959	1963	1967	rBV2	601	1132	0.11%	0.011%
87	13.109	1969	1972	1975	rBV3	378	554	0.05%	0.006%
88	13.201	1984	1987	1988	rBV	366	308	0.03%	0.003%
89	13.317	2003	2006	2008	rBV	568	586	0.06%	0.006%
90	13.780	2080	2082	2084	rBV	820	864	0.08%	0.009%
91	13.969	2111	2113	2114	rBV2	655	457	0.04%	0.005%
92	14.170	2144	2146	2147	rVB2	496	326	0.03%	0.003%
93	14.591	2213	2215	2216	rBV	676	443	0.04%	0.005%
94	14.865	2258	2260	2261	rVB	771	339	0.03%	0.003%
95	14.920	2267	2269	2270	rBV	561	331	0.03%	0.003%
96	14.981	2275	2279	2281	rBV3	715	976	0.09%	0.010%
97	15.505	2363	2365	2366	rBV2	970	681	0.06%	0.007%
98	15.798	2412	2413	2417	rBV2	683	820	0.08%	0.008%
99	16.212	2479	2481	2482	rBV	567	389	0.04%	0.004%
100	16.718	2563	2564	2567	rBV3	605	702	0.07%	0.007%




Sum of corrected areas: 9844366

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030471.D
Acq On : 06 Aug 2022 17:53
Operator : JC/MD
Sample : N4021-16DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E22DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

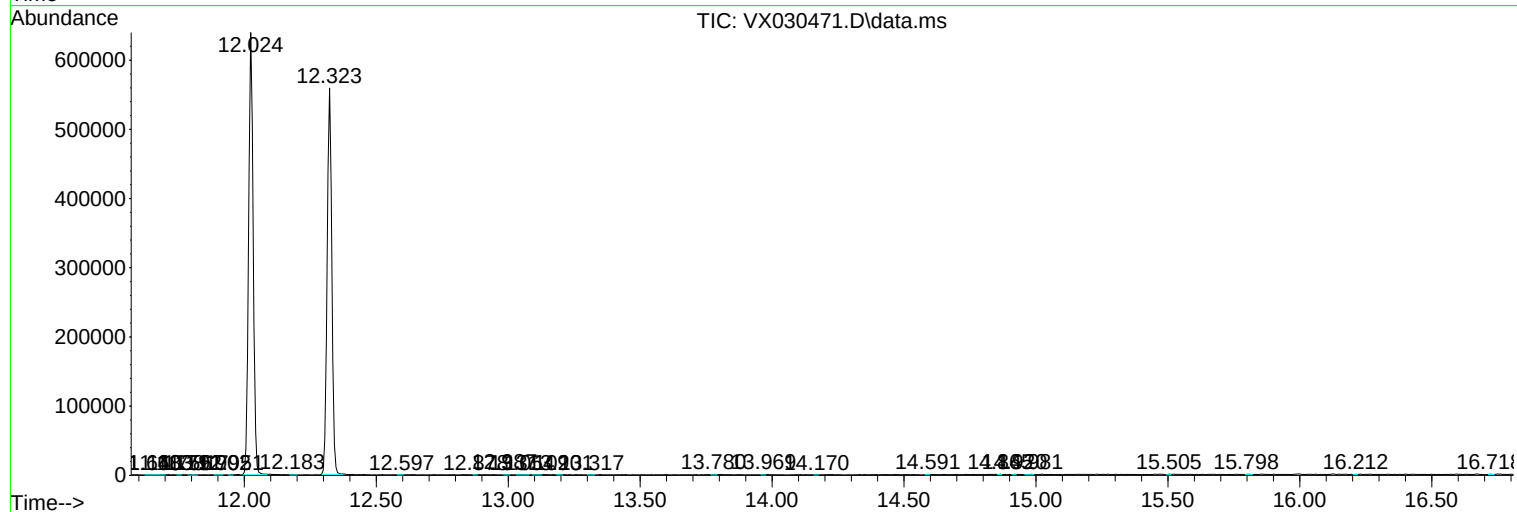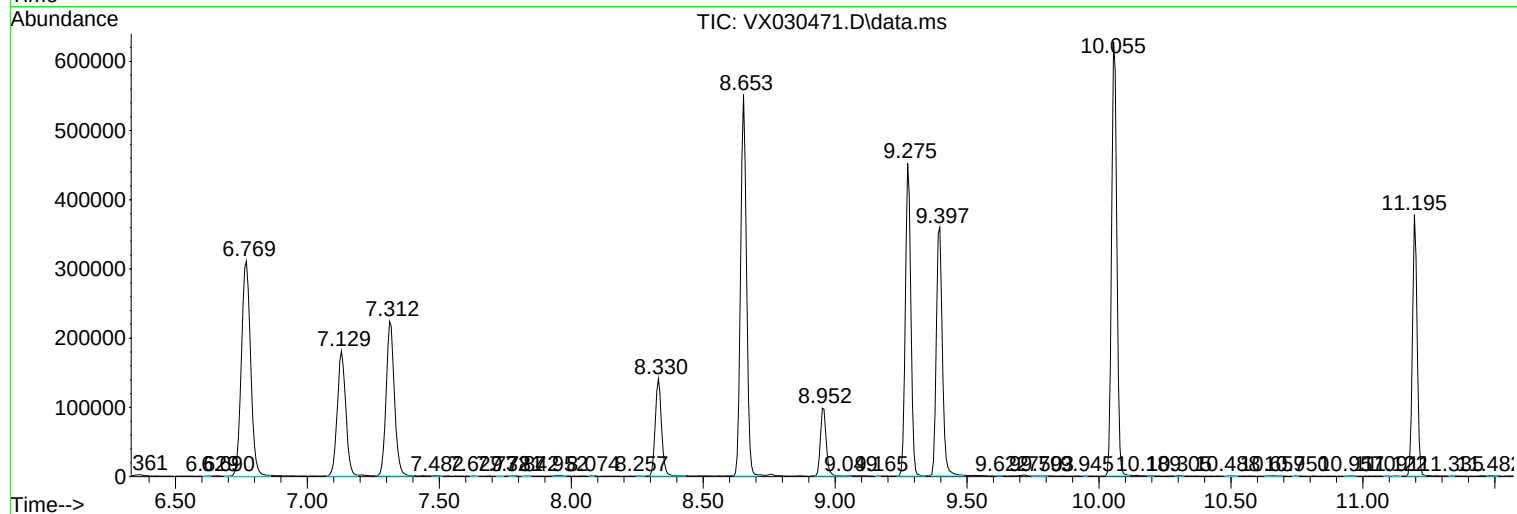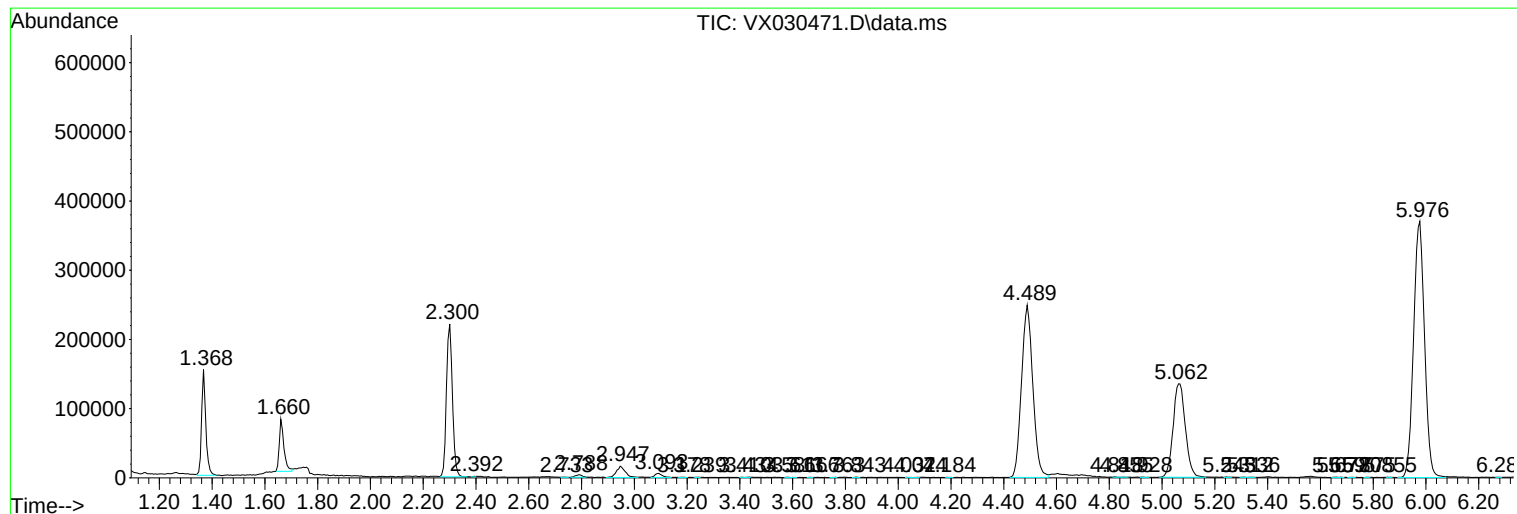

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030471.D
Acq On : 06 Aug 2022 17:53
Operator : JC/MD
Sample : N4021-16DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E22DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030471.D
Acq On : 06 Aug 2022 17:53
Operator : JC/MD
Sample : N4021-16DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E22DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc