

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030472.D
 Acq On : 06 Aug 2022 18:16
 Operator : JC/MD
 Sample : N4021-15DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E21DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030472.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB2	145010	164692	15.45%	1.752%
2	1.660	91	94	99	rBV	76412	91342	8.57%	0.972%
3	2.300	193	199	209	rVB	202654	326592	30.64%	3.474%
4	2.544	238	239	241	rBV2	426	340	0.03%	0.004%
5	2.788	273	279	286	rVB3	5278	10029	0.94%	0.107%
6	2.892	293	296	297	rVB	720	557	0.05%	0.006%
7	2.947	297	305	319	rBV	18499	46313	4.35%	0.493%
8	3.093	322	329	337	rVB6	4266	9652	0.91%	0.103%
9	3.215	346	349	350	rBV	496	555	0.05%	0.006%
10	3.233	350	352	354	rVB	467	436	0.04%	0.005%
11	3.312	363	365	366	rVV2	561	449	0.04%	0.005%
12	3.331	366	368	371	rVV3	411	434	0.04%	0.005%
13	3.392	376	378	381	rVB	394	323	0.03%	0.003%
14	3.520	397	399	402	rVB	563	471	0.04%	0.005%
15	3.568	405	407	410	rVV	465	424	0.04%	0.005%
16	3.605	410	413	415	rVV	488	388	0.04%	0.004%
17	3.745	432	436	439	rVB	369	544	0.05%	0.006%
18	3.776	439	441	446	rBV2	296	508	0.05%	0.005%
19	3.879	456	458	459	rVV	649	389	0.04%	0.004%
20	3.910	461	463	465	rVV2	629	469	0.04%	0.005%
21	4.123	495	498	499	rBV2	411	475	0.04%	0.005%
22	4.239	514	517	521	rBV2	431	530	0.05%	0.006%
23	4.276	521	523	526	rVB	547	431	0.04%	0.005%
24	4.361	533	537	538	rBV2	436	446	0.04%	0.005%
25	4.483	545	557	571	rBV2	173430	551781	51.77%	5.869%
26	4.824	612	613	617	rVB2	1003	810	0.08%	0.009%
27	4.995	638	641	642	rBV3	525	568	0.05%	0.006%
28	5.062	642	652	667	rVV	134248	431919	40.52%	4.594%
29	5.324	694	695	697	rBV	476	430	0.04%	0.005%
30	5.385	703	705	707	rBV2	1177	1192	0.11%	0.013%
31	5.550	727	732	735	rBV3	1498	2897	0.27%	0.031%
32	5.733	761	762	763	rBV	662	354	0.03%	0.004%
33	5.812	774	775	778	rBV	408	419	0.04%	0.004%
34	5.977	788	802	819	rBV2	366534	1065844	100.00%	11.338%
35	6.208	836	840	844	rBV2	574	1028	0.10%	0.011%
36	6.348	858	863	864	rBV2	2213	2395	0.22%	0.025%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030472.D
 Acq On : 06 Aug 2022 18:16
 Operator : JC/MD
 Sample : N4021-15DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E21DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.884	1770	1771	1776	rVB2	450	449	0.04%	0.005%
78	12.024	1789	1794	1804	rBV	614331	736749	69.12%	7.837%
79	12.323	1838	1843	1850	rBV	523311	659626	61.89%	7.017%
80	12.561	1880	1882	1884	rBV2	494	378	0.04%	0.004%
81	12.786	1918	1919	1921	rBV	576	336	0.03%	0.004%
82	13.109	1970	1972	1973	rBV	426	334	0.03%	0.004%
83	13.207	1987	1988	1990	rBV	429	375	0.04%	0.004%
84	13.262	1995	1997	1998	rVV	499	395	0.04%	0.004%
85	13.298	2001	2003	2005	rBV2	415	376	0.04%	0.004%
86	13.353	2010	2012	2014	rBV2	519	465	0.04%	0.005%
87	13.524	2038	2040	2044	rBV2	474	555	0.05%	0.006%
88	13.646	2058	2060	2063	rBV2	524	534	0.05%	0.006%
89	13.749	2076	2077	2081	rBV2	522	574	0.05%	0.006%
90	13.786	2081	2083	2086	rVB3	583	558	0.05%	0.006%
91	13.817	2086	2088	2090	rBV	363	386	0.04%	0.004%
92	14.170	2144	2146	2147	rBV	555	430	0.04%	0.005%
93	14.457	2190	2193	2194	rBV2	671	510	0.05%	0.005%
94	14.871	2259	2261	2262	rBV	582	449	0.04%	0.005%
95	14.926	2269	2270	2272	rBV2	638	501	0.05%	0.005%
96	15.176	2309	2311	2313	rBV3	705	650	0.06%	0.007%
97	16.103	2461	2463	2465	rBV2	913	530	0.05%	0.006%
98	16.145	2469	2470	2472	rBV	686	363	0.03%	0.004%
99	16.261	2487	2489	2492	rBV2	664	807	0.08%	0.009%
100	16.377	2506	2508	2509	rBV	972	499	0.05%	0.005%




Sum of corrected areas: 9400889

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030472.D
Acq On : 06 Aug 2022 18:16
Operator : JC/MD
Sample : N4021-15DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E21DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

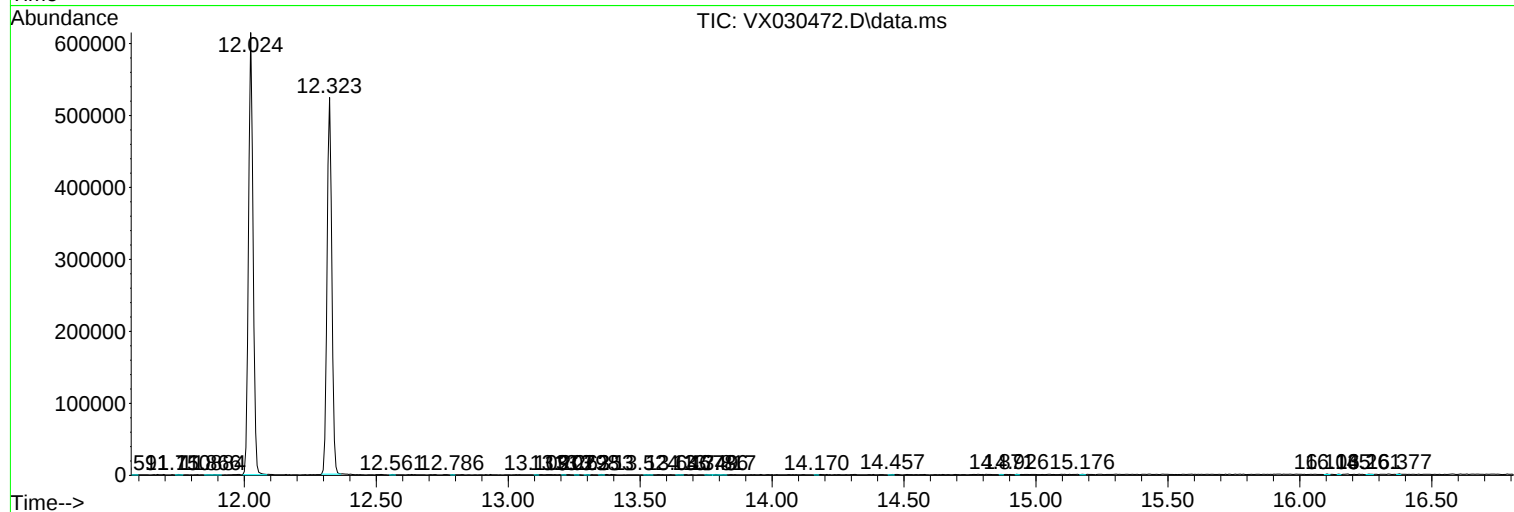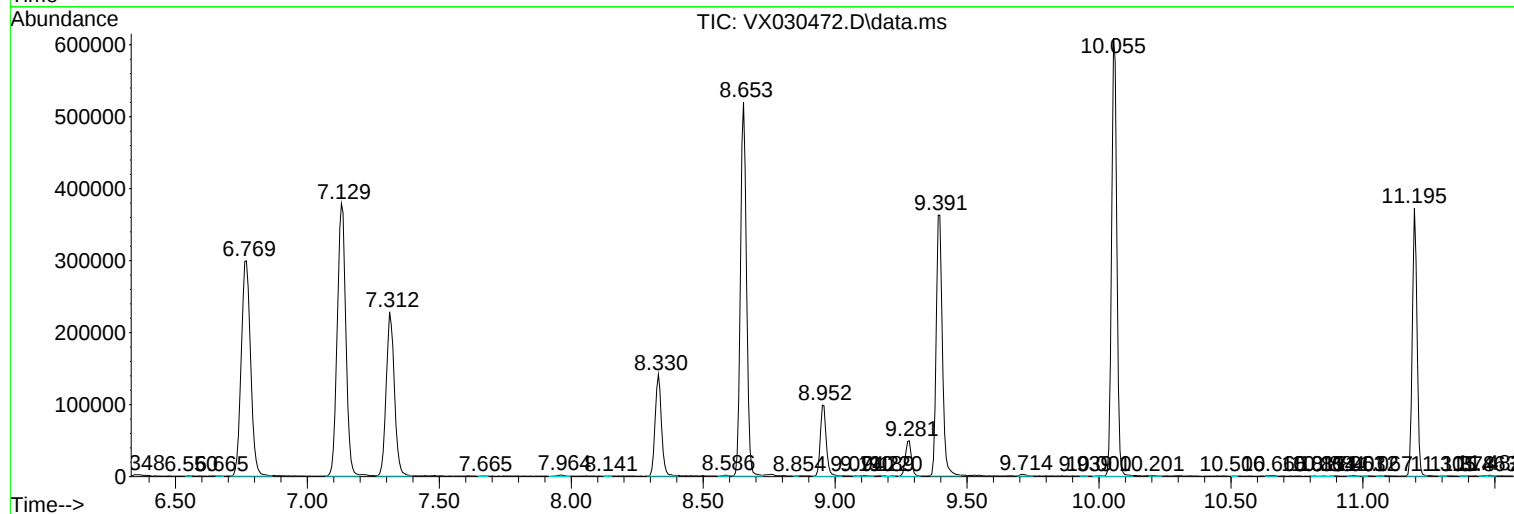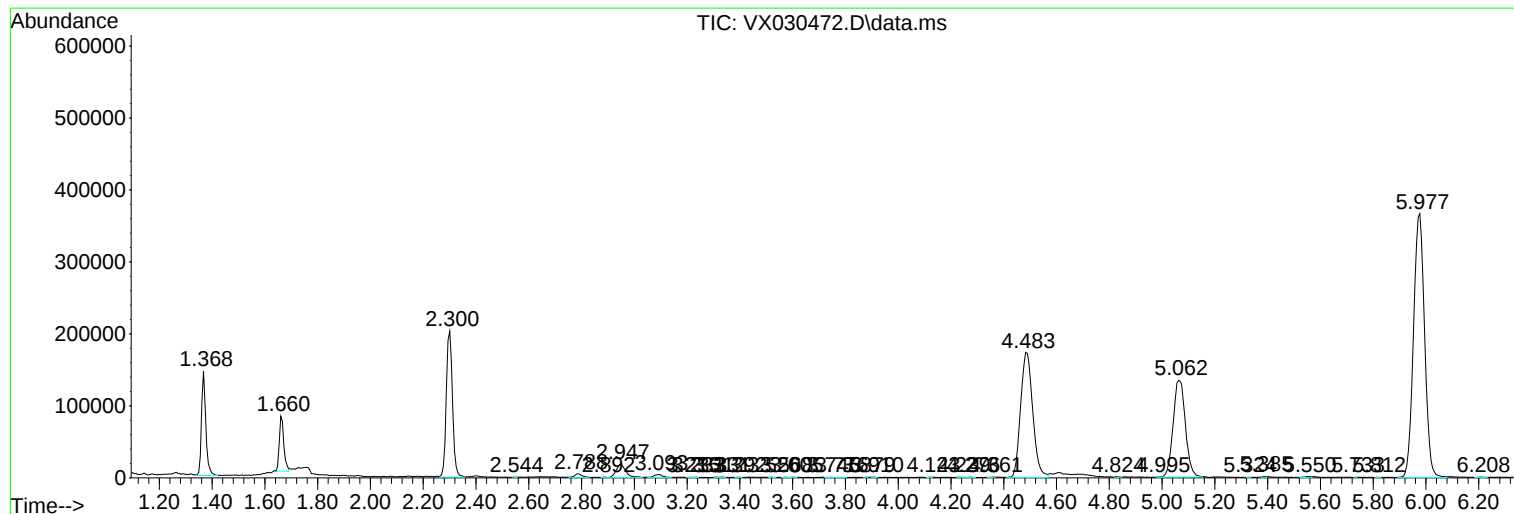

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030472.D
Acq On : 06 Aug 2022 18:16
Operator : JC/MD
Sample : N4021-15DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E21DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030472.D
Acq On : 06 Aug 2022 18:16
Operator : JC/MD
Sample : N4021-15DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E21DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc