

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030474.D
 Acq On : 06 Aug 2022 19:03
 Operator : JC/MD
 Sample : N4066-02DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D93DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030474.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	60	rVB2	208271	253047	23.37%	2.764%
2	1.660	91	94	104	rBV	78594	94957	8.77%	1.037%
3	2.300	193	199	208	rVB	217321	335392	30.98%	3.664%
4	2.788	270	279	289	rBV5	5838	14110	1.30%	0.154%
5	2.953	297	306	312	rBV2	11100	27216	2.51%	0.297%
6	3.093	322	329	333	rBV3	13834	30137	2.78%	0.329%
7	3.203	345	347	350	rVB3	322	311	0.03%	0.003%
8	3.373	373	375	378	rBV2	390	403	0.04%	0.004%
9	3.404	378	380	382	rVV2	408	321	0.03%	0.004%
10	3.660	419	422	423	rBV2	545	518	0.05%	0.006%
11	3.800	441	445	446	rBV2	482	561	0.05%	0.006%
12	4.099	491	494	496	rVB2	340	354	0.03%	0.004%
13	4.294	522	526	535	rVB6	1895	4689	0.43%	0.051%
14	4.361	535	537	538	rBV2	437	370	0.03%	0.004%
15	4.489	546	558	571	rBV2	261301	793980	73.33%	8.673%
16	4.989	638	640	641	rBV	421	370	0.03%	0.004%
17	5.062	641	652	669	rVV	145109	434733	40.15%	4.749%
18	5.184	669	672	676	rVB3	517	769	0.07%	0.008%
19	5.397	701	707	711	rBV5	1199	2586	0.24%	0.028%
20	5.556	727	733	739	rBV2	1478	3081	0.28%	0.034%
21	5.605	739	741	744	rVB2	578	466	0.04%	0.005%
22	5.855	779	782	784	rBV2	645	601	0.06%	0.007%
23	5.879	784	786	788	rVB	515	429	0.04%	0.005%
24	5.970	788	801	822	rBV3	365822	1082738	100.00%	11.827%
25	6.147	828	830	834	rBV3	756	1128	0.10%	0.012%
26	6.257	847	848	854	rVB2	739	827	0.08%	0.009%
27	6.306	854	856	858	rBV2	385	431	0.04%	0.005%
28	6.361	860	865	867	rBV4	1907	3814	0.35%	0.042%
29	6.458	879	881	884	rBV	496	419	0.04%	0.005%
30	6.543	889	895	896	rBV2	649	1067	0.10%	0.012%
31	6.659	912	914	916	rBV2	586	406	0.04%	0.004%
32	6.769	921	932	948	rBV	310477	748612	69.14%	8.177%
33	7.129	982	991	1000	rBV3	71687	166155	15.35%	1.815%
34	7.312	1013	1021	1039	rVB	223363	493159	45.55%	5.387%
35	7.476	1045	1048	1049	rBV2	674	768	0.07%	0.008%
36	7.702	1082	1085	1090	rBV2	557	1027	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030474.D
 Acq On : 06 Aug 2022 19:03
 Operator : JC/MD
 Sample : N4066-02DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D93DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.964	1118	1128	1134	rVB6	1662	3973	0.37%	0.043%
38	8.019	1134	1137	1139	rBV2	514	503	0.05%	0.005%
39	8.043	1139	1141	1145	rBV	537	679	0.06%	0.007%
40	8.177	1161	1163	1164	rBV	650	331	0.03%	0.004%
41	8.196	1164	1166	1169	rVB2	358	352	0.03%	0.004%
42	8.226	1169	1171	1173	rVB	373	355	0.03%	0.004%
43	8.330	1181	1188	1202	rBV	138731	232236	21.45%	2.537%
44	8.592	1228	1231	1232	rBV3	398	355	0.03%	0.004%
45	8.653	1234	1241	1254	rVV	532370	830439	76.70%	9.071%
46	8.958	1285	1291	1301	rVV	98196	151440	13.99%	1.654%
47	9.086	1310	1312	1313	rVB	521	331	0.03%	0.004%
48	9.110	1313	1316	1317	rBV	411	392	0.04%	0.004%
49	9.275	1339	1343	1353	rVB3	13923	21836	2.02%	0.239%
50	9.391	1356	1362	1379	rBV	374133	591729	54.65%	6.464%
51	9.604	1396	1397	1402	rVB2	732	777	0.07%	0.008%
52	9.714	1410	1415	1424	rBV3	3165	6499	0.60%	0.071%
53	9.878	1439	1442	1443	rBV	437	547	0.05%	0.006%
54	9.994	1458	1461	1462	rBV2	666	806	0.07%	0.009%
55	10.055	1465	1471	1485	rVV	632655	869496	80.31%	9.498%
56	10.317	1512	1514	1518	rVB2	678	691	0.06%	0.008%
57	10.366	1518	1522	1524	rBV2	472	725	0.07%	0.008%
58	10.415	1528	1530	1531	rBV2	529	331	0.03%	0.004%
59	10.524	1546	1548	1550	rBV	427	347	0.03%	0.004%
60	10.683	1572	1574	1575	rBV	489	323	0.03%	0.004%
61	10.842	1599	1600	1602	rBV2	427	311	0.03%	0.003%
62	10.866	1602	1604	1608	rVV3	336	395	0.04%	0.004%
63	11.195	1652	1658	1667	rBV	381069	479973	44.33%	5.243%
64	11.305	1675	1676	1680	rVB3	659	549	0.05%	0.006%
65	11.341	1680	1682	1685	rVB2	439	512	0.05%	0.006%
66	11.476	1703	1704	1708	rVV	932	691	0.06%	0.008%
67	11.512	1708	1710	1713	rVB	536	432	0.04%	0.005%
68	11.604	1722	1725	1726	rBV2	347	425	0.04%	0.005%
69	11.707	1740	1742	1743	rBV2	606	417	0.04%	0.005%
70	12.024	1789	1794	1804	rBV	635136	752307	69.48%	8.218%
71	12.183	1816	1820	1824	rBV2	481	942	0.09%	0.010%
72	12.323	1837	1843	1850	rBV	563860	688794	63.62%	7.524%
73	12.457	1862	1865	1868	rBV3	464	761	0.07%	0.008%
74	12.518	1873	1875	1877	rBV	412	407	0.04%	0.004%
75	12.658	1896	1898	1900	rBV2	544	476	0.04%	0.005%
76	12.695	1900	1904	1905	rBV2	301	424	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030474.D
 Acq On : 06 Aug 2022 19:03
 Operator : JC/MD
 Sample : N4066-02DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D93DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.762	1913	1915	1917	rVV2	641	641	0.06%	0.007%
78	12.823	1921	1925	1927	rBV2	277	408	0.04%	0.004%
79	12.859	1929	1931	1935	rVV2	393	420	0.04%	0.005%
80	13.024	1957	1958	1963	rBV	439	539	0.05%	0.006%
81	13.067	1963	1965	1967	rVB2	409	314	0.03%	0.003%
82	13.115	1970	1973	1975	rBV2	485	458	0.04%	0.005%
83	13.274	1997	1999	2002	rBV2	466	453	0.04%	0.005%
84	13.469	2029	2031	2032	rVV	606	315	0.03%	0.003%
85	13.548	2041	2044	2046	rBV2	437	483	0.04%	0.005%
86	13.573	2046	2048	2050	rVB	503	429	0.04%	0.005%
87	13.591	2050	2051	2052	rBV	719	388	0.04%	0.004%
88	13.609	2052	2054	2058	rVB	590	687	0.06%	0.008%
89	13.640	2058	2059	2062	rBV	599	492	0.05%	0.005%
90	13.707	2069	2070	2072	rVV	598	317	0.03%	0.003%
91	13.762	2075	2079	2080	rVB	424	465	0.04%	0.005%
92	13.853	2091	2094	2095	rBV2	480	413	0.04%	0.005%
93	13.945	2107	2109	2111	rVB2	669	442	0.04%	0.005%
94	14.219	2152	2154	2156	rVB2	599	496	0.05%	0.005%
95	14.286	2161	2165	2167	rBV2	531	559	0.05%	0.006%
96	14.310	2167	2169	2171	rVB2	724	584	0.05%	0.006%
97	14.347	2171	2175	2176	rBV3	575	725	0.07%	0.008%
98	14.646	2221	2224	2226	rBV	567	679	0.06%	0.007%
99	14.749	2239	2241	2242	rVB	724	427	0.04%	0.005%
100	15.054	2289	2291	2293	rBV	489	347	0.03%	0.004%




Sum of corrected areas: 9154742

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030474.D
Acq On : 06 Aug 2022 19:03
Operator : JC/MD
Sample : N4066-02DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D93DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

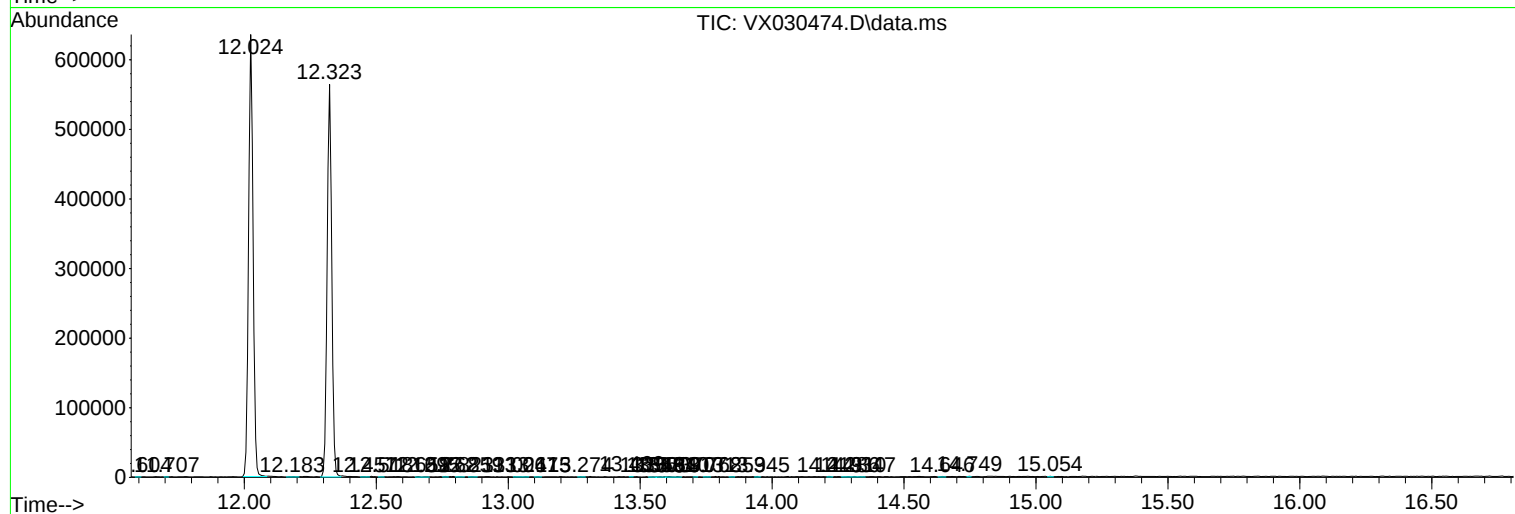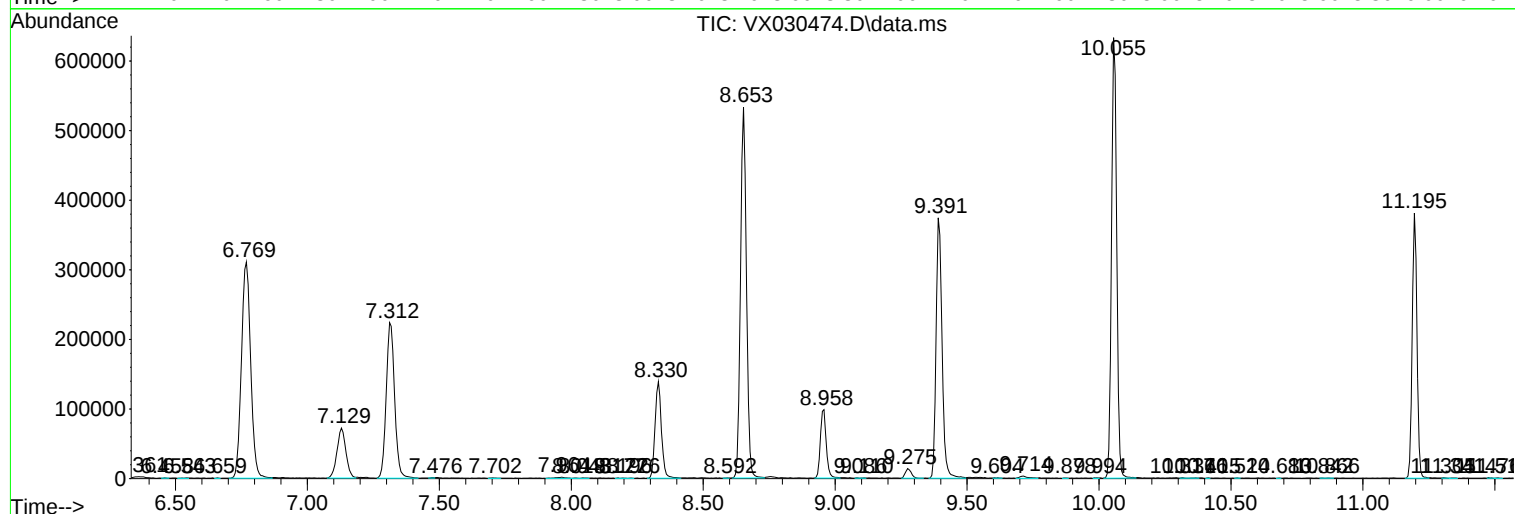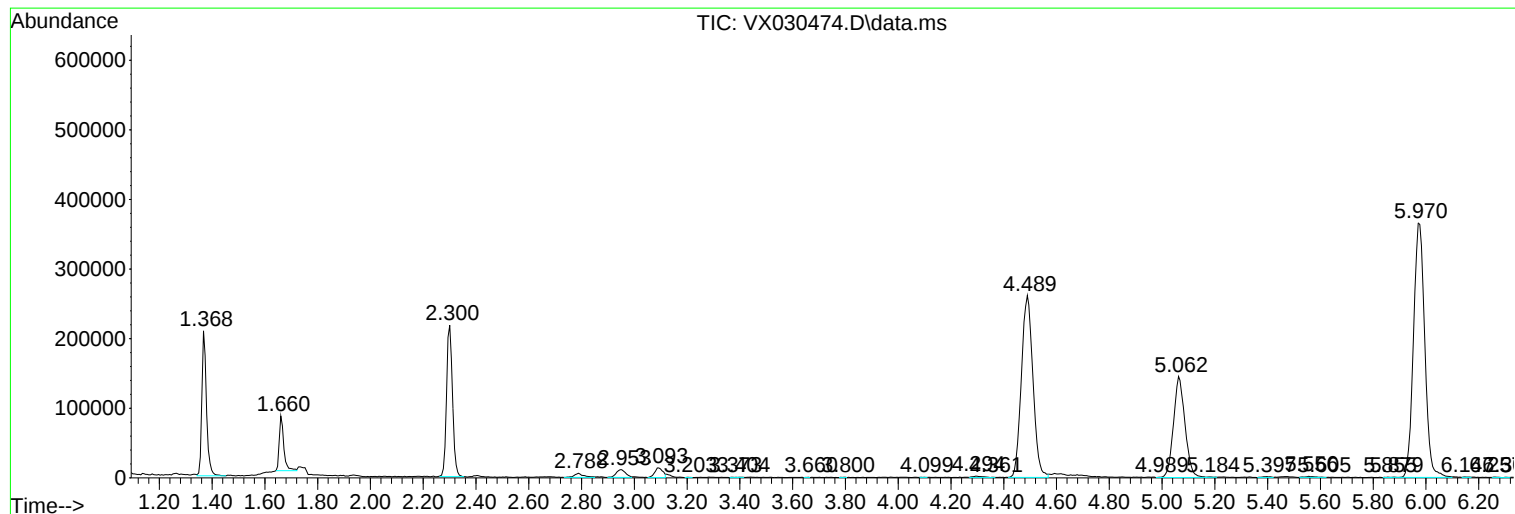

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030474.D
Acq On : 06 Aug 2022 19:03
Operator : JC/MD
Sample : N4066-02DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D93DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030474.D
Acq On : 06 Aug 2022 19:03
Operator : JC/MD
Sample : N4066-02DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D93DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc