

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030475.D
 Acq On : 06 Aug 2022 19:27
 Operator : JC/MD
 Sample : N4066-03DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D94DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030475.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	58	rVB2	216564	247516	22.82%	2.702%
2	1.660	91	94	100	rBV	75024	88538	8.16%	0.967%
3	2.300	193	199	211	rVB	217197	347579	32.05%	3.795%
4	2.648	254	256	257	rBV	575	346	0.03%	0.004%
5	2.788	273	279	288	rBV6	3616	8492	0.78%	0.093%
6	2.947	298	305	316	rBV2	14406	35047	3.23%	0.383%
7	3.038	318	320	322	rVV2	841	782	0.07%	0.009%
8	3.093	322	329	346	rVB4	14198	37662	3.47%	0.411%
9	3.288	359	361	363	rVB2	397	422	0.04%	0.005%
10	3.373	371	375	377	rBV2	449	550	0.05%	0.006%
11	3.434	384	385	387	rVV2	540	351	0.03%	0.004%
12	3.611	410	414	416	rBV2	445	624	0.06%	0.007%
13	3.642	416	419	421	rVV2	287	380	0.04%	0.004%
14	4.020	479	481	483	rVB	581	410	0.04%	0.004%
15	4.056	483	487	491	rBV2	490	858	0.08%	0.009%
16	4.111	491	496	498	rBV	455	690	0.06%	0.008%
17	4.294	521	526	534	rVB3	1830	4474	0.41%	0.049%
18	4.489	545	558	570	rBV2	264741	788027	72.66%	8.604%
19	4.812	609	611	614	rBV3	531	619	0.06%	0.007%
20	4.977	635	638	640	rVB2	399	360	0.03%	0.004%
21	5.062	640	652	667	rBV	141988	431354	39.77%	4.709%
22	5.391	701	706	708	rBV4	619	1077	0.10%	0.012%
23	5.544	730	731	733	rBV2	728	664	0.06%	0.007%
24	5.818	774	776	778	rBV	395	403	0.04%	0.004%
25	5.971	788	801	823	rBV2	371977	1084520	100.00%	11.841%
26	6.367	859	866	876	rVB3	2811	7268	0.67%	0.079%
27	6.611	904	906	907	rBV3	420	381	0.04%	0.004%
28	6.769	922	932	944	rBV	316211	751109	69.26%	8.201%
29	6.946	960	961	963	rBV	394	372	0.03%	0.004%
30	7.031	973	975	977	rVB2	645	499	0.05%	0.005%
31	7.050	977	978	980	rBV2	540	396	0.04%	0.004%
32	7.129	980	991	1001	rBV3	72165	170004	15.68%	1.856%
33	7.312	1012	1021	1040	rBV	220557	490173	45.20%	5.352%
34	7.482	1044	1049	1050	rBV2	761	817	0.08%	0.009%
35	7.623	1071	1072	1075	rVB2	563	403	0.04%	0.004%
36	7.665	1075	1079	1081	rBV2	397	481	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030475.D
 Acq On : 06 Aug 2022 19:27
 Operator : JC/MD
 Sample : N4066-03DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D94DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.702	1081	1085	1086	rBV2	408	461	0.04%	0.005%
38	7.787	1097	1099	1102	rVV3	496	485	0.04%	0.005%
39	7.842	1105	1108	1111	rBV2	446	619	0.06%	0.007%
40	7.934	1119	1123	1124	rVV3	480	538	0.05%	0.006%
41	7.952	1124	1126	1133	rVB5	1527	2321	0.21%	0.025%
42	8.074	1144	1146	1147	rVB2	806	459	0.04%	0.005%
43	8.086	1147	1148	1151	rBV2	618	508	0.05%	0.006%
44	8.165	1157	1161	1162	rBV	387	462	0.04%	0.005%
45	8.190	1163	1165	1168	rVV2	621	500	0.05%	0.005%
46	8.244	1172	1174	1177	rVB2	379	388	0.04%	0.004%
47	8.330	1182	1188	1198	rBV	135261	229718	21.18%	2.508%
48	8.586	1228	1230	1232	rBV2	623	681	0.06%	0.007%
49	8.653	1234	1241	1251	rBV	546833	835338	77.02%	9.120%
50	8.952	1285	1290	1298	rBV	97090	149938	13.83%	1.637%
51	9.116	1315	1317	1319	rBV2	746	687	0.06%	0.008%
52	9.153	1321	1323	1327	rVV2	435	422	0.04%	0.005%
53	9.275	1337	1343	1349	rBV2	12954	20169	1.86%	0.220%
54	9.391	1356	1362	1378	rBV	364734	587376	54.16%	6.413%
55	9.714	1411	1415	1423	rVB5	2954	5070	0.47%	0.055%
56	9.799	1426	1429	1430	rBV2	522	553	0.05%	0.006%
57	9.897	1442	1445	1447	rBV3	451	460	0.04%	0.005%
58	10.055	1466	1471	1481	rVV	655434	875713	80.75%	9.561%
59	10.165	1487	1489	1492	rBV3	752	772	0.07%	0.008%
60	10.317	1512	1514	1517	rBV2	451	516	0.05%	0.006%
61	10.378	1522	1524	1526	rBV	479	386	0.04%	0.004%
62	10.421	1530	1531	1534	rBV	415	466	0.04%	0.005%
63	10.488	1540	1542	1549	rVB2	534	932	0.09%	0.010%
64	10.543	1549	1551	1554	rBV2	435	398	0.04%	0.004%
65	10.677	1572	1573	1575	rVV	787	473	0.04%	0.005%
66	10.835	1596	1599	1603	rBV3	608	996	0.09%	0.011%
67	11.043	1631	1633	1635	rVV2	556	449	0.04%	0.005%
68	11.195	1653	1658	1668	rVV	364806	465534	42.93%	5.083%
69	11.482	1703	1705	1711	rVB3	793	916	0.08%	0.010%
70	11.622	1726	1728	1730	rVB2	395	348	0.03%	0.004%
71	11.762	1750	1751	1755	rBV	481	508	0.05%	0.006%
72	12.024	1789	1794	1803	rVV	643439	770572	71.05%	8.413%
73	12.323	1837	1843	1849	rBV	562969	685880	63.24%	7.488%
74	12.439	1860	1862	1864	rVB	870	701	0.06%	0.008%
75	12.463	1864	1866	1870	rBV	513	532	0.05%	0.006%
76	12.610	1887	1890	1893	rVB2	408	461	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030475.D
 Acq On : 06 Aug 2022 19:27
 Operator : JC/MD
 Sample : N4066-03DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D94DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	13.006	1952	1955	1957	rVB2	500	545	0.05%	0.006%
78	13.128	1973	1975	1978	rBV2	374	429	0.04%	0.005%
79	13.238	1989	1993	1994	rBV2	419	444	0.04%	0.005%
80	13.280	1998	2000	2002	rVV2	565	461	0.04%	0.005%
81	13.305	2002	2004	2006	rVB2	422	357	0.03%	0.004%
82	13.481	2032	2033	2035	rVB	716	474	0.04%	0.005%
83	13.506	2035	2037	2039	rBV2	391	437	0.04%	0.005%
84	13.670	2062	2064	2066	rBV2	303	373	0.03%	0.004%
85	13.865	2094	2096	2098	rBV	618	409	0.04%	0.004%
86	13.969	2111	2113	2118	rVB2	517	712	0.07%	0.008%
87	14.402	2183	2184	2187	rVB2	526	385	0.04%	0.004%
88	14.627	2220	2221	2223	rBV	498	389	0.04%	0.004%
89	14.719	2235	2236	2239	rBV2	596	609	0.06%	0.007%
90	14.792	2246	2248	2249	rBV2	593	380	0.04%	0.004%
91	14.963	2274	2276	2278	rBV2	487	411	0.04%	0.004%
92	15.225	2317	2319	2320	rBV	863	474	0.04%	0.005%
93	15.554	2369	2373	2375	rBV3	900	1191	0.11%	0.013%
94	15.755	2405	2406	2409	rBV2	509	443	0.04%	0.005%
95	15.938	2435	2436	2438	rBV2	744	374	0.03%	0.004%
96	15.957	2438	2439	2441	rVV	537	389	0.04%	0.004%
97	16.066	2455	2457	2458	rBV2	810	393	0.04%	0.004%
98	16.280	2490	2492	2493	rBV2	698	482	0.04%	0.005%
99	16.493	2525	2527	2531	rBV2	715	832	0.08%	0.009%
100	16.749	2567	2569	2572	rBV2	533	532	0.05%	0.006%


Sum of corrected areas: 9159279

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030475.D
Acq On : 06 Aug 2022 19:27
Operator : JC/MD
Sample : N4066-03DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D94DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

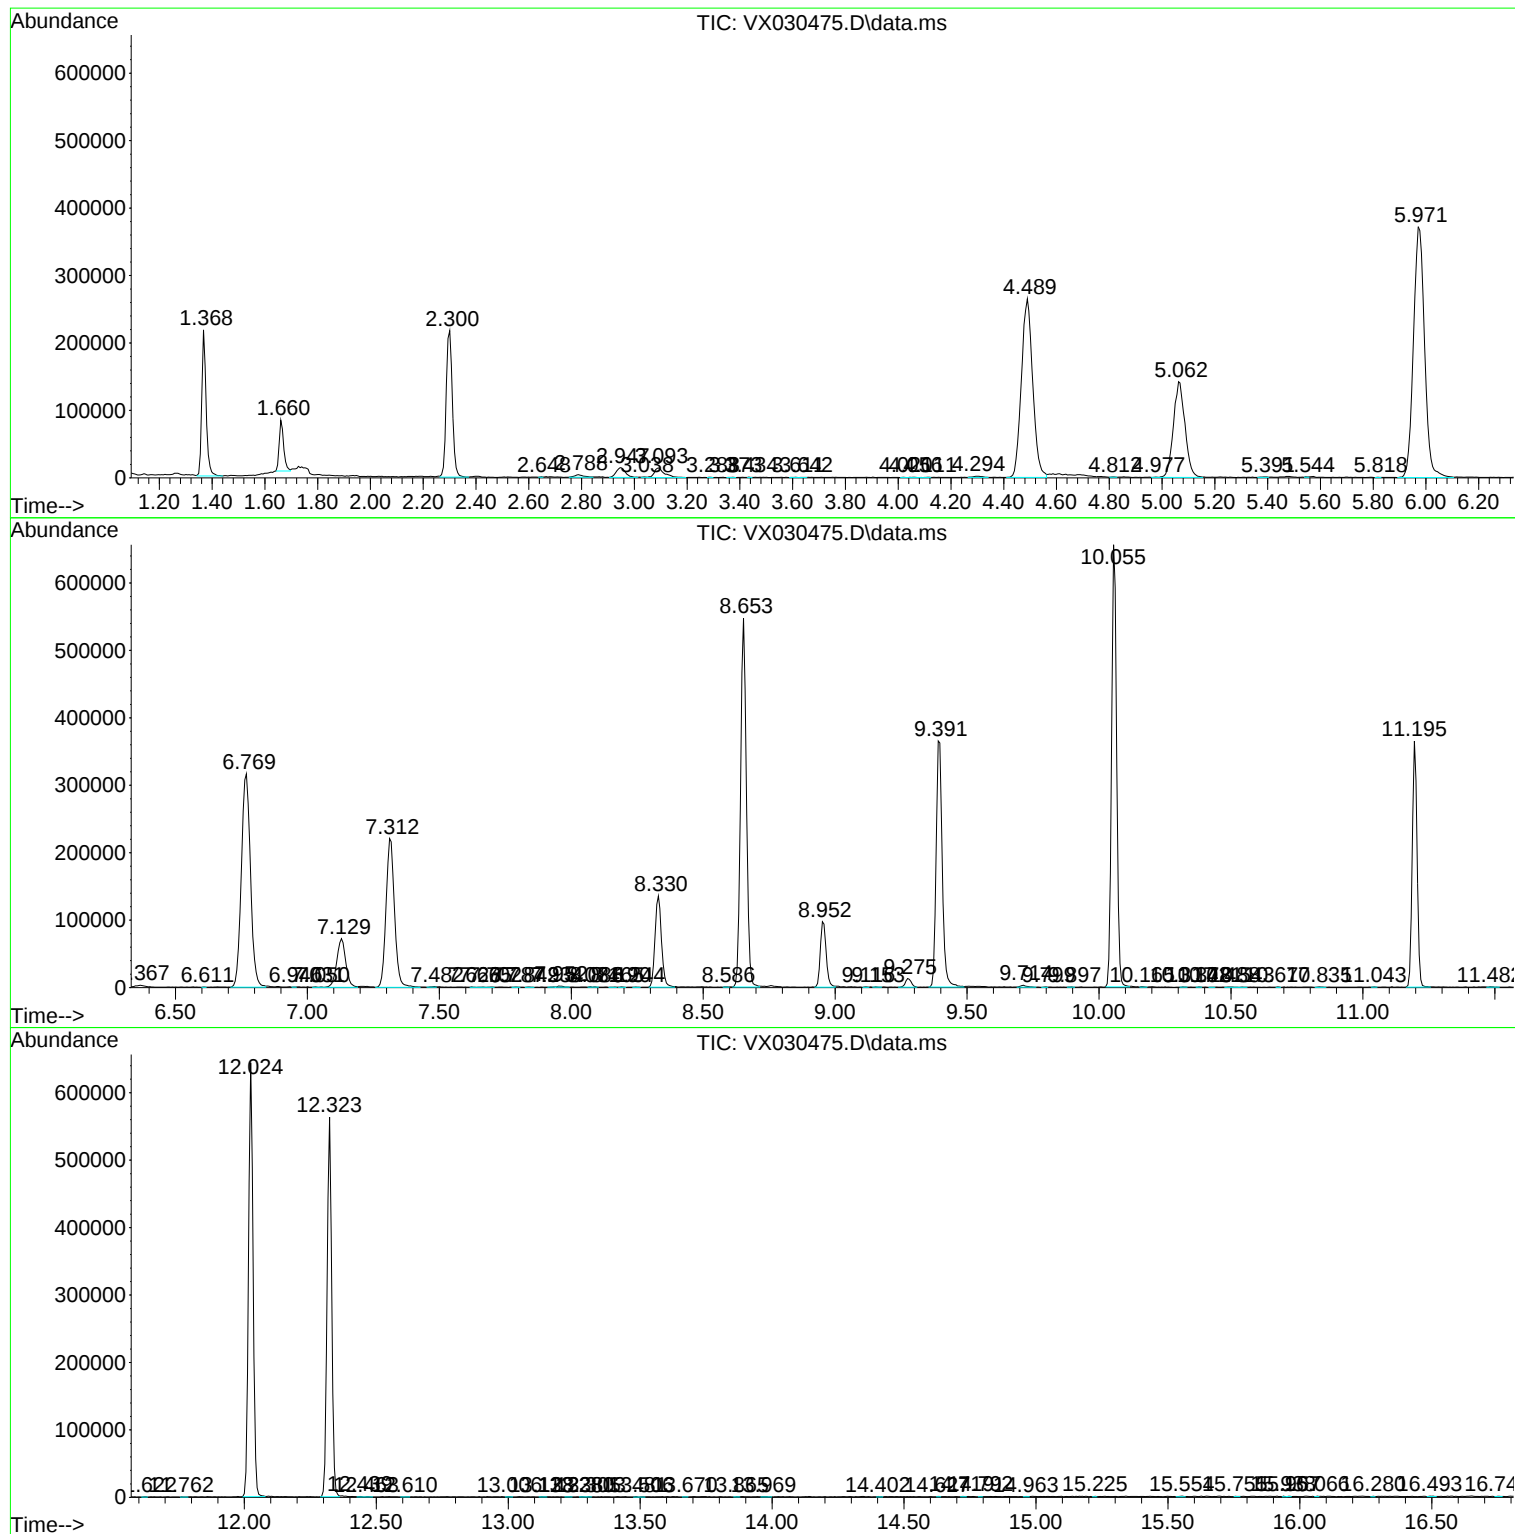

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030475.D
Acq On : 06 Aug 2022 19:27
Operator : JC/MD
Sample : N4066-03DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D94DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030475.D
Acq On : 06 Aug 2022 19:27
Operator : JC/MD
Sample : N4066-03DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D94DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc