

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030476.D
 Acq On : 06 Aug 2022 19:50
 Operator : JC/MD
 Sample : N4066-04DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E23DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030476.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	56	rVB2	156864	162319	15.65%	1.879%
2	1.666	91	95	102	rVB	106739	128665	12.40%	1.489%
3	2.306	194	200	210	rVB	208836	323396	31.18%	3.743%
4	2.520	231	235	237	rBV3	559	803	0.08%	0.009%
5	2.581	239	245	247	rBV2	1331	2245	0.22%	0.026%
6	2.794	275	280	285	rVB2	2737	4465	0.43%	0.052%
7	2.947	299	305	315	rBV	7453	16958	1.63%	0.196%
8	3.032	317	319	320	rBV2	546	359	0.03%	0.004%
9	3.099	323	330	337	rVB6	2674	6163	0.59%	0.071%
10	3.178	340	343	347	rBV2	548	1041	0.10%	0.012%
11	3.422	382	383	386	rBV	365	465	0.04%	0.005%
12	3.538	400	402	406	rVB	508	541	0.05%	0.006%
13	3.574	406	408	410	rBV	516	534	0.05%	0.006%
14	3.629	414	417	421	rVB2	616	893	0.09%	0.010%
15	3.666	421	423	426	rBV2	479	588	0.06%	0.007%
16	3.776	439	441	444	rBV2	506	500	0.05%	0.006%
17	3.898	460	461	464	rVB	502	425	0.04%	0.005%
18	3.959	468	471	472	rVV	482	391	0.04%	0.005%
19	3.989	474	476	478	rBV2	521	381	0.04%	0.004%
20	4.489	546	558	570	rBV3	186364	632765	61.00%	7.323%
21	4.806	608	610	613	rVB2	560	500	0.05%	0.006%
22	4.836	613	615	617	rBV2	551	432	0.04%	0.005%
23	4.873	620	621	624	rVB2	663	504	0.05%	0.006%
24	4.934	627	631	633	rBV3	554	741	0.07%	0.009%
25	5.068	641	653	666	rBV	133025	415036	40.01%	4.803%
26	5.233	678	680	683	rVB3	679	723	0.07%	0.008%
27	5.257	683	684	687	rVB	567	484	0.05%	0.006%
28	5.288	687	689	690	rBV	435	440	0.04%	0.005%
29	5.416	708	710	713	rVB2	733	849	0.08%	0.010%
30	5.574	729	736	745	rVB5	1273	3420	0.33%	0.040%
31	5.653	747	749	751	rBV2	589	561	0.05%	0.006%
32	5.976	790	802	820	rBV2	357030	1037354	100.00%	12.006%
33	6.214	839	841	843	rVV2	459	473	0.05%	0.005%
34	6.251	846	847	850	rVV2	614	519	0.05%	0.006%
35	6.281	850	852	855	rVB2	475	437	0.04%	0.005%
36	6.361	864	865	867	rVB2	538	375	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030476.D
 Acq On : 06 Aug 2022 19:50
 Operator : JC/MD
 Sample : N4066-04DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E23DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.452	876	880	882	rBV2	387	510	0.05%	0.006%
38	6.550	893	896	900	rVB3	723	849	0.08%	0.010%
39	6.592	900	903	906	rBV3	526	671	0.06%	0.008%
40	6.629	906	909	912	rVV	214	355	0.03%	0.004%
41	6.769	922	932	946	rBV	304859	744747	71.79%	8.619%
42	7.031	973	975	977	rVB	668	406	0.04%	0.005%
43	7.117	983	989	997	rBV6	12789	31064	2.99%	0.360%
44	7.251	1010	1011	1013	rVV	417	409	0.04%	0.005%
45	7.318	1013	1022	1045	rVB	215900	482553	46.52%	5.585%
46	7.476	1045	1048	1049	rBV2	557	594	0.06%	0.007%
47	7.568	1059	1063	1066	rVB3	359	514	0.05%	0.006%
48	7.598	1066	1068	1071	rVB2	445	427	0.04%	0.005%
49	7.629	1071	1073	1076	rBV2	390	418	0.04%	0.005%
50	7.872	1110	1113	1115	rVV3	362	400	0.04%	0.005%
51	8.019	1136	1137	1141	rVB	585	563	0.05%	0.007%
52	8.330	1182	1188	1198	rBV	141214	227402	21.92%	2.632%
53	8.580	1227	1229	1233	rBV2	742	687	0.07%	0.008%
54	8.653	1234	1241	1251	rBV	536964	815799	78.64%	9.442%
55	8.958	1285	1291	1299	rVV	94229	146717	14.14%	1.698%
56	9.098	1312	1314	1315	rVB	622	385	0.04%	0.004%
57	9.177	1323	1327	1328	rBV2	533	464	0.04%	0.005%
58	9.275	1341	1343	1347	rVB3	918	1201	0.12%	0.014%
59	9.336	1350	1353	1355	rBV2	641	545	0.05%	0.006%
60	9.390	1356	1362	1374	rBV	419682	603613	58.19%	6.986%
61	9.653	1403	1405	1406	rBV	538	439	0.04%	0.005%
62	9.708	1410	1414	1416	rVV2	3267	3875	0.37%	0.045%
63	9.836	1433	1435	1437	rBV2	455	423	0.04%	0.005%
64	9.909	1445	1447	1451	rBV	302	354	0.03%	0.004%
65	10.055	1465	1471	1480	rBV	637072	866509	83.53%	10.028%
66	10.250	1501	1503	1506	rBV4	756	1098	0.11%	0.013%
67	10.482	1539	1541	1544	rBV2	509	623	0.06%	0.007%
68	10.610	1560	1562	1564	rVB	532	402	0.04%	0.005%
69	10.634	1564	1566	1568	rBV	367	400	0.04%	0.005%
70	10.780	1586	1590	1596	rVB2	519	890	0.09%	0.010%
71	10.848	1598	1601	1603	rBV	521	483	0.05%	0.006%
72	10.872	1603	1605	1606	rVV2	551	403	0.04%	0.005%
73	10.909	1609	1611	1614	rBV2	327	380	0.04%	0.004%
74	11.140	1647	1649	1651	rVB2	673	377	0.04%	0.004%
75	11.195	1651	1658	1668	rBV	382503	481984	46.46%	5.578%
76	11.268	1668	1670	1672	rVB3	808	459	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030476.D
 Acq On : 06 Aug 2022 19:50
 Operator : JC/MD
 Sample : N4066-04DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E23DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.354	1682	1684	1687	rVB	705	468	0.05%	0.005%
78	11.640	1729	1731	1733	rBV2	407	354	0.03%	0.004%
79	11.963	1781	1784	1786	rVB2	401	423	0.04%	0.005%
80	12.024	1789	1794	1800	rBV	667256	782706	75.45%	9.059%
81	12.183	1818	1820	1823	rVB	685	427	0.04%	0.005%
82	12.225	1823	1827	1831	rBV2	436	742	0.07%	0.009%
83	12.323	1838	1843	1851	rBV	546617	679272	65.48%	7.861%
84	12.463	1862	1866	1867	rBV2	412	510	0.05%	0.006%
85	12.725	1907	1909	1913	rVB3	582	594	0.06%	0.007%
86	12.823	1923	1925	1926	rBV	579	518	0.05%	0.006%
87	13.097	1968	1970	1972	rVV	537	533	0.05%	0.006%
88	13.122	1972	1974	1978	rVV2	557	593	0.06%	0.007%
89	13.164	1978	1981	1983	rVB2	452	517	0.05%	0.006%
90	13.225	1989	1991	1993	rVB2	483	424	0.04%	0.005%
91	13.250	1993	1995	1996	rBV	549	404	0.04%	0.005%
92	13.536	2040	2042	2046	rBV3	484	457	0.04%	0.005%
93	13.676	2063	2065	2069	rBV	720	689	0.07%	0.008%
94	13.743	2073	2076	2077	rVB2	543	496	0.05%	0.006%
95	13.896	2099	2101	2103	rVB2	650	372	0.04%	0.004%
96	14.091	2131	2133	2136	rBV2	526	729	0.07%	0.008%
97	14.255	2156	2160	2163	rBV3	434	499	0.05%	0.006%
98	14.310	2166	2169	2172	rBV3	451	678	0.07%	0.008%
99	15.359	2339	2341	2342	rBV2	643	449	0.04%	0.005%
100	15.883	2426	2427	2429	rBV2	717	542	0.05%	0.006%




Sum of corrected areas: 8640533

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030476.D
Acq On : 06 Aug 2022 19:50
Operator : JC/MD
Sample : N4066-04DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E23DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

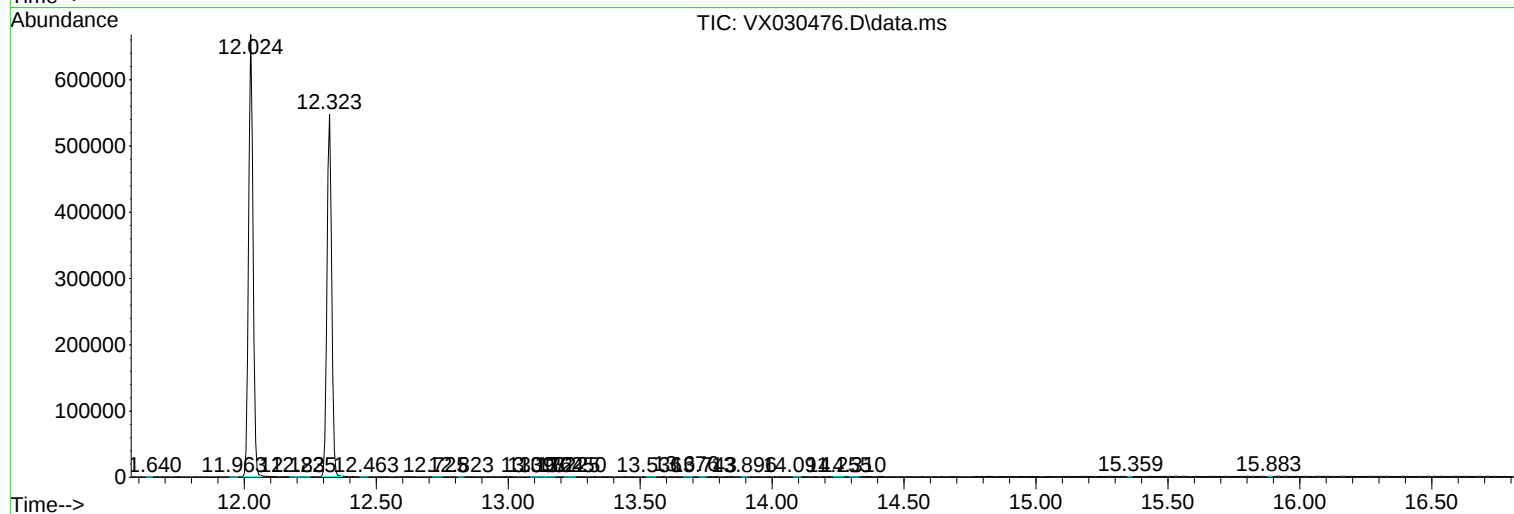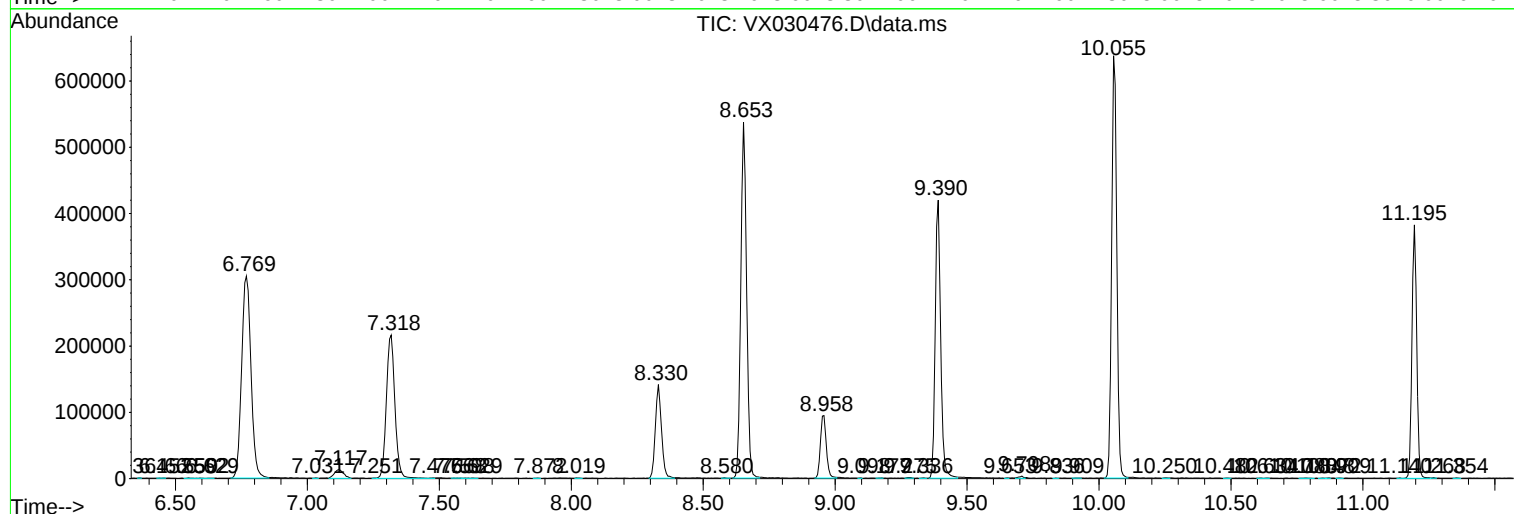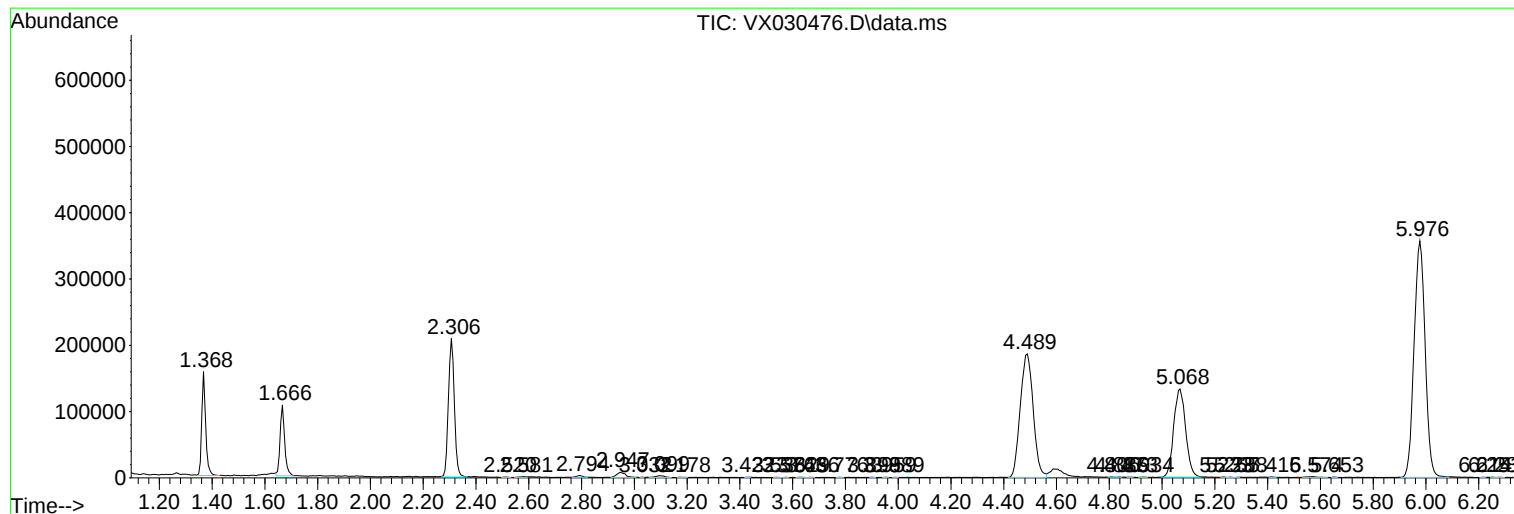

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030476.D
Acq On : 06 Aug 2022 19:50
Operator : JC/MD
Sample : N4066-04DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E23DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030476.D
Acq On : 06 Aug 2022 19:50
Operator : JC/MD
Sample : N4066-04DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E23DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc