

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030477.D
 Acq On : 06 Aug 2022 20:14
 Operator : JC/MD
 Sample : N4066-05DL 4X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E25DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030477.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB2	142540	168301	16.05%	1.793%
2	1.660	91	94	101	rBV	75064	86702	8.27%	0.924%
3	2.300	192	199	210	rVB	221098	338797	32.31%	3.609%
4	2.483	228	229	233	rBV2	523	513	0.05%	0.005%
5	2.788	274	279	288	rBV3	4168	7498	0.72%	0.080%
6	2.947	298	305	320	rBV	15467	37627	3.59%	0.401%
7	3.087	323	328	338	rVB2	10506	20088	1.92%	0.214%
8	3.196	344	346	349	rVB2	395	435	0.04%	0.005%
9	3.233	349	352	353	rVB	598	470	0.04%	0.005%
10	3.556	403	405	408	rVB2	387	360	0.03%	0.004%
11	3.593	408	411	413	rBV2	542	672	0.06%	0.007%
12	3.721	431	432	435	rVB3	405	372	0.04%	0.004%
13	3.867	452	456	458	rVB2	395	450	0.04%	0.005%
14	4.001	476	478	481	rVB	477	372	0.04%	0.004%
15	4.044	483	485	488	rBV2	433	482	0.05%	0.005%
16	4.196	506	510	513	rVB	300	423	0.04%	0.005%
17	4.294	524	526	529	rBV2	547	662	0.06%	0.007%
18	4.324	529	531	536	rBV2	791	626	0.06%	0.007%
19	4.483	545	557	573	rBV2	232925	720028	68.67%	7.671%
20	5.062	640	652	669	rVV	132354	424262	40.46%	4.520%
21	5.391	703	706	707	rBV2	580	644	0.06%	0.007%
22	5.483	718	721	723	rVV2	497	715	0.07%	0.008%
23	5.568	729	735	739	rVV3	1440	3248	0.31%	0.035%
24	5.659	748	750	752	rVV2	494	466	0.04%	0.005%
25	5.970	791	801	817	rBV2	360848	1048588	100.00%	11.171%
26	6.220	841	842	844	rBV	552	369	0.04%	0.004%
27	6.361	860	865	877	rVB4	2452	6946	0.66%	0.074%
28	6.452	877	880	881	rBV2	315	412	0.04%	0.004%
29	6.550	893	896	897	rVV	338	450	0.04%	0.005%
30	6.769	921	932	951	rBV	312753	752736	71.79%	8.020%
31	7.129	982	991	1000	rBV2	130866	285854	27.26%	3.045%
32	7.312	1011	1021	1037	rBV	222176	487812	46.52%	5.197%
33	7.476	1045	1048	1054	rVB7	836	1649	0.16%	0.018%
34	7.610	1067	1070	1072	rVV2	551	671	0.06%	0.007%
35	7.635	1072	1074	1078	rVB3	426	417	0.04%	0.004%
36	7.848	1106	1109	1111	rBV	466	599	0.06%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030477.D
 Acq On : 06 Aug 2022 20:14
 Operator : JC/MD
 Sample : N4066-05DL 4X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E25DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.909	1116	1119	1120	rBV2	296	379	0.04%	0.004%
38	7.927	1120	1122	1123	rVV	489	382	0.04%	0.004%
39	7.964	1123	1128	1131	rVV5	1194	2584	0.25%	0.028%
40	8.257	1174	1176	1178	rBV	512	611	0.06%	0.007%
41	8.330	1181	1188	1202	rVV	132881	226517	21.60%	2.413%
42	8.580	1227	1229	1233	rBV3	490	801	0.08%	0.009%
43	8.653	1233	1241	1252	rBV	537573	831912	79.34%	8.863%
44	8.958	1285	1291	1301	rBV	96051	147608	14.08%	1.573%
45	9.086	1311	1312	1314	rBV2	515	433	0.04%	0.005%
46	9.110	1314	1316	1324	rVB3	942	1735	0.17%	0.018%
47	9.177	1324	1327	1329	rBV	352	388	0.04%	0.004%
48	9.208	1329	1332	1334	rBV2	365	392	0.04%	0.004%
49	9.275	1337	1343	1350	rBV	246588	360063	34.34%	3.836%
50	9.397	1357	1363	1379	rBV	358533	575188	54.85%	6.128%
51	9.653	1404	1405	1408	rBV	533	452	0.04%	0.005%
52	9.714	1411	1415	1420	rVB2	2746	4030	0.38%	0.043%
53	9.811	1430	1431	1432	rBV	769	370	0.04%	0.004%
54	9.866	1438	1440	1443	rVB2	635	680	0.06%	0.007%
55	10.055	1465	1471	1480	rBV	659337	885387	84.44%	9.433%
56	10.250	1502	1503	1505	rBV2	529	366	0.03%	0.004%
57	10.299	1509	1511	1512	rVV	503	390	0.04%	0.004%
58	10.342	1516	1518	1520	rVB2	553	463	0.04%	0.005%
59	10.488	1538	1542	1543	rBV	367	402	0.04%	0.004%
60	10.713	1576	1579	1581	rVV	268	399	0.04%	0.004%
61	10.908	1610	1611	1614	rBV	476	368	0.04%	0.004%
62	11.195	1652	1658	1667	rBV	379029	467029	44.54%	4.976%
63	11.347	1681	1683	1684	rBV	557	424	0.04%	0.005%
64	11.384	1687	1689	1691	rVV	490	374	0.04%	0.004%
65	11.463	1695	1702	1703	rBV2	776	967	0.09%	0.010%
66	11.482	1703	1705	1709	rVB2	1001	928	0.09%	0.010%
67	11.518	1709	1711	1714	rBV2	572	597	0.06%	0.006%
68	11.561	1717	1718	1721	rBV2	512	580	0.06%	0.006%
69	11.750	1747	1749	1750	rBV2	495	372	0.04%	0.004%
70	11.860	1765	1767	1770	rBV2	325	371	0.04%	0.004%
71	12.024	1789	1794	1805	rBV	647003	770435	73.47%	8.208%
72	12.140	1810	1813	1816	rVB3	856	960	0.09%	0.010%
73	12.177	1816	1819	1821	rBV2	333	451	0.04%	0.005%
74	12.195	1821	1822	1825	rBV2	579	479	0.05%	0.005%
75	12.323	1837	1843	1852	rBV	555946	683076	65.14%	7.277%
76	12.500	1871	1872	1874	rBV	802	504	0.05%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030477.D
 Acq On : 06 Aug 2022 20:14
 Operator : JC/MD
 Sample : N4066-05DL 4X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E25DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.567	1878	1883	1885	rBV2	633	833	0.08%	0.009%
78	12.878	1930	1934	1937	rVV2	599	884	0.08%	0.009%
79	13.054	1960	1963	1965	rBV	451	559	0.05%	0.006%
80	13.262	1994	1997	1999	rBV	586	497	0.05%	0.005%
81	13.292	1999	2002	2005	rVV2	336	535	0.05%	0.006%
82	13.506	2035	2037	2040	rBV2	489	512	0.05%	0.005%
83	13.634	2057	2058	2061	rVB	618	475	0.05%	0.005%
84	13.670	2061	2064	2066	rVB2	557	728	0.07%	0.008%
85	13.926	2104	2106	2109	rVB2	657	721	0.07%	0.008%
86	13.963	2109	2112	2114	rBV2	645	912	0.09%	0.010%
87	14.298	2165	2167	2169	rVB	524	434	0.04%	0.005%
88	14.323	2169	2171	2173	rBV2	430	423	0.04%	0.005%
89	14.530	2200	2205	2210	rVB	843	1309	0.12%	0.014%
90	14.566	2210	2211	2214	rBV2	585	599	0.06%	0.006%
91	14.597	2214	2216	2219	rBV3	399	394	0.04%	0.004%
92	15.005	2277	2283	2285	rBV3	725	1221	0.12%	0.013%
93	15.188	2311	2313	2317	rVB3	816	915	0.09%	0.010%
94	15.316	2332	2334	2336	rVB2	820	503	0.05%	0.005%
95	15.481	2359	2361	2364	rBV3	500	639	0.06%	0.007%
96	15.902	2428	2430	2434	rVB3	622	390	0.04%	0.004%
97	15.932	2434	2435	2438	rBV3	660	571	0.05%	0.006%
98	16.304	2495	2496	2499	rBV3	696	513	0.05%	0.005%
99	16.505	2528	2529	2531	rBV	593	482	0.05%	0.005%
100	16.615	2545	2547	2551	rVB2	748	694	0.07%	0.007%




Sum of corrected areas: 9386306

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030477.D
Acq On : 06 Aug 2022 20:14
Operator : JC/MD
Sample : N4066-05DL 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E25DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

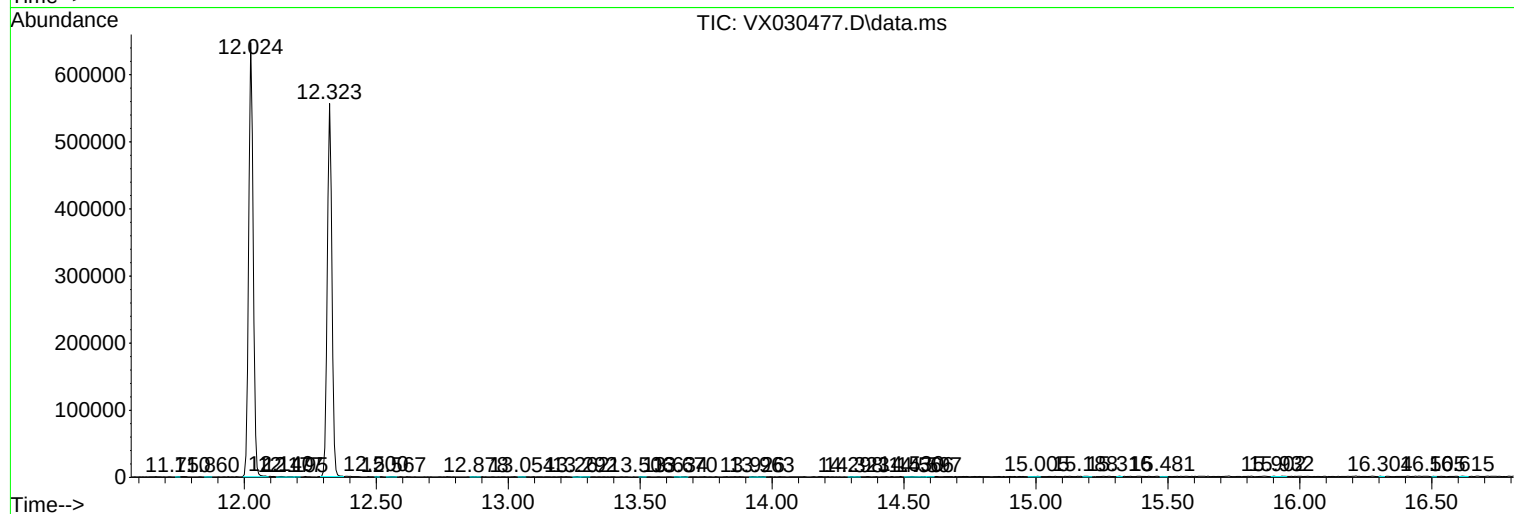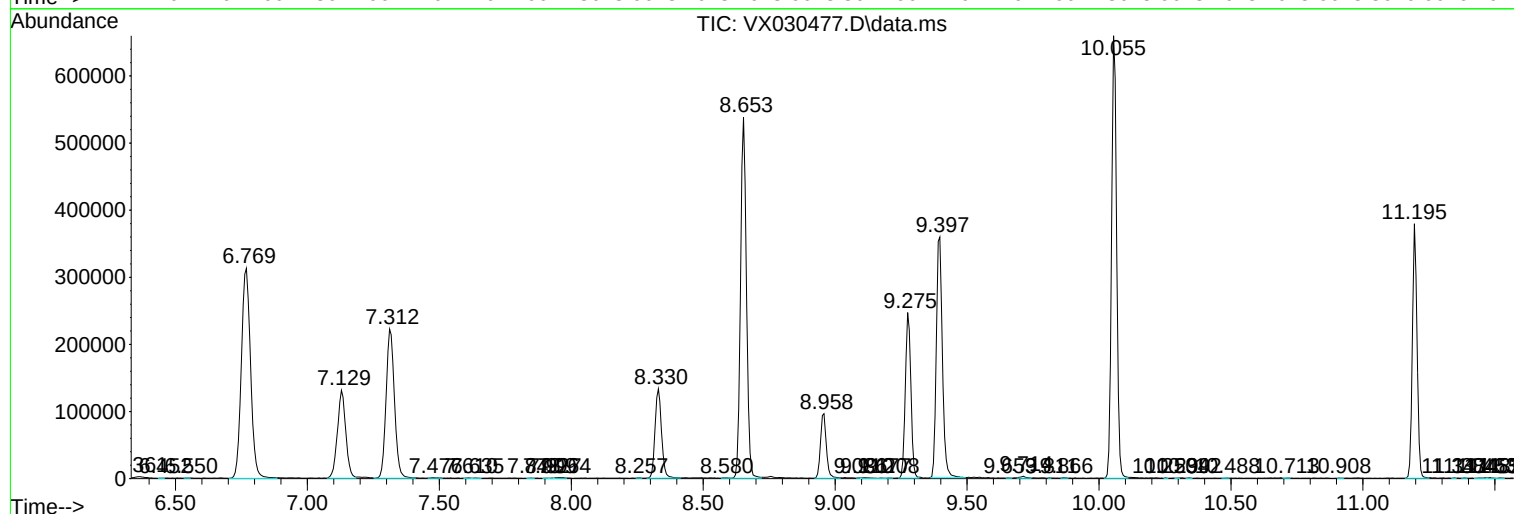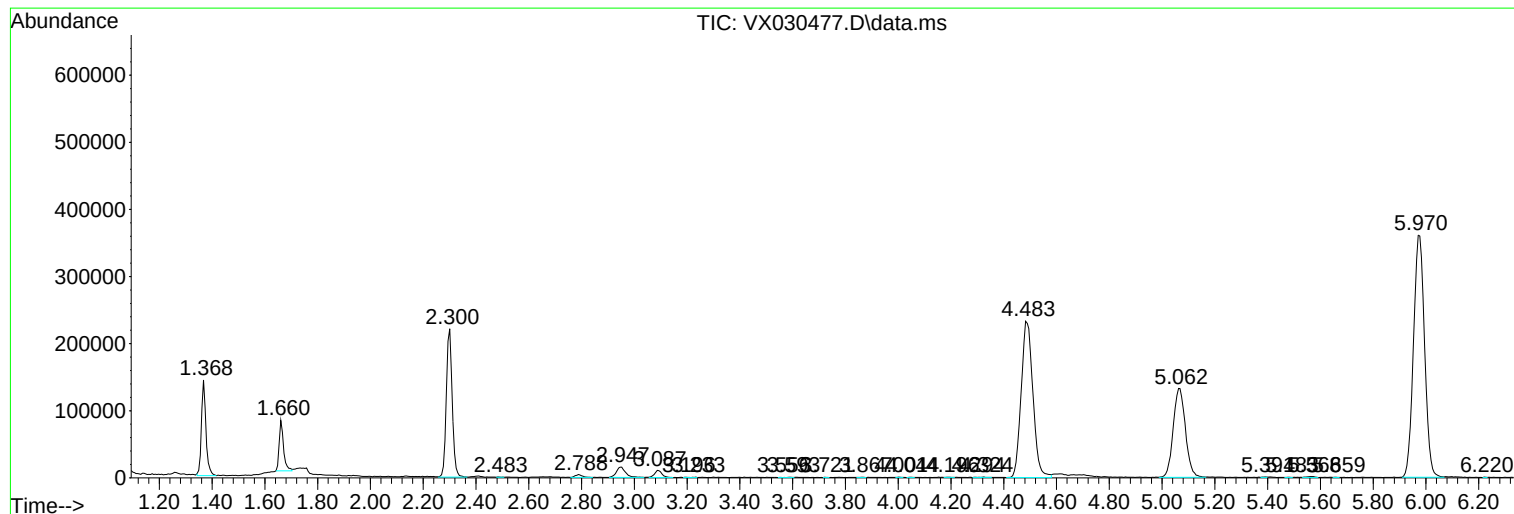

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030477.D
Acq On : 06 Aug 2022 20:14
Operator : JC/MD
Sample : N4066-05DL 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E25DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030477.D
Acq On : 06 Aug 2022 20:14
Operator : JC/MD
Sample : N4066-05DL 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E25DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc