

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030479.D
 Acq On : 06 Aug 2022 21:24
 Operator : JC/MD
 Sample : VX0806WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK672

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030479.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rVB	120002	122170	11.90%	1.497%
2	1.666	91	95	102	rVB	109377	126459	12.32%	1.549%
3	2.306	194	200	210	rVB	205022	318339	31.02%	3.900%
4	2.508	230	233	237	rVB2	2983	4202	0.41%	0.051%
5	2.690	261	263	272	rVB2	534	703	0.07%	0.009%
6	2.794	275	280	287	rVB3	3014	5152	0.50%	0.063%
7	2.947	298	305	313	rBV	4875	10971	1.07%	0.134%
8	3.093	325	329	335	rVB5	1718	2596	0.25%	0.032%
9	3.184	341	344	346	rBV2	674	866	0.08%	0.011%
10	3.300	360	363	368	rBV3	417	934	0.09%	0.011%
11	3.611	412	414	417	rVV3	440	461	0.04%	0.006%
12	3.666	420	423	425	rVB	367	345	0.03%	0.004%
13	3.727	431	433	435	rBV2	339	411	0.04%	0.005%
14	4.056	485	487	489	rVB2	425	351	0.03%	0.004%
15	4.074	489	490	494	rVB	475	353	0.03%	0.004%
16	4.184	506	508	511	rBV2	306	408	0.04%	0.005%
17	4.373	536	539	541	rBV3	427	518	0.05%	0.006%
18	4.471	546	555	568	rBV	101781	299548	29.19%	3.670%
19	4.745	597	600	604	rVB4	641	965	0.09%	0.012%
20	5.068	642	653	666	rBV	141048	426848	41.59%	5.229%
21	5.324	692	695	698	rVV	498	714	0.07%	0.009%
22	5.446	713	715	717	rBV2	697	864	0.08%	0.011%
23	5.568	727	735	738	rBV3	939	2195	0.21%	0.027%
24	5.666	749	751	754	rBV2	637	800	0.08%	0.010%
25	5.976	788	802	819	rBV2	346338	1026210	100.00%	12.572%
26	6.312	854	857	860	rVB2	522	692	0.07%	0.008%
27	6.348	860	863	865	rBV2	529	720	0.07%	0.009%
28	6.769	923	932	949	rVV	315382	717548	69.92%	8.791%
29	6.897	951	953	955	rVB2	768	503	0.05%	0.006%
30	7.116	981	989	998	rBV5	14043	32930	3.21%	0.403%
31	7.312	1012	1021	1039	rVV	219673	491638	47.91%	6.023%
32	7.732	1087	1090	1093	rBV2	580	559	0.05%	0.007%
33	7.933	1121	1123	1125	rBV	546	418	0.04%	0.005%
34	8.330	1179	1188	1197	rBV	134259	221018	21.54%	2.708%
35	8.592	1229	1231	1233	rVB2	729	527	0.05%	0.006%
36	8.653	1233	1241	1251	rBV	493070	755163	73.59%	9.251%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030479.D
 Acq On : 06 Aug 2022 21:24
 Operator : JC/MD
 Sample : VX0806WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK672

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	8.817	1266	1268	1271	rVB3	576	506	0.05%	0.006%
38	8.952	1284	1290	1301	rBV	94911	146797	14.30%	1.798%
39	9.104	1313	1315	1318	rBV	446	467	0.05%	0.006%
40	9.128	1318	1319	1322	rVB3	485	412	0.04%	0.005%
41	9.159	1322	1324	1327	rVB2	534	515	0.05%	0.006%
42	9.232	1334	1336	1340	rBV2	368	390	0.04%	0.005%
43	9.281	1340	1344	1350	rVB3	2925	4484	0.44%	0.055%
44	9.390	1356	1362	1374	rBV	444114	643751	62.73%	7.887%
45	9.701	1410	1413	1419	rBV5	2332	4020	0.39%	0.049%
46	9.878	1441	1442	1446	rVB3	685	737	0.07%	0.009%
47	9.915	1446	1448	1451	rBV2	496	582	0.06%	0.007%
48	9.945	1451	1453	1456	rVV4	519	647	0.06%	0.008%
49	9.970	1456	1457	1459	rVB	725	361	0.04%	0.004%
50	10.055	1464	1471	1486	rBV	605506	817305	79.64%	10.013%
51	10.201	1490	1495	1499	rVB4	1853	2781	0.27%	0.034%
52	10.305	1509	1512	1516	rBV3	2757	3152	0.31%	0.039%
53	10.360	1519	1521	1524	rVB2	604	607	0.06%	0.007%
54	10.512	1542	1546	1547	rBV2	422	660	0.06%	0.008%
55	10.524	1547	1548	1550	rVB	637	385	0.04%	0.005%
56	10.585	1555	1558	1563	rVV3	642	1061	0.10%	0.013%
57	10.659	1565	1570	1577	rVV5	2737	5935	0.58%	0.073%
58	10.719	1577	1580	1582	rVV	379	461	0.04%	0.006%
59	10.744	1582	1584	1586	rVV3	531	426	0.04%	0.005%
60	10.908	1609	1611	1615	rVB2	302	417	0.04%	0.005%
61	10.969	1617	1621	1624	rBV3	2772	3416	0.33%	0.042%
62	11.097	1639	1642	1644	rBV	550	657	0.06%	0.008%
63	11.195	1652	1658	1665	rBV	414994	510142	49.71%	6.250%
64	11.384	1687	1689	1690	rBV	504	464	0.05%	0.006%
65	11.457	1698	1701	1704	rVV3	1953	2668	0.26%	0.033%
66	11.646	1730	1732	1737	rBV2	598	826	0.08%	0.010%
67	11.719	1742	1744	1746	rVV	529	480	0.05%	0.006%
68	11.756	1746	1750	1758	rVB3	2643	4500	0.44%	0.055%
69	11.853	1764	1766	1768	rBV2	371	449	0.04%	0.006%
70	11.908	1770	1775	1777	rVB3	455	798	0.08%	0.010%
71	11.933	1777	1779	1782	rBV2	469	366	0.04%	0.004%
72	11.975	1782	1786	1789	rBV3	3622	4900	0.48%	0.060%
73	12.024	1789	1794	1804	rVB	595807	721966	70.35%	8.845%
74	12.158	1814	1816	1819	rBV	617	540	0.05%	0.007%
75	12.323	1837	1843	1851	rVV	532830	659314	64.25%	8.077%
76	12.469	1865	1867	1869	rBV	449	545	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030479.D
 Acq On : 06 Aug 2022 21:24
 Operator : JC/MD
 Sample : VX0806WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK672

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.658	1896	1898	1901	rVB	569	602	0.06%	0.007%
78	12.689	1901	1903	1907	rBV2	508	606	0.06%	0.007%
79	12.817	1920	1924	1925	rBV2	450	544	0.05%	0.007%
80	12.945	1942	1945	1946	rBV	302	358	0.03%	0.004%
81	13.115	1969	1973	1979	rVB3	5276	6411	0.62%	0.079%
82	13.304	2002	2004	2006	rBV	588	463	0.05%	0.006%
83	13.365	2009	2014	2016	rBV2	505	665	0.06%	0.008%
84	13.396	2016	2019	2022	rBV2	502	652	0.06%	0.008%
85	13.439	2025	2026	2031	rVB2	501	530	0.05%	0.006%
86	13.591	2047	2051	2057	rVV5	5524	7037	0.69%	0.086%
87	13.719	2069	2072	2073	rBV2	394	376	0.04%	0.005%
88	13.786	2078	2083	2086	rVB	4591	6212	0.61%	0.076%
89	13.963	2108	2112	2120	rVB4	4918	6780	0.66%	0.083%
90	14.103	2132	2135	2138	rBV3	535	703	0.07%	0.009%
91	14.134	2138	2140	2142	rBV	401	443	0.04%	0.005%
92	14.194	2149	2150	2156	rVB2	510	519	0.05%	0.006%
93	14.353	2171	2176	2179	rBV	663	1053	0.10%	0.013%
94	14.444	2189	2191	2193	rBV	428	385	0.04%	0.005%
95	14.499	2198	2200	2202	rBV3	460	480	0.05%	0.006%
96	14.572	2210	2212	2215	rVB2	564	509	0.05%	0.006%
97	14.768	2242	2244	2245	rBV2	713	455	0.04%	0.006%
98	14.896	2263	2265	2266	rBV	704	653	0.06%	0.008%
99	16.664	2553	2555	2557	rVB	1260	815	0.08%	0.010%
100	16.688	2557	2559	2563	rBV2	931	1394	0.14%	0.017%

Sum of corrected areas: 8162634




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030479.D
Acq On : 06 Aug 2022 21:24
Operator : JC/MD
Sample : VX0806WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK672

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

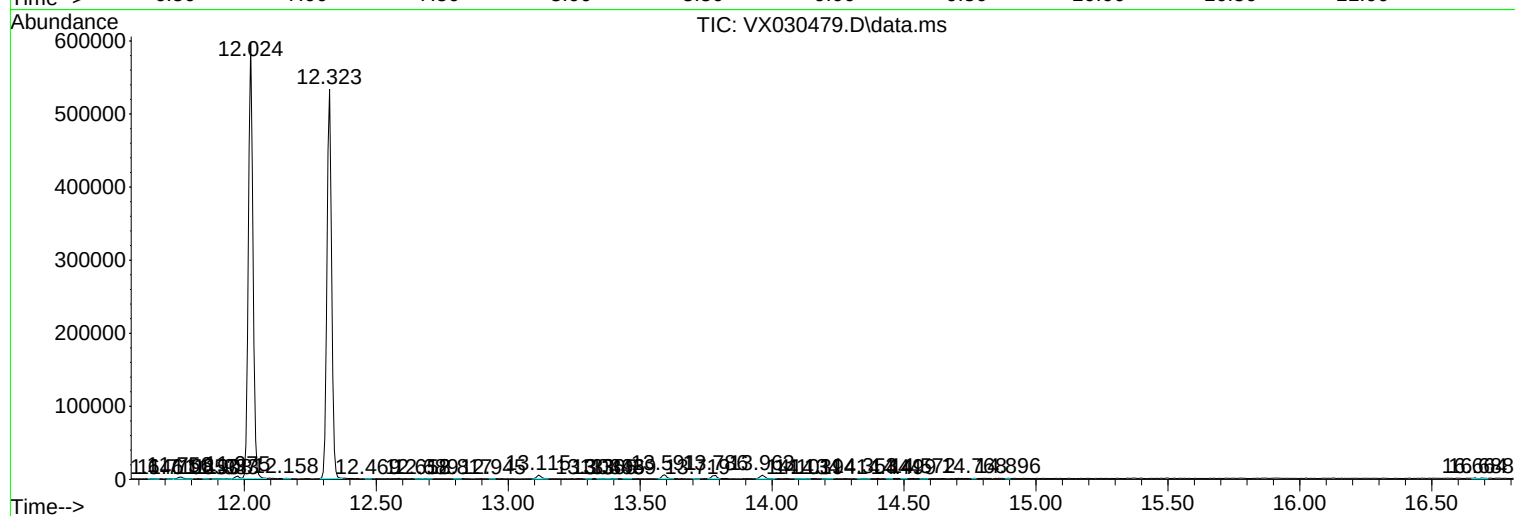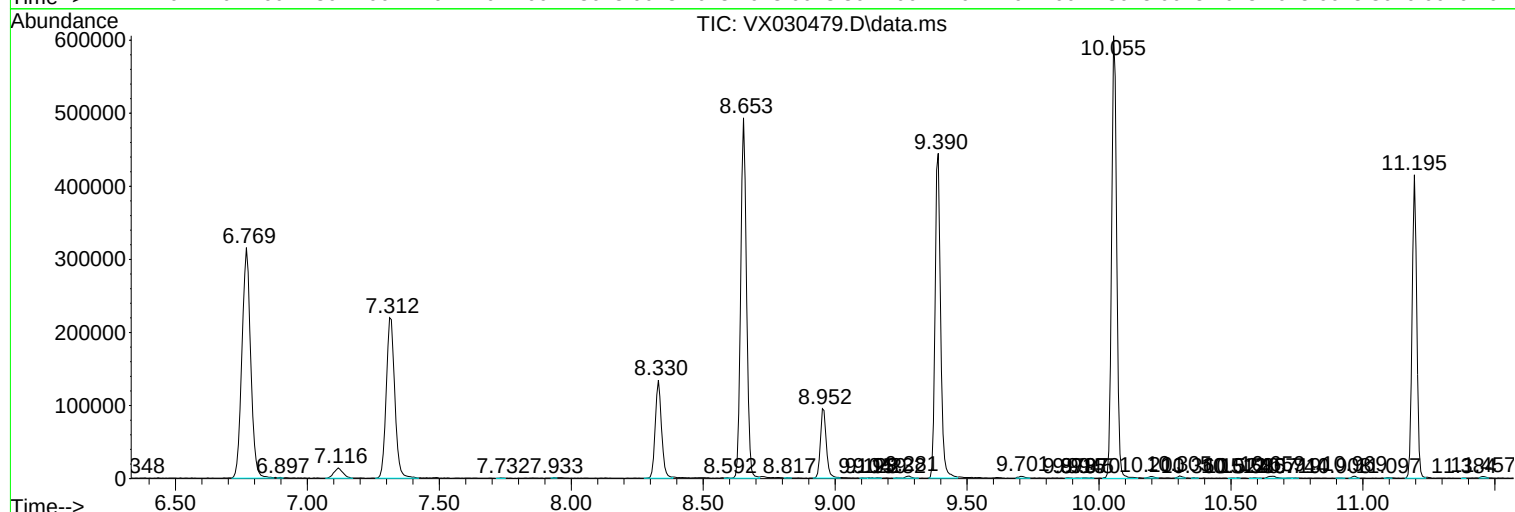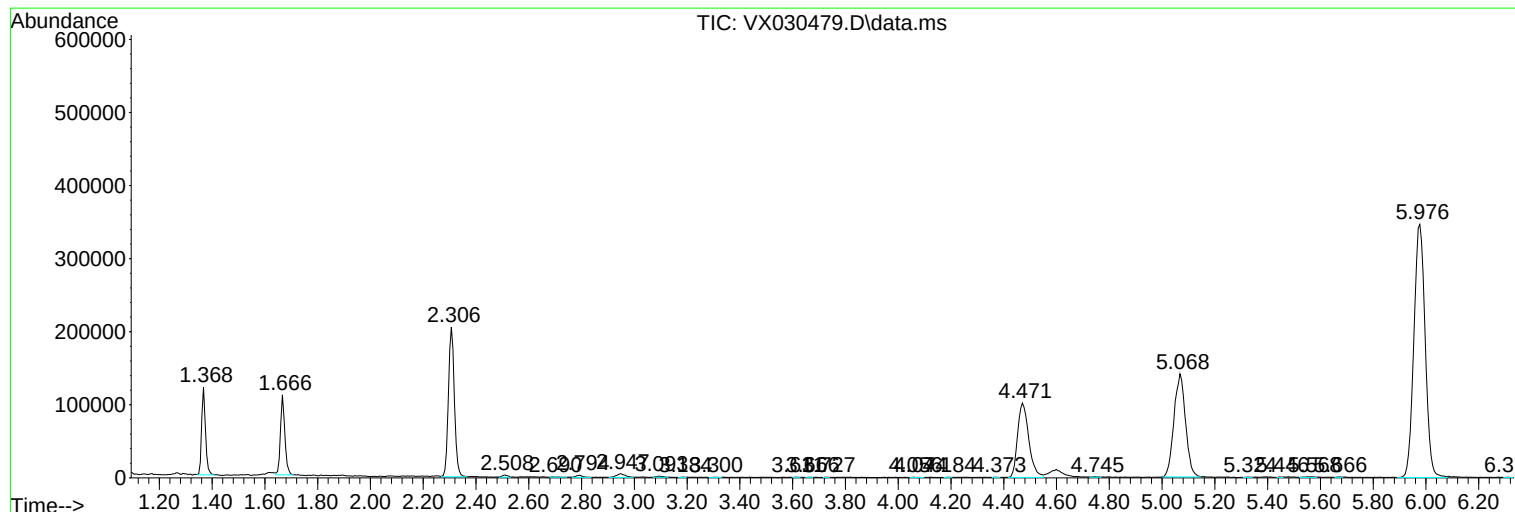

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030479.D
Acq On : 06 Aug 2022 21:24
Operator : JC/MD
Sample : VX0806WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK672

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030479.D
Acq On : 06 Aug 2022 21:24
Operator : JC/MD
Sample : VX0806WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK672

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc