

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030480.D
 Acq On : 06 Aug 2022 22:11
 Operator : JC/MD
 Sample : N4066-06DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E26DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030480.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	59	rVB	125620	142348	13.57%	1.566%
2	1.660	91	94	102	rBV	74456	93312	8.89%	1.026%
3	2.300	193	199	210	rVB	214334	326680	31.13%	3.593%
4	2.398	213	215	216	rBV	1266	788	0.08%	0.009%
5	2.508	229	233	236	rBV3	1282	1595	0.15%	0.018%
6	2.788	274	279	285	rBV3	4232	7451	0.71%	0.082%
7	2.904	295	298	299	rBV2	694	624	0.06%	0.007%
8	2.947	299	305	312	rBV	17295	36175	3.45%	0.398%
9	3.087	322	328	335	rVB3	1813	3541	0.34%	0.039%
10	3.282	358	360	363	rVB	623	410	0.04%	0.005%
11	3.373	373	375	378	rVB2	548	502	0.05%	0.006%
12	3.398	378	379	382	rBV	312	408	0.04%	0.004%
13	3.428	382	384	385	rVV	523	429	0.04%	0.005%
14	3.446	385	387	391	rVV2	763	784	0.07%	0.009%
15	3.501	395	396	399	rVB	427	350	0.03%	0.004%
16	3.532	399	401	404	rBV3	399	443	0.04%	0.005%
17	3.745	435	436	439	rVB2	526	458	0.04%	0.005%
18	4.257	518	520	521	rBV	580	474	0.05%	0.005%
19	4.391	538	542	543	rBV	498	496	0.05%	0.005%
20	4.483	546	557	572	rBV2	142132	459679	43.81%	5.055%
21	5.068	639	653	671	rBV2	137976	430078	40.99%	4.730%
22	5.275	685	687	689	rBV	533	460	0.04%	0.005%
23	5.544	729	731	732	rBV	1084	816	0.08%	0.009%
24	5.806	771	774	778	rVB	398	529	0.05%	0.006%
25	5.861	780	783	787	rVB2	441	560	0.05%	0.006%
26	5.976	789	802	817	rBV2	360360	1049312	100.00%	11.540%
27	6.196	835	838	841	rBV3	597	873	0.08%	0.010%
28	6.263	848	849	851	rBV	496	446	0.04%	0.005%
29	6.367	859	866	872	rBV6	2029	5243	0.50%	0.058%
30	6.543	890	895	896	rVV3	662	818	0.08%	0.009%
31	6.580	898	901	902	rVV2	502	478	0.05%	0.005%
32	6.769	922	932	946	rBV	308592	739539	70.48%	8.133%
33	7.129	982	991	1001	rBV	271306	612182	58.34%	6.733%
34	7.312	1013	1021	1037	rVV	216966	482034	45.94%	5.301%
35	7.610	1069	1070	1073	rBV2	494	388	0.04%	0.004%
36	7.769	1092	1096	1099	rBV3	584	935	0.09%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030480.D
 Acq On : 06 Aug 2022 22:11
 Operator : JC/MD
 Sample : N4066-06DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E26DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.891	1113	1116	1118	rBV2	617	845	0.08%	0.009%
38	8.250	1171	1175	1177	rBV2	428	433	0.04%	0.005%
39	8.330	1181	1188	1197	rBV	133293	224322	21.38%	2.467%
40	8.537	1219	1222	1225	rBV2	437	614	0.06%	0.007%
41	8.567	1225	1227	1228	rBV	632	440	0.04%	0.005%
42	8.653	1234	1241	1252	rBV	530473	815440	77.71%	8.968%
43	8.811	1265	1267	1269	rBV	598	491	0.05%	0.005%
44	8.952	1285	1290	1302	rBV	96111	146815	13.99%	1.615%
45	9.110	1314	1316	1317	rBV2	549	405	0.04%	0.004%
46	9.275	1337	1343	1351	rVB	122767	182692	17.41%	2.009%
47	9.397	1357	1363	1373	rBV	370178	578257	55.11%	6.360%
48	9.567	1389	1391	1393	rVB	734	561	0.05%	0.006%
49	9.708	1412	1414	1419	rVB3	2566	2973	0.28%	0.033%
50	10.055	1465	1471	1482	rBV	626134	866005	82.53%	9.524%
51	10.195	1492	1494	1497	rBV2	739	760	0.07%	0.008%
52	10.305	1509	1512	1514	rBV3	821	901	0.09%	0.010%
53	10.378	1521	1524	1525	rVB2	566	516	0.05%	0.006%
54	10.543	1548	1551	1553	rBV2	454	413	0.04%	0.005%
55	10.579	1553	1557	1559	rBV2	486	544	0.05%	0.006%
56	10.646	1566	1568	1573	rBV3	663	1032	0.10%	0.011%
57	10.768	1586	1588	1590	rVV2	485	386	0.04%	0.004%
58	10.823	1596	1597	1600	rVB2	394	349	0.03%	0.004%
59	10.896	1607	1609	1612	rBV2	339	402	0.04%	0.004%
60	10.927	1612	1614	1617	rVV3	450	425	0.04%	0.005%
61	10.963	1617	1620	1625	rVB2	623	952	0.09%	0.010%
62	11.024	1625	1630	1633	rBV4	531	755	0.07%	0.008%
63	11.067	1635	1637	1639	rVV2	410	382	0.04%	0.004%
64	11.091	1639	1641	1643	rVB2	728	561	0.05%	0.006%
65	11.195	1653	1658	1665	rBV	374549	462221	44.05%	5.083%
66	11.427	1692	1696	1698	rBV	449	568	0.05%	0.006%
67	11.457	1698	1701	1704	rVV3	613	709	0.07%	0.008%
68	11.488	1704	1706	1708	rVB2	586	446	0.04%	0.005%
69	11.524	1710	1712	1714	rBV2	388	346	0.03%	0.004%
70	11.622	1725	1728	1729	rBV	571	458	0.04%	0.005%
71	11.713	1740	1743	1744	rBV	373	437	0.04%	0.005%
72	11.939	1779	1780	1782	rBV	534	346	0.03%	0.004%
73	11.969	1782	1785	1788	rBV4	991	1333	0.13%	0.015%
74	12.024	1789	1794	1801	rBV	607312	738404	70.37%	8.121%
75	12.213	1822	1825	1826	rBV	624	616	0.06%	0.007%
76	12.323	1837	1843	1851	rBV	522424	641912	61.17%	7.060%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030480.D
 Acq On : 06 Aug 2022 22:11
 Operator : JC/MD
 Sample : N4066-06DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E26DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.500	1870	1872	1874	rBV2	457	435	0.04%	0.005%
78	12.524	1874	1876	1881	rBV	370	577	0.05%	0.006%
79	12.652	1895	1897	1901	rVB3	435	549	0.05%	0.006%
80	12.689	1901	1903	1906	rVB2	415	401	0.04%	0.004%
81	12.725	1906	1909	1912	rBV2	703	653	0.06%	0.007%
82	12.841	1927	1928	1932	rVB	657	512	0.05%	0.006%
83	12.878	1932	1934	1935	rBV2	480	374	0.04%	0.004%
84	12.896	1935	1937	1939	rBV2	412	407	0.04%	0.004%
85	12.963	1946	1948	1950	rBV	383	368	0.04%	0.004%
86	13.115	1971	1973	1976	rVB2	965	1195	0.11%	0.013%
87	13.207	1986	1988	1991	rBV2	355	415	0.04%	0.005%
88	13.256	1995	1996	1998	rBV	562	455	0.04%	0.005%
89	13.597	2049	2052	2055	rVB3	815	1039	0.10%	0.011%
90	13.725	2071	2073	2076	rVB3	432	385	0.04%	0.004%
91	13.774	2079	2081	2087	rVV3	1028	1659	0.16%	0.018%
92	13.963	2110	2112	2114	rBV	606	636	0.06%	0.007%
93	14.042	2123	2125	2130	rVB2	662	854	0.08%	0.009%
94	14.548	2206	2208	2210	rVB	822	498	0.05%	0.005%
95	14.664	2226	2227	2229	rBV	581	436	0.04%	0.005%
96	14.737	2237	2239	2242	rBV	496	396	0.04%	0.004%
97	16.109	2462	2464	2465	rVB	717	361	0.03%	0.004%
98	16.645	2548	2552	2553	rBV4	717	785	0.07%	0.009%
99	16.664	2553	2555	2557	rVB2	964	703	0.07%	0.008%
100	16.694	2558	2560	2564	rVB3	703	550	0.05%	0.006%




Sum of corrected areas: 9092748

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030480.D
Acq On : 06 Aug 2022 22:11
Operator : JC/MD
Sample : N4066-06DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E26DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

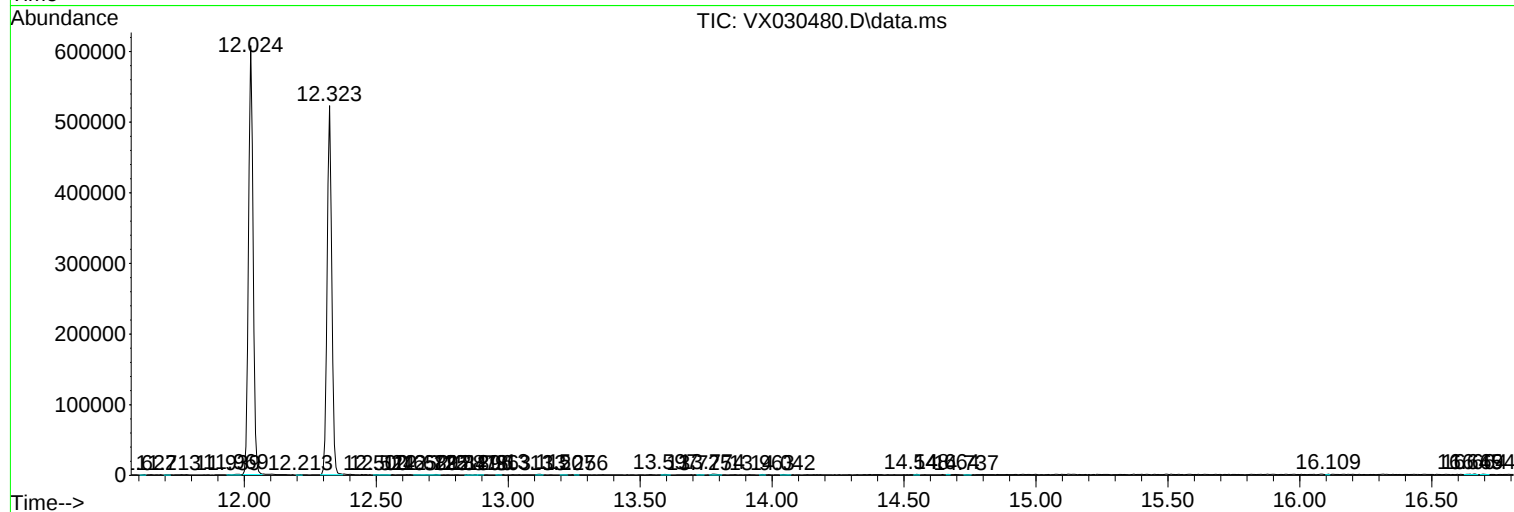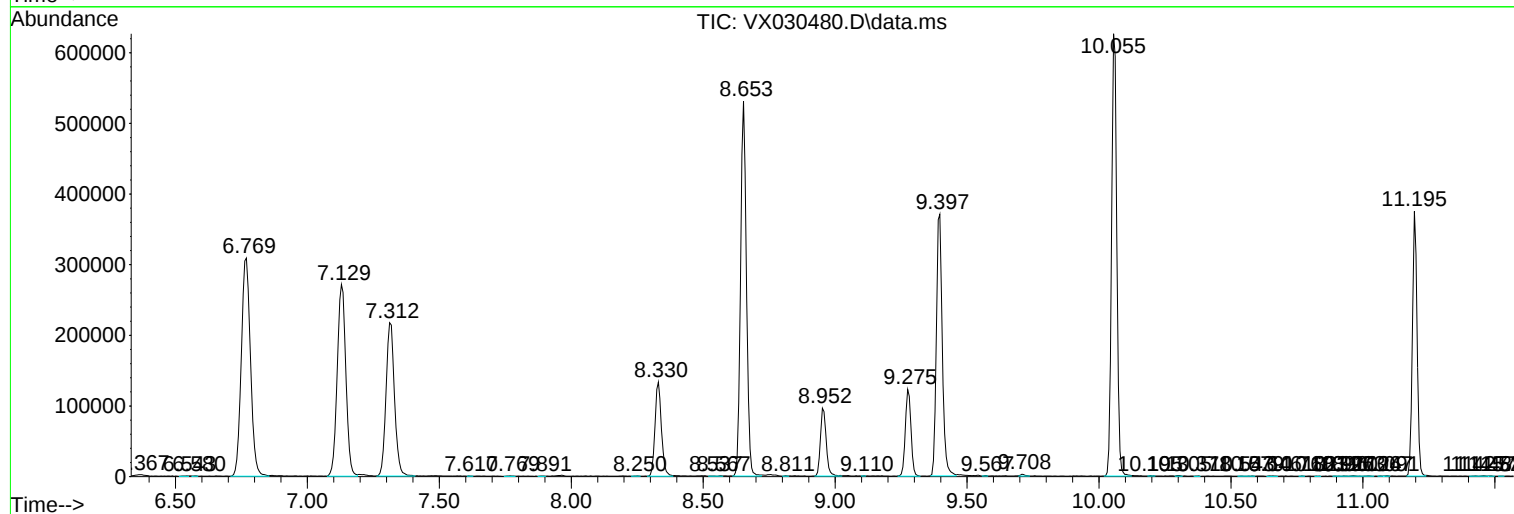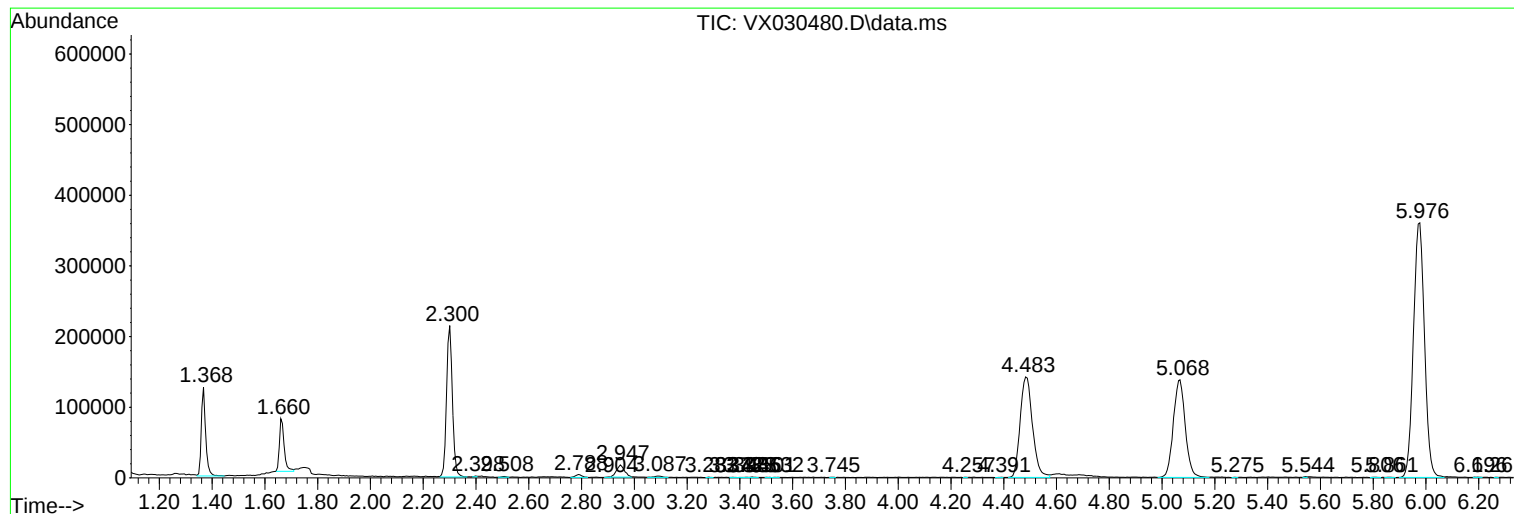

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030480.D
Acq On : 06 Aug 2022 22:11
Operator : JC/MD
Sample : N4066-06DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E26DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030480.D
Acq On : 06 Aug 2022 22:11
Operator : JC/MD
Sample : N4066-06DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E26DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc